


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061119\
Data File : BE099912.D
Acq On : 11 Jun 2019 7:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 14:57:20 2019

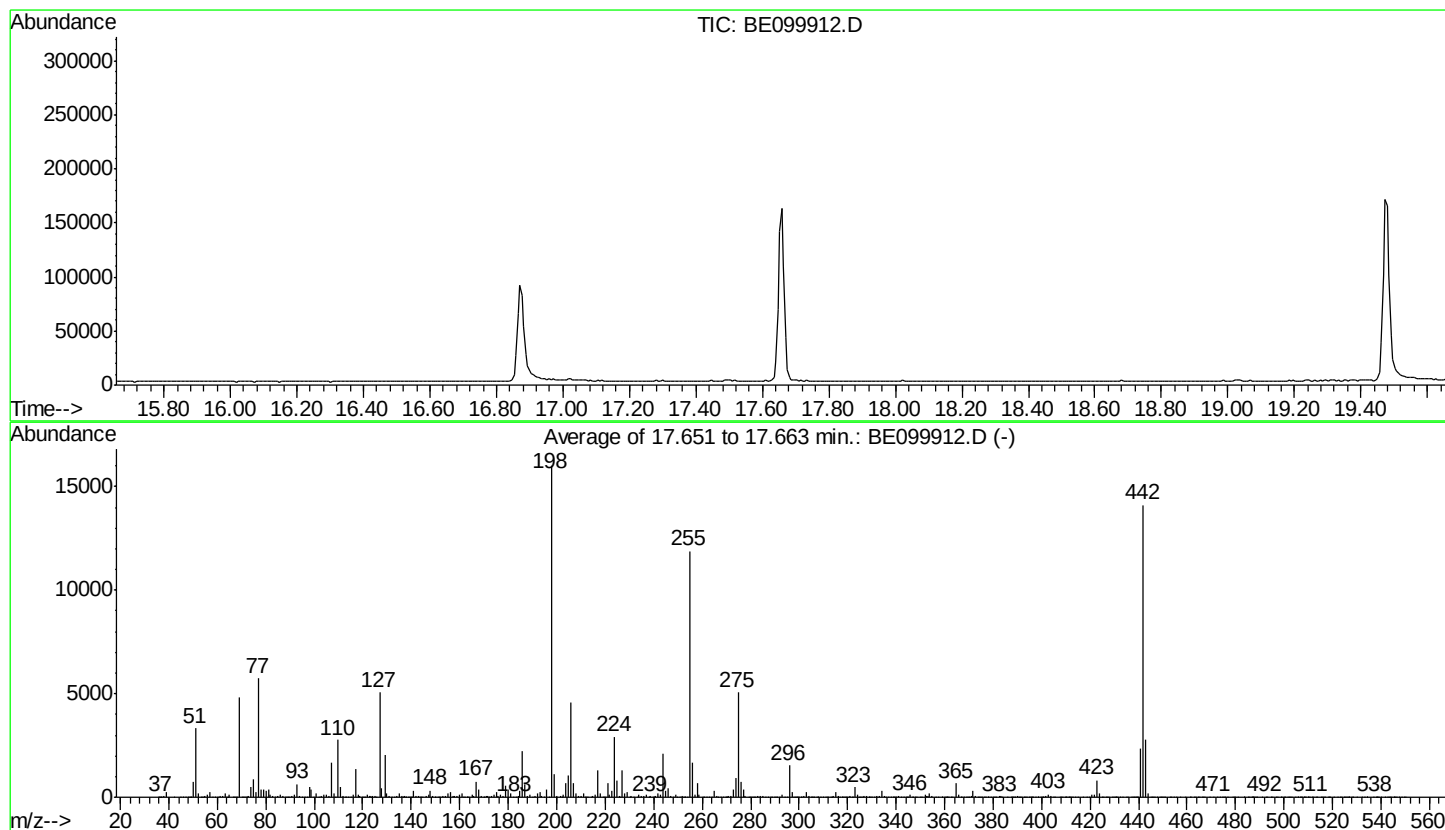

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	3316	PASS
68	69	0.00	2	0.7	32	PASS
69	198	0.00	100	30.2	4836	PASS
70	69	0.00	2	0.5	23	PASS
127	198	10	80	31.6	5061	PASS
197	198	0.00	2	0.1	24	PASS
198	198	100	100	100.0	16018	PASS
199	198	5	9	7.1	1135	PASS
275	198	10	60	31.6	5067	PASS
365	198	1	100	4.2	670	PASS
441	198	0.01	100	14.6	2344	PASS
442	198	50	100	88.2	14123	PASS
443	442	15	24	19.8	2790	PASS