


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061119\
 Data File : BE099926.D
 Acq On : 11 Jun 2019 16:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

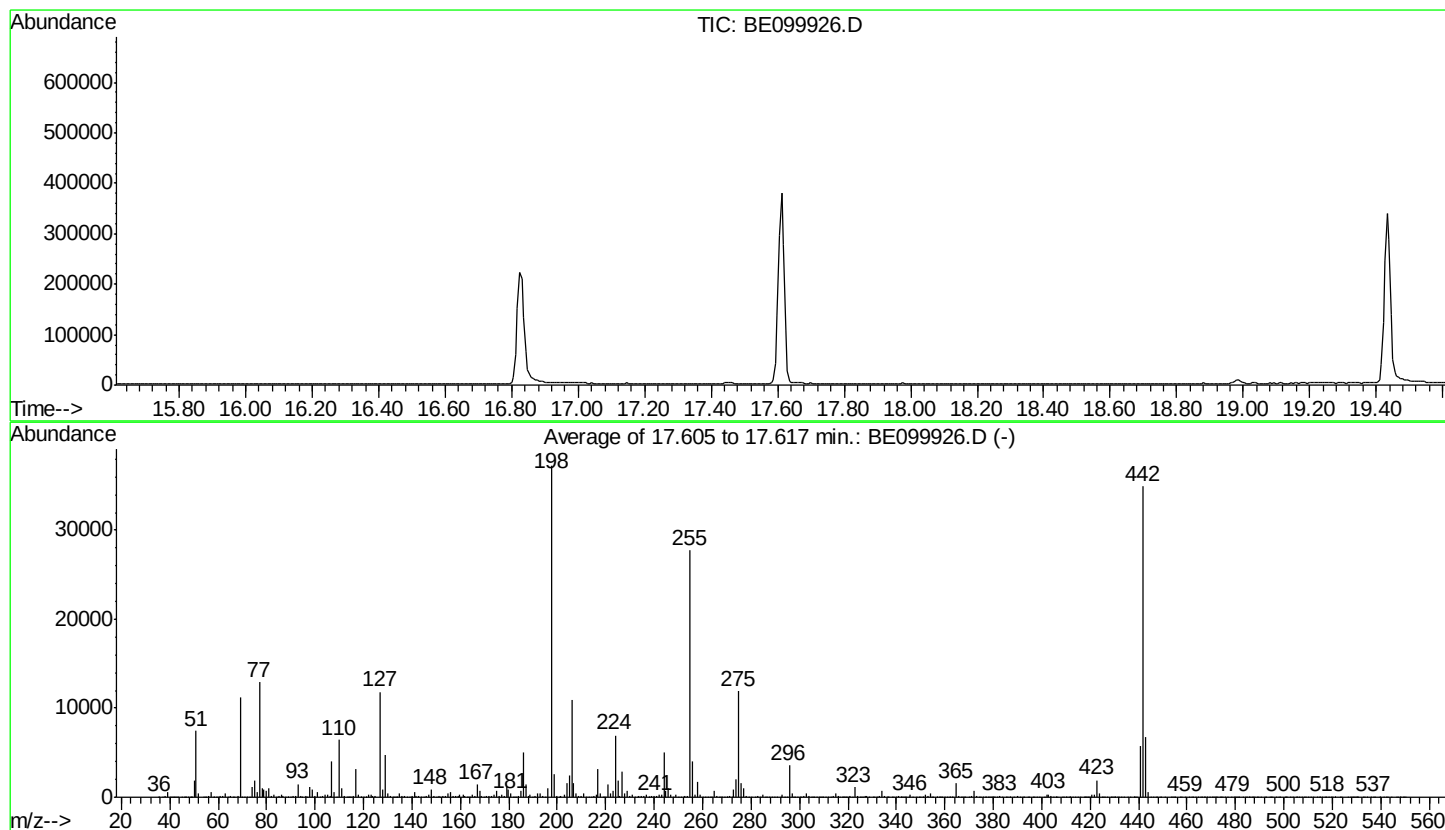

AutoFind: Scans 2556, 2557, 2558; Background Corrected with Scan 2548

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.0	7464	PASS
68	69	0.00	2	1.4	151	PASS
69	198	0.00	100	29.9	11157	PASS
70	69	0.00	2	0.7	73	PASS
127	198	10	80	31.7	11817	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37253	PASS
199	198	5	9	6.9	2558	PASS
275	198	10	60	32.0	11922	PASS
365	198	1	100	4.2	1548	PASS
441	198	0.01	100	15.4	5744	PASS
442	198	50	100	93.8	34928	PASS
443	442	15	24	19.2	6708	PASS