

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061219\
 Data File : BE099973.D
 Acq On : 13 Jun 2019 1:14
 Operator : JU/SJ
 Sample : K3255-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 RE126D3-20190604

Quant Time: Jun 13 05:48:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 10 14:57:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	1026	0.40	ng	-0.01
7) Naphthalene-d8	10.60	136	3490	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	2659	0.40	ng	0.00
19) Phenanthrene-d10	17.21	188	7582	0.40	ng	0.00
27) Chrysene-d12	21.39	240	10586	0.40	ng	-0.01
34) Perylene-d12	23.92	264	12165	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.35	112	379	0.14	ng	0.00
5) Phenol-d6	6.97	99	291	0.08	ng	0.00
8) Nitrobenzene-d5	8.98	82	1169	0.35	ng	0.01
11) 2-Methylnaphthalene-d10	12.21	152	2143	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.97	330	467	0.24	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	4313	0.43	ng	-0.02
25) Fluoranthene-d10	19.24	212	40728	0.37	ng	-0.01
29) Terphenyl-d14	19.84	244	10686	0.56	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.27	88	955	0.629	ng	Qvalue # 83
32) Bis(2-ethylhexyl)phthalate	21.29	149	4709	0.104	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061219\
Data File : BE099973.D
Acq On : 13 Jun 2019 1:14
Operator : JU/SJ
Sample : K3255-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
RE126D3-20190604

Quant Time: Jun 13 05:48:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 10 14:57:20 2019
Response via : Initial Calibration

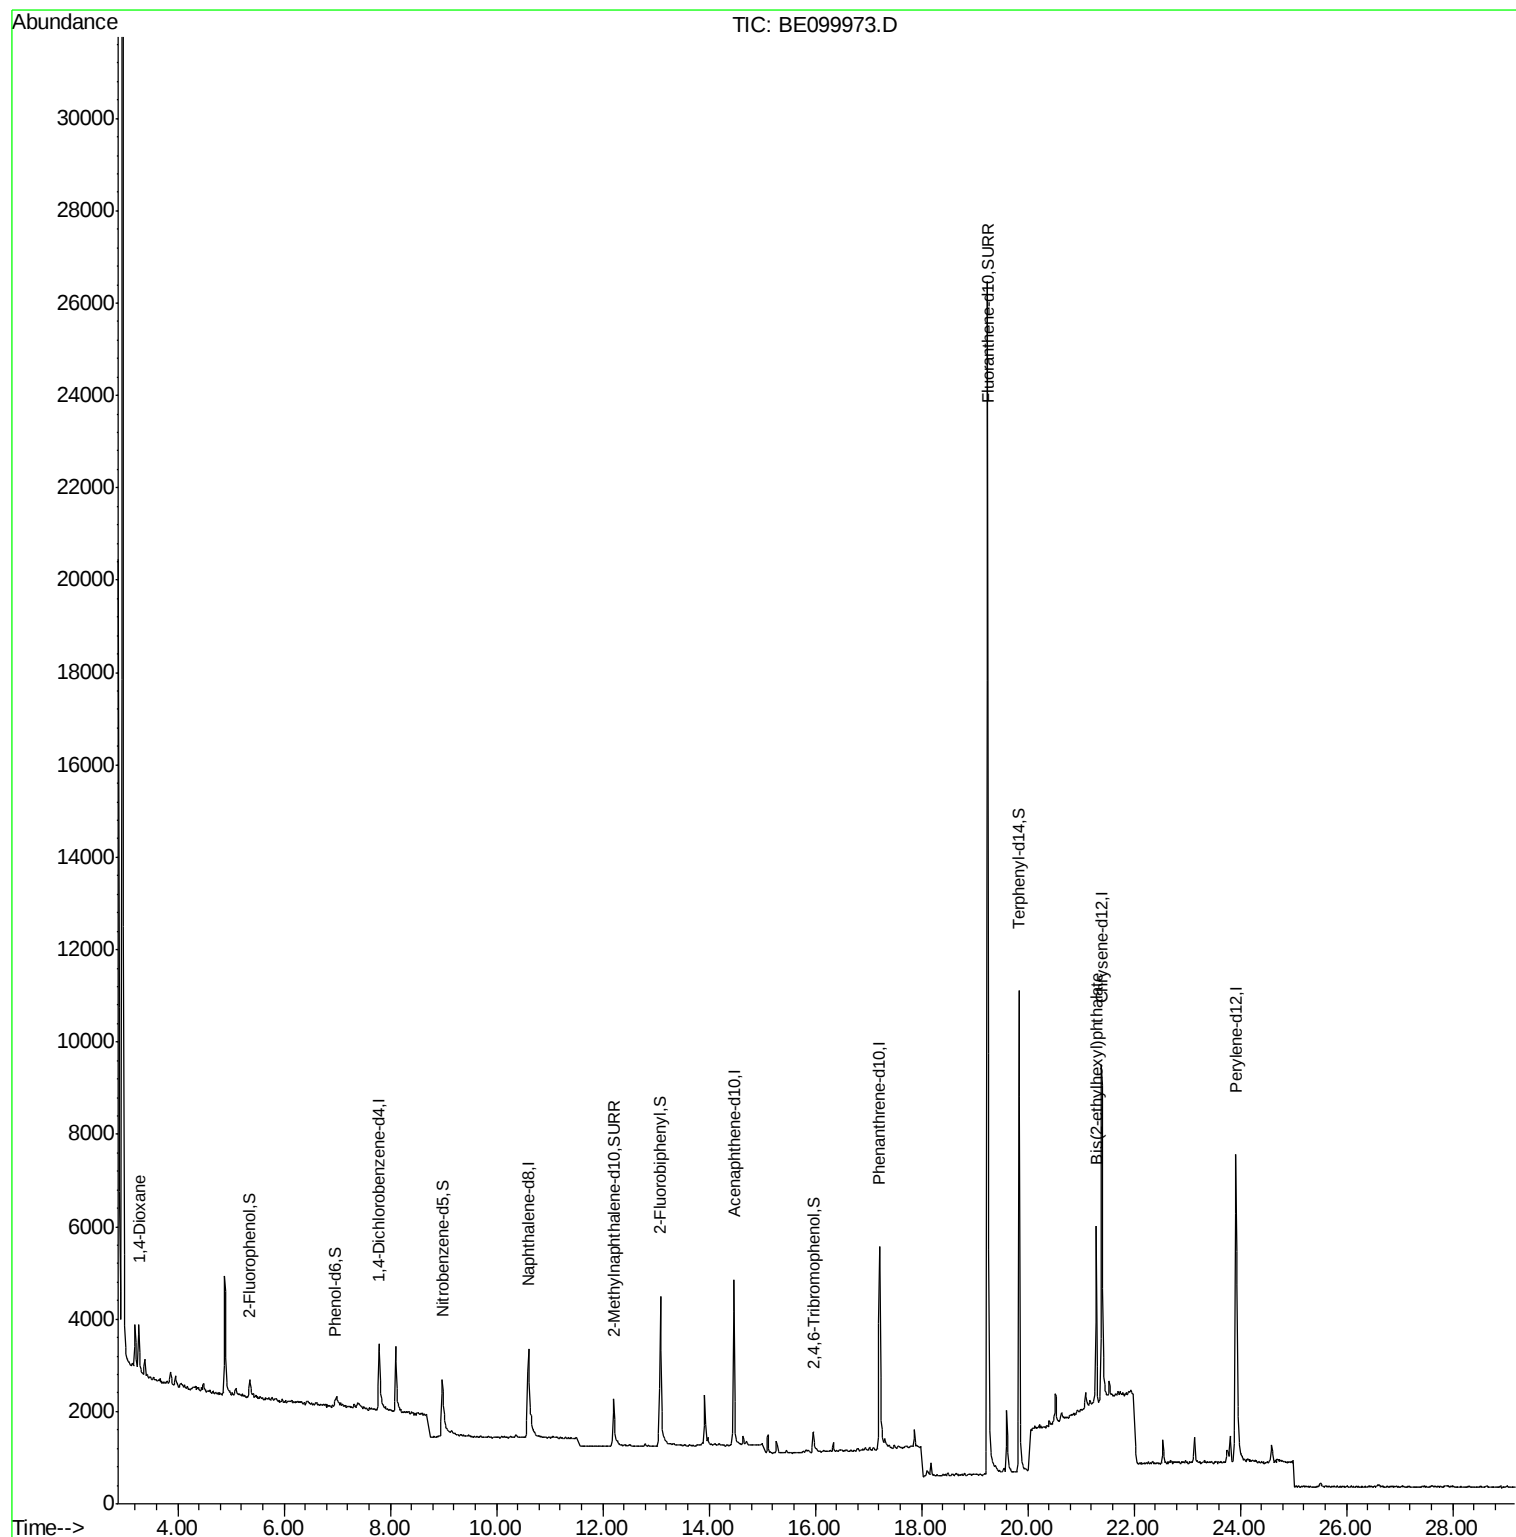

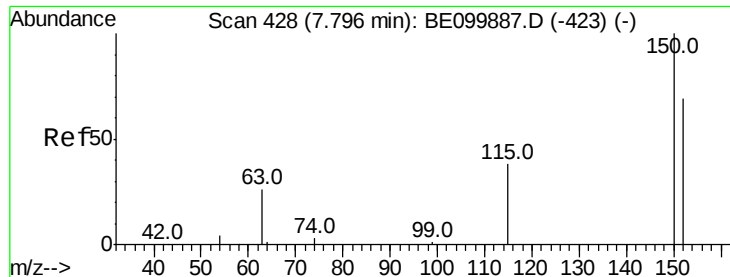


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.78 min Scan# 427
Delta R.T. -0.01 min
Lab File: BE099973.D
Acq: 13 Jun 2019 1:14

Instrument :
BNA_E
ClientSampleId :
RE126D3-20190604

Tot Ion:152 Resp: 1026
Ion Ratio Lower Upper
152 100
150 140.8 111.0 166.6
115 67.7 50.7 76.1

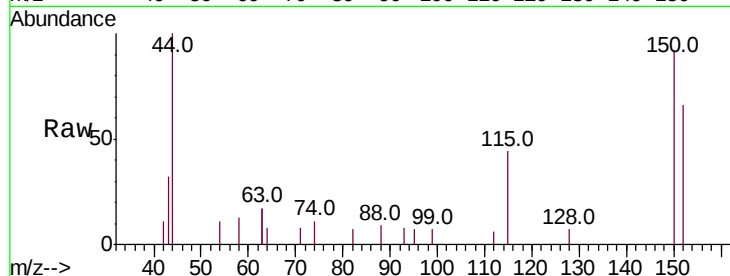


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

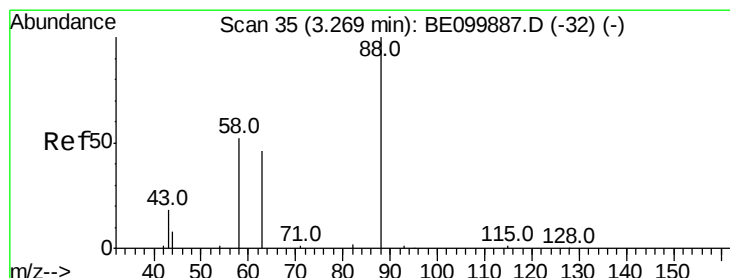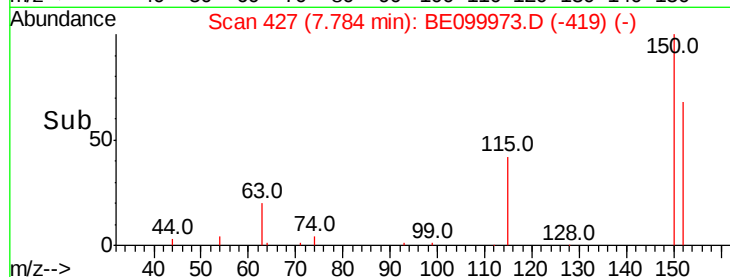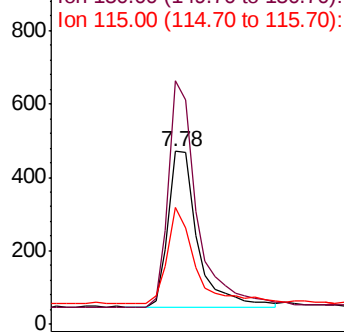



#2


1,4-Dioxane
Concen: 0.629 ng
RT: 3.27 min Scan# 35
Delta R.T. 0.00 min
Lab File: BE099973.D
Acq: 13 Jun 2019 1:14

Tgt Ion: 88 Resp: 955
Ion Ratio Lower Upper
88 100
58 51.1 48.8 73.2
43 37.8 19.0 28.6#

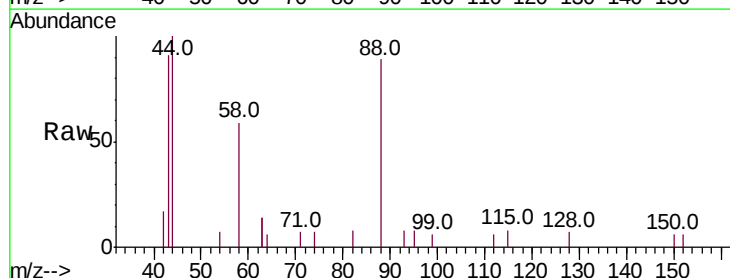

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

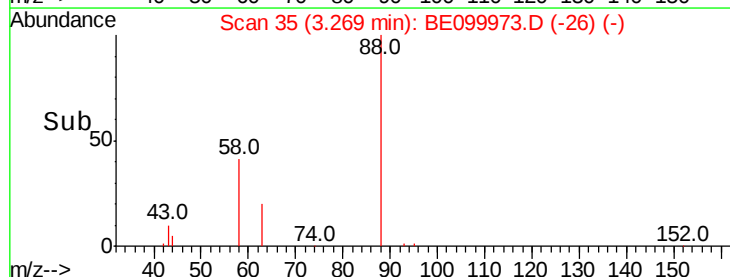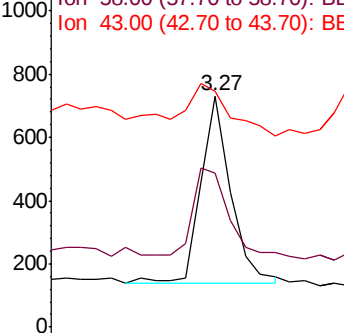

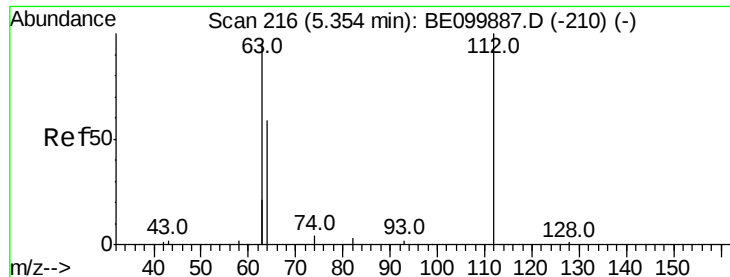

#4

2-Fluorophenol

Concen: 0.137 ng

RT: 5.35 min Scan# 216

Delta R.T. 0.00 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14

Instrument :

BNA_E

ClientSampleId :

RE126D3-20190604


Tot Ion:112 Resp: 379

Ion Ratio Lower Upper

112 100

64 52.2 44.1 66.1




63 118.5 87.8 131.6

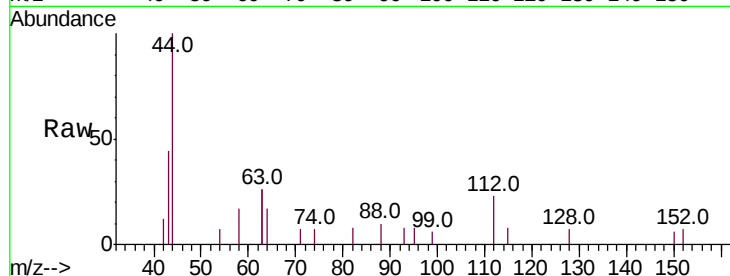

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

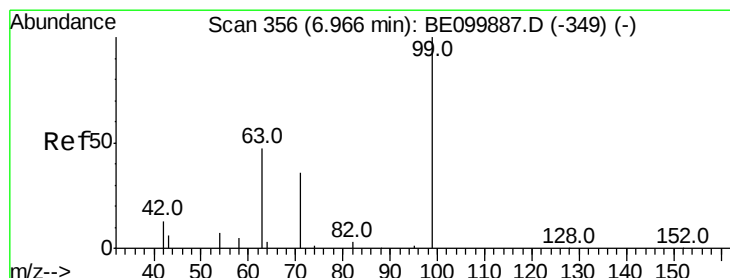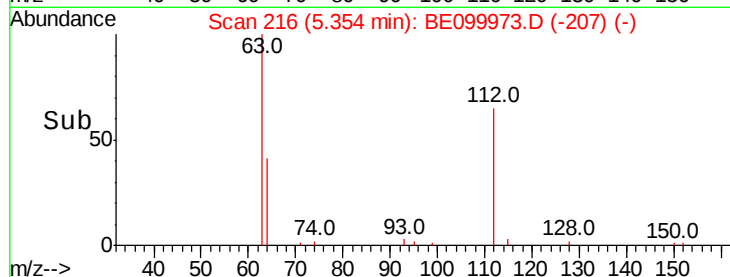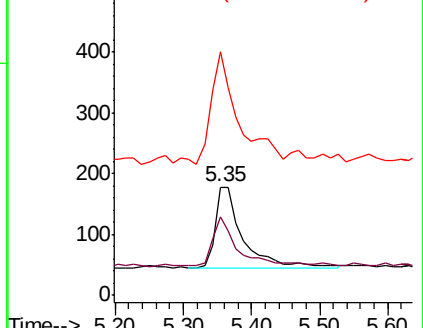

#5

Phenol-d6

Concen: 0.082 ng

RT: 6.97 min Scan# 356

Delta R.T. 0.00 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14


Tgt Ion: 99 Resp: 291

Ion Ratio Lower Upper

99 100

42 0.0 15.9 23.9#



71 38.8 34.6 52.0

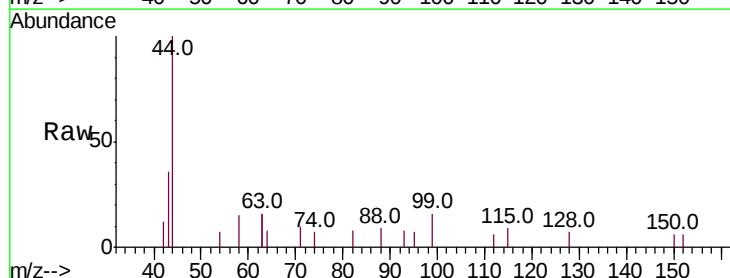


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

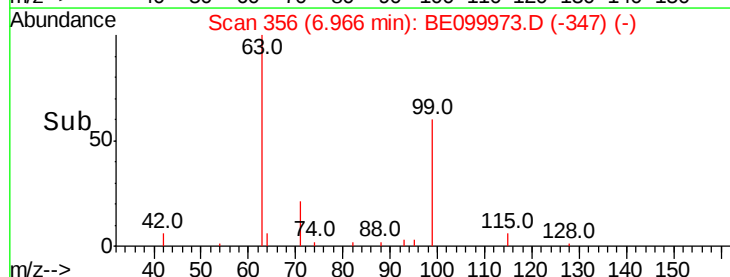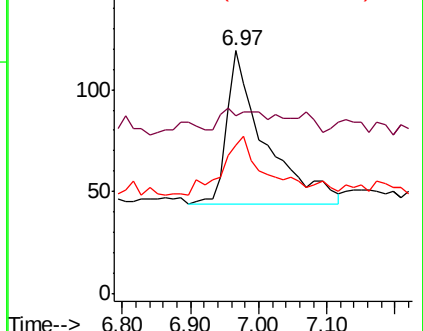



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. -0.00 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14

Instrument :

BNA_E

ClientSampleId :

RE126D3-20190604

Tot Ion: 136 Resp: 3490



Ion Ratio Lower Upper

136 100

137 13.6 12.3 18.5

54 32.5 28.2 42.4

68 8.1 7.8 11.8


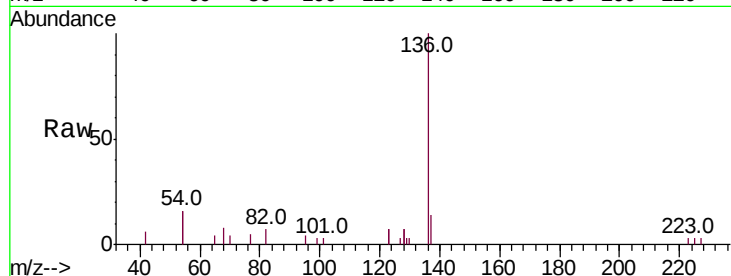


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

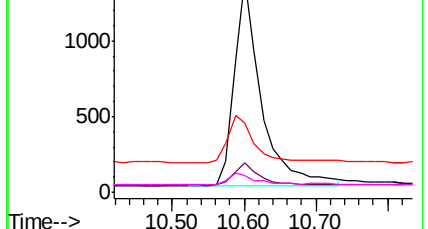

#8

Nitrobenzene-d5

Concen: 0.354 ng

RT: 8.98 min Scan# 524

Delta R.T. 0.01 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14



Tgt Ion: 82 Resp: 1169

Ion Ratio Lower Upper

82 100

128 179.6 137.3 205.9


54 168.5 129.7 194.5




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0




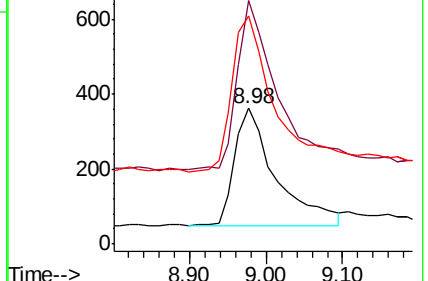


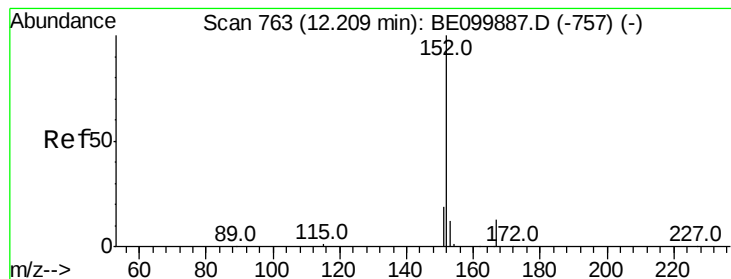

#11
 2-Methylnaphthalene-d10
 Concen: 0.352 ng
 RT: 12.21 min Scan# 763
 Delta R.T. -0.00 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14




Instrument :
 BNA_E
 ClientSampleId :
 RE126D3-20190604


Tot Ion:152 Resp: 2143
 Ion Ratio Lower Upper
 152 100
 151 20.3 15.2 22.8

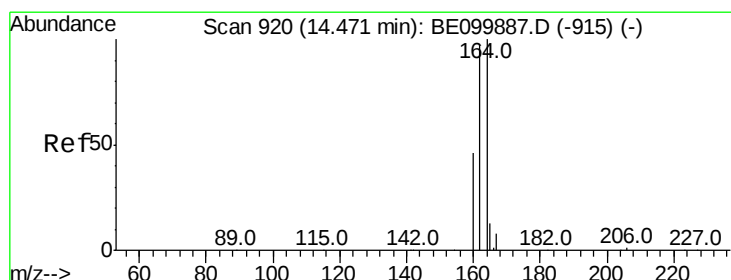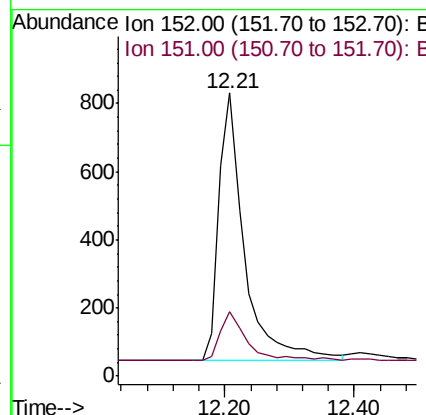

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.47 min Scan# 920
 Delta R.T. -0.00 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14

Tgt Ion:164 Resp: 2659
 Ion Ratio Lower Upper
 164 100
 162 97.7 77.8 116.8
 160 49.1 38.2 57.4

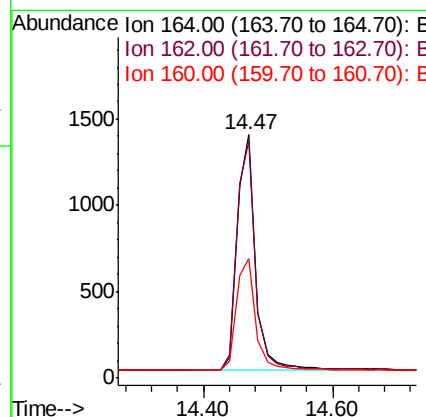







#14
 2,4,6-Tribromophenol
 Concen: 0.238 ng
 RT: 15.97 min Scan# 1026
 Delta R.T. -0.00 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14

Instrument :
 BNA_E
 ClientSampleId :
 RE126D3-20190604

Tot Ion:330 Resp: 467
 Ion Ratio Lower Upper
 330 100
 332 96.6 76.7 115.1
 141 27.8 21.0 31.6

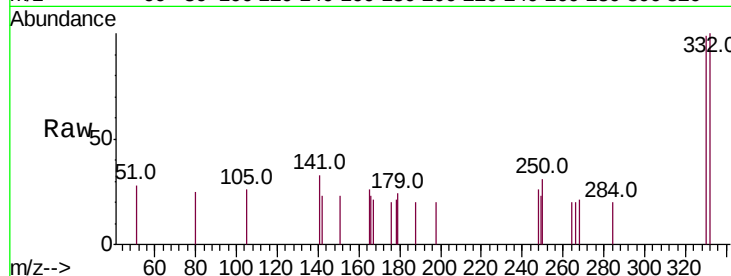


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

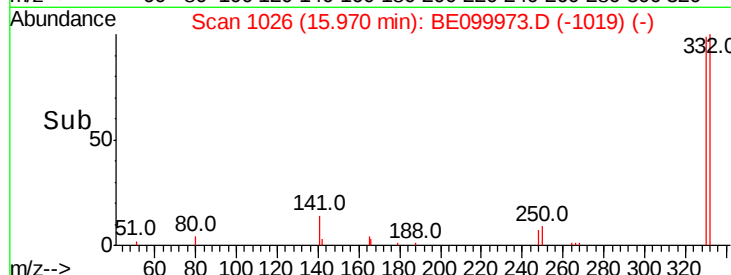
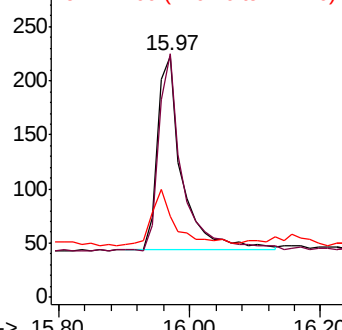



#15
 2-Fluorobiphenyl
 Concen: 0.428 ng
 RT: 13.09 min Scan# 824
 Delta R.T. -0.02 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14

Tgt Ion:172 Resp: 4313
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.2 43.8
 170 25.5 21.2 31.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

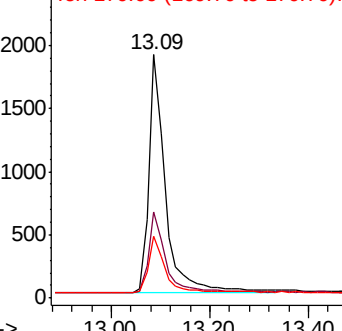

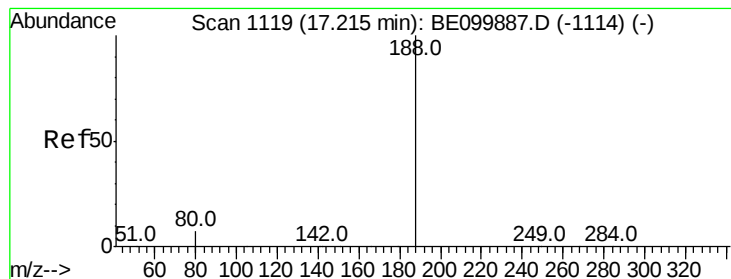

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.21 min Scan# 1119

Delta R.T. -0.00 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14

Instrument :

BNA_E

ClientSampleId :

RE126D3-20190604


Tot Ion:188 Resp: 7582

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 6.4 6.4 9.6



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

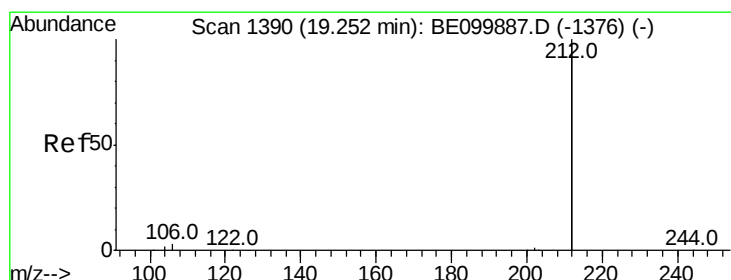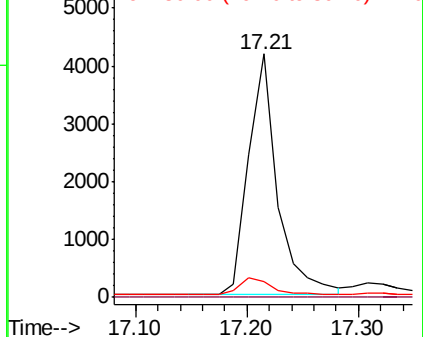

#25

Fluoranthene-d10

Concen: 0.369 ng

RT: 19.24 min Scan# 1388

Delta R.T. -0.01 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14


Tgt Ion:212 Resp: 40728

Ion Ratio Lower Upper

212 100

106 1.9 1.4 2.2



104 1.2 0.9 1.3




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

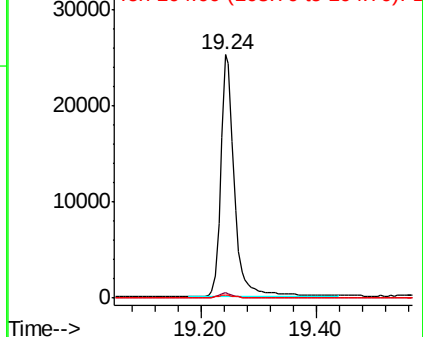







#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.39 min Scan# 1632
 Delta R.T. -0.01 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14

Instrument :
 BNA_E
 ClientSampleId :
 RE126D3-20190604

Tot Ion:240 Resp: 10586
 Ion Ratio Lower Upper
 240 100
 120 8.7 3.8 5.6#
 236 28.5 22.0 33.0

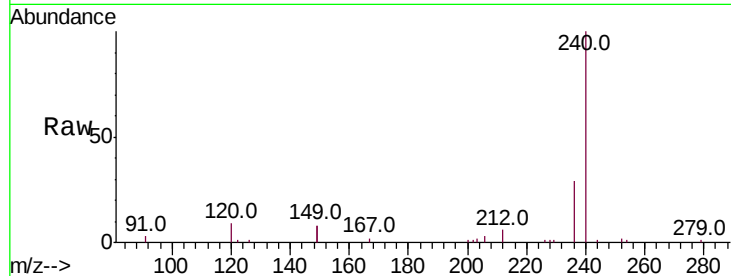


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E


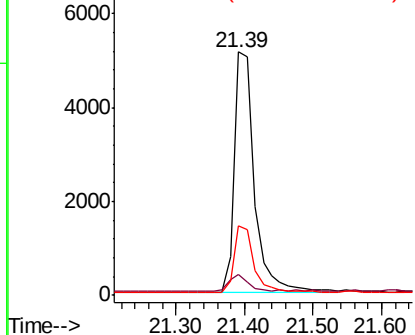



#29
 Terphenyl-d14
 Concen: 0.561 ng
 RT: 19.84 min Scan# 1492
 Delta R.T. -0.01 min
 Lab File: BE099973.D
 Acq: 13 Jun 2019 1:14

Tgt Ion:244 Resp: 10686
 Ion Ratio Lower Upper
 244 100
 212 31.8 25.7 38.5
 122 6.5 5.5 8.3

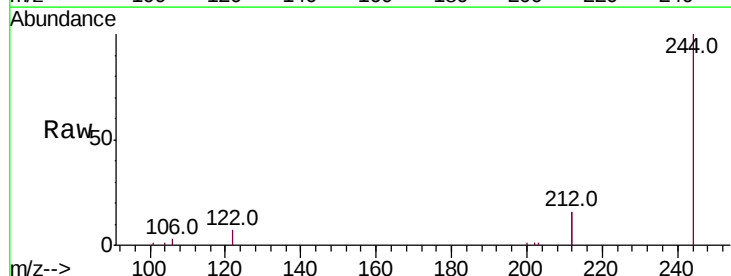

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

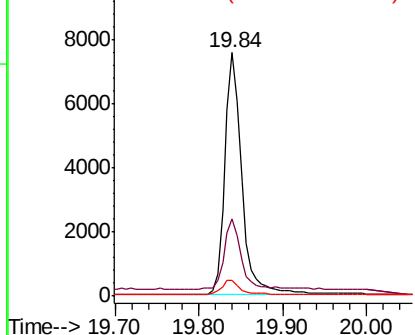



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.104 ng

RT: 21.29 min Scan# 1624

Delta R.T. 0.00 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14

Instrument :

BNA_E

ClientSampleId :

RE126D3-20190604


Tot Ion:149 Resp: 4709

Ion Ratio Lower Upper

149 100

167 7.5 5.9 8.9




279 1.3 1.2 1.8



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

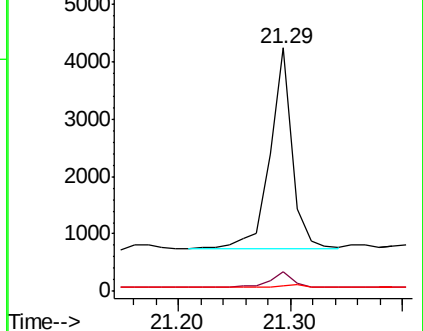

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.92 min Scan# 2215

Delta R.T. -0.01 min

Lab File: BE099973.D

Acq: 13 Jun 2019 1:14


Tgt Ion:264 Resp: 12165

Ion Ratio Lower Upper

264 100

260 25.6 20.2 30.2

265 29.2 22.0 33.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

