


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061219\
 Data File : BE099945.D
 Acq On : 12 Jun 2019 7:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

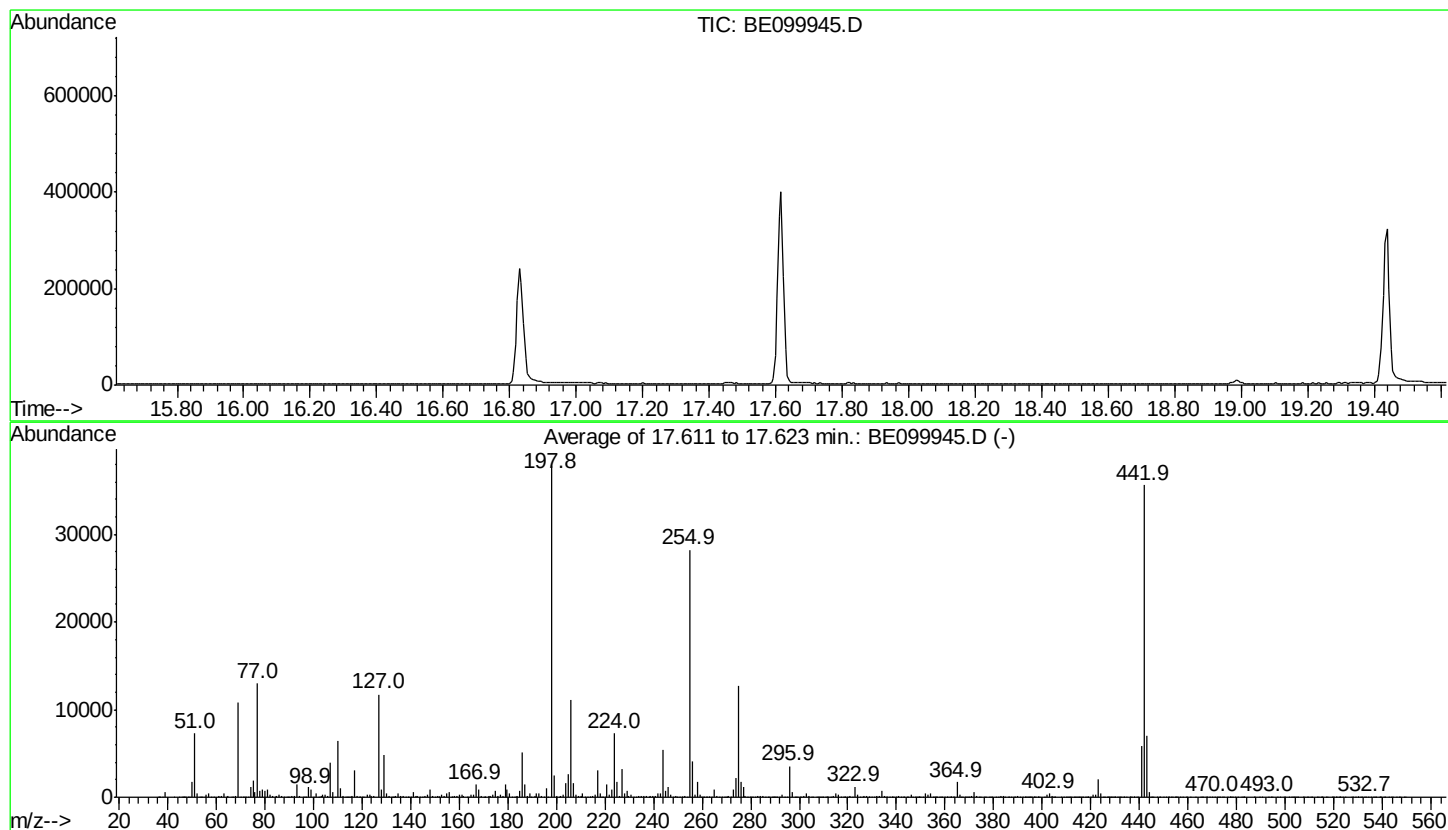

AutoFind: Scans 2557, 2558, 2559; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.2	7273	PASS
68	69	0.00	2	1.7	187	PASS
69	198	0.00	100	28.6	10831	PASS
70	69	0.00	2	0.5	56	PASS
127	198	10	80	31.1	11754	PASS
197	198	0.00	2	0.1	54	PASS
198	198	100	100	100.0	37851	PASS
199	198	5	9	6.7	2521	PASS
275	198	10	60	33.5	12691	PASS
365	198	1	100	4.5	1687	PASS
441	198	0.01	100	15.3	5810	PASS
442	198	50	100	94.1	35600	PASS
443	442	15	24	19.6	6961	PASS