


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061219\
 Data File : BE099959.D
 Acq On : 12 Jun 2019 16:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

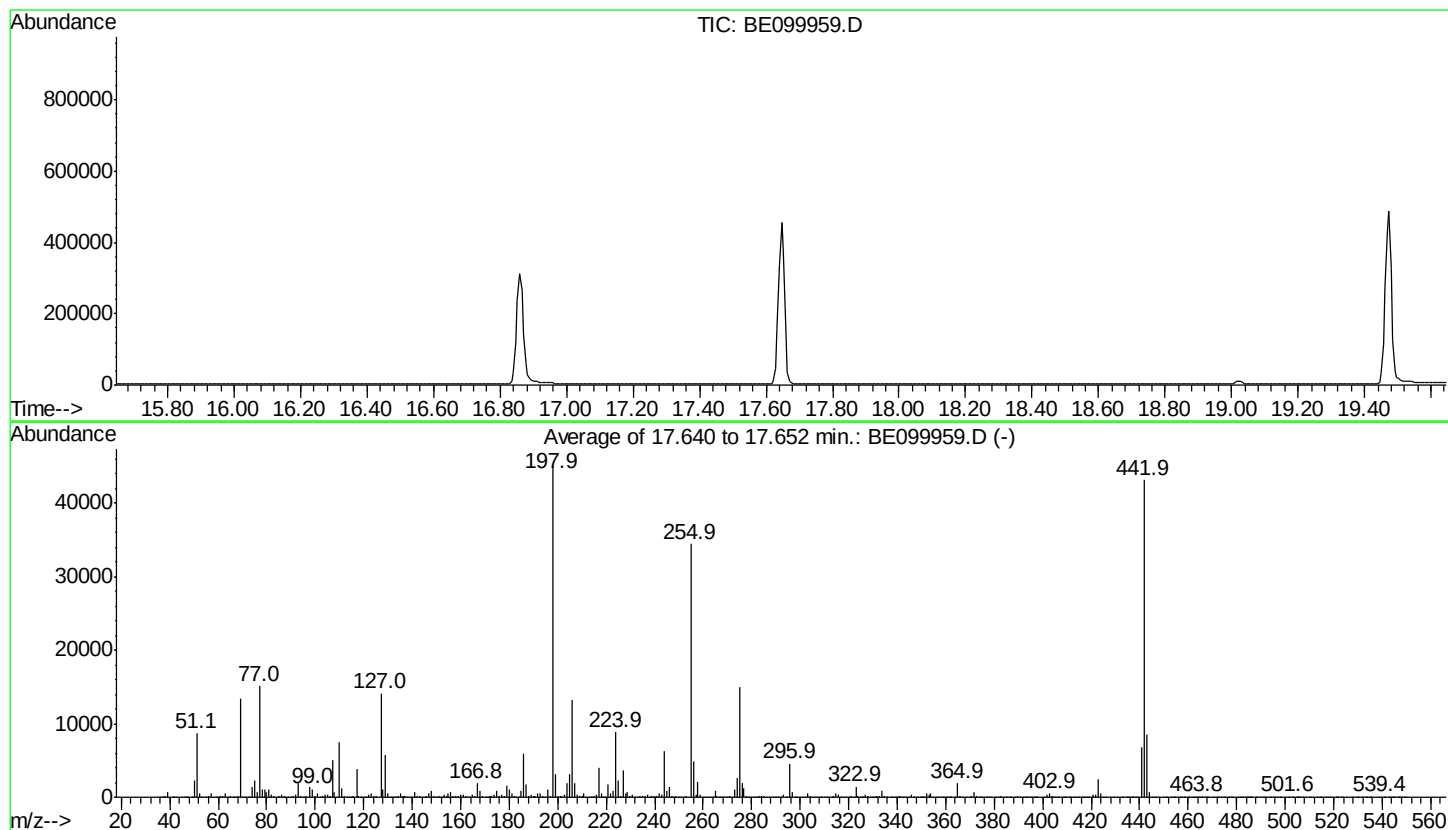

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	8690	PASS
68	69	0.00	2	1.6	219	PASS
69	198	0.00	100	29.6	13360	PASS
70	69	0.00	2	0.5	71	PASS
127	198	10	80	31.1	14026	PASS
197	198	0.00	2	0.4	160	PASS
198	198	100	100	100.0	45085	PASS
199	198	5	9	6.8	3063	PASS
275	198	10	60	33.0	14894	PASS
365	198	1	100	4.1	1848	PASS
441	198	0.01	100	15.1	6791	PASS
442	198	50	100	95.6	43104	PASS
443	442	15	24	19.9	8596	PASS