


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061319\
 Data File : BE099978.D
 Acq On : 13 Jun 2019 8:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

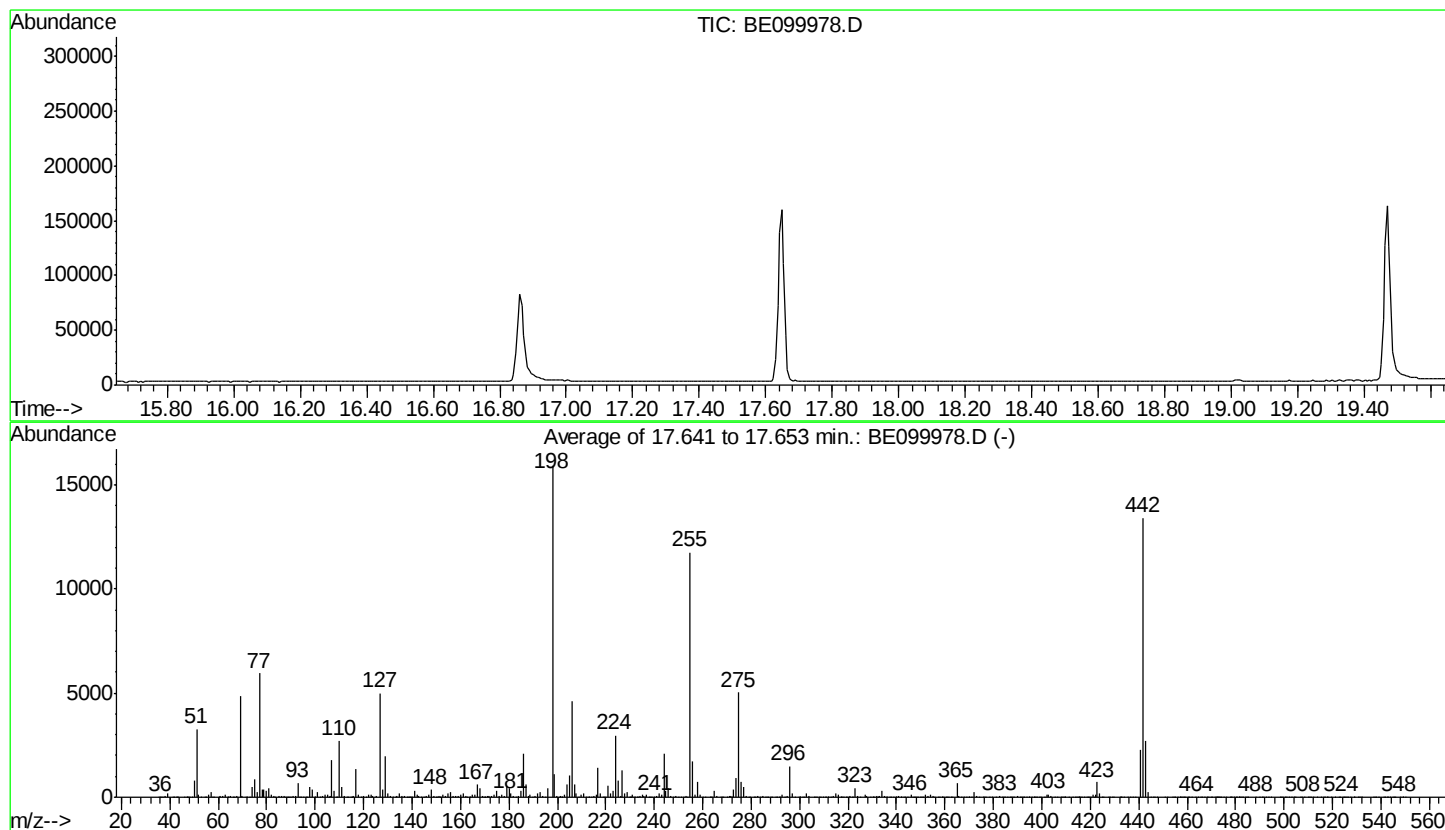

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.6	3288	PASS
68	69	0.00	2	1.7	81	PASS
69	198	0.00	100	30.4	4847	PASS
70	69	0.00	2	0.8	39	PASS
127	198	10	80	31.4	4993	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15925	PASS
199	198	5	9	6.8	1086	PASS
275	198	10	60	31.5	5020	PASS
365	198	1	100	4.4	693	PASS
441	198	0.01	100	14.1	2251	PASS
442	198	50	100	84.2	13410	PASS
443	442	15	24	20.0	2679	PASS