


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061319\
Data File : BE099992.D
Acq On : 13 Jun 2019 16:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 14:57:20 2019

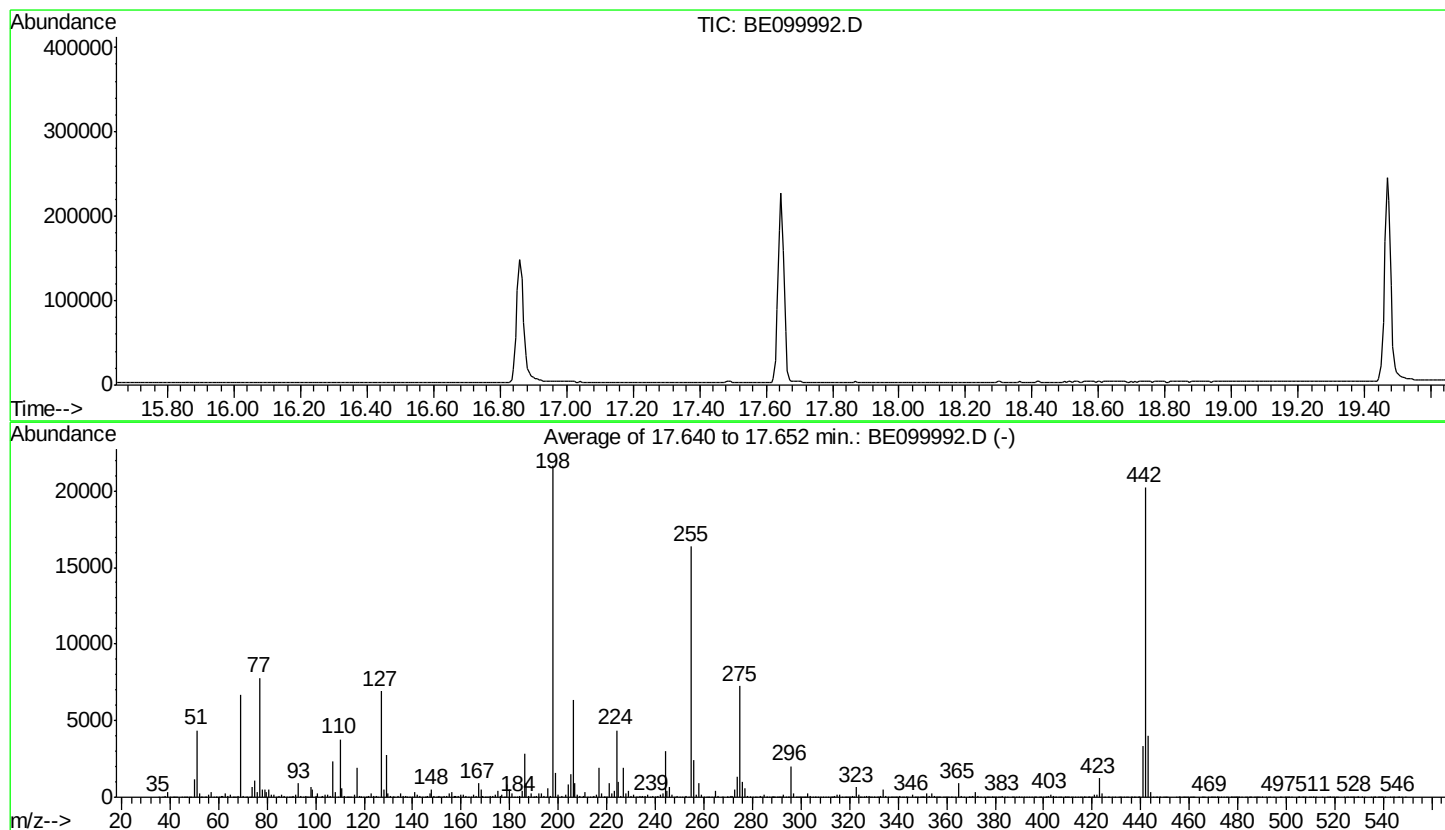

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.2	4381	PASS
68	69	0.00	2	1.6	106	PASS
69	198	0.00	100	30.8	6678	PASS
70	69	0.00	2	0.8	51	PASS
127	198	10	80	32.0	6932	PASS
197	198	0.00	2	0.2	54	PASS
198	198	100	100	100.0	21647	PASS
199	198	5	9	7.5	1626	PASS
275	198	10	60	33.5	7259	PASS
365	198	1	100	4.2	906	PASS
441	198	0.01	100	15.6	3380	PASS
442	198	50	100	93.3	20204	PASS
443	442	15	24	20.1	4053	PASS