
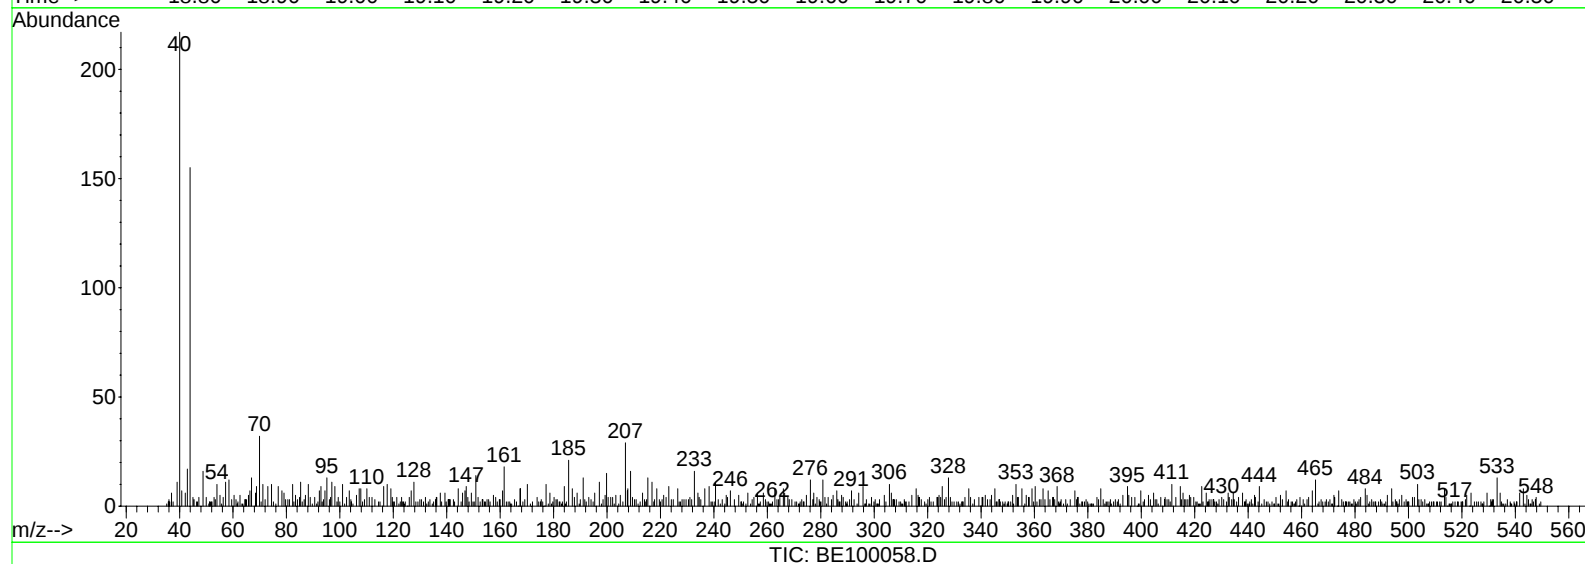


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061719\
Data File : BE100058.D
Acq On : 17 Jun 2019 8:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:20:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

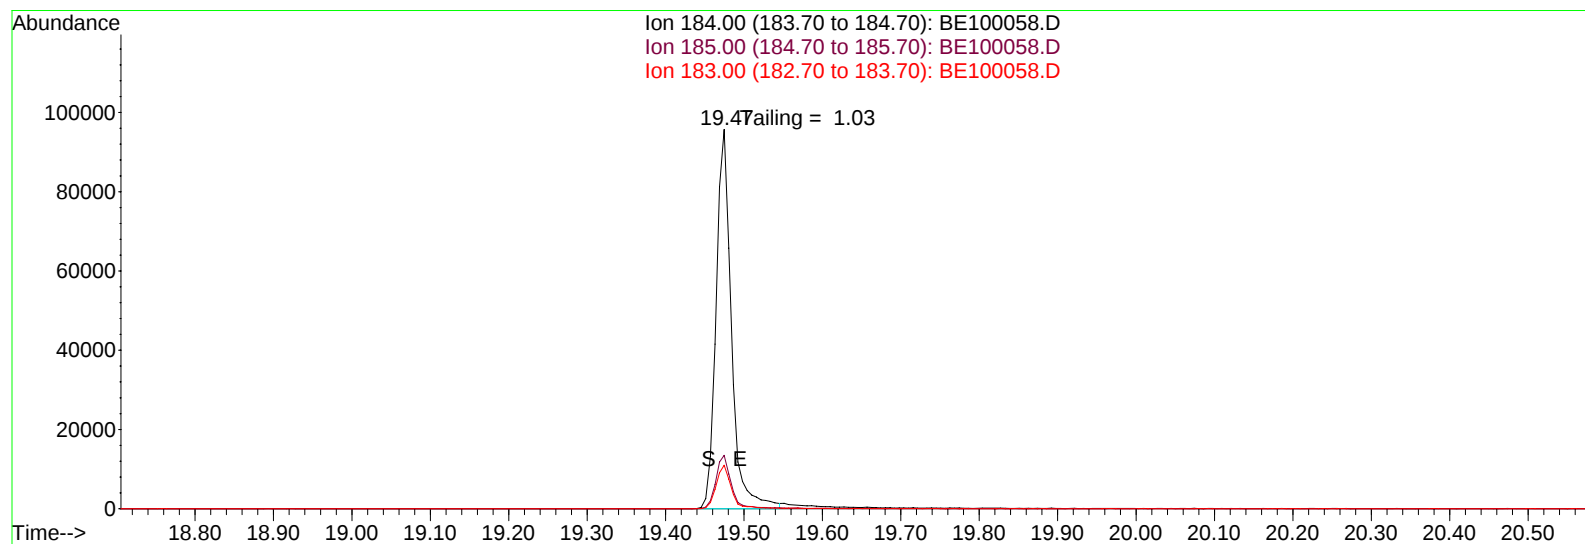

(76) Benzidine



14.868min (+0.278) 56.38ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	230.00#
183.00	12.20	30.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061719\
Data File : BE100058.D
Acq On : 17 Jun 2019 8:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 05:20:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

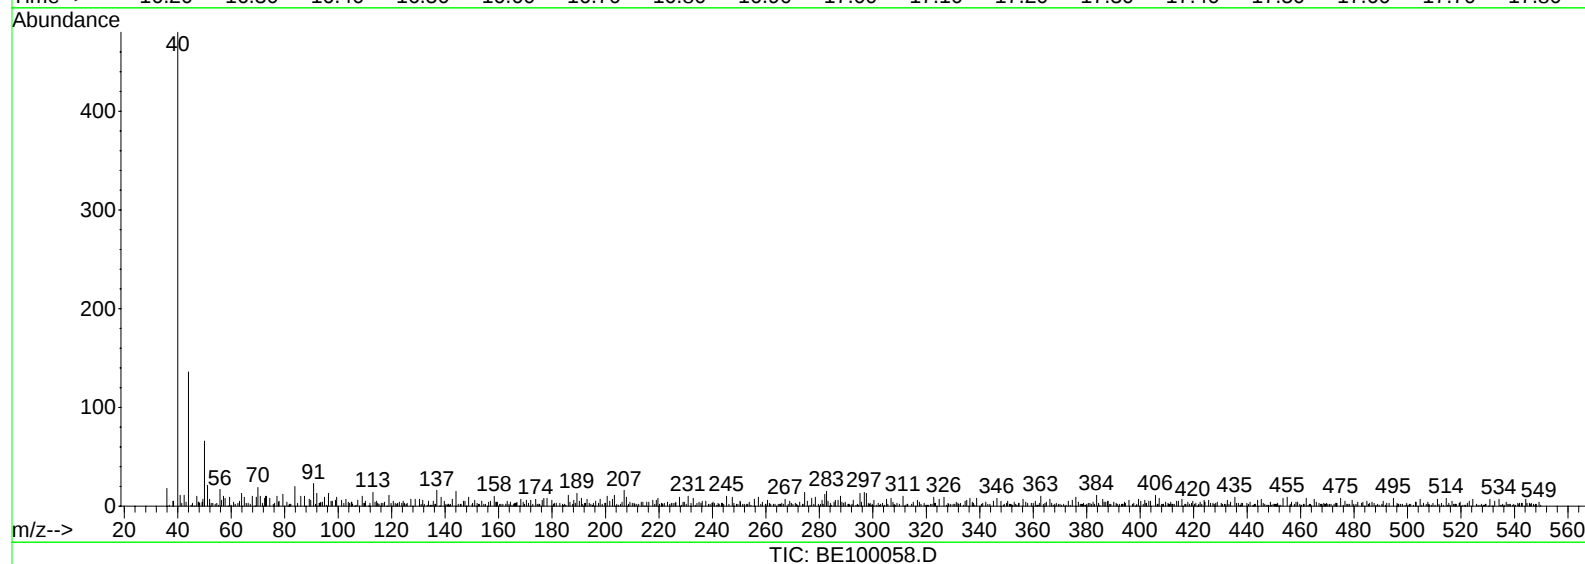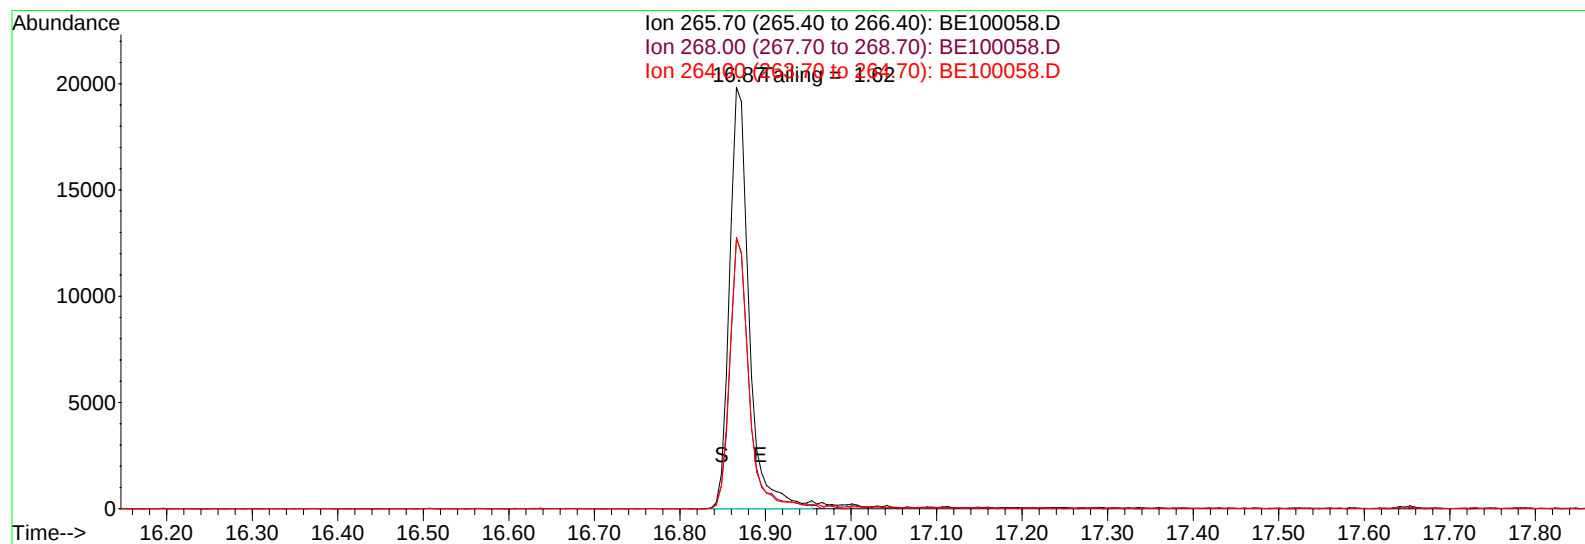

TIC: BE100058.D

(69) Pentachlorophenol (C)

12.348min (+0.261) 100.19ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	40.00#
264.00	65.00	40.00#
0.00	0.00	0.00