


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061719\
 Data File : BE100058.D
 Acq On : 17 Jun 2019 8:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 17 17:23:36 2019

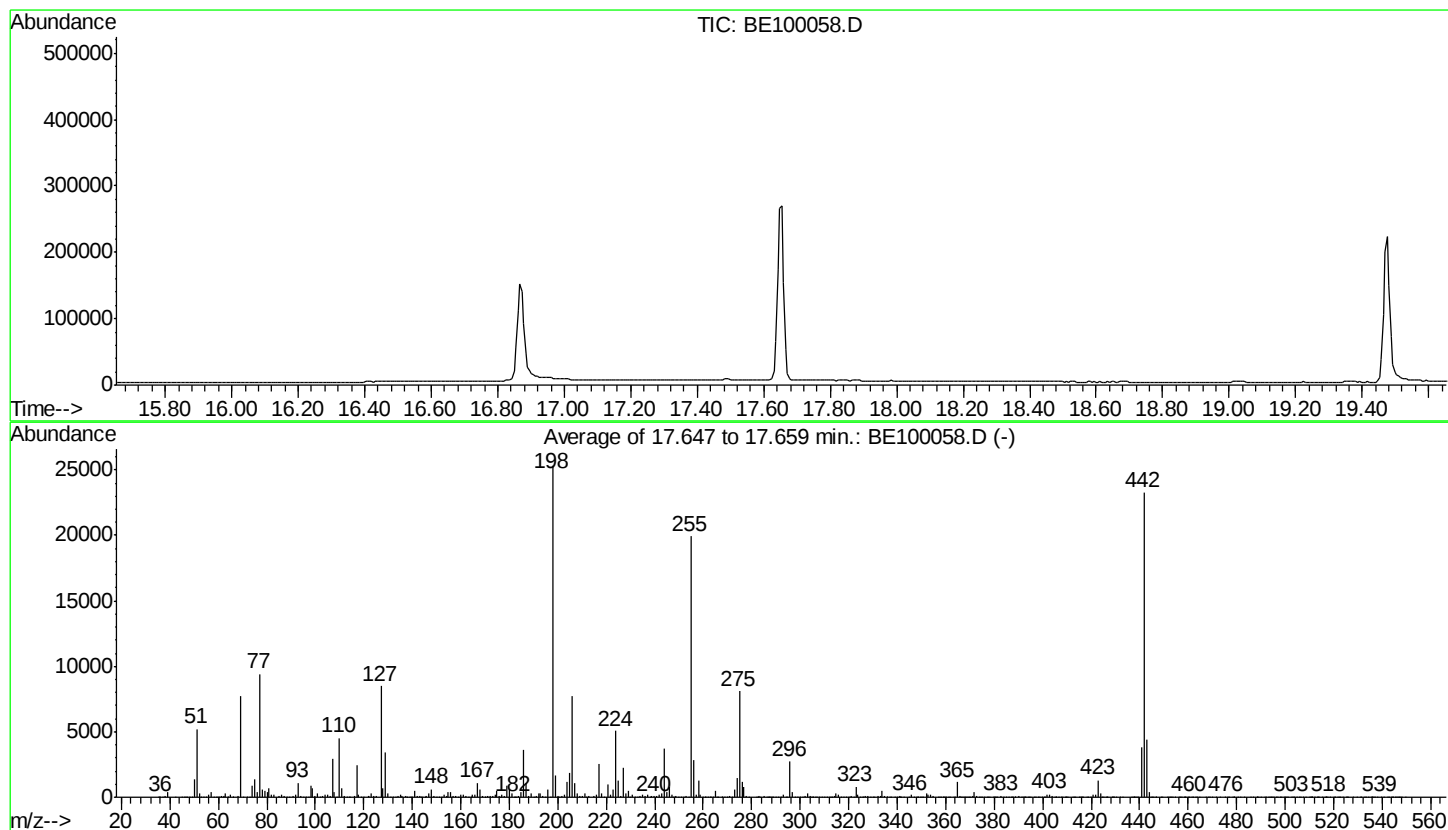

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	5202	PASS
68	69	0.00	2	1.1	87	PASS
69	198	0.00	100	30.4	7705	PASS
70	69	0.00	2	0.2	16	PASS
127	198	10	80	33.5	8486	PASS
197	198	0.00	2	0.2	39	PASS
198	198	100	100	100.0	25329	PASS
199	198	5	9	6.6	1668	PASS
275	198	10	60	32.0	8108	PASS
365	198	1	100	4.5	1151	PASS
441	198	0.01	100	14.9	3771	PASS
442	198	50	100	91.8	23261	PASS
443	442	15	24	18.9	4385	PASS