

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061818\
 Data File : BE096821.D
 Acq On : 18 Jun 2018 22:56
 Operator : SJ/JU
 Sample : J3467-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 19 01:26:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 18 13:28:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	3884	0.40	ng	0.00
7) Naphthalene-d8	10.16	136	22087	0.40	ng	0.00
13) Acenaphthene-d10	13.99	164	119571	0.40	ng	-0.03
19) Phenanthrene-d10	16.78	188	40555	0.40	ng	0.00
27) Chrysene-d12	20.98	240	30791	0.40	ng	0.00
34) Perylene-d12	23.22	264	31535	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.06	112	3236	0.38	ng	0.00
5) Phenol-d6	6.60	99	2648	0.21	ng	0.00
8) Nitrobenzene-d5	8.60	82	79727	6.49	ng	0.07
11) 2-Methylnaphthalene-d10	11.74	152	18971	0.54	ng	0.00
14) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
15) 2-Fluorobiphenyl	12.64	172	22946	0.05	ng	0.00
25) Fluoranthene-d10	18.83	212	125029	0.31	ng	0.02
29) Terphenyl-d14	19.44	244	36558	0.52	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) n-Nitrosodimethylamine	3.38	42	1551	0.234	ng	# 1
6) bis(2-Chloroethyl)ether	6.81	93	6155	0.410	ng	# 1
9) Naphthalene	10.21	128	12159952	56.031	ng	100
12) 2-Methylnaphthalene	11.82	142	1769675	48.627	ng	99
16) Acenaphthylene	13.75	152	21517	0.038	ng	# 1
17) Acenaphthene	14.09	154	18608	0.049	ng	92
22) Pentachlorophenol	16.44	266	85	0.109	ng	92
23) Phenanthrene	16.82	178	28055	0.254	ng	# 69
24) Anthracene	16.92	178	2421	0.027	ng	# 62
28) Pyrene	19.22	202	2700	0.027	ng	# 92
32) Bis(2-ethylhexyl)phthalate	20.94	149	76318	1.361	ng	100
38) Dibenzo(a,h)anthracene	25.54	278	31	0.077	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061818\
Data File : BE096821.D
Acq On : 18 Jun 2018 22:56
Operator : SJ/JU
Sample : J3467-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 19 01:26:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 18 13:28:13 2018
Response via : Initial Calibration

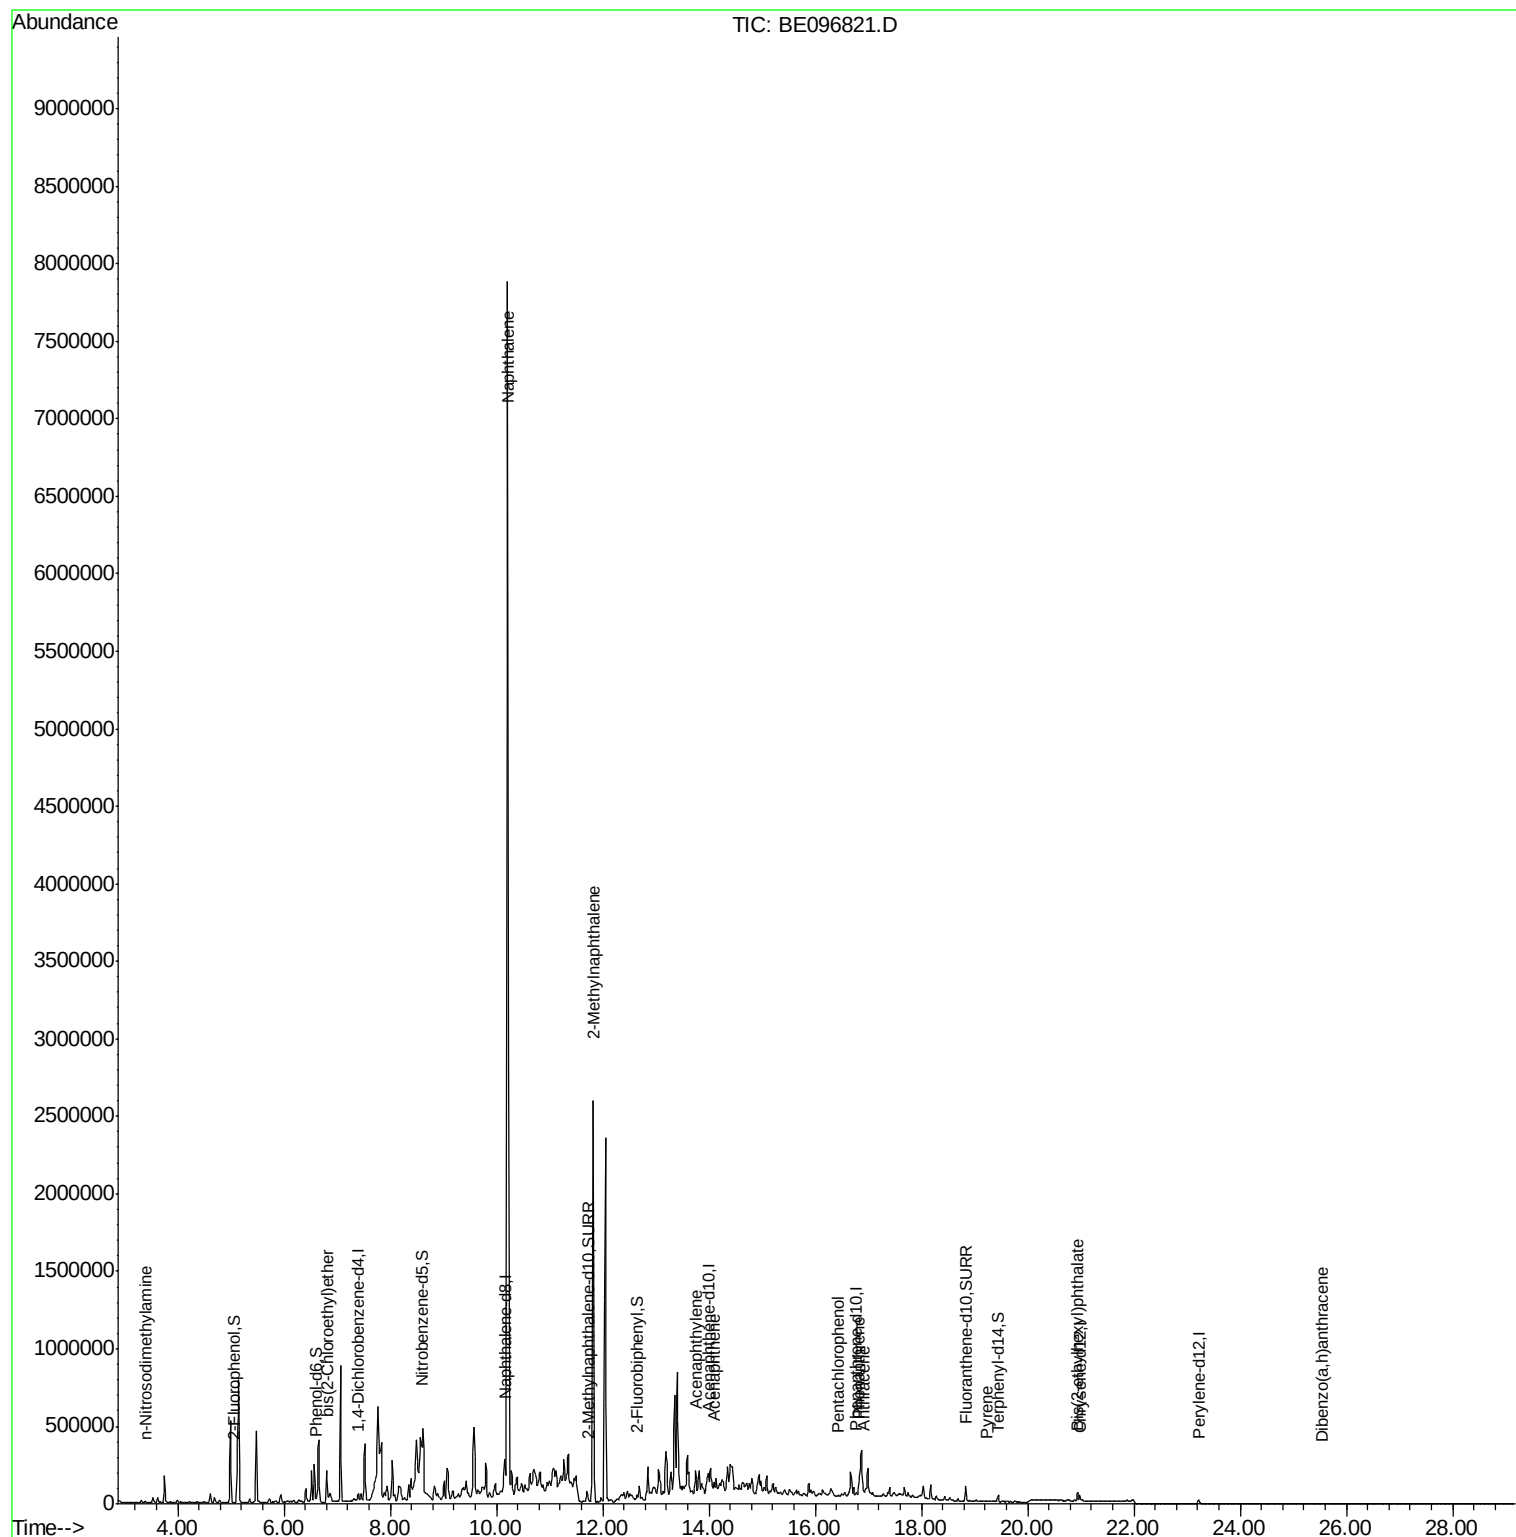




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.40 min Scan# 394
Delta R.T. 0.00 min
Lab File: BE096821.D
Acq: 18 Jun 2018 22:56

Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 3884
Ion Ratio Lower Upper
152 100
150 152.2 117.2 175.8
115 71.1 57.0 85.6

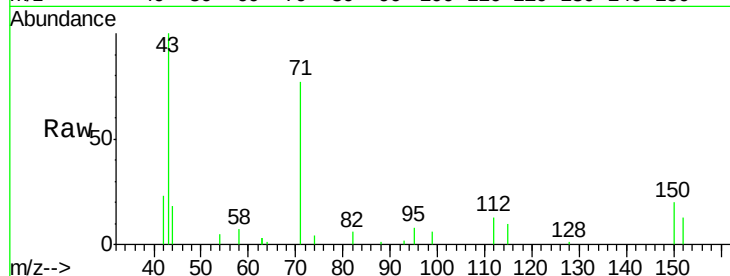


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

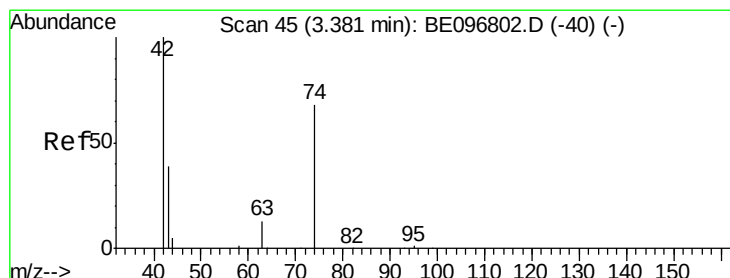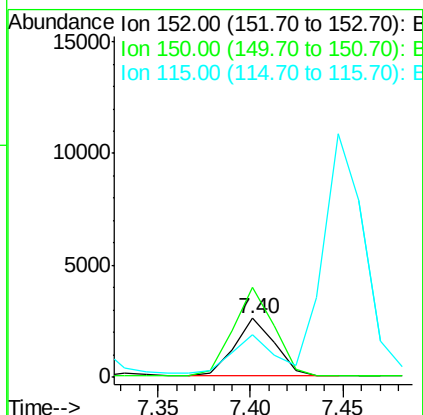



#3


n-Nitrosodimethylamine
Concen: 0.234 ng
RT: 3.38 min Scan# 45
Delta R.T. 0.00 min
Lab File: BE096821.D
Acq: 18 Jun 2018 22:56

Tgt Ion: 42 Resp: 1551
Ion Ratio Lower Upper
42 100
74 0.0 96.0 144.0#
44 24.6 12.0 18.0#

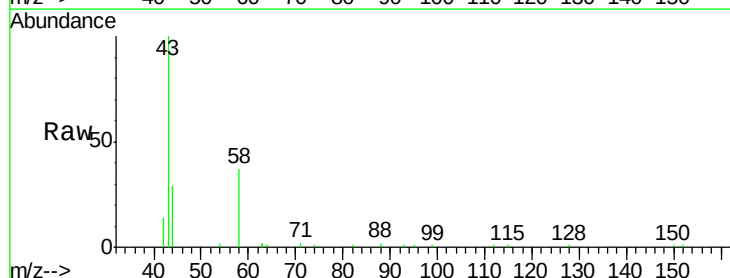

Abundance Ion 42.00 (41.70 to 42.70): BE0
Ion 74.00 (73.70 to 74.70): BE0
Ion 44.00 (43.70 to 44.70): BE0

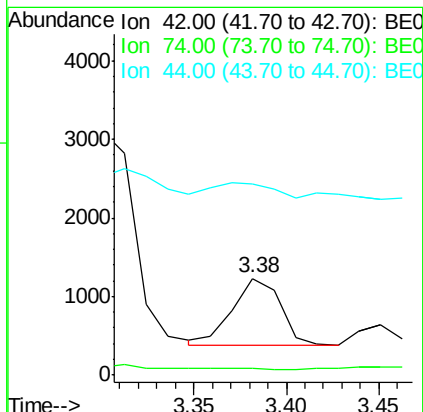

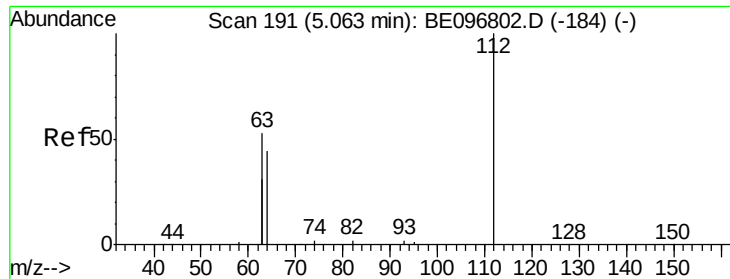

#4

2-Fluorophenol

Concen: 0.381 ng

RT: 5.06 min Scan# 191





Delta R.T. 0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :
BNA_E
ClientSampled :

Tot Ion:112 Resp: 3236
Ion Ratio Lower Upper
112 100
64 0.0 60.1 90.1#
63 0.0 116.8 175.2#

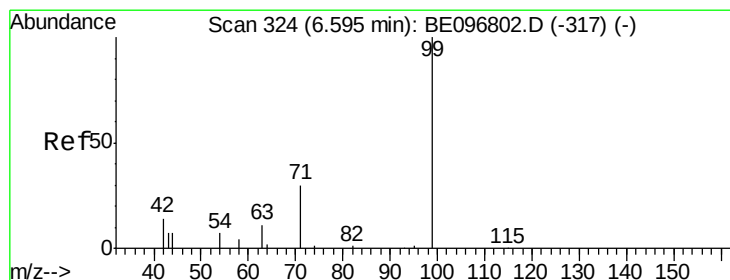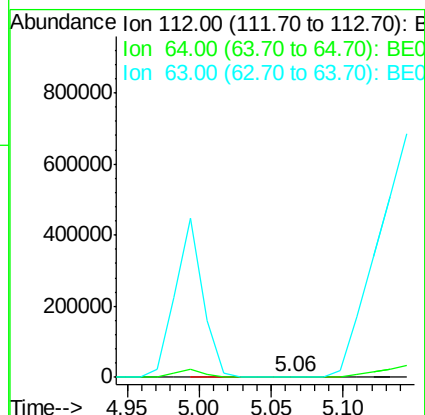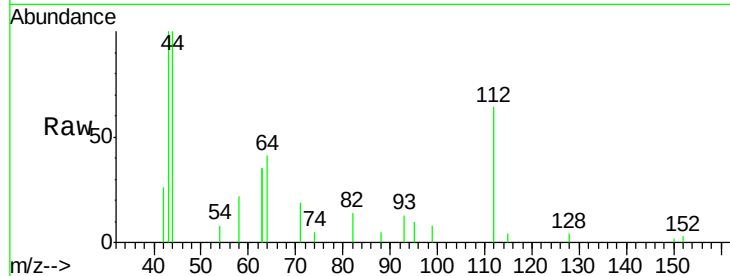

#5

Phenol-d6

Concen: 0.208 ng




RT: 6.60 min Scan# 324


Delta R.T. 0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Tgt Ion: 99 Resp: 2648
Ion Ratio Lower Upper
99 100
42 0.0 20.2 30.2#
71 156.4 28.4 42.6#

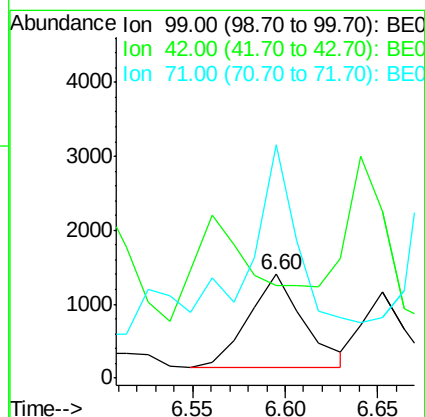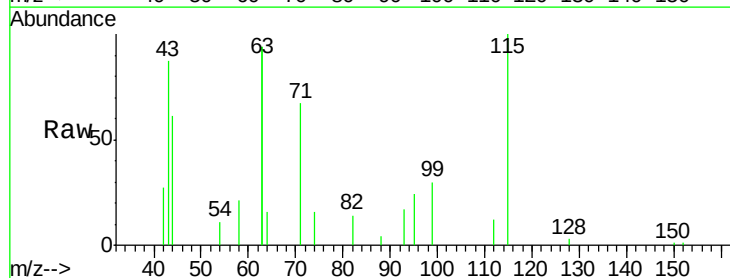

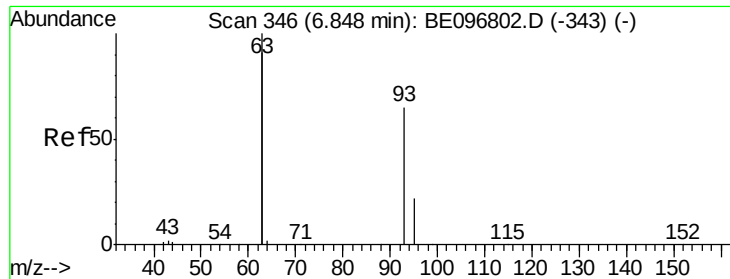

#6

bis(2-Chloroethyl)ether

Concen: 0.410 ng

RT: 6.81 min Scan# 343

Delta R.T. -0.03 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :





Tot Ion: 93 Resp: 6155

Ion Ratio Lower Upper

93 100

63 3576.1 275.3 412.9#

95 76.2 25.2 37.8#

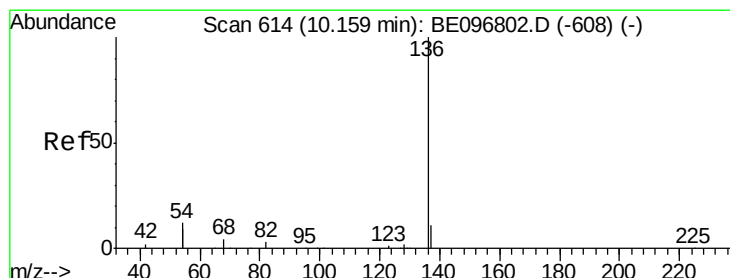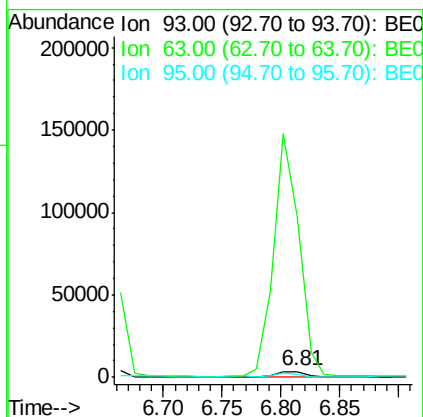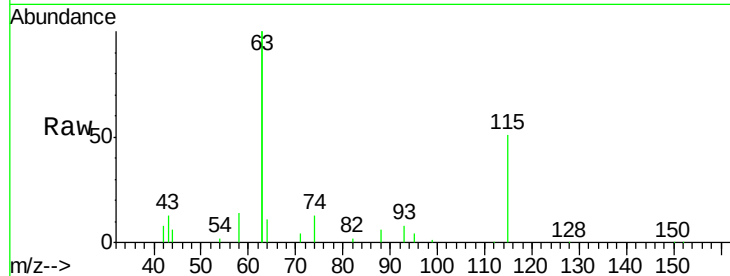

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.16 min Scan# 614

Delta R.T. -0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Tgt Ion: 136 Resp: 22087




Ion Ratio Lower Upper


136 100

137 16.6 9.5 14.3#

54 247.3 29.1 43.7#

68 60.3 6.2 9.2#

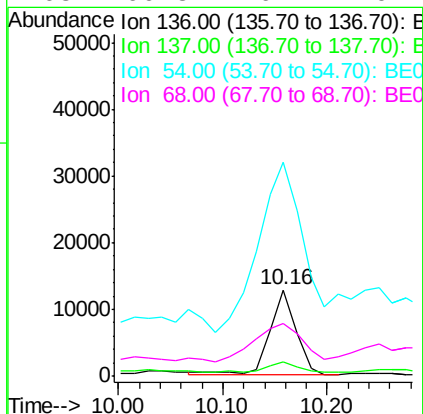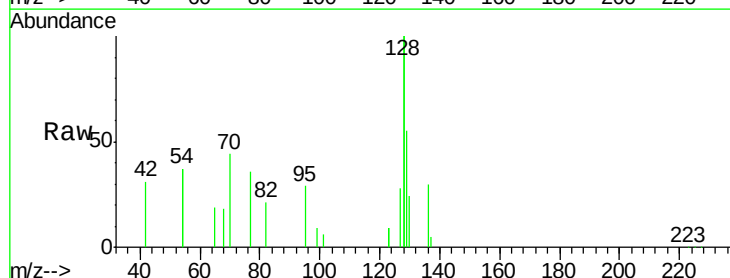



#8

Nitrobenzene-d5

Concen: 6.490 ng

RT: 8.60 min Scan# 498

Delta R.T. 0.07 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampled :


Tot Ion: 82 Resp: 79727

Ion Ratio Lower Upper

82 100

128 5.7 24.0 36.0#




54 57.8 40.0 60.0

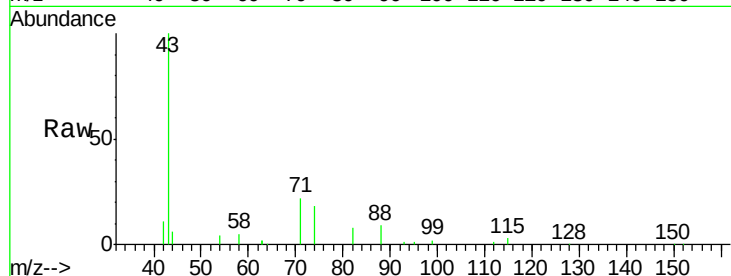

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

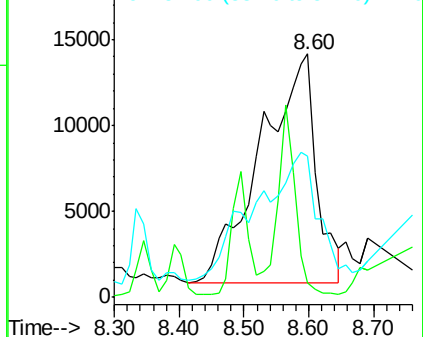

#9

Naphthalene

Concen: 56.031 ng

RT: 10.21 min Scan# 618

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56


Tgt Ion:128 Resp:12159952

Ion Ratio Lower Upper

128 100

129 3.1 2.6 3.8



127 3.5 2.8 4.2




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

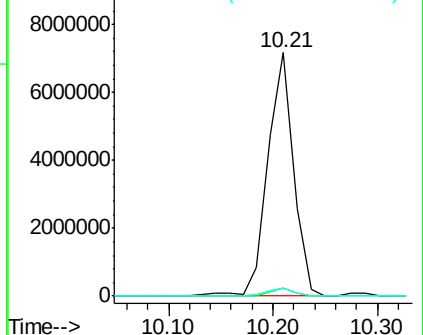

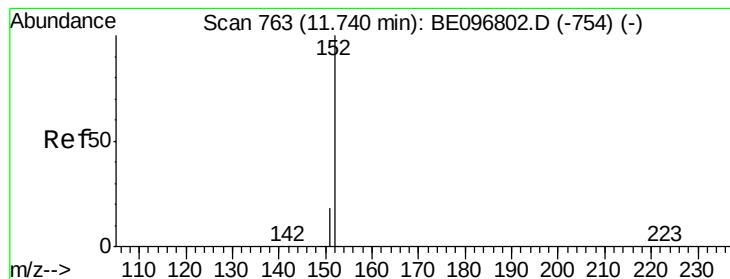

#11

2-Methylnaphthalene-d10

Concen: 0.538 ng

RT: 11.74 min Scan# 764

Delta R.T. 0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E


ClientSampleId :

Tot Ion:152 Resp: 18971

Ion Ratio Lower Upper

152 100

151 26.9 15.4 23.0#

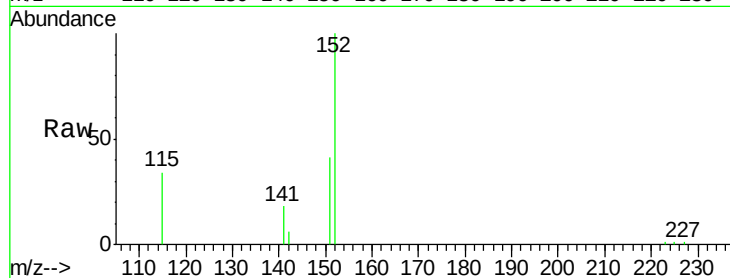

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

11.74

10000

8000

6000



4000

2000

0

Time-->

11.65 11.70 11.75 11.80

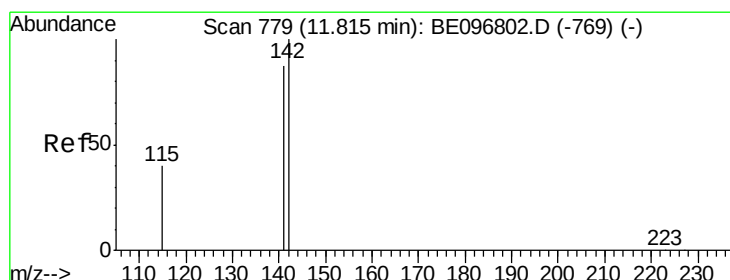

#12

2-Methylnaphthalene

Concen: 48.627 ng

RT: 11.82 min Scan# 780

Delta R.T. 0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56


Tgt Ion:142 Resp: 1769675

Ion Ratio Lower Upper

142 100

141 89.5 70.4 105.6

115 39.5 31.7 47.5

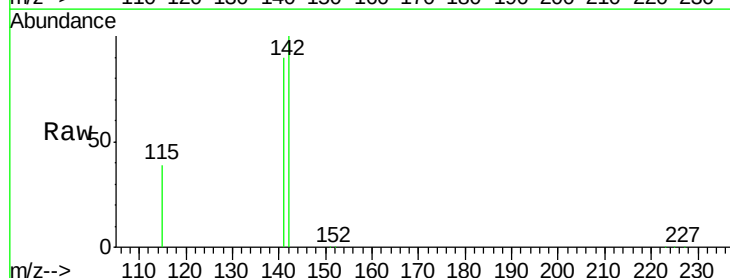

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

11.82

1500000


1000000


500000

0

Time-->

11.70 11.80 11.90



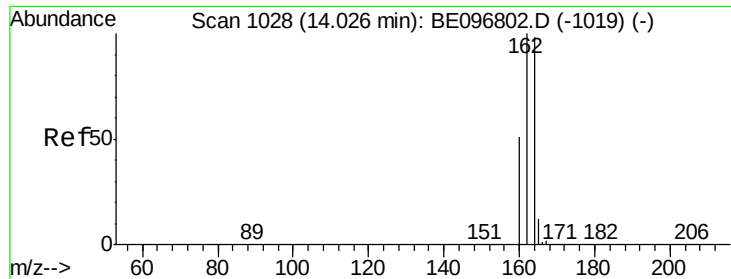

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 13.99 min Scan# 1026

Delta R.T. -0.03 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :


Tot Ion:164 Resp: 119571

Ion Ratio Lower Upper

164 100

162 22.7 83.1 124.7#




160 23.3 37.1 55.7#

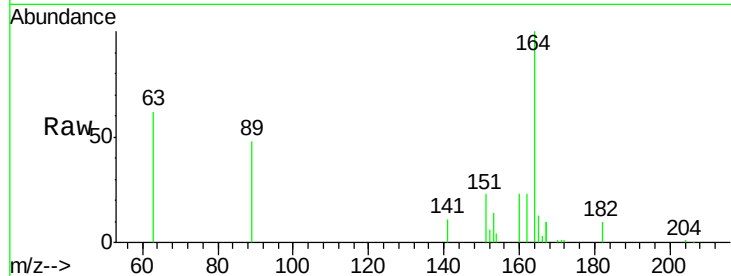

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

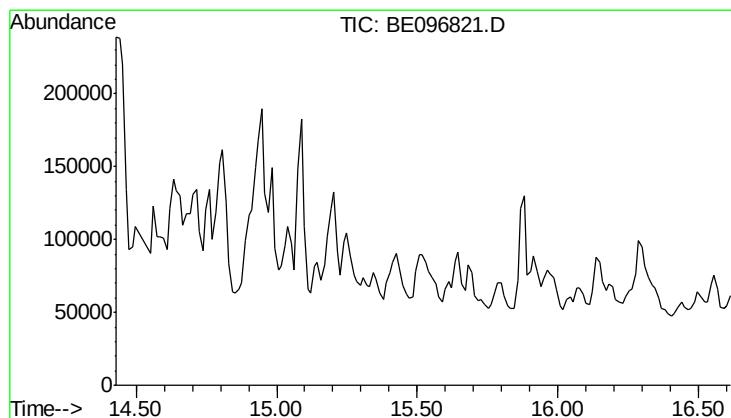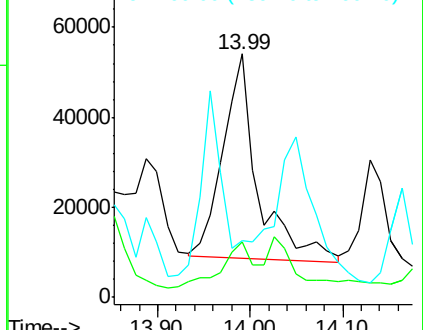

#14

2,4,6-Tribromophenol

Concen: 0.000 ng

Expected RT: 15.52 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56


Tgt Ion: 330


Sig Exp Ratio

330 100

332 190.9

141 42.1

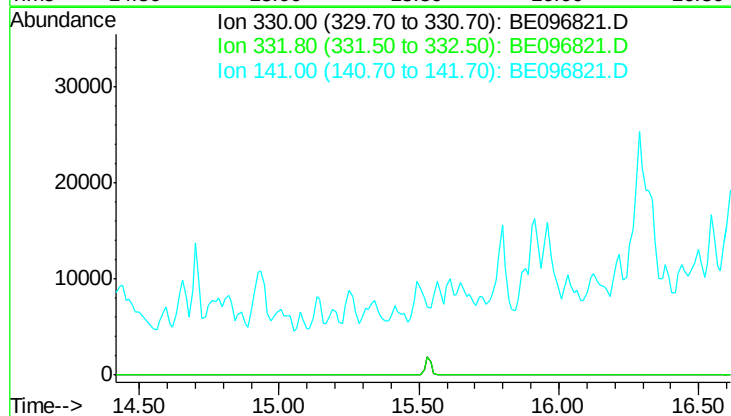

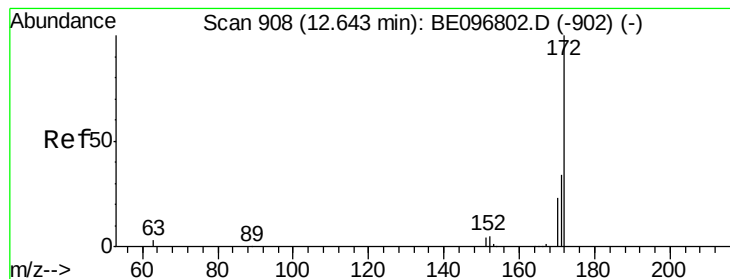

#15

2-Fluorobiphenyl

Concen: 0.047 ng

RT: 12.64 min Scan# 909

Delta R.T. 0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :


Tot Ion:172 Resp: 22946

Ion Ratio Lower Upper

172 100

171 36.5 29.9 44.9




170 28.3 21.8 32.8

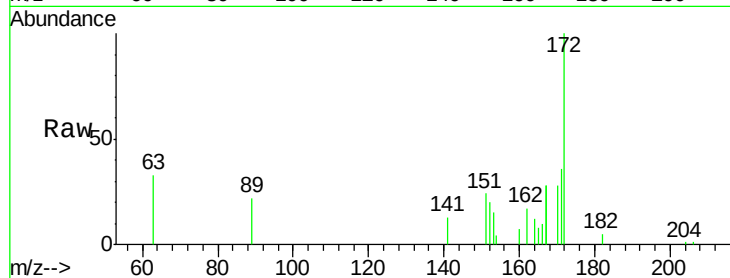

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

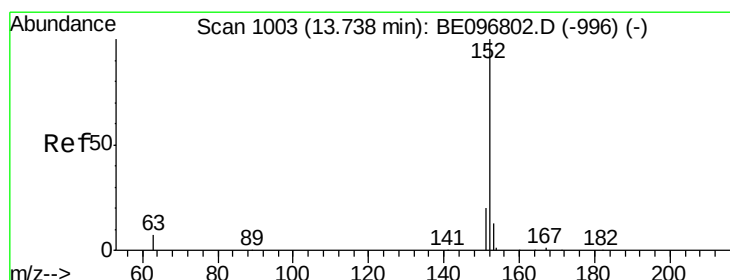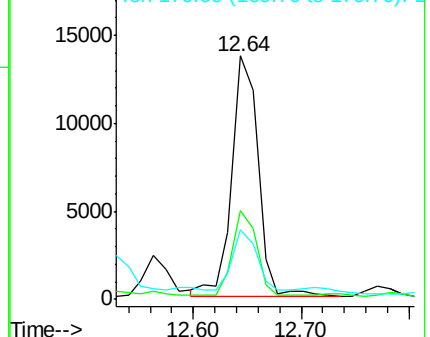

#16

Acenaphthylene

Concen: 0.038 ng

RT: 13.75 min Scan# 1005

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56


Tgt Ion:152 Resp: 21517

Ion Ratio Lower Upper

152 100

151 32.8 15.7 23.5#



153 179.3 10.5 15.7#

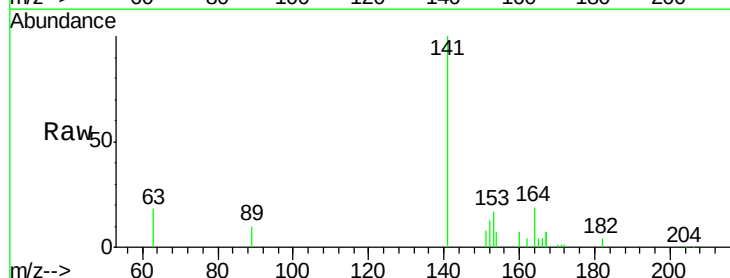


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

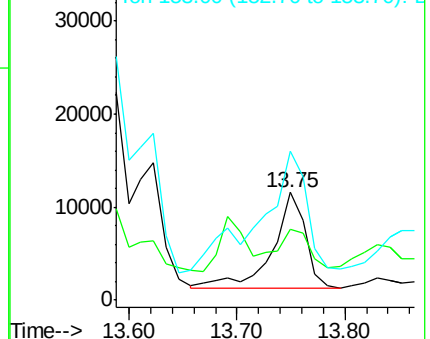

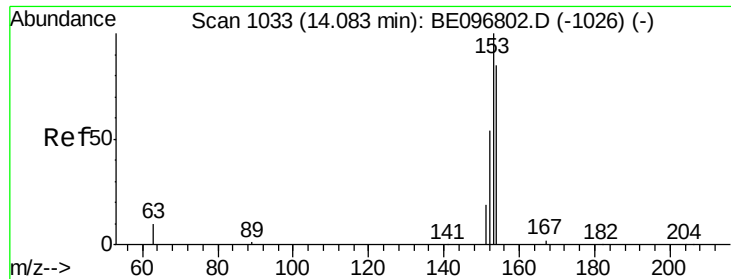

#17

Acenaphthene

Concen: 0.049 ng

RT: 14.09 min Scan# 1035

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :





Tot Ion:154 Resp: 18608

Ion Ratio Lower Upper

154 100

153 102.2 89.2 133.8

152 56.6 42.0 63.0

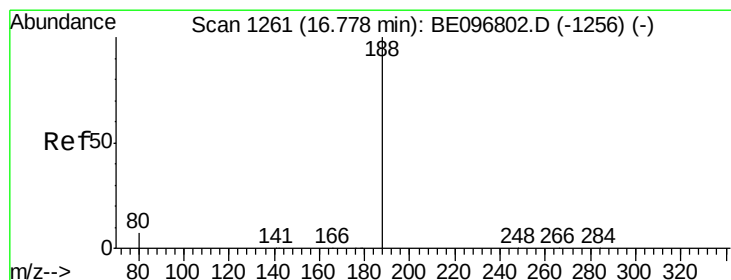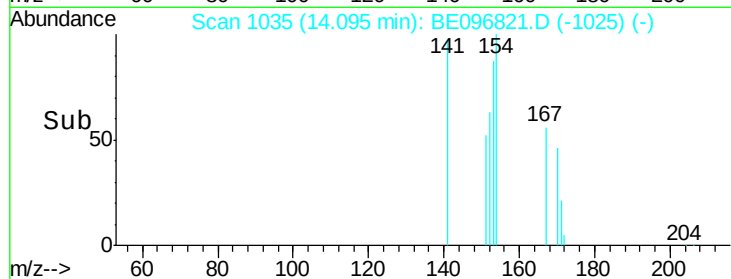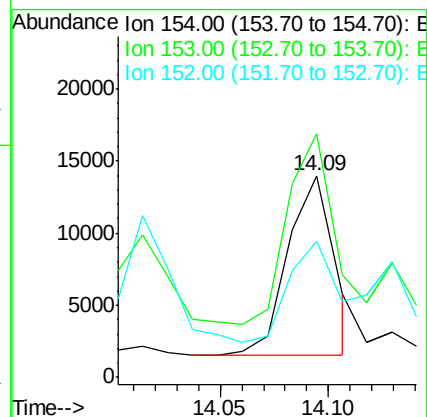

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.78 min Scan# 1262

Delta R.T. -0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56




Tgt Ion:188 Resp: 40555


Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#

80 36.8 3.6 5.4#


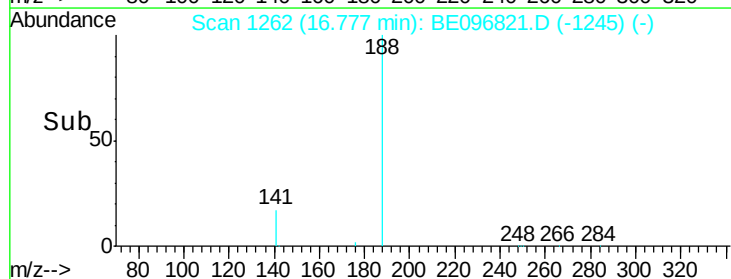
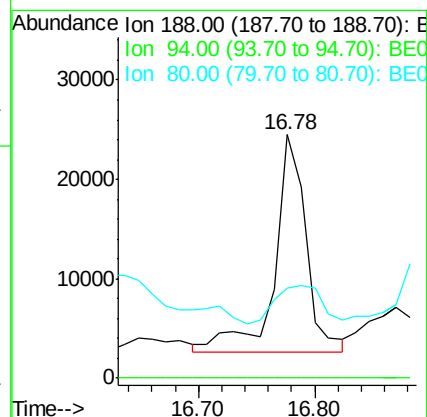
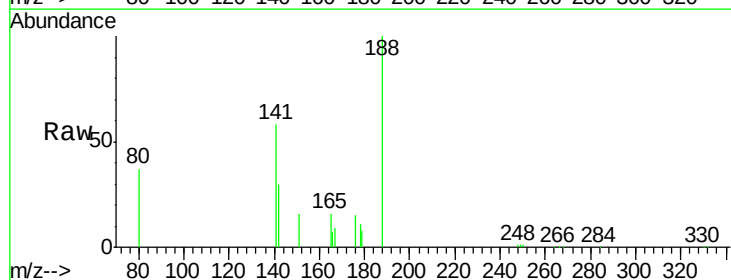


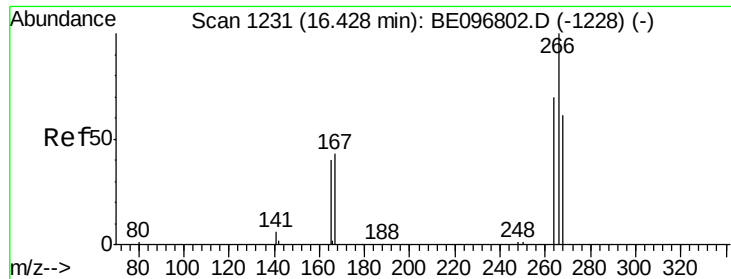

#22
 Pentachlorophenol
 Concen: 0.109 ng
 RT: 16.44 min Scan# 1233
 Delta R.T. 0.01 min
 Lab File: BE096821.D
 Acq: 18 Jun 2018 22:56




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 85
 Ion Ratio Lower Upper
 266 100
 264 89.3 72.5 108.7
 268 106.6 73.8 110.6

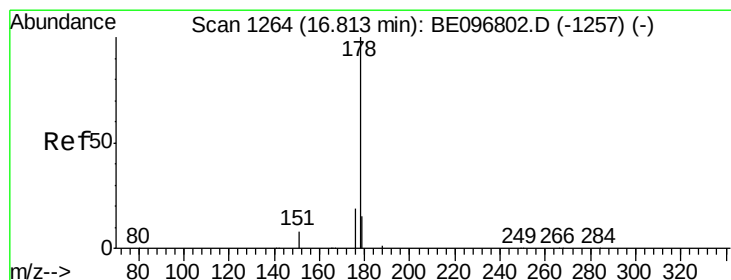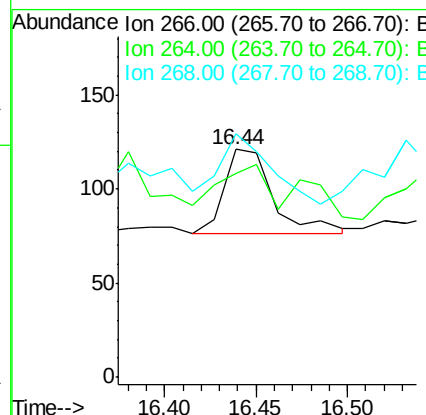

#23
 Phenanthrene
 Concen: 0.254 ng
 RT: 16.82 min Scan# 1266
 Delta R.T. 0.01 min
 Lab File: BE096821.D
 Acq: 18 Jun 2018 22:56

Tgt Ion:178 Resp: 28055
 Ion Ratio Lower Upper
 178 100
 176 39.5 15.1 22.7#
 179 19.6 11.8 17.6#

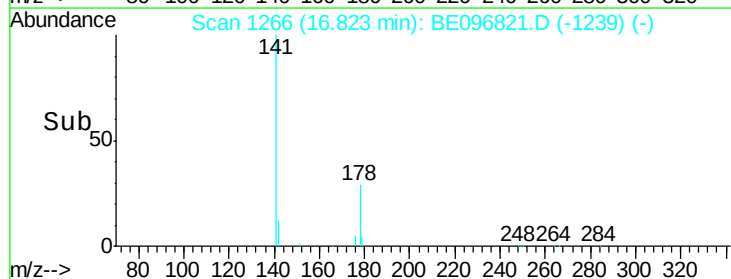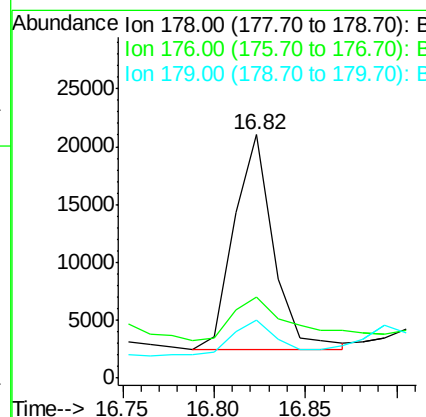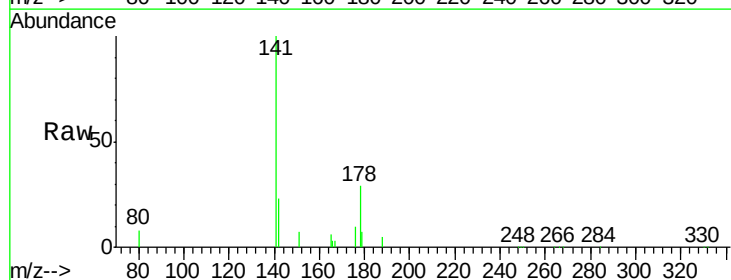



#24

Anthracene

Concen: 0.027 ng

RT: 16.92 min Scan# 1274

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampled :





Tot Ion:178 Resp: 2421

Ion Ratio Lower Upper

178 100

176 0.0 12.8 19.2#

179 0.0 13.0 19.6#

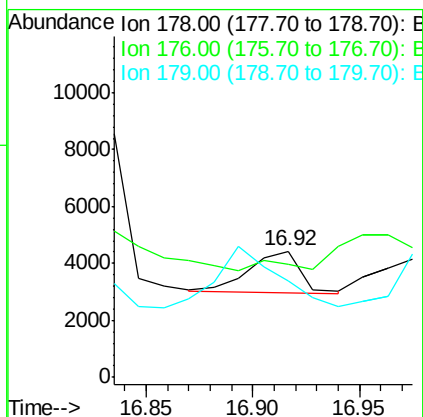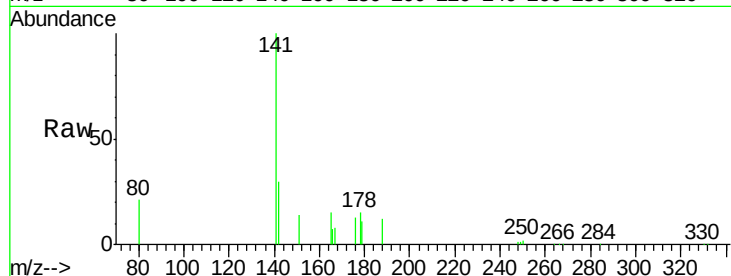

#25

Fluoranthene-d10

Concen: 0.315 ng

RT: 18.83 min Scan# 1507

Delta R.T. 0.02 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56




Tgt Ion:212 Resp: 125029


Ion Ratio Lower Upper

212 100

106 4.3 2.8 4.2#

104 2.4 1.6 2.4#

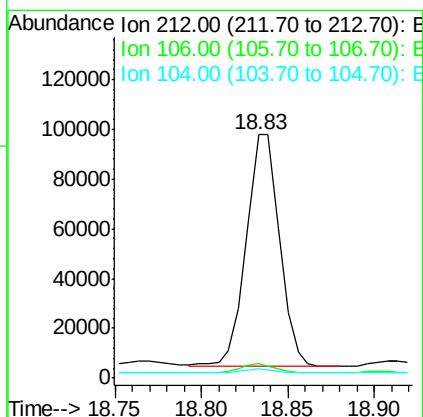



#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.98 min Scan# 1788

Delta R.T. -0.00 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 30791

Ion Ratio Lower Upper

240 100

120 13.6 5.5 8.3#




236 29.5 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

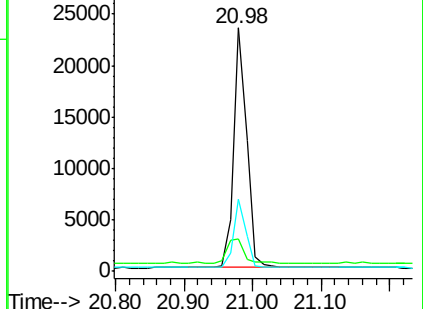

#28

Pyrene

Concen: 0.027 ng

RT: 19.22 min Scan# 1574

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56


Tgt Ion:202 Resp: 2700

Ion Ratio Lower Upper

202 100

200 23.9 16.6 25.0



203 21.9 13.8 20.8#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

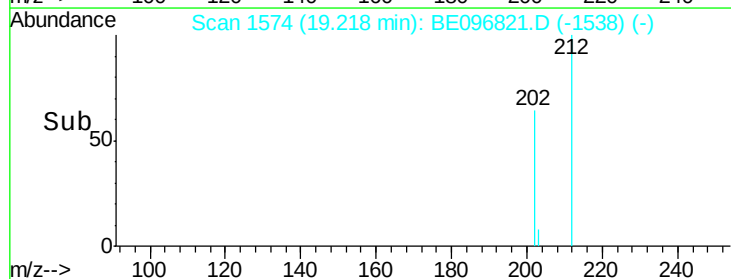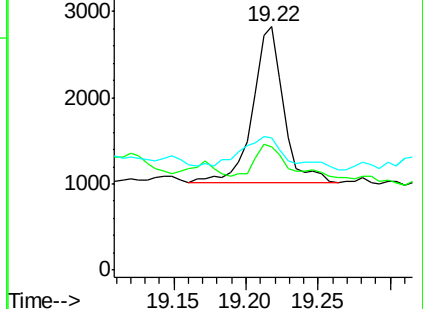

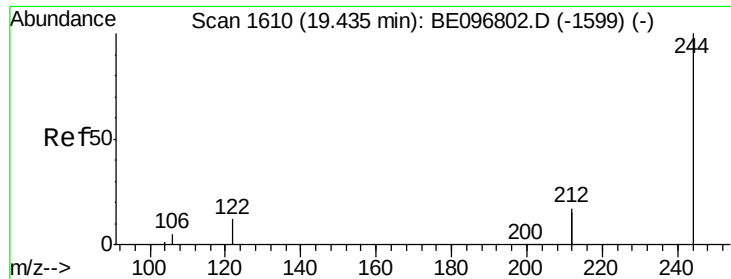

#29

Terphenyl-d14

Concen: 0.524 ng

RT: 19.44 min Scan# 1613

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56

Instrument :

BNA_E

ClientSampleId :





Tot Ion:244 Resp: 36558

Ion Ratio Lower Upper

244 100

212 38.0 25.4 38.0

122 16.2 8.1 12.1#

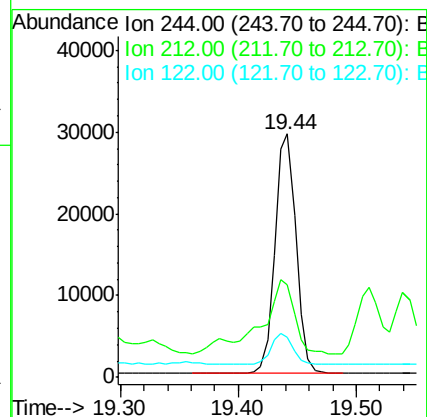

#32

Bis(2-ethylhexyl)phthalate

Concen: 1.361 ng

RT: 20.94 min Scan# 1785

Delta R.T. 0.01 min

Lab File: BE096821.D

Acq: 18 Jun 2018 22:56




Tgt Ion:149 Resp: 76318




Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0

279 1.0 0.7 1.1



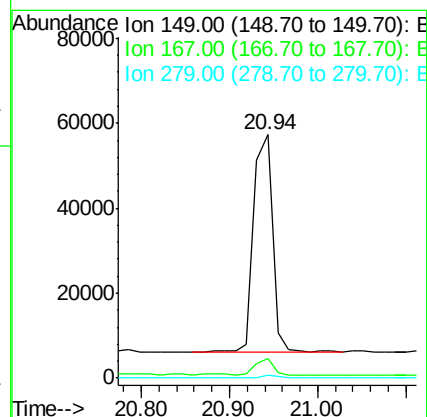



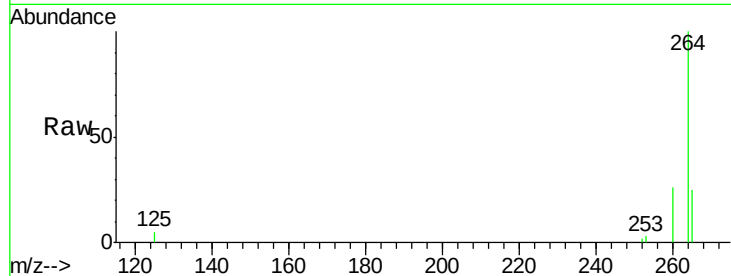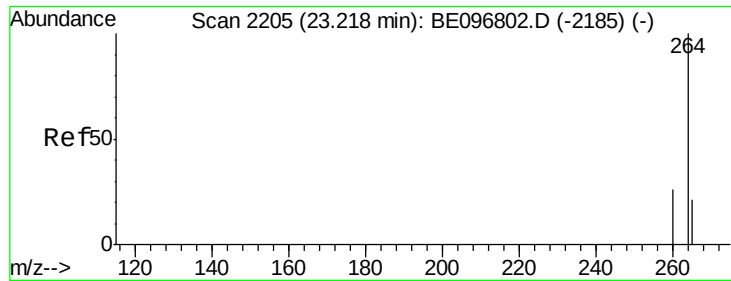

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.22 min Scan# 2207
 Delta R.T. -0.00 min
 Lab File: BE096821.D
 Acq: 18 Jun 2018 22:56

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:264 Resp: 31535
 Ion Ratio Lower Upper
 264 100
 260 26.1 20.5 30.7
 265 24.8 22.8 34.2

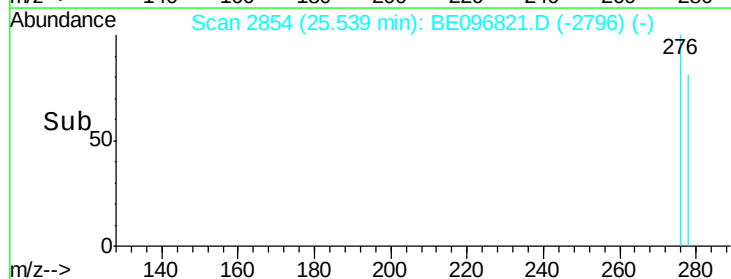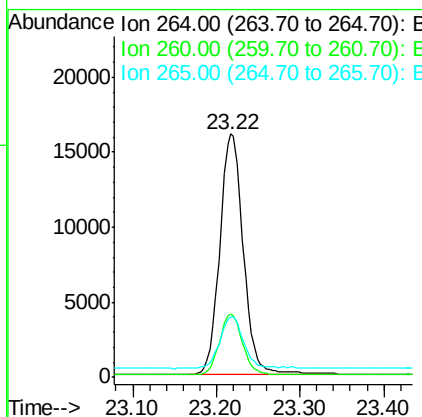

#38
 Dibenzo(a,h)anthracene
 Concen: 0.077 ng
 RT: 25.54 min Scan# 2854
 Delta R.T. 0.01 min
 Lab File: BE096821.D
 Acq: 18 Jun 2018 22:56

Tgt Ion:278 Resp: 31
 Ion Ratio Lower Upper
 278 100
 139 238.8 16.0 24.0#
 279 121.6 20.0 30.0#

