
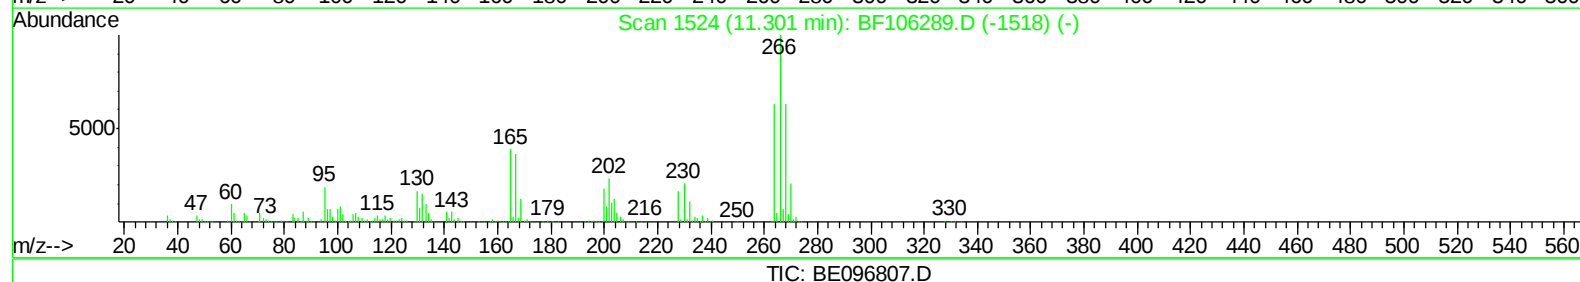
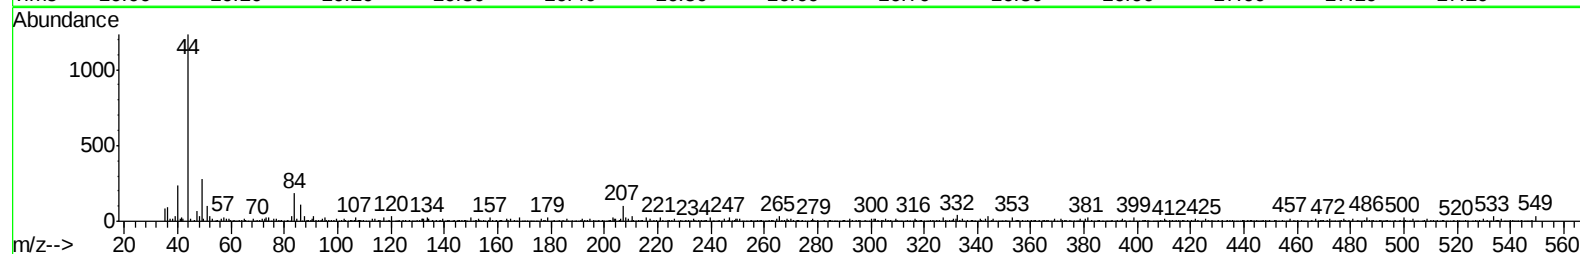


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061818\
 Data File : BE096807.D
 Acq On : 18 Jun 2018 14:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:44:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 15 11:11:47 2018
 Response via : Initial Calibration

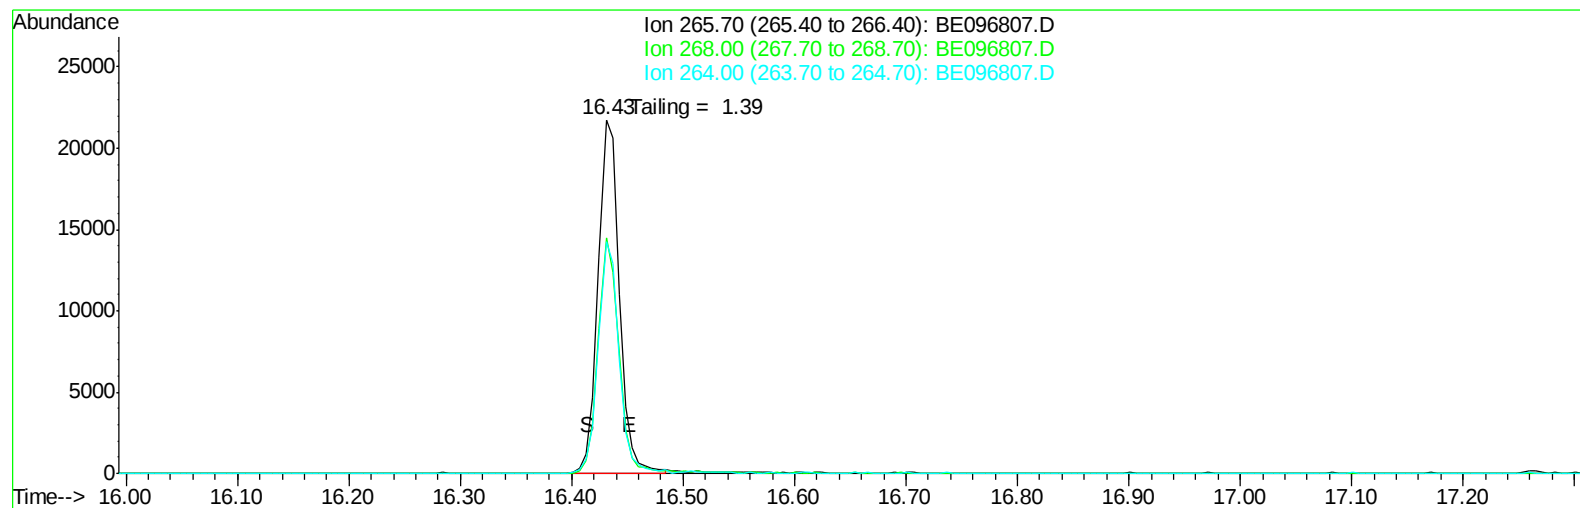

TIC: BE096807.D

(69) Pentachlorophenol (C)




11.478min (+0.171) 138.52ng

response 19

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.25
264.00	61.90	56.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061818\
Data File : BE096807.D
Acq On : 18 Jun 2018 14:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:44:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 15 11:11:47 2018
Response via : Initial Calibration

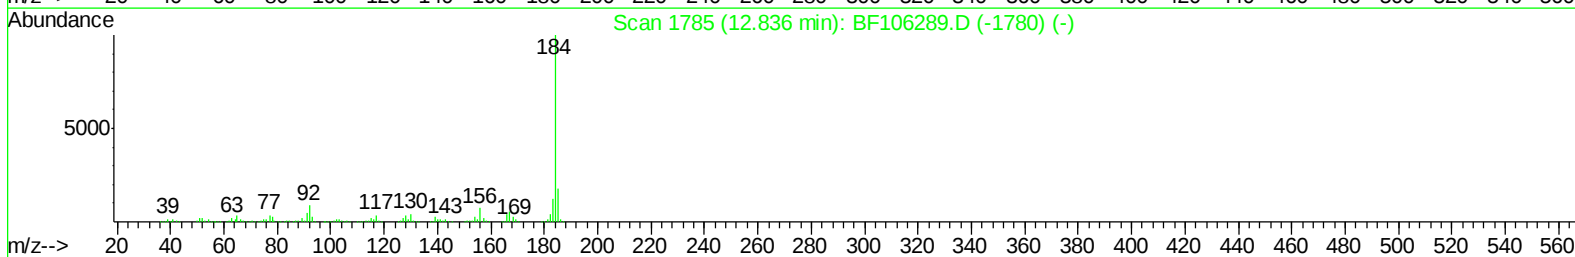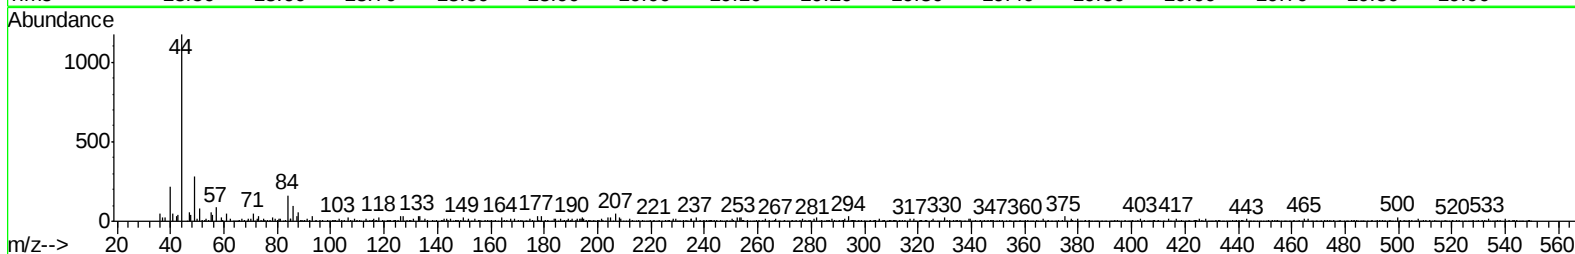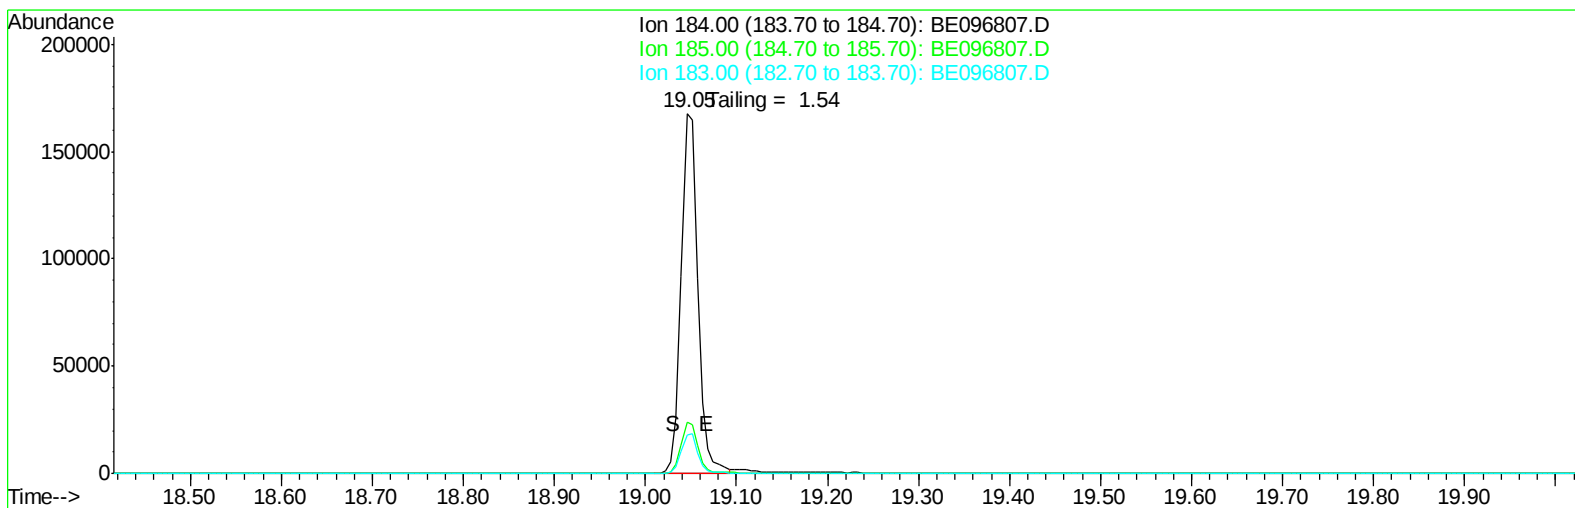

TIC: BE096807.D

(76) Benzidine

12.853min (+0.017) 28.42ng

response 35

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	9.38#
183.00	11.60	53.13#
0.00	0.00	0.00