


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061818\
 Data File : BE096799.D
 Acq On : 18 Jun 2018 9:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 18 13:28:13 2018

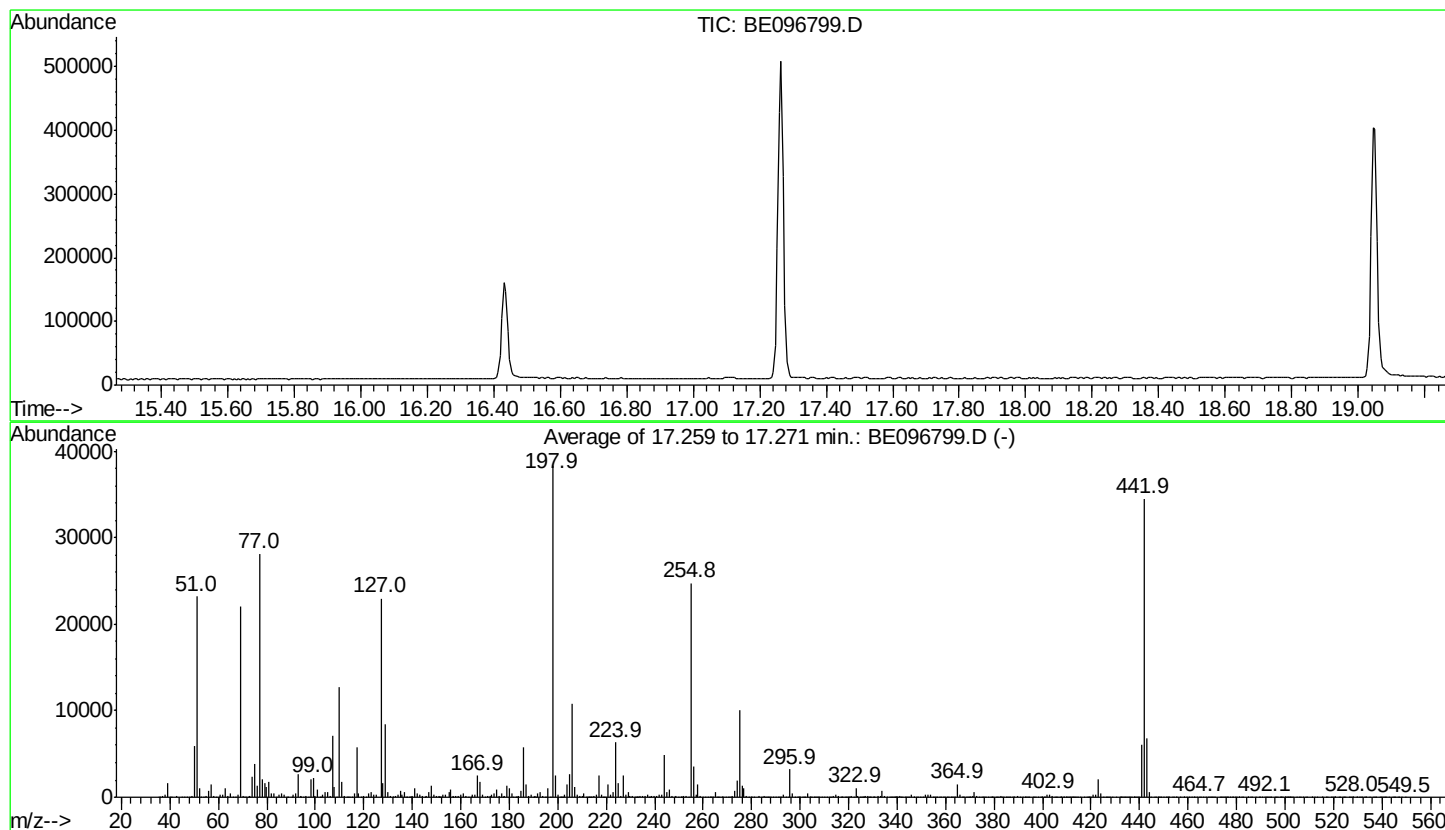

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	23194	PASS
68	69	0.00	2	1.3	284	PASS
69	198	0.00	100	57.5	22029	PASS
70	69	0.00	2	0.7	146	PASS
127	198	10	80	60.0	22994	PASS
197	198	0.00	2	0.1	51	PASS
198	198	100	100	100.0	38336	PASS
199	198	5	9	6.6	2525	PASS
275	198	10	60	26.4	10128	PASS
365	198	1	100	4.0	1528	PASS
441	443	0.01	100	88.6	6036	PASS
442	198	50	100	90.1	34554	PASS
443	442	15	24	19.7	6816	PASS