


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061818\
Data File : BE096807.D
Acq On : 18 Jun 2018 14:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 18 13:28:13 2018

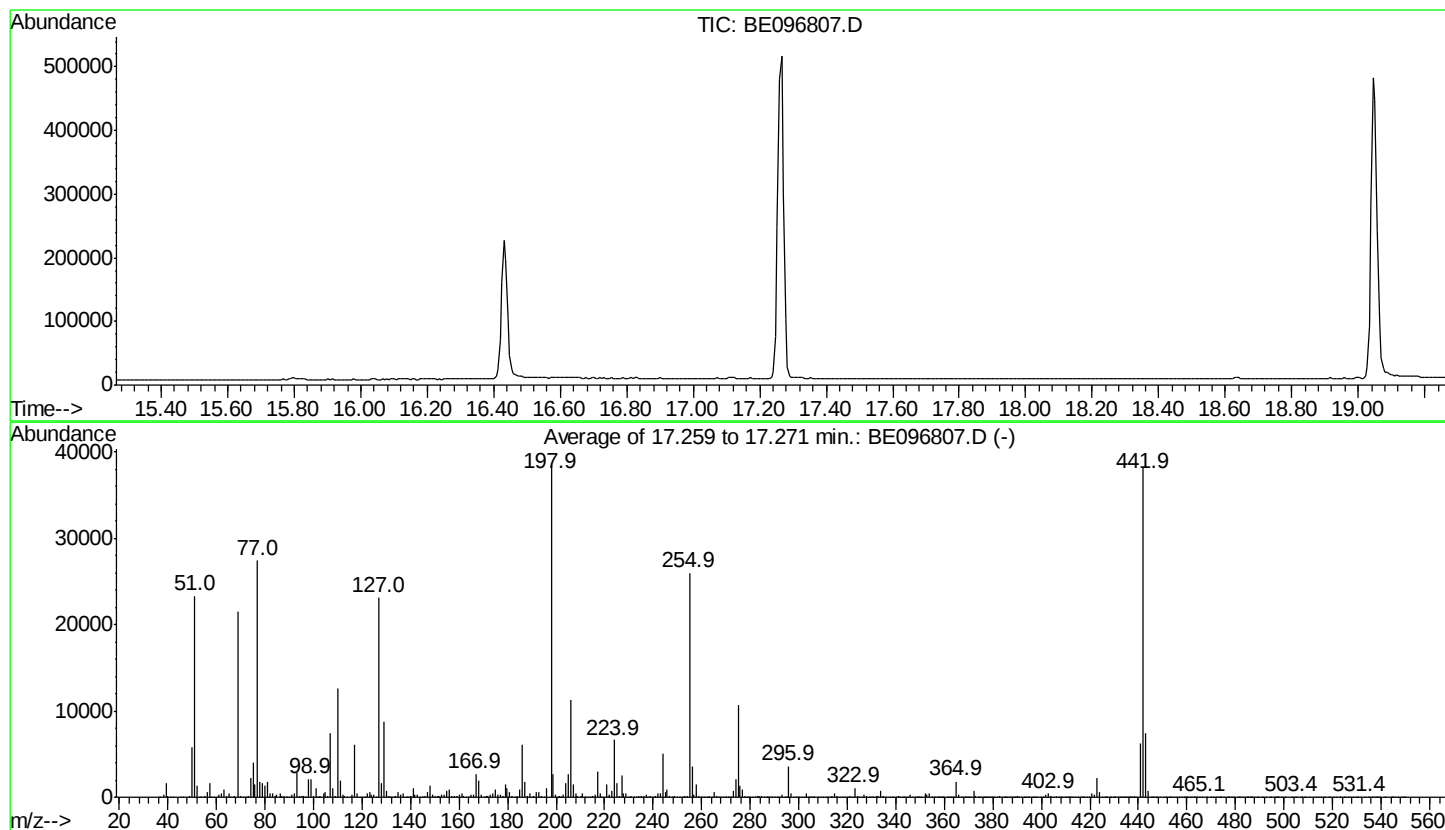

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	23339	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.1	21559	PASS
70	69	0.00	2	0.6	120	PASS
127	198	10	80	60.1	23089	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38440	PASS
199	198	5	9	7.0	2693	PASS
275	198	10	60	27.7	10667	PASS
365	198	1	100	4.7	1812	PASS
441	443	0.01	100	84.8	6248	PASS
442	198	50	100	99.7	38317	PASS
443	442	15	24	19.2	7368	PASS