

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE061919\
 Data File : BE100087.D
 Acq On : 19 Jun 2019 18:02
 Operator : JU/SJ
 Sample : PB120491BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB120491BL

Quant Time: Jun 20 03:50:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 19 15:07:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	493	0.40	ng	0.01
7) Naphthalene-d8	10.58	136	1697	0.40	ng	0.04
13) Acenaphthene-d10	14.43	164	1283	0.40	ng	0.01
19) Phenanthrene-d10	17.19	188	3650	0.40	ng	0.03
27) Chrysene-d12	21.35	240	5297	0.40	ng	0.01
34) Perylene-d12	23.85	264	6906	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.32	112	325	0.32	ng	0.01
5) Phenol-d6	7.02	99	429	0.31	ng	0.09
8) Nitrobenzene-d5	9.00	82	378	0.23	ng	0.09
11) 2-Methylnaphthalene-d10	12.21	152	861	0.27	ng	0.06
14) 2,4,6-Tribromophenol	15.97	330	63	0.09	ng	0.05
15) 2-Fluorobiphenyl	13.07	172	1631	0.32	ng	0.03
25) Fluoranthene-d10	19.21	212	14277	0.27	ng	0.02
29) Terphenyl-d14	19.81	244	3551	0.34	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.60	42	4	0.349	ng	Qvalue # 100
6) bis(2-Chloroethyl)ether	7.22	93	6	0.038	ng	# 1
22) Pentachlorophenol	16.91	266	3	0.246	ng	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE061919\
Data File : BE100087.D
Acq On : 19 Jun 2019 18:02
Operator : JU/SJ
Sample : PB120491BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB120491BL

Quant Time: Jun 20 03:50:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 19 15:07:24 2019
Response via : Initial Calibration

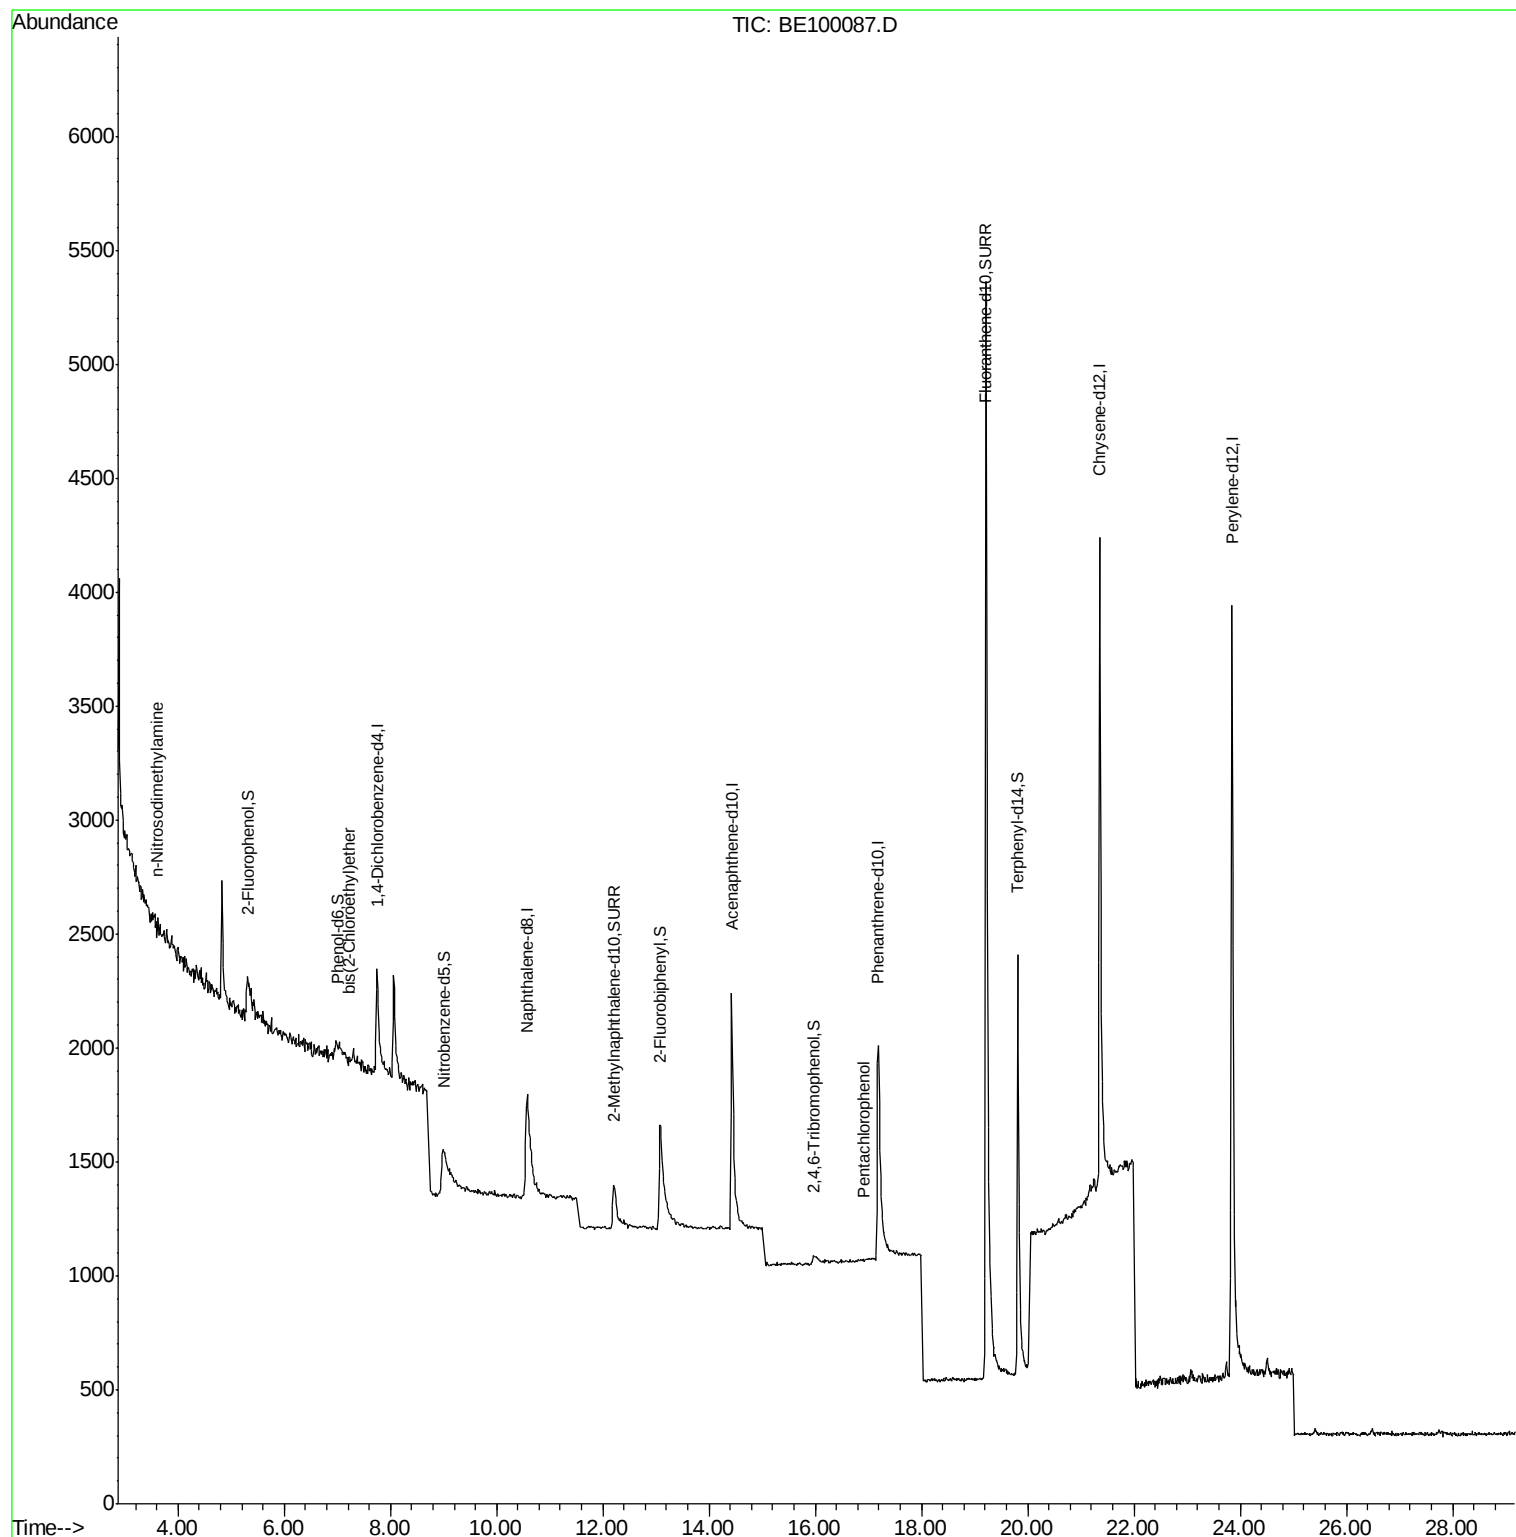

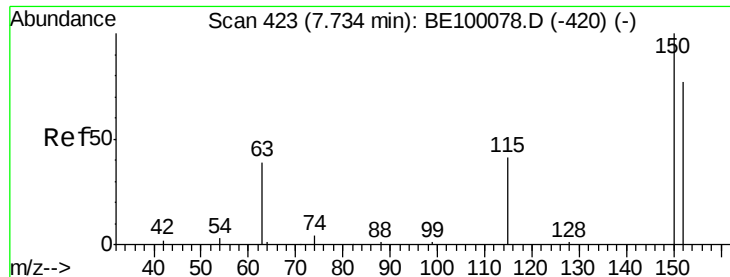

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.75 min Scan# 424

Delta R.T. 0.01 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL


Tgt Ion:152 Resp: 493

Ion Ratio Lower Upper

152 100

150 135.5 99.8 149.8




115 76.5 51.3 76.9

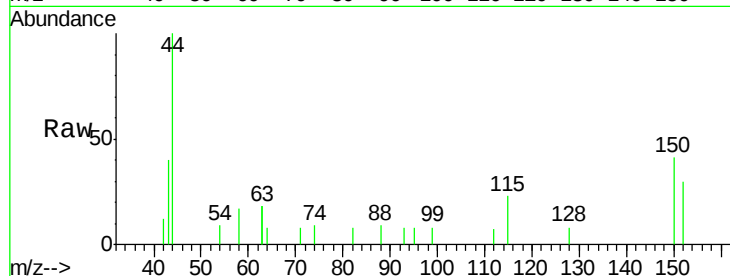

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

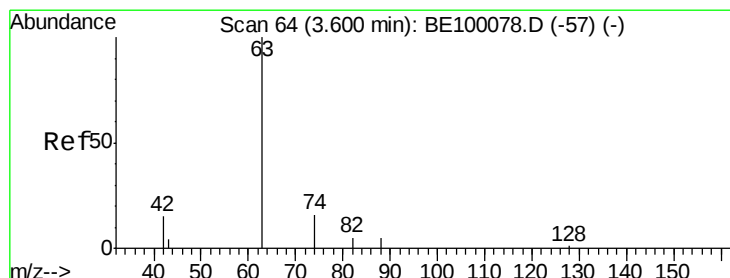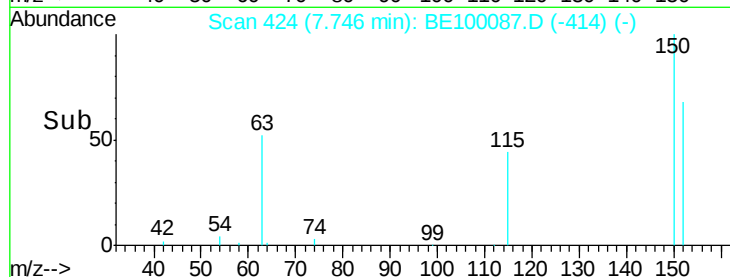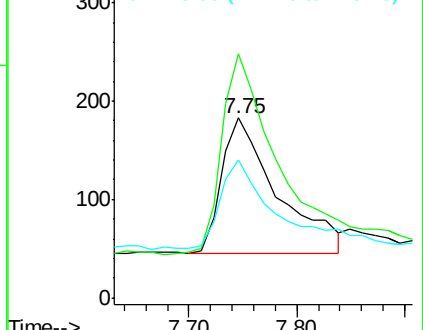

#3

n-Nitrosodimethylamine

Concen: 0.349 ng

RT: 3.60 min Scan# 64

Delta R.T. 0.00 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02


Tgt Ion: 42 Resp: 4

Ion Ratio Lower Upper

42 100

74 0.0 0.0 0.0



44 0.0 0.0 0.0



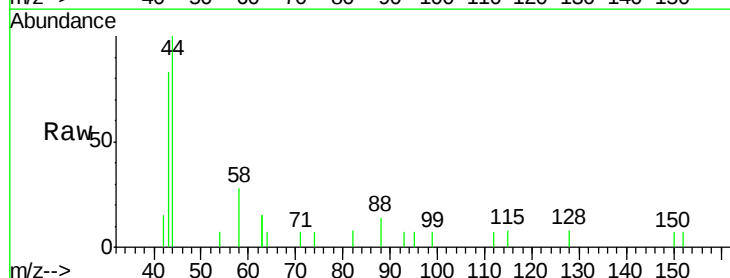


Abundance Ion 42.00 (41.70 to 42.70): BE1

Ion 74.00 (73.70 to 74.70): BE1

Ion 44.00 (43.70 to 44.70): BE1

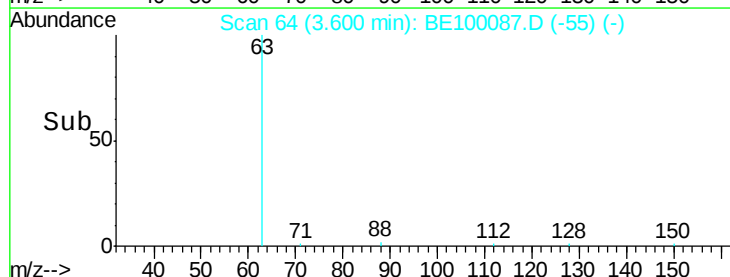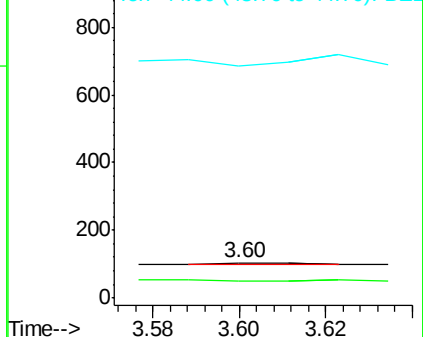

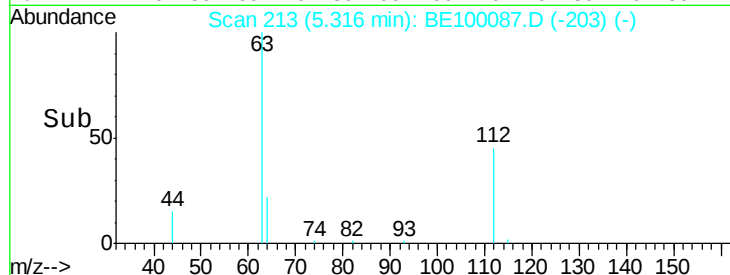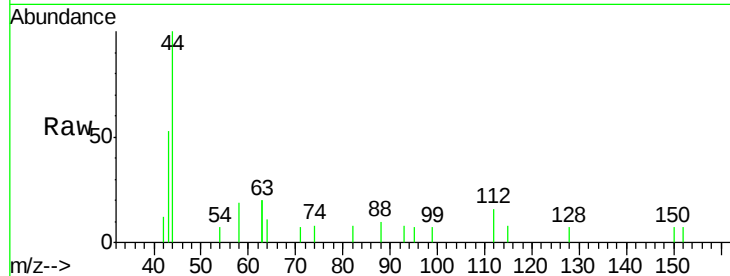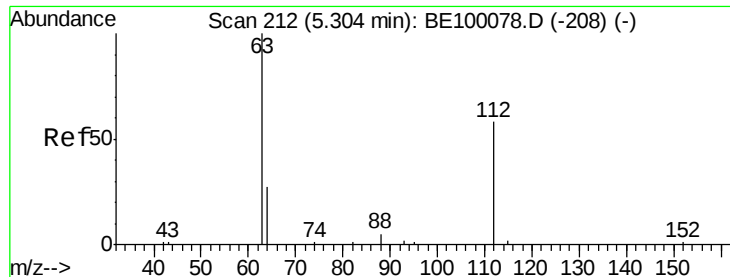

#4

2-Fluorophenol

Concen: 0.318 ng

RT: 5.32 min Scan# 213

Delta R.T. 0.01 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL





Tgt Ion: 112 Resp: 325

Ion Ratio Lower Upper

112 100

64 32.6 22.0 33.0

63 151.7 121.8 182.6

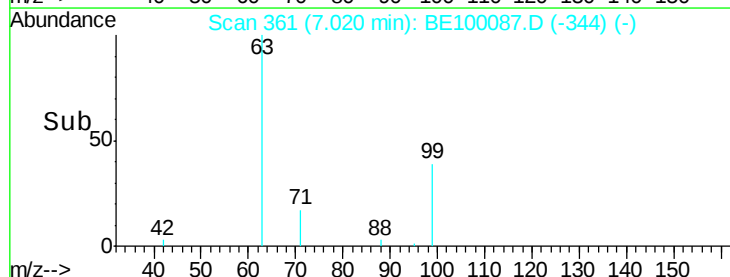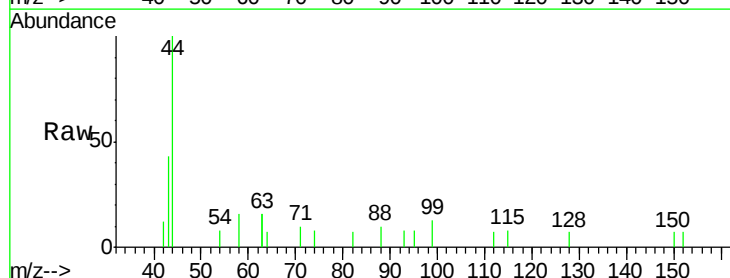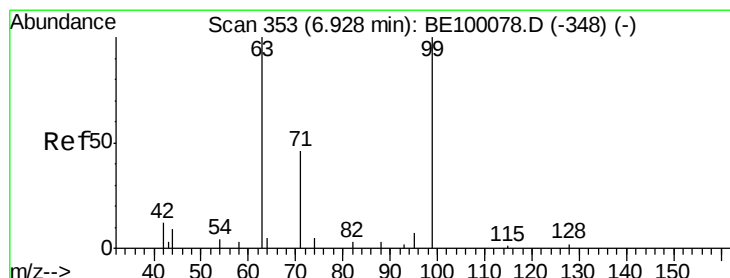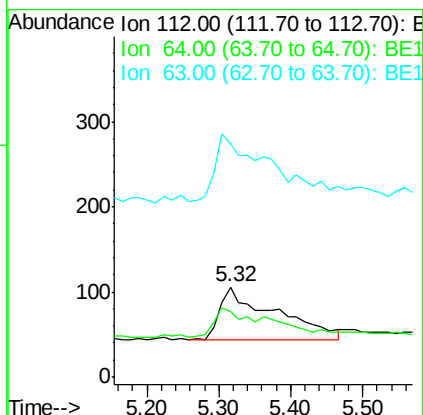

#5

Phenol-d6

Concen: 0.305 ng

RT: 7.02 min Scan# 361

Delta R.T. 0.09 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02


Tgt Ion: 99 Resp: 429


Ion Ratio Lower Upper

99 100

42 1.9 0.0 0.0#

71 0.0 37.6 56.4#

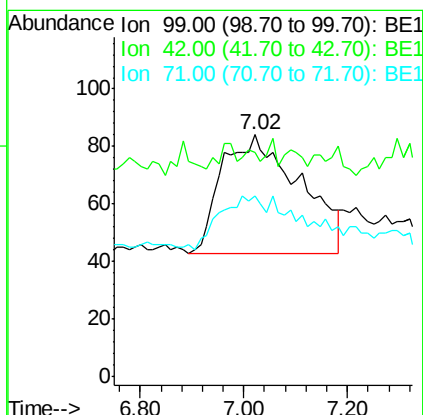

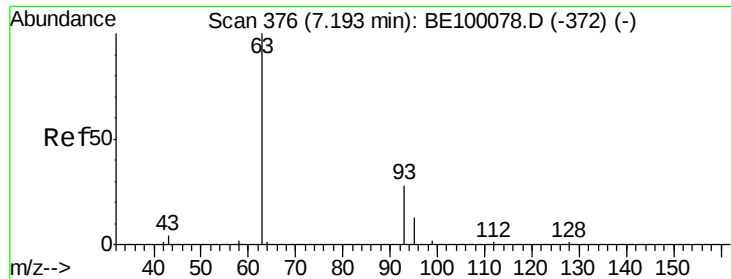

#6

bis(2-Chloroethyl)ether

Concen: 0.038 ng

RT: 7.22 min Scan# 378

Delta R.T. 0.02 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL


Tgt Ion: 93 Resp: 6

Ion Ratio Lower Upper

93 100

63 0.0 200.0 300.0#




95 200.0 24.0 36.0#

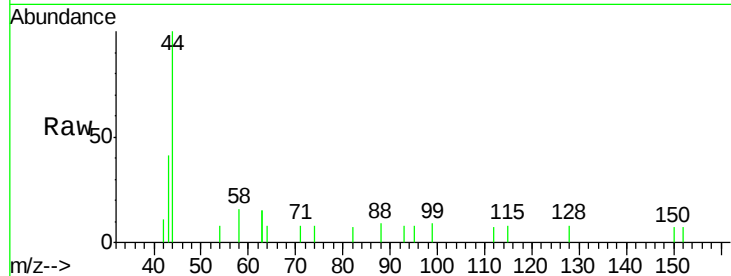

Abundance Ion 93.00 (92.70 to 93.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

Ion 95.00 (94.70 to 95.70): BE1

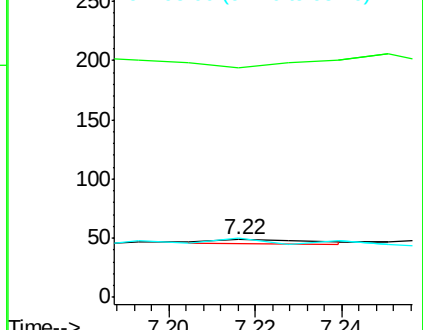

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.58 min Scan# 647

Delta R.T. 0.04 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Tgt Ion: 136 Resp: 1697


Ion Ratio Lower Upper

136 100

137 21.2 11.6 17.4#

54 70.8 33.9 50.9#

68 18.7 7.8 11.8#






Abundance Ion 136.00 (135.70 to 136.70): BE1

Ion 137.00 (136.70 to 137.70): BE1

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

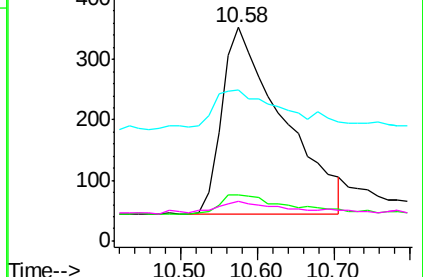



#8

Nitrobenzene-d5

Concen: 0.230 ng

RT: 9.00 min Scan# 526

Delta R.T. 0.09 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL


Tgt Ion: 82 Resp: 378

Ion Ratio Lower Upper

82 100

128 249.5 128.0 192.0#




54 251.5 143.4 215.0#

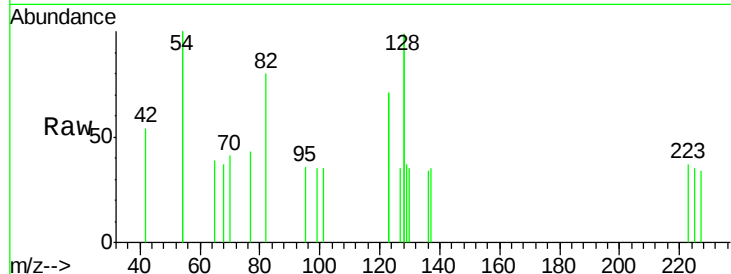

Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): BE1

Ion 54.00 (53.70 to 54.70): BE1

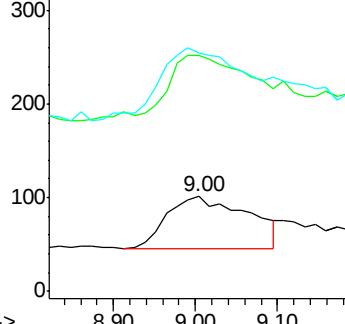

#11

2-Methylnaphthalene-d10

Concen: 0.267 ng

RT: 12.21 min Scan# 763

Delta R.T. 0.06 min

Lab File: BE100087.D


Acq: 19 Jun 2019 18:02

Tgt Ion: 152 Resp: 861

Ion Ratio Lower Upper



152 100


151 16.6 16.3 24.5

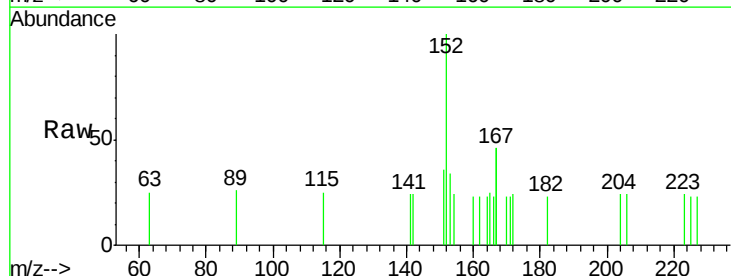

Abundance Ion 152.00 (151.70 to 152.70): BE1

Ion 151.00 (150.70 to 151.70): BE1

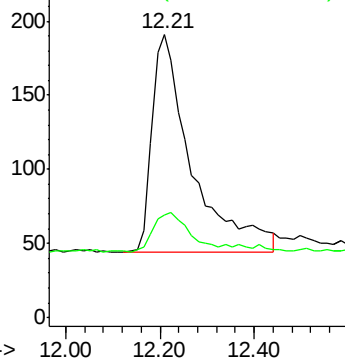

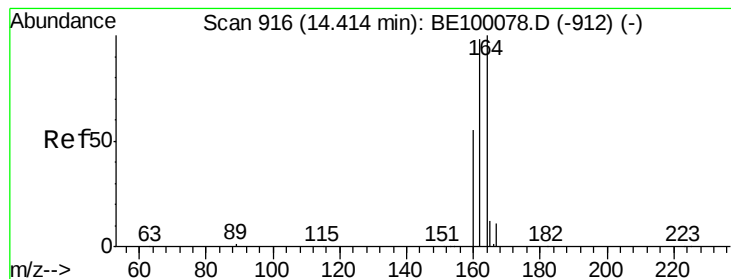

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.43 min Scan# 917

Delta R.T. 0.01 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL


Tgt Ion:164 Resp: 1283

Ion Ratio Lower Upper

164 100

162 97.1 78.2 117.2


160 65.5 45.6 68.4

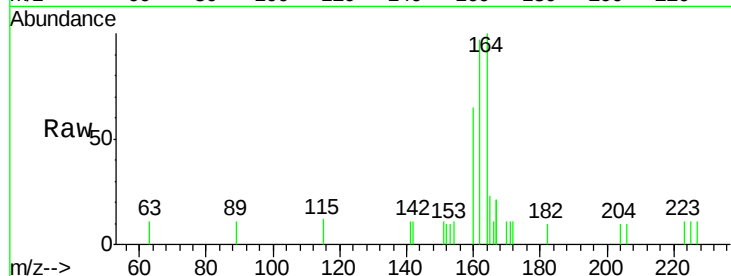



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

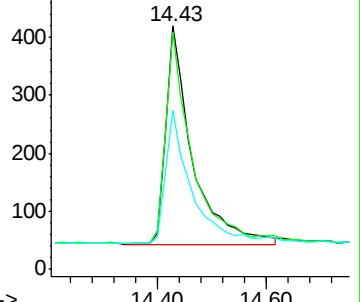

Time-->

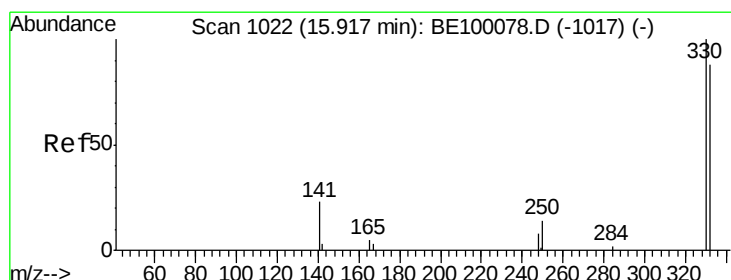

#14

2,4,6-Tribromophenol

Concen: 0.089 ng

RT: 15.97 min Scan# 1026

Delta R.T. 0.05 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02


Tgt Ion:330 Resp: 63

Ion Ratio Lower Upper

330 100

332 114.3 73.3 109.9#


141 47.6 22.2 33.2#




Abundance Ion 330.00 (329.70 to 330.70): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

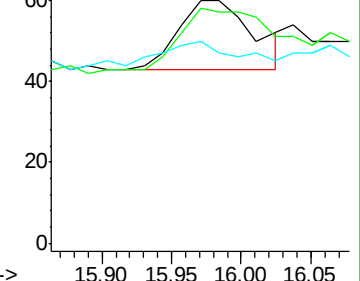

Time-->







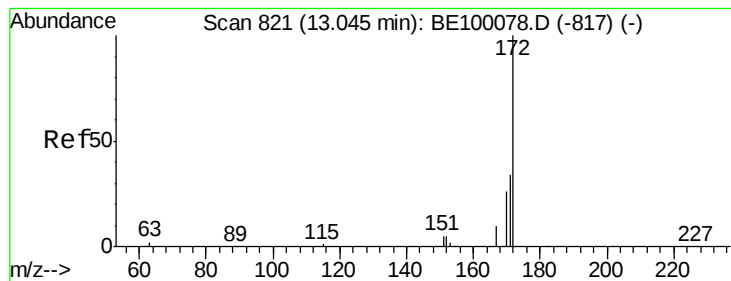

#15
2-Fluorobiphenyl
Concen: 0.323 ng
RT: 13.07 min Scan# 823
Delta R.T. 0.03 min
Lab File: BE100087.D
Acq: 19 Jun 2019 18:02




Instrument :
BNA_E
ClientSampleId :
PB120491BL


Tgt Ion:172 Resp: 1631
Ion Ratio Lower Upper
172 100
171 43.4 29.8 44.8
170 33.9 23.2 34.8

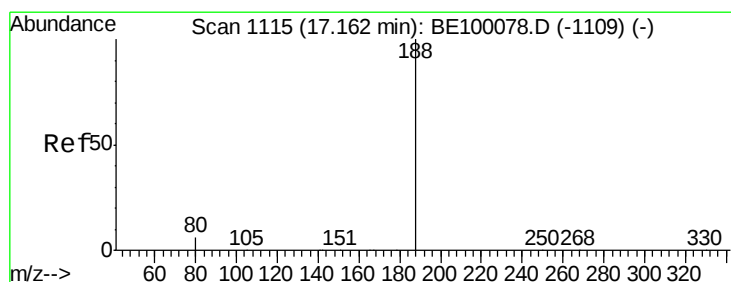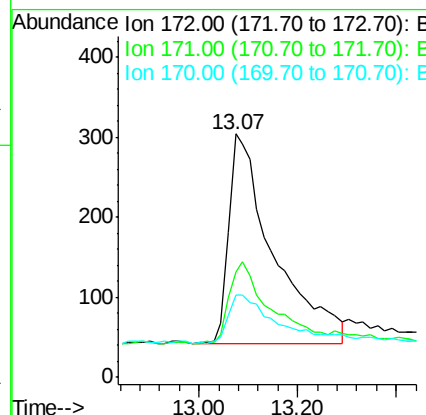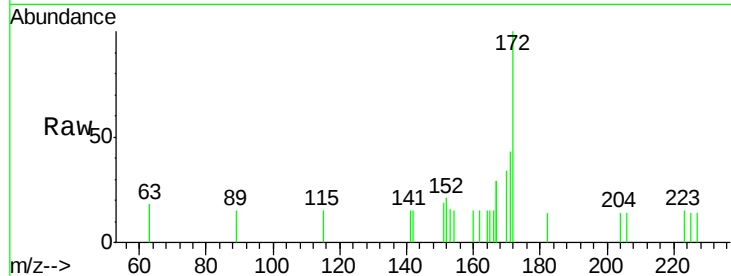

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.19 min Scan# 1117
Delta R.T. 0.03 min
Lab File: BE100087.D
Acq: 19 Jun 2019 18:02

Tgt Ion:188 Resp: 3650
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.2 6.3 9.5#

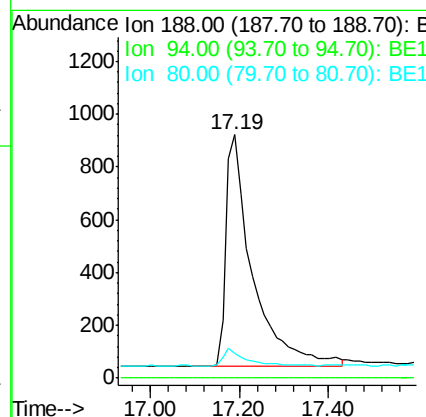

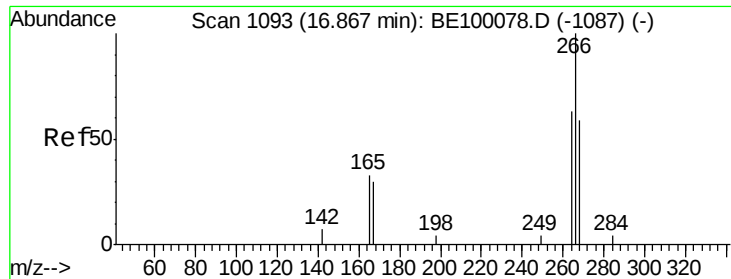

#22

Pentachlorophenol

Concen: 0.246 ng

RT: 16.91 min Scan# 1096

Delta R.T. 0.04 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02





Instrument :

BNA_E

ClientSampleId :

PB120491BL

Tgt Ion:	266	Resp:	3
Ion	Ratio	Lower	Upper
266	100		
264	93.5	67.8	101.6
268	102.2	70.0	105.0

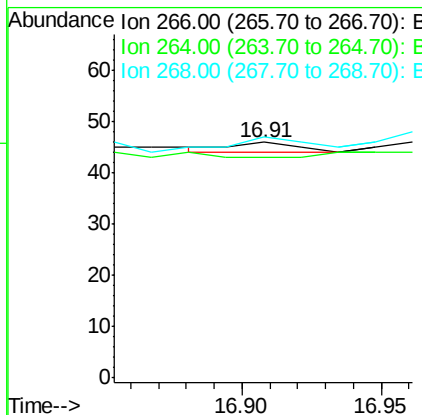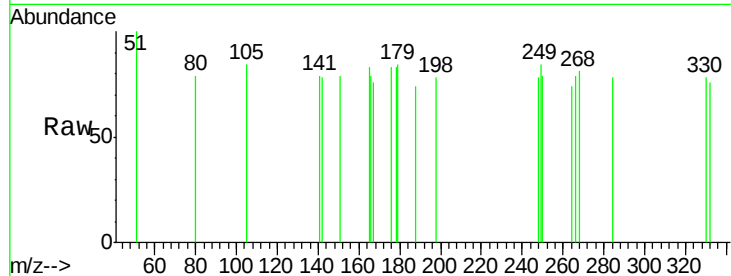

#25

Fluoranthene-d10

Concen: 0.274 ng




RT: 19.21 min Scan# 1383


Delta R.T. 0.02 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Tgt Ion:	212	Resp:	14277
Ion	Ratio	Lower	Upper
212	100		
106	1.7	1.4	2.0
104	0.9	0.8	1.2


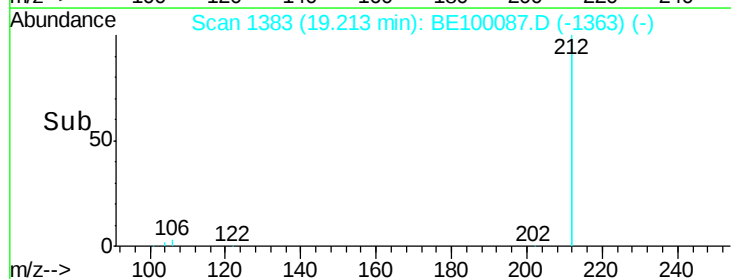
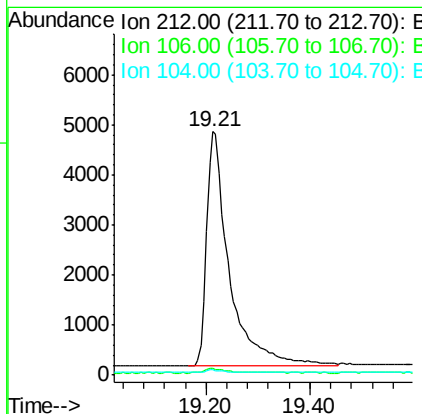





#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.35 min Scan# 1629
 Delta R.T. 0.01 min
 Lab File: BE100087.D
 Acq: 19 Jun 2019 18:02




Instrument :
 BNA_E
 ClientSampled :
 PB120491BL




Tgt Ion:240 Resp: 5297
 Ion Ratio Lower Upper
 240 100
 120 8.1 6.6 10.0
 236 29.6 23.8 35.6

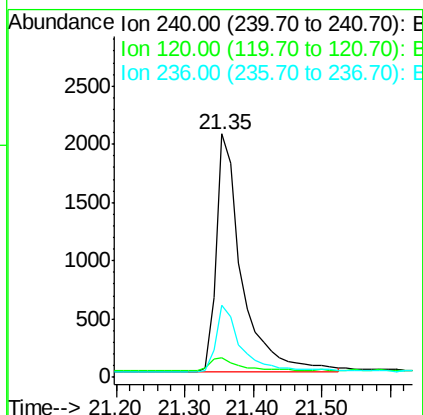

#29
 Terphenyl-d14
 Concen: 0.335 ng
 RT: 19.81 min Scan# 1487
 Delta R.T. 0.01 min
 Lab File: BE100087.D
 Acq: 19 Jun 2019 18:02

Tgt Ion:244 Resp: 3551
 Ion Ratio Lower Upper
 244 100
 212 41.8 29.8 44.8
 122 9.5 6.1 9.1#

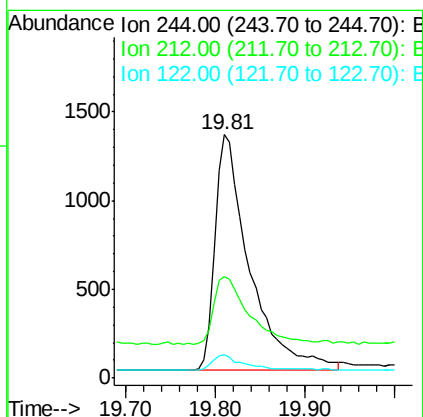

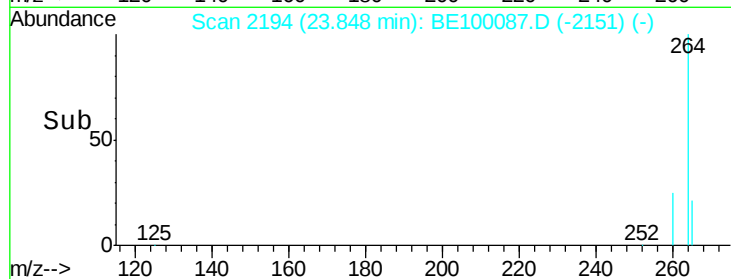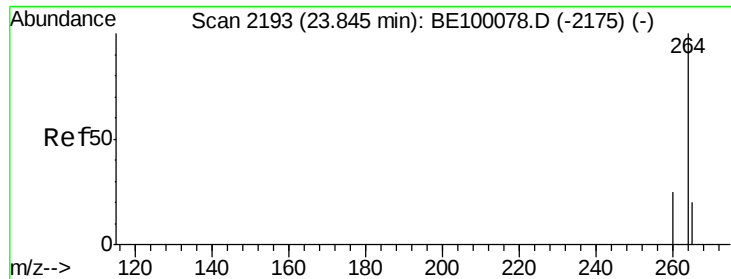

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.85 min Scan# 2194

Delta R.T. 0.00 min

Lab File: BE100087.D

Acq: 19 Jun 2019 18:02

Instrument :

BNA_E

ClientSampleId :

PB120491BL

Tgt Ion:264 Resp: 6906

Ion Ratio Lower Upper

264 100

260 26.0 20.8 31.2

265 29.7 23.2 34.8

