

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE061919\
 Data File : BE100096.D
 Acq On : 19 Jun 2019 23:28
 Operator : JU/SJ
 Sample : K3309-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 LF016MW001-190610

Quant Time: Jun 20 03:52:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 19 15:07:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	844	0.40	ng	-0.01
7) Naphthalene-d8	10.52	136	2998	0.40	ng	-0.01
13) Acenaphthene-d10	14.41	164	2425	0.40	ng	0.00
19) Phenanthrene-d10	17.16	188	7769	0.40	ng	0.00
27) Chrysene-d12	21.34	240	10724	0.40	ng	0.00
34) Perylene-d12	23.84	264	12369	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.30	112	311	0.18	ng	0.00
5) Phenol-d6	6.89	99	265	0.11	ng	-0.03
8) Nitrobenzene-d5	8.90	82	1065	0.37	ng	-0.01
11) 2-Methylnaphthalene-d10	12.14	152	1527	0.27	ng	-0.01
14) 2,4,6-Tribromophenol	15.90	330	647	0.48	ng	-0.01
15) 2-Fluorobiphenyl	13.03	172	3146	0.33	ng	-0.01
25) Fluoranthene-d10	19.20	212	31267	0.28	ng	0.00
29) Terphenyl-d14	19.79	244	8311	0.39	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.20	88	193	0.143	ng	# 41
3) n-Nitrosodimethylamine	3.61	42	21	0.365	ng	# 100
6) bis(2-Chloroethyl)ether	7.24	93	6	0.036	ng	# 1
9) Naphthalene	10.58	128	684	0.021	ng	# 77
22) Pentachlorophenol	16.81	266	58	0.277	ng	94
23) Phenanthrene	17.20	178	848	0.046	ng	# 86
26) Fluoranthene	19.22	202	698	0.023	ng	# 59
28) Pyrene	19.59	202	769	0.028	ng	# 63
32) Bis(2-ethylhexyl)phthalate	21.25	149	8881	0.295	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE061919\
Data File : BE100096.D
Acq On : 19 Jun 2019 23:28
Operator : JU/SJ
Sample : K3309-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
LF016MW001-190610

Quant Time: Jun 20 03:52:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 19 15:07:24 2019
Response via : Initial Calibration

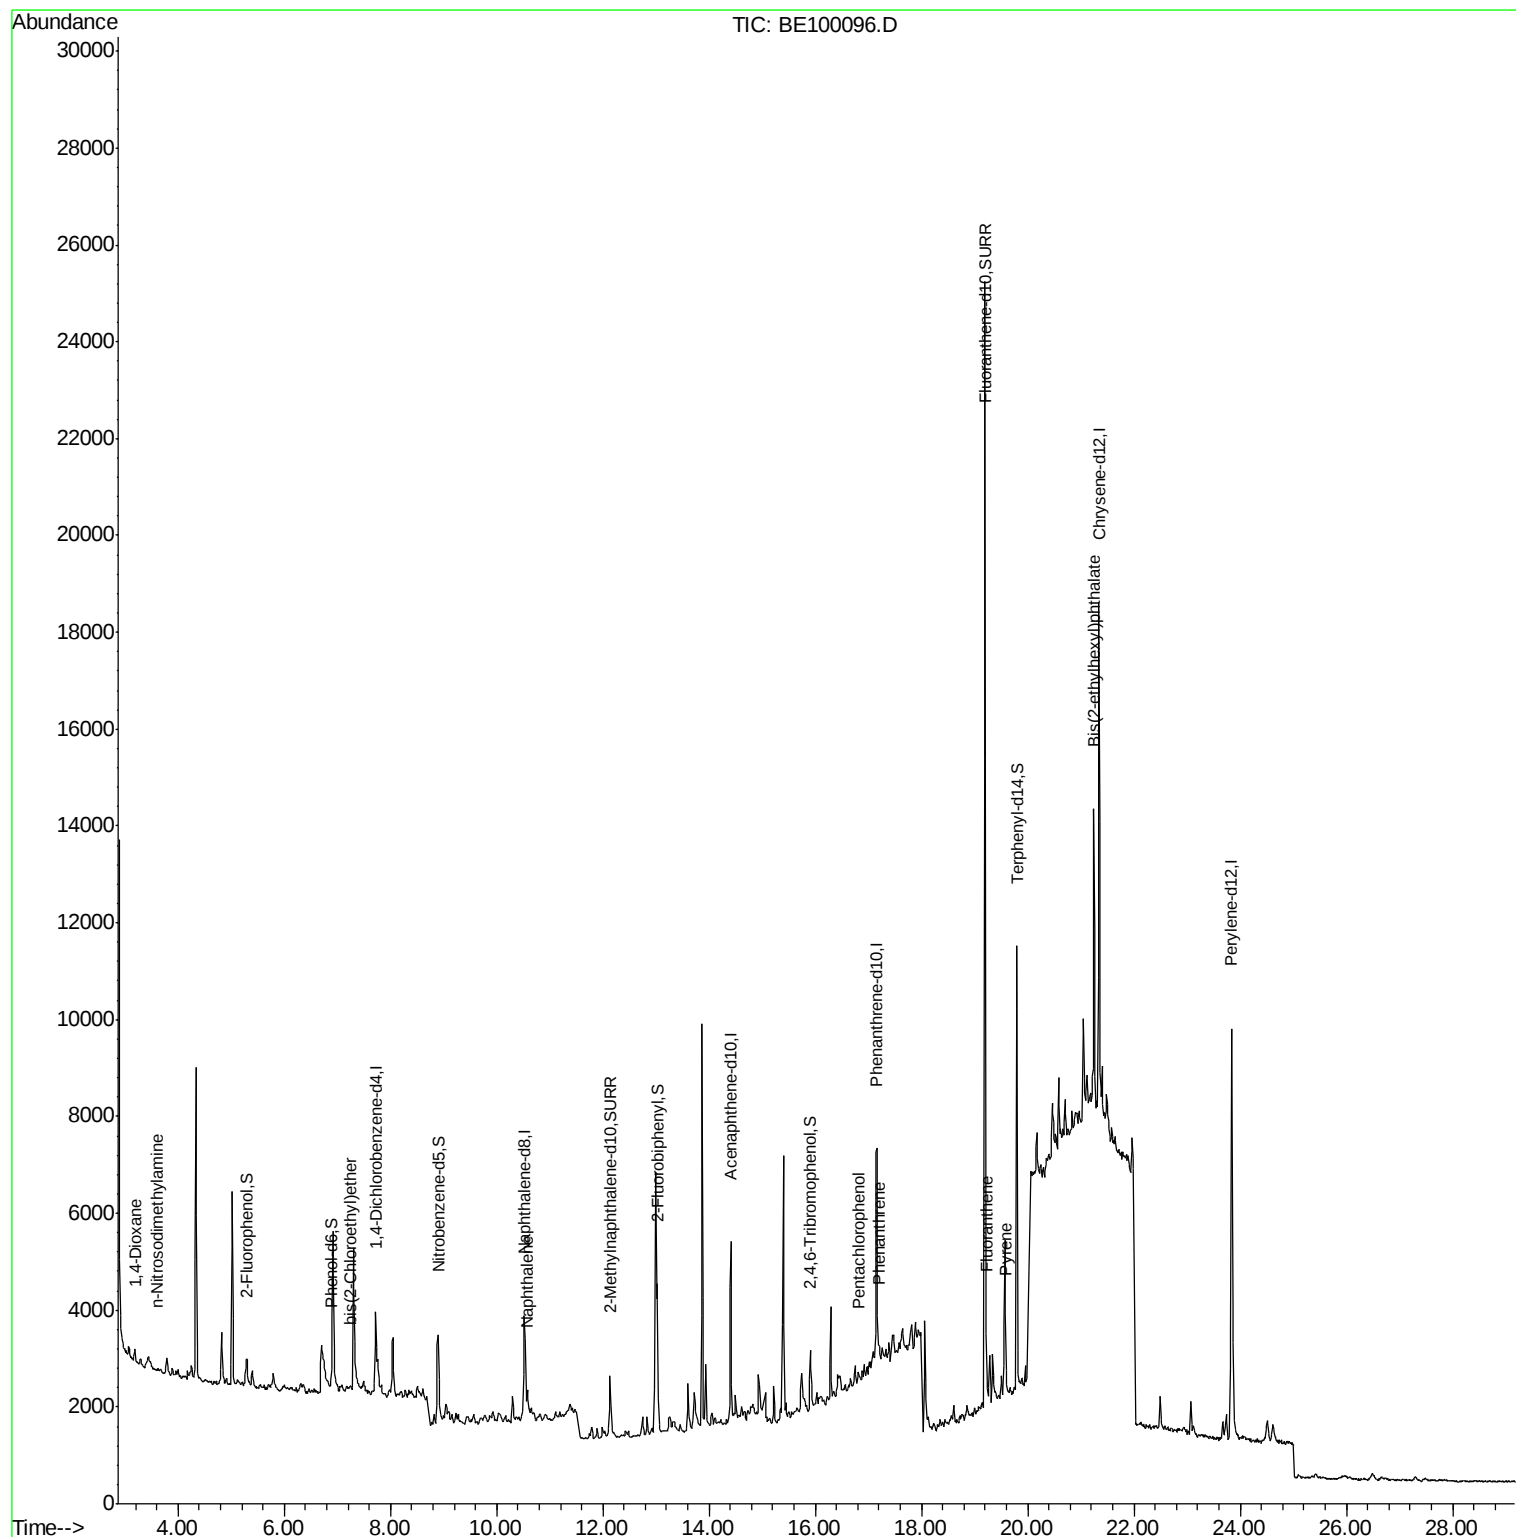







#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 422
Delta R.T. -0.01 min
Lab File: BE100096.D
Acq: 19 Jun 2019 23:28

Instrument :
BNA_E
ClientSampleId :
LF016MW001-190610




Tgt Ion: 152 Resp: 844
Ion Ratio Lower Upper
152 100
150 141.9 99.8 149.8
115 65.1 51.3 76.9

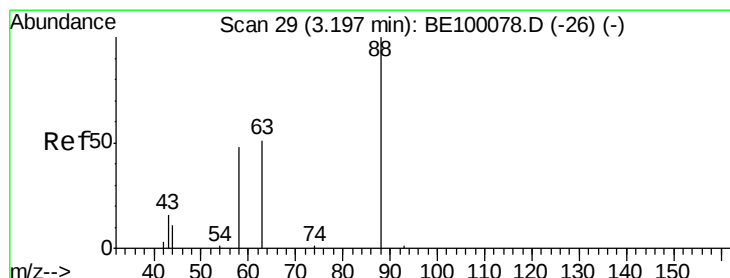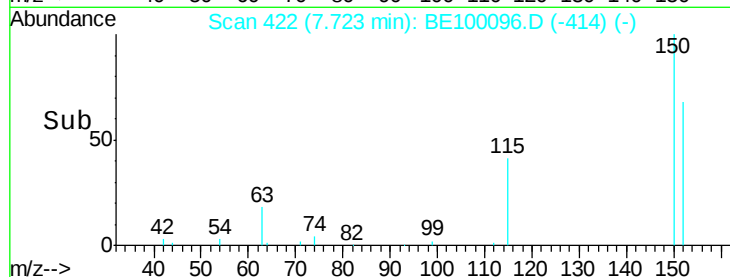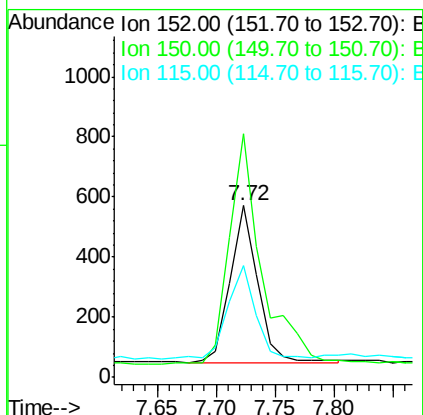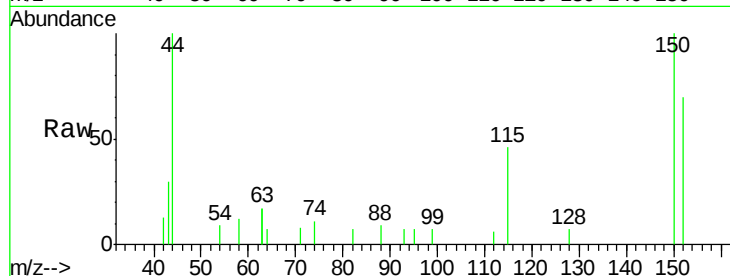

#2

1,4-Dioxane
Concen: 0.143 ng
RT: 3.20 min Scan# 29
Delta R.T. 0.00 min
Lab File: BE100096.D
Acq: 19 Jun 2019 23:28

Tgt Ion: 88 Resp: 193
Ion Ratio Lower Upper
88 100
58 55.4 51.1 76.7
43 116.6 21.7 32.5#

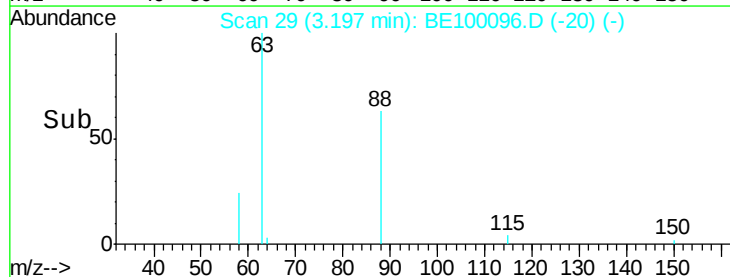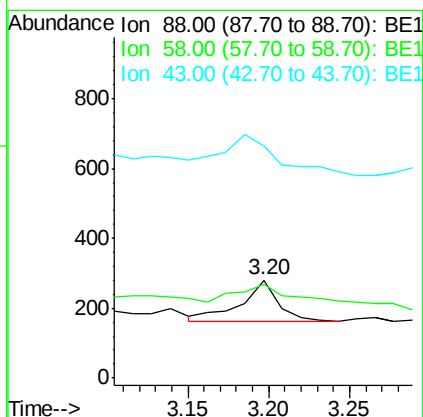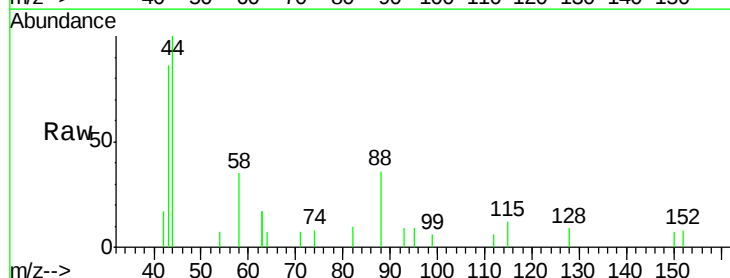



#3

n-Nitrosodimethylamine

Concen: 0.365 ng

RT: 3.61 min Scan# 65

Delta R.T. 0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28





Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610

Tgt Ion:	42	Resp:	21
Ion	Ratio	Lower	Upper
42	100		
74	0.0	0.0	0.0
44	395.2	0.0	0.0#

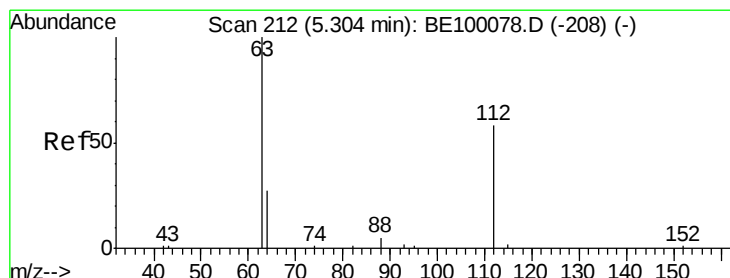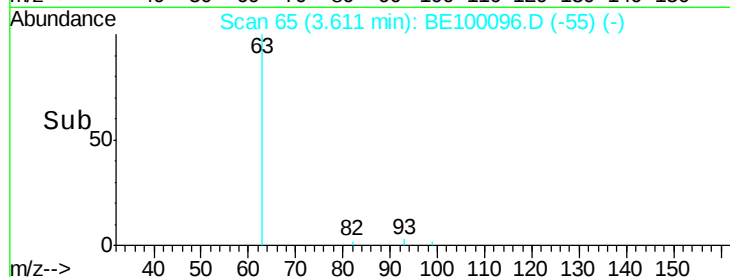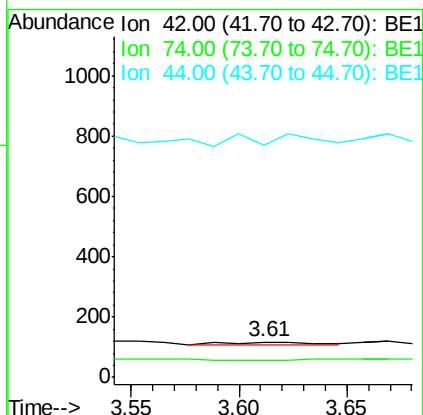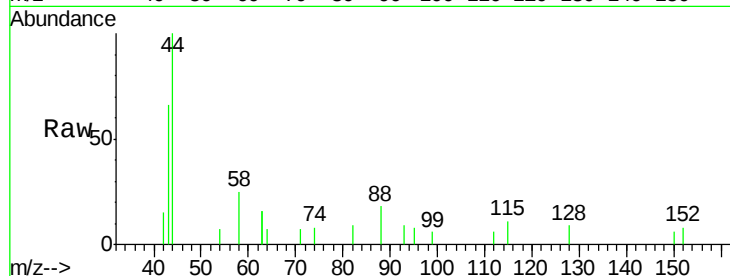

#4

2-Fluorophenol

Concen: 0.178 ng




RT: 5.30 min Scan# 212


Delta R.T. 0.00 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Tgt Ion:	112	Resp:	311
Ion	Ratio	Lower	Upper
112	100		
64	56.3	22.0	33.0#
63	118.6	121.8	182.6#

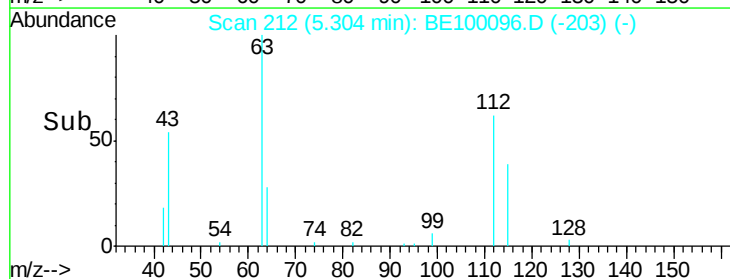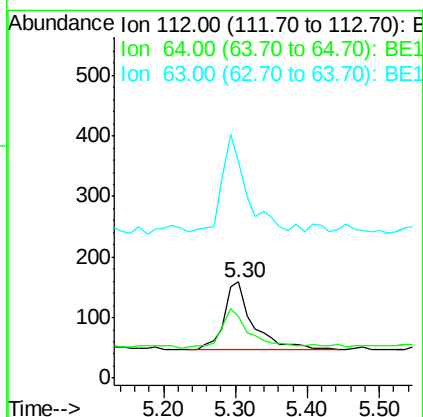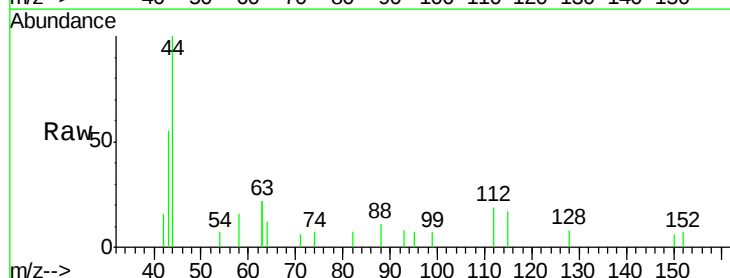



#5

Phenol-d6

Concen: 0.110 ng

RT: 6.89 min Scan# 350

Delta R.T. -0.03 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610


Tgt Ion: 99 Resp: 265

Ion Ratio Lower Upper




99 100

42 0.0 0.0 0.0

71 60.4 37.6 56.4#

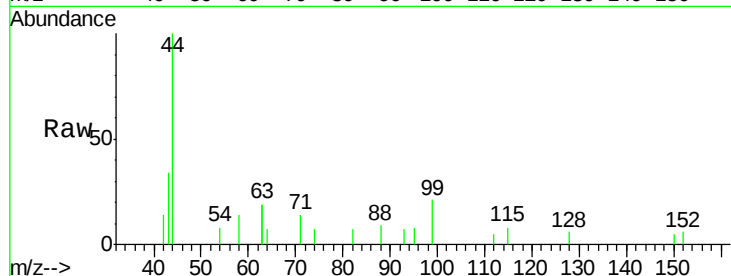

Abundance Ion 99.00 (98.70 to 99.70): BE1
Ion 42.00 (41.70 to 42.70): BE1
Ion 71.00 (70.70 to 71.70): BE1

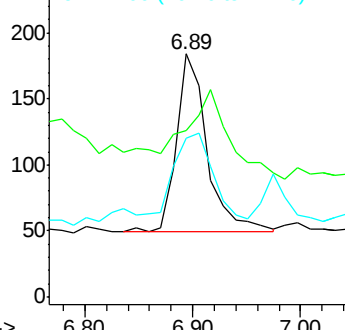

#6

bis(2-Chloroethyl)ether

Concen: 0.036 ng

RT: 7.24 min Scan# 380

Delta R.T. 0.05 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28


Tgt Ion: 93 Resp: 6

Ion Ratio Lower Upper



93 100

63 0.0 200.0 300.0#

95 83.3 24.0 36.0#



Abundance Ion 93.00 (92.70 to 93.70): BE1
Ion 63.00 (62.70 to 63.70): BE1
Ion 95.00 (94.70 to 95.70): BE1

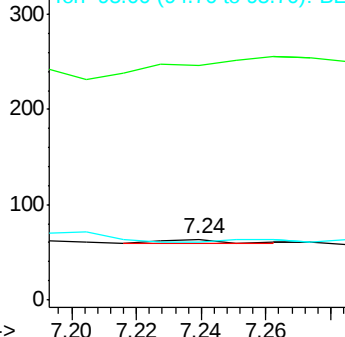



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.52 min Scan# 643

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610

Tgt Ion: 136 Resp: 2998


Ion Ratio Lower Upper

136 100

137 14.3 11.6 17.4

54 41.6 33.9 50.9

68 10.4 7.8 11.8



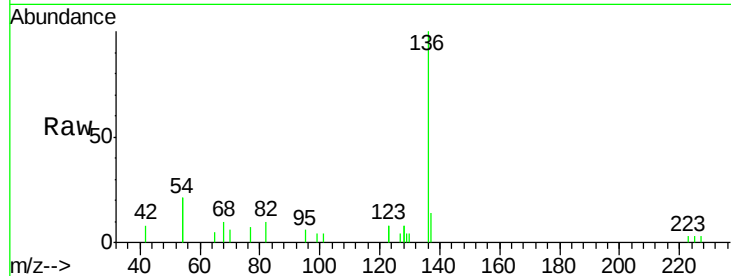


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE1

Ion 68.00 (67.70 to 68.70): BE1

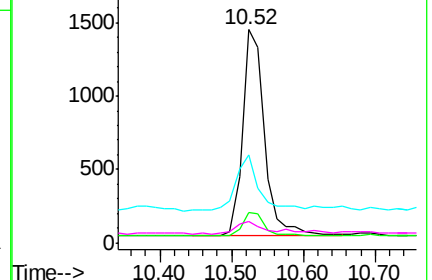

#8

Nitrobenzene-d5

Concen: 0.366 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28


Tgt Ion: 82 Resp: 1065

Ion Ratio Lower Upper

82 100

128 204.7 128.0 192.0#



54 154.2 143.4 215.0




Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE1

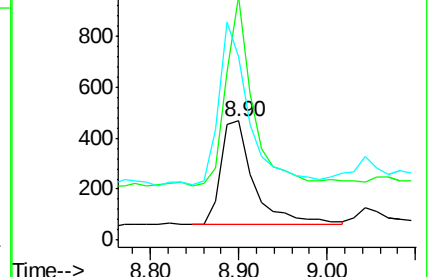

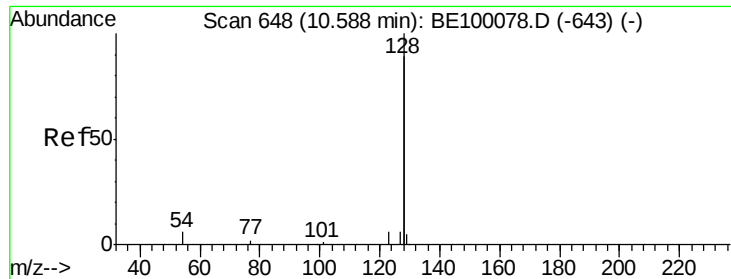

#9

Naphthalene

Concen: 0.021 ng

RT: 10.58 min Scan# 647

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610


Tgt Ion:128 Resp: 684

Ion Ratio Lower Upper

128 100

129 12.8 3.1 4.7#




127 10.7 3.4 5.2#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

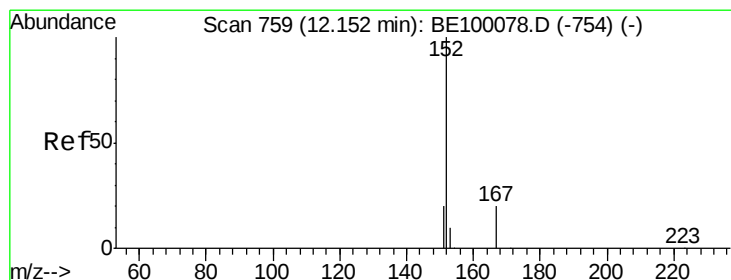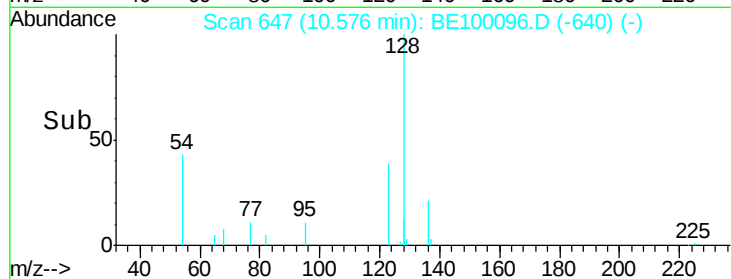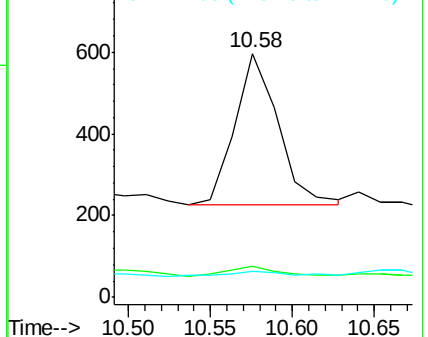

#11

2-Methylnaphthalene-d10

Concen: 0.268 ng

RT: 12.14 min Scan# 758

Delta R.T. -0.01 min

Lab File: BE100096.D


Acq: 19 Jun 2019 23:28

Tgt Ion:152 Resp: 1527

Ion Ratio Lower Upper



152 100


151 23.2 16.3 24.5



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

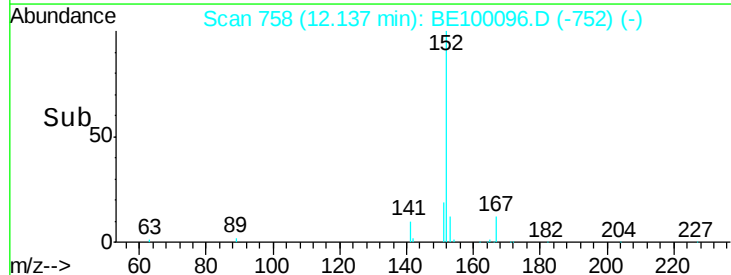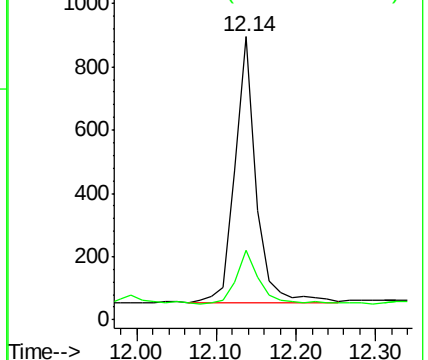

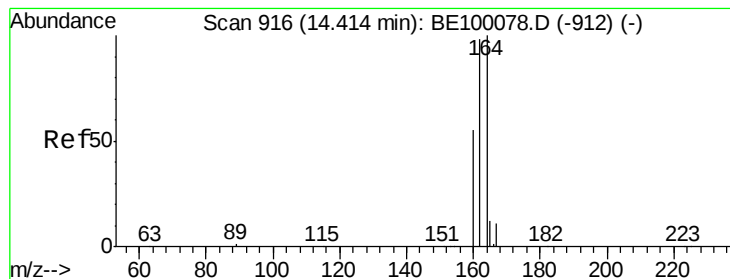

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.41 min Scan# 916

Delta R.T. 0.00 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610


Tgt Ion:164 Resp: 2425

Ion Ratio Lower Upper

164 100

162 94.9 78.2 117.2




160 47.6 45.6 68.4

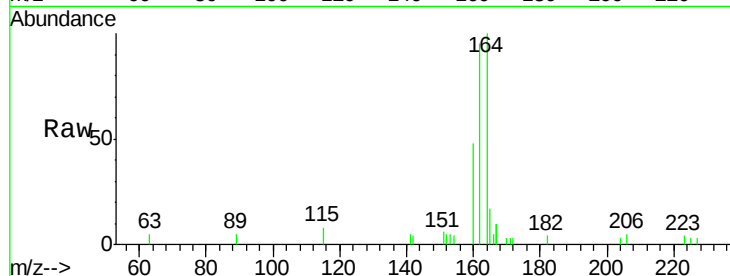

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

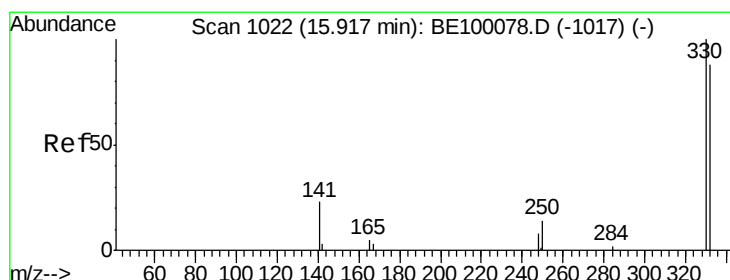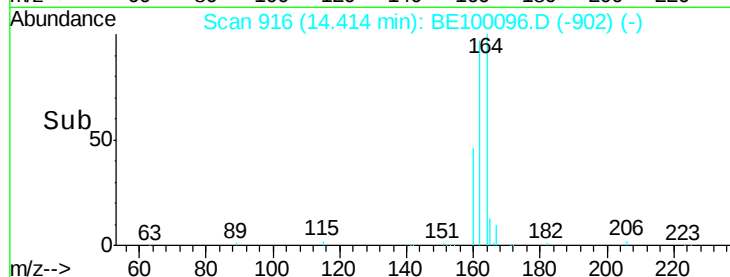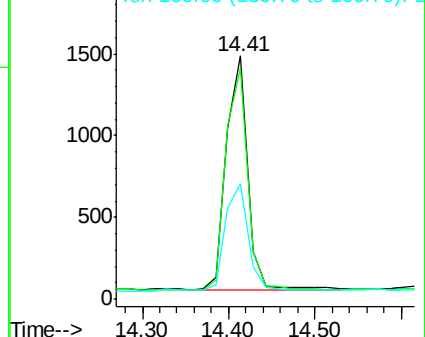

#14

2,4,6-Tribromophenol

Concen: 0.483 ng

RT: 15.90 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28


Tgt Ion:330 Resp: 647

Ion Ratio Lower Upper

330 100

332 93.7 73.3 109.9



141 34.5 22.2 33.2#

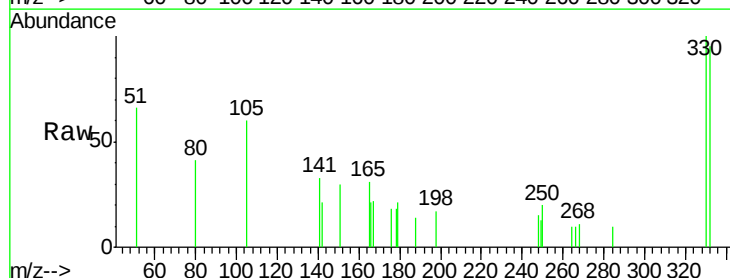


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



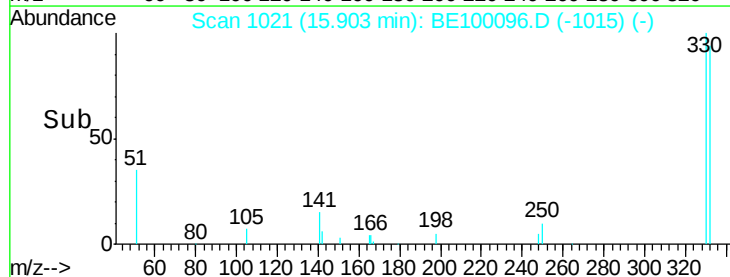
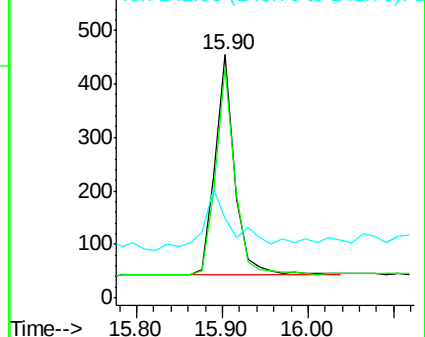


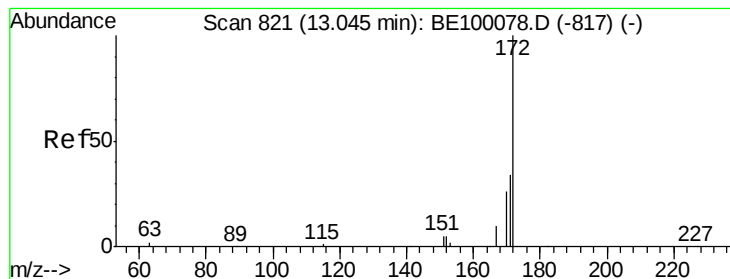

#15
 2-Fluorobiphenyl
 Concen: 0.330 ng
 RT: 13.03 min Scan# 820
 Delta R.T. -0.01 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28




Instrument :
 BNA_E
 ClientSampleId :
 LF016MW001-190610


Tgt Ion:172 Resp: 3146
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.8 44.8
 170 25.1 23.2 34.8

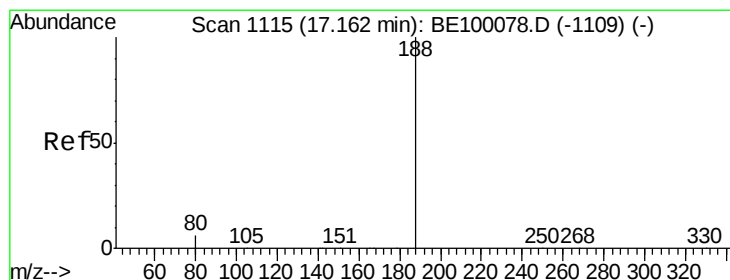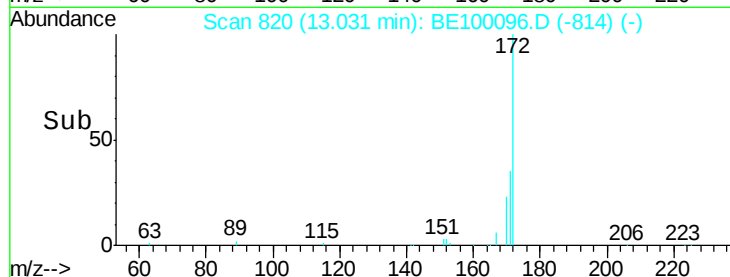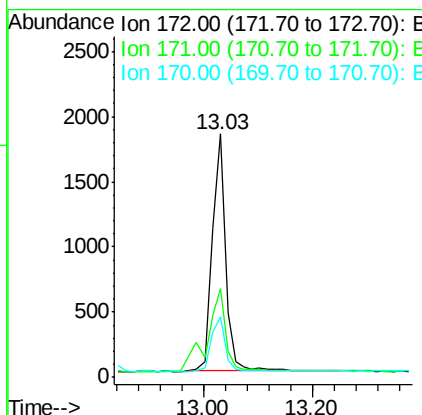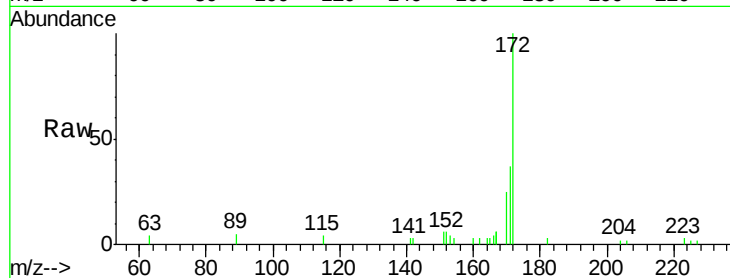

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.16 min Scan# 1115
 Delta R.T. 0.00 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28

Tgt Ion:188 Resp: 7769
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 8.1 6.3 9.5


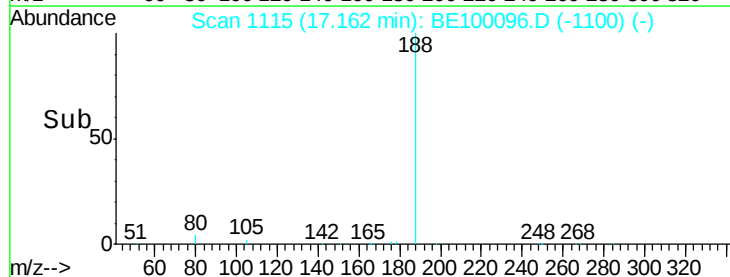
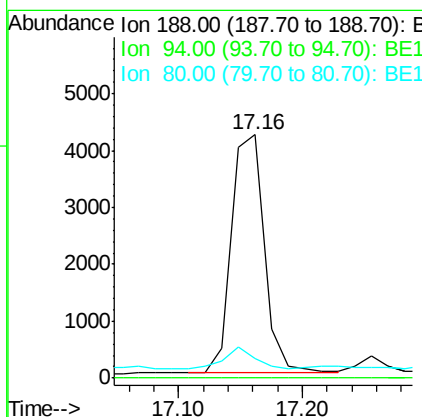
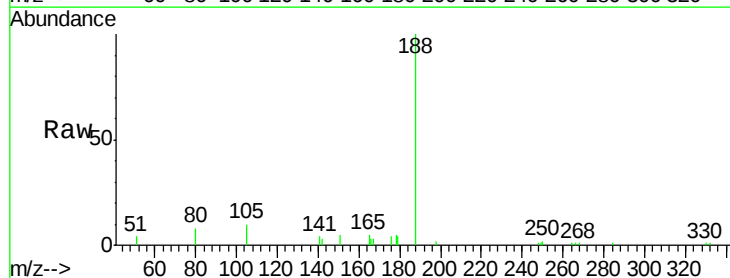


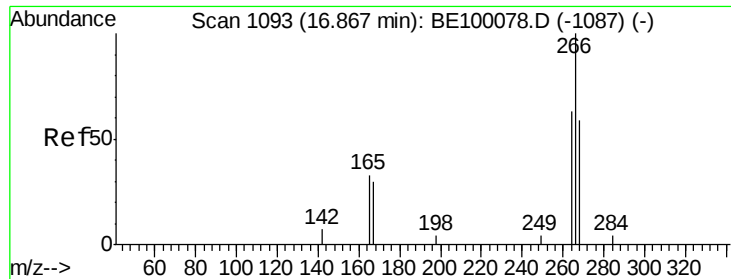

#22
 Pentachlorophenol
 Concen: 0.277 ng
 RT: 16.81 min Scan# 1089
 Delta R.T. -0.05 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28




Instrument :
 BNA_E
 ClientSampleId :
 LF016MW001-190610


Tgt Ion: 266 Resp: 58
 Ion Ratio Lower Upper
 266 100
 264 81.3 67.8 101.6
 268 80.2 70.0 105.0

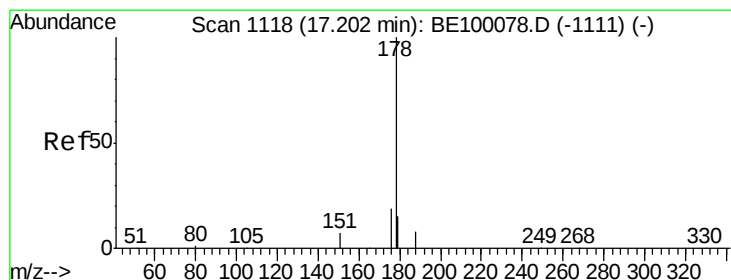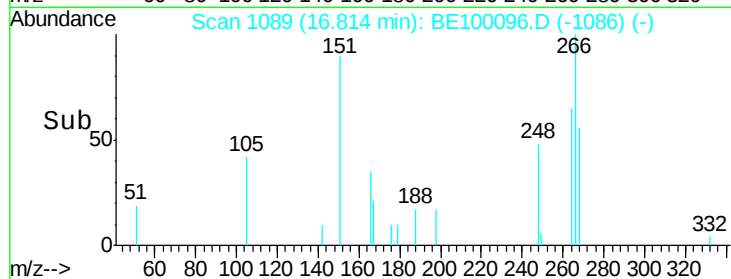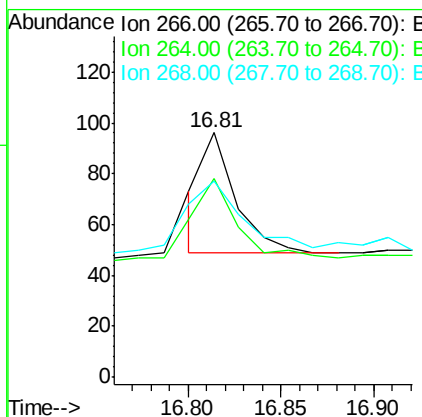

#23
 Phenanthrene
 Concen: 0.046 ng
 RT: 17.20 min Scan# 1118
 Delta R.T. 0.00 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28

Tgt Ion: 178 Resp: 848
 Ion Ratio Lower Upper
 178 100
 176 13.0 15.9 23.9#
 179 10.7 13.1 19.7#


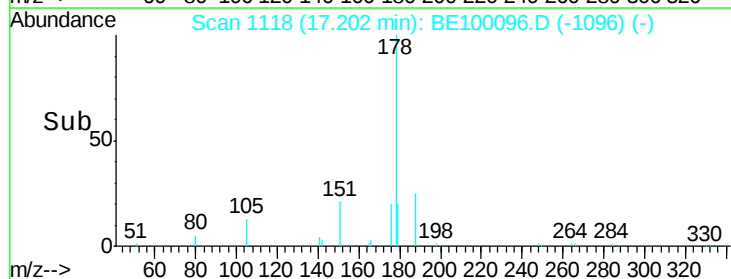
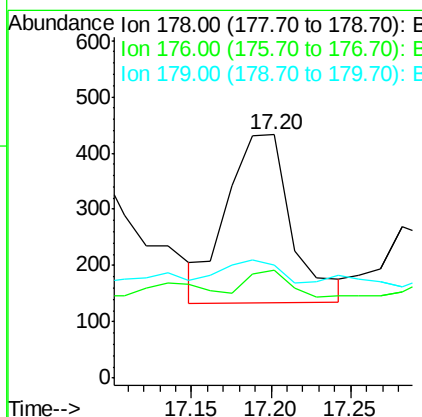
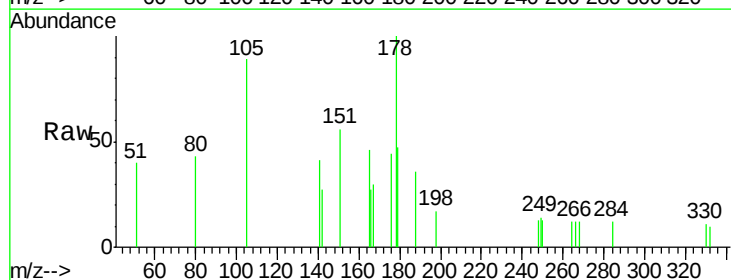




#25
 Fluoranthene-d10
 Concen: 0.282 ng
 RT: 19.20 min Scan# 1380
 Delta R.T. 0.00 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28




Instrument :
 BNA_E
 ClientSampleId :
 LF016MW001-190610


Tgt Ion: 212 Resp: 31267
 Ion Ratio Lower Upper
 212 100
 106 1.9 1.4 2.0
 104 1.1 0.8 1.2

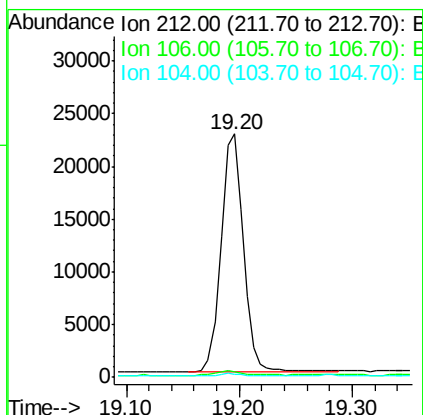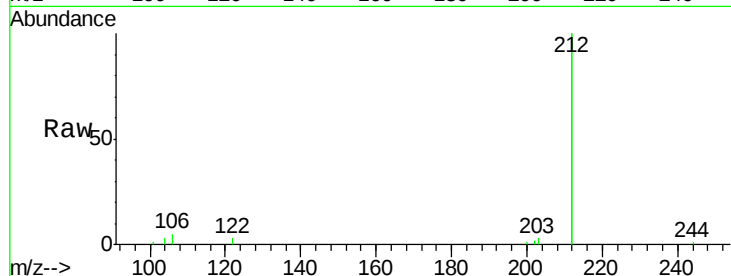

#26
 Fluoranthene
 Concen: 0.023 ng
 RT: 19.22 min Scan# 1385
 Delta R.T. -0.01 min
 Lab File: BE100096.D
 Acq: 19 Jun 2019 23:28

Tgt Ion: 202 Resp: 698
 Ion Ratio Lower Upper
 202 100
 101 27.9 5.0 7.4#
 203 31.2 13.7 20.5#

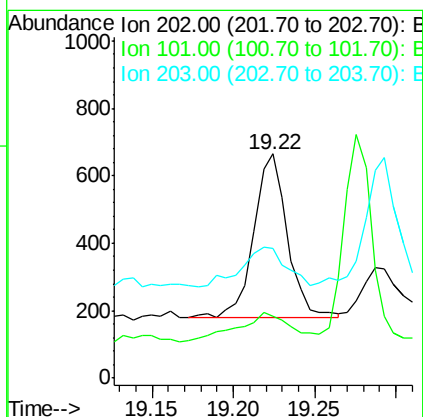



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.34 min Scan# 1628

Delta R.T. 0.00 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610


Tgt Ion:240 Resp: 10724

Ion Ratio Lower Upper

240 100

120 7.5 6.6 10.0




236 29.9 23.8 35.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

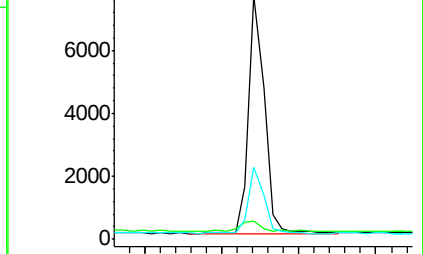

#28

Pyrene

Concen: 0.028 ng

RT: 19.59 min Scan# 1448

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28


Tgt Ion:202 Resp: 769

Ion Ratio Lower Upper

202 100

200 36.0 15.6 23.4#



203 33.8 13.9 20.9#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

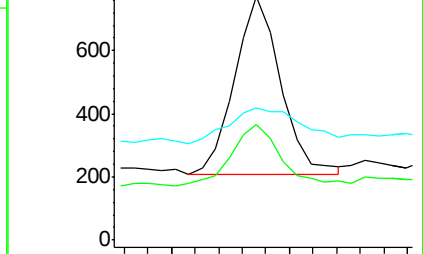

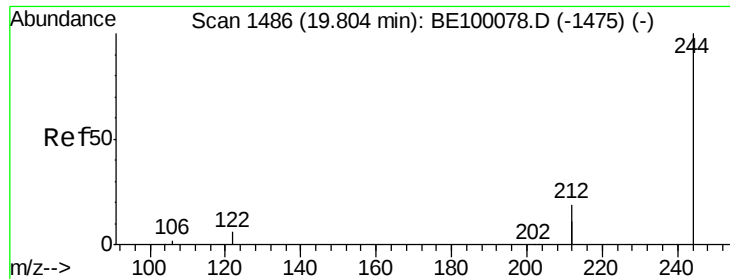

#29

Terphenyl-d14

Concen: 0.388 ng

RT: 19.79 min Scan# 1484

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610


Tgt Ion:244 Resp: 8311

Ion Ratio Lower Upper

244 100

212 36.4 29.8 44.8




122 8.7 6.1 9.1

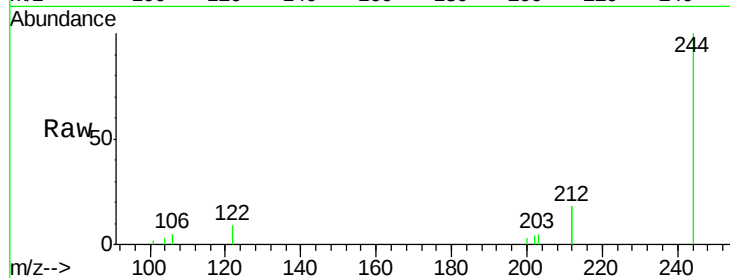

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

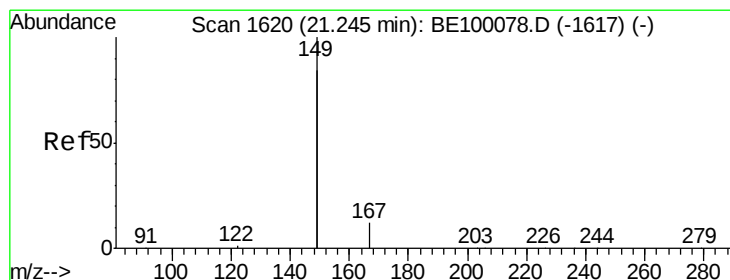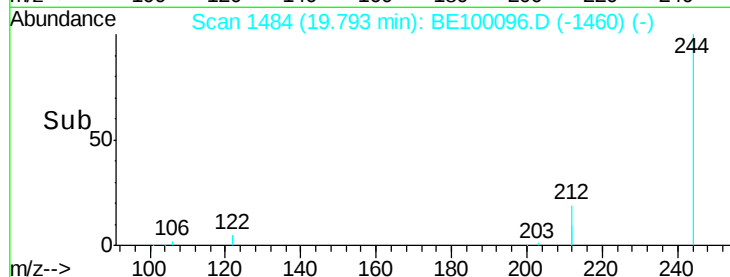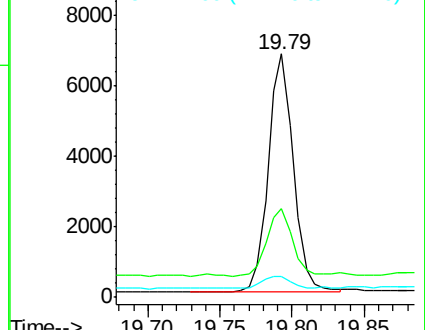

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.295 ng

RT: 21.25 min Scan# 1620

Delta R.T. 0.00 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28


Tgt Ion:149 Resp: 8881

Ion Ratio Lower Upper

149 100

167 7.0 5.8 8.6



279 1.3 1.1 1.7



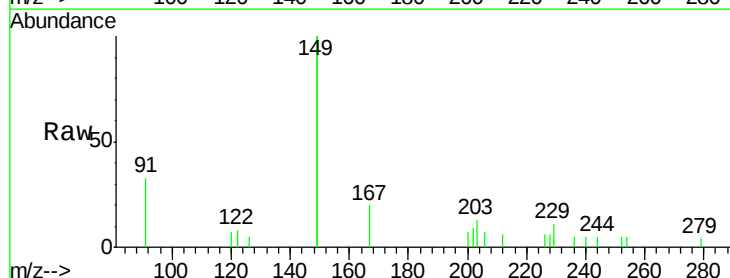


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

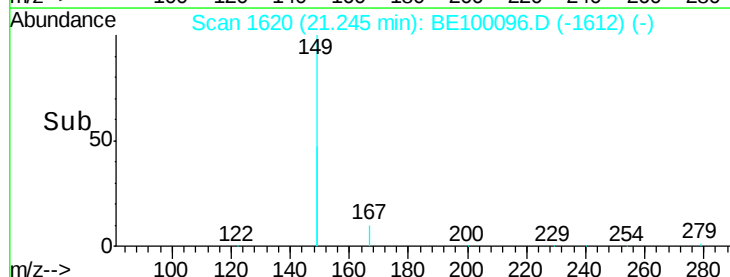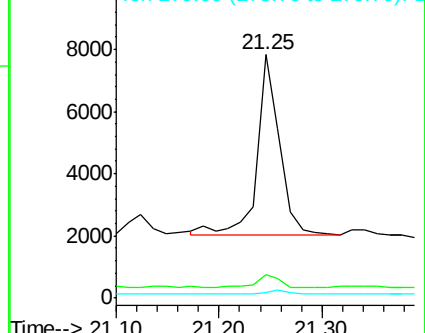

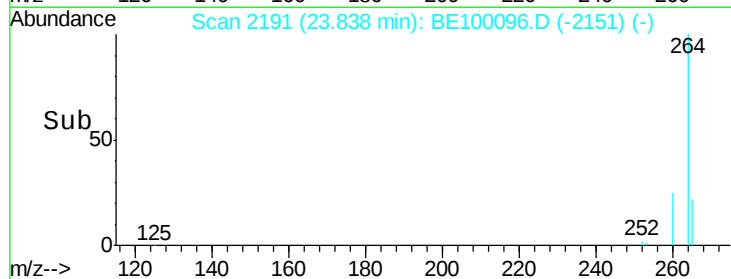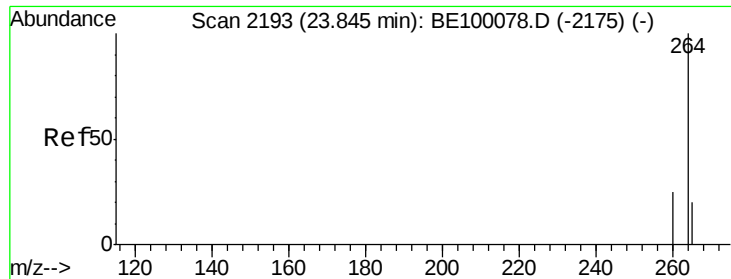

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.84 min Scan# 2191

Delta R.T. -0.01 min

Lab File: BE100096.D

Acq: 19 Jun 2019 23:28

Instrument :

BNA_E

ClientSampleId :

LF016MW001-190610

Tgt Ion:264 Resp: 12369

Ion Ratio Lower Upper

264 100

260 26.3 20.8 31.2

265 30.1 23.2 34.8

