
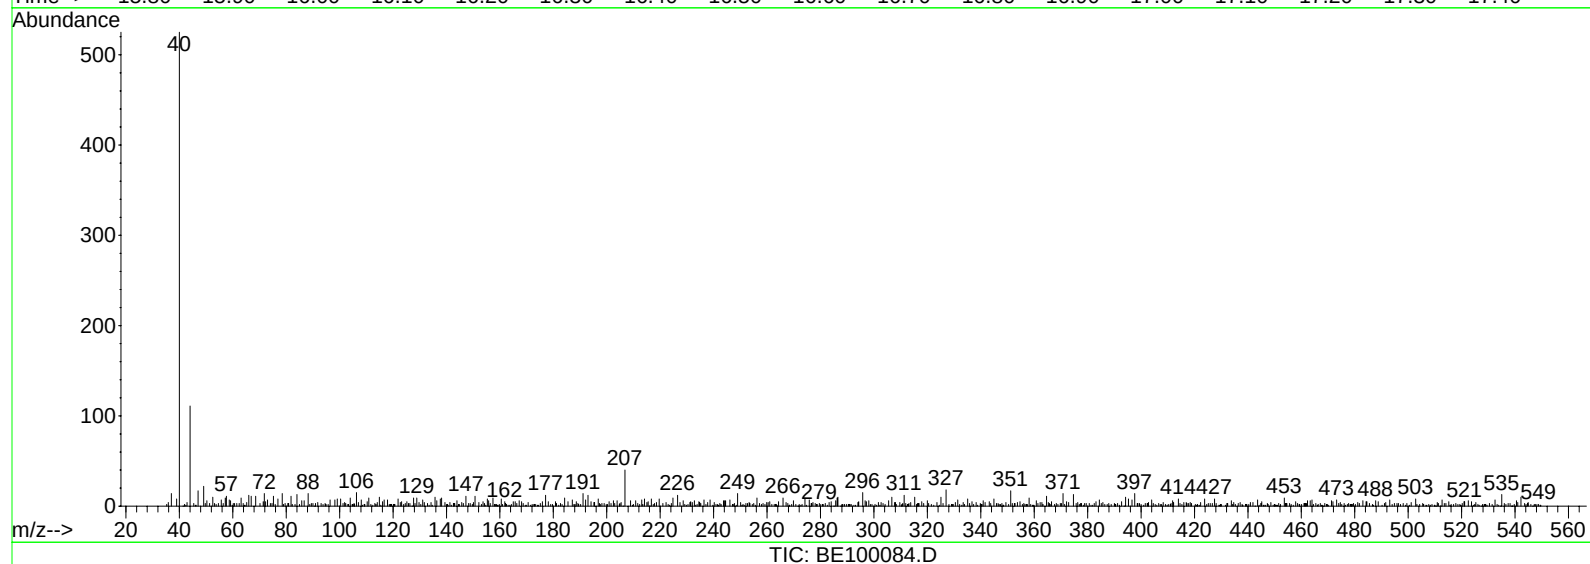


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061919\
Data File : BE100084.D
Acq On : 19 Jun 2019 15:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:59:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

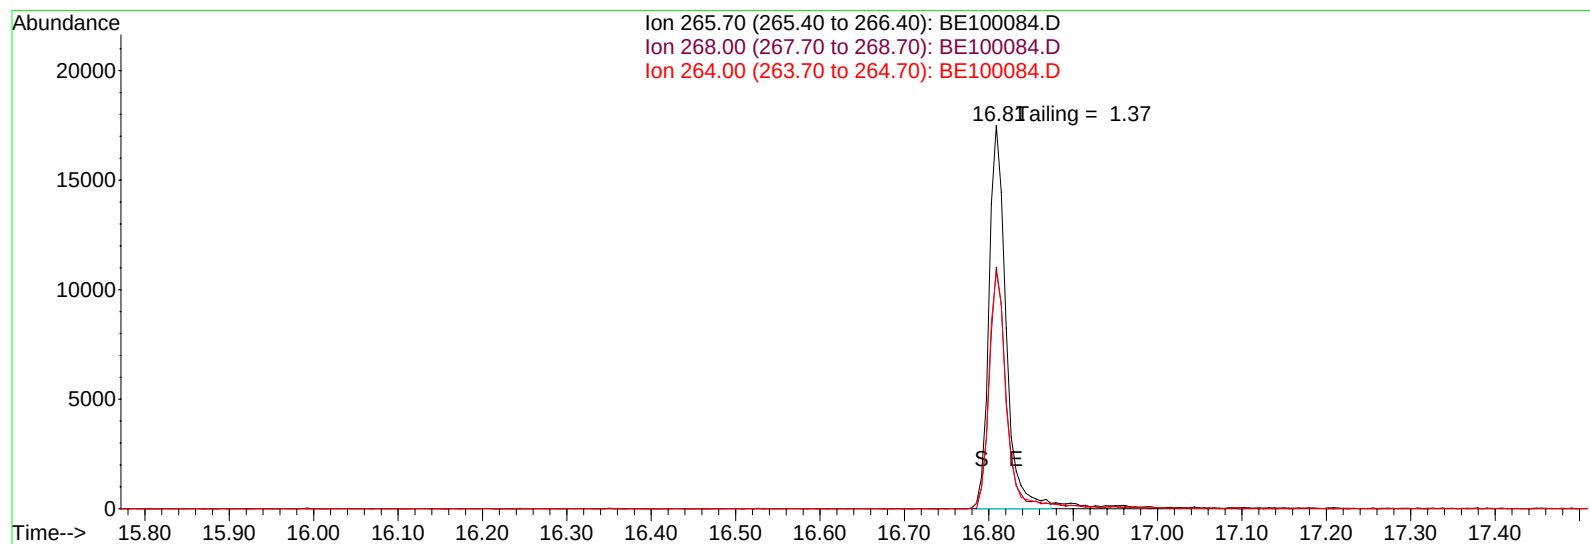

(69) Pentachlorophenol (C)



12.032min (-0.055) 144.28ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	55.56
264.00	65.00	66.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE061919\
Data File : BE100084.D
Acq On : 19 Jun 2019 15:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:59:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

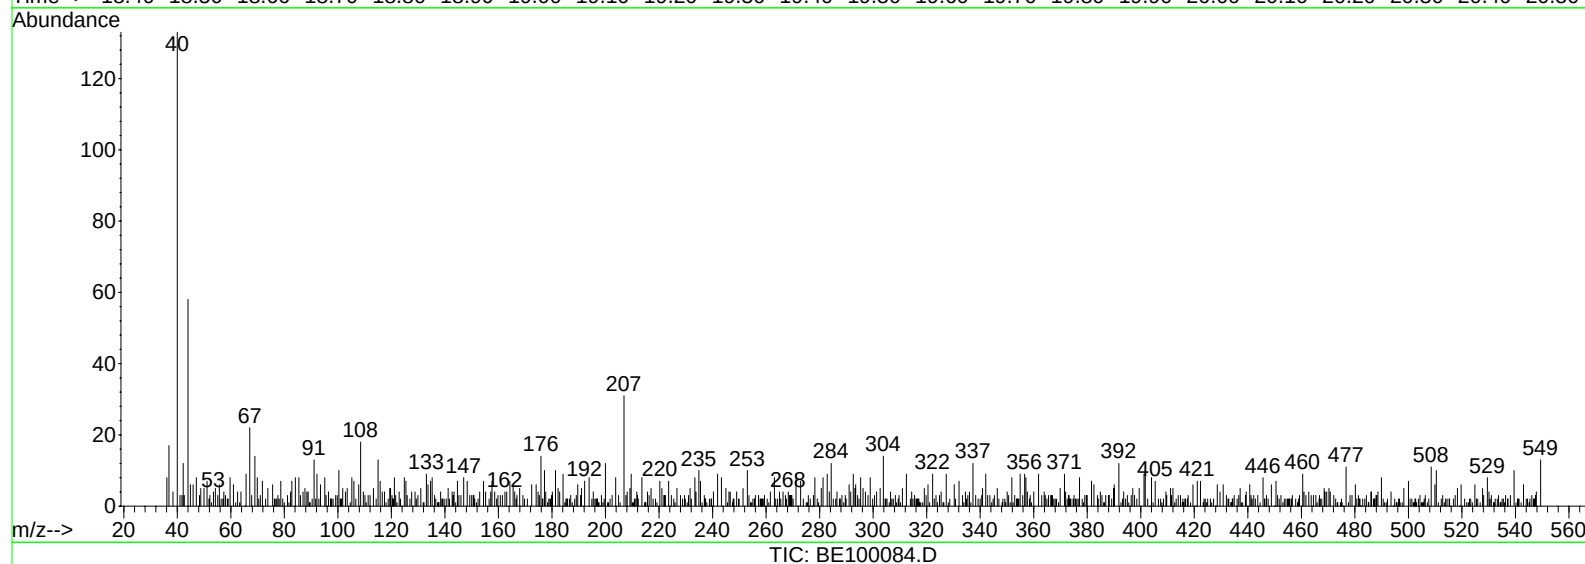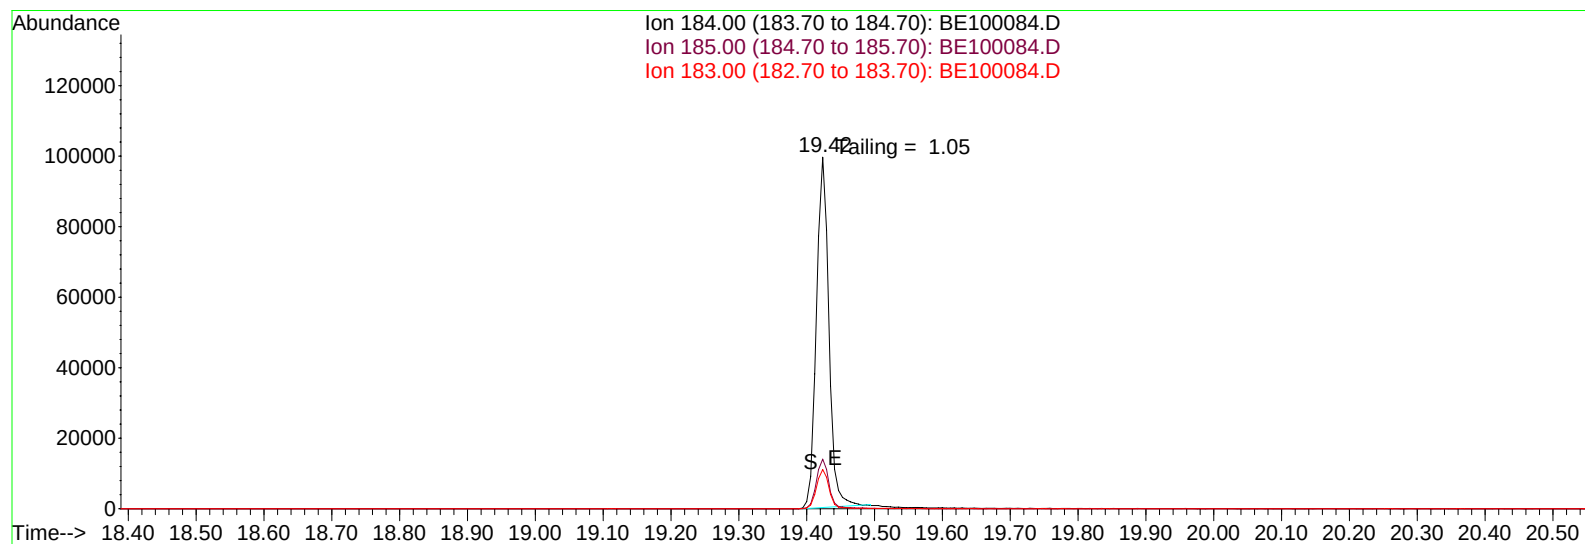

(76) Benzidine

14.594min (+0.004) 147.99ng

response 9

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	55.56#
183.00	12.20	44.44#
0.00	0.00	0.00