

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061919\
 Data File : BE100086.D
 Acq On : 19 Jun 2019 16:51
 Operator : JU/SJ
 Sample : PB120501BS
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB120501BS

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:20:30 AM

Quant Time: Jun 19 18:36:13 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061919.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 19 15:07:24 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	858	0.40	ng	0.00
7) Naphthalene-d8	10.54	136	2786	0.40	ng	0.00
13) Acenaphthene-d10	14.41	164	1754	0.40	ng	0.00
19) Phenanthrene-d10	17.16	188	4899	0.40	ng	0.00
27) Chrysene-d12	21.35	240	5829	0.40	ng	0.01
34) Perylene-d12	23.84	264	7231	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.30	112	695	0.39	ng	0.00
5) Phenol-d6	6.92	99	904	0.37	ng	-0.01
8) Nitrobenzene-d5	8.90	82	945	0.35	ng	-0.01
11) 2-Methylnaphthalene-d10	12.15	152	2387	0.45	ng	0.00
14) 2,4,6-Tribromophenol	15.92	330	223	0.23	ng	0.00
15) 2-Fluorobiphenyl	13.04	172	2571	0.37	ng	0.00
25) Fluoranthene-d10	19.20	212	19564	0.28	ng	0.00
29) Terphenyl-d14	19.80	244	3959	0.34	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.20	88	1084	0.787	ng	# 84
3) n-Nitrosodimethylamine	3.57	42	195	0.557	ng	# 100
6) bis(2-Chloroethyl)ether	7.17	93	974	0.420	ng	# 64
9) Naphthalene	10.59	128	10547	0.348	ng	99
10) Hexachlorobutadiene	10.86	225	1002	0.337	ng	96
12) 2-Methylnaphthalene	12.22	142	1733	0.348	ng	95
16) Acenaphthylene	14.14	152	2988	0.359	ng	99
17) Acenaphthene	14.47	154	1635	0.351	ng	99
18) Fluorene	15.46	166	2312	0.333	ng	98
20) 4-Bromophenyl-phenylether	16.36	248	1011	0.347	ng	97
21) Hexachlorobenzene	16.47	284	1107	0.344	ng	99
22) Pentachlorophenol	16.88	266	90	0.328	ng	97
23) Phenanthrene	17.20	178	4038	0.344	ng	99
24) Anthracene	17.30	178	3190	0.322	ng	99
26) Fluoranthene	19.23	202	5769	0.306	ng	99
28) Pyrene	19.59	202	5746	0.384	ng	99
30) Benzo(a)anthracene	21.33	228	5966	0.344	ng	100
31) Chrysene	21.39	228	7422	0.368	ng	100
32) Bis(2-ethylhexyl)phthalate	21.24	149	4939	0.302	ng	100
33) Indeno(1,2,3-cd)pyrene	26.48	276	11391	0.502	ng	# 95
35) Benzo(b)fluoranthene	23.07	252	8043m	0.379	ng	
36) Benzo(k)fluoranthene	23.12	252	8354	0.346	ng	98
37) Benzo(a)pyrene	23.73	252	7413	0.362	ng	# 96
38) Dibenzo(a,h)anthracene	26.51	278	9360	0.446	ng	99
39) Benzo(g,h,i)perylene	27.29	276	9649	0.442	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061919\
Data File : BE100086.D
Acq On : 19 Jun 2019 16:51
Operator : JU/SJ
Sample : PB120501BS
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
PB120501BS

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM

Quant Time: Jun 19 18:36:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 19 15:07:24 2019
Response via : Initial Calibration



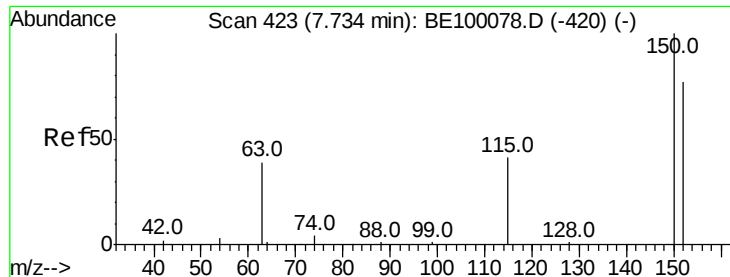

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.73 min Scan# 423

Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS




Tot Ion:	152	Resp:	858
Ion	Ratio	Lower	Upper
152	100		
150	132.6	99.8	149.8
115	55.6	51.3	76.9

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 0.787 ng


RT: 3.20 min Scan# 29

Delta R.T. 0.00 min



Lab File: BE100086.D


Acq: 19 Jun 2019 16:51

Tgt Ion:	88	Resp:	1084
Ion	Ratio	Lower	Upper
88	100		
58	51.5	51.1	76.7
43	35.8	21.7	32.5#



Abundance Ion 88.00 (87.70 to 88.70): BE1
Ion 58.00 (57.70 to 58.70): BE1
Ion 43.00 (42.70 to 43.70): BE1





#3

n-Nitrosodimethylamine

Concen: 0.557 ng

RT: 3.57 min Scan# 61

Delta R.T. -0.03 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E





ClientSampleId :

PB120501BS

Tot Ion	42	Resp:	195
Ion	Ratio	Lower	Upper
42	100		
74	153.3	0.0	0.0#
44	39.5	0.0	0.0#

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#4

2-Fluorophenol

Concen: 0.390 ng




RT: 5.30 min Scan# 212




Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion	112	Resp:	695
Ion	Ratio	Lower	Upper
112	100		
64	50.8	22.0	33.0#
63	136.4	121.8	182.6





#5

Phenol-d6

Concen: 0.370 ng

RT: 6.92 min Scan# 352

Delta R.T. -0.01 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tot Ion:	99	Resp:	904
Ion	Ratio	Lower	Upper
99	100		
42	14.5	0.0	0.0#
71	42.1	37.6	56.4

Instrument :





BNA_E

ClientSampleId :

PB120501BS

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#6

bis(2-Chloroethyl)ether

Concen: 0.420 ng


RT: 7.17 min Scan# 374


Delta R.T. -0.02 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion:	93	Resp:	974
Ion	Ratio	Lower	Upper
93	100		
63	182.0	200.0	300.0#
95	24.9	24.0	36.0





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.54 min Scan# 644

Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E





ClientSampleId :

PB120501BS

Tot Ion	Ratio	Lower	Upper
136	100		
137	14.2	11.6	17.4
54	31.1	33.9	50.9#
68	7.7	7.8	11.8#

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#8

Nitrobenzene-d5

Concen: 0.350 ng




RT: 8.90 min Scan# 518


Delta R.T. -0.01 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
82	100		
128	136.5	128.0	192.0
54	176.6	143.4	215.0





#9

Naphthalene

Concen: 0.348 ng

RT: 10.59 min Scan# 648

Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS




Tot Ion:	128	Resp:	10547
Ion Ratio	Lower	Upper	
128	100		
129	3.6	3.1	4.7
127	4.2	3.4	5.2

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E



#10

Hexachlorobutadiene

Concen: 0.337 ng

RT: 10.86 min Scan# 669




Delta R.T. -0.00 min


Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion:	225	Resp:	1002
Ion Ratio	Lower	Upper	
225	100		
223	63.3	52.2	78.4
227	61.9	53.0	79.6

Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E









#11
 2-Methylnaphthalene-d10
 Concen: 0.450 ng
 RT: 12.15 min Scan# 759
 Delta R.T. -0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Instrument :
 BNA_E
 ClientSampleId :
 PB120501BS

Tot Ion	Ratio	Lower	Upper
152	100		
151	13.6	16.3	24.5#




Manual Integrations
 APPROVED


mohammad
 6/21/2019 8:20:30 AM



#12
 2-Methylnaphthalene
 Concen: 0.348 ng
 RT: 12.22 min Scan# 764
 Delta R.T. -0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.5	74.1	111.1
115	45.3	40.9	61.3






#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.41 min Scan# 916
 Delta R.T. -0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Instrument :
 BNA_E
 ClientSampleId :
 PB120501BS




Tot Ion	Ratio	Lower	Upper
164	100		
162	99.5	78.2	117.2
160	60.0	45.6	68.4

Manual Integrations
 APPROVED

mohammad
 6/21/2019 8:20:30 AM




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E






#14
 2,4,6-Tribromophenol
 Concen: 0.230 ng
 RT: 15.92 min Scan# 1022
 Delta R.T. 0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
330	100		
332	98.7	73.3	109.9
141	21.1	22.2	33.2#



Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E









#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 13.04 min Scan# 821
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Instrument :
BNA_E
ClientSampled :
PB120501BS

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.9	29.8	44.8
170	25.0	23.2	34.8




Manual Integrations
APPROVED


mohammad
6/21/2019 8:20:30 AM



#16
Acenaphthylene
Concen: 0.359 ng
RT: 14.14 min Scan# 897
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.9	23.9
153	12.6	10.1	15.1






#17
Acenaphthene
Concen: 0.351 ng
RT: 14.47 min Scan# 920
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Instrument :
BNA_E
ClientSampleId :
PB120501BS

Tot Ion	Ratio	Lower	Upper
154	100		
153	120.7	95.5	143.3
152	70.2	54.9	82.3

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM






Abundance

Ion 154.00 (153.70 to 154.70): E


Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



#18
Fluorene
Concen: 0.333 ng
RT: 15.46 min Scan# 988
Delta R.T. 0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
166	100		
165	102.2	79.8	119.8
167	13.0	10.2	15.4






Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.16 min Scan# 1115
Delta R.T. 0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Instrument :
BNA_E
ClientSampleId :
PB120501BS

Tot Ion	Ratio	Resp	Lower	Upper
188	100			
94	0.0	0.0	0.0	
80	7.6	6.3	9.5	




Manual Integrations
APPROVED


mohammad
6/21/2019 8:20:30 AM



#20
4-Bromophenyl-phenylether
Concen: 0.347 ng
RT: 16.36 min Scan# 1055
Delta R.T. 0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Resp	Lower	Upper
248	100			
250	97.5	80.6	120.8	
141	49.2	38.8	58.2	





#21

Hexachlorobenzene

Concen: 0.344 ng

RT: 16.47 min Scan# 1063

Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS




Tot Ion:	284	Resp:	1107
Ion Ratio	Lower	Upper	
284	100		
142	25.5	20.7	31.1
249	33.6	26.6	39.8

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E



#22

Pentachlorophenol

Concen: 0.328 ng


RT: 16.88 min Scan# 1094

Delta R.T. 0.01 min



Lab File: BE100086.D


Acq: 19 Jun 2019 16:51

Tgt Ion:	266	Resp:	90
Ion Ratio	Lower	Upper	
266	100		
264	83.1	67.8	101.6
268	83.1	70.0	105.0



Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E





#23

Phenanthrene

Concen: 0.344 ng

RT: 17.20 min Scan# 1118

Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E





ClientSampleId :

PB120501BS

Tot Ion:	178	Resp:	4038
Ion	Ratio	Lower	Upper
178	100		
176	19.8	15.9	23.9
179	15.4	13.1	19.7

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#24

Anthracene

Concen: 0.322 ng




RT: 17.30 min Scan# 1125


Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion:	178	Resp:	3190
Ion	Ratio	Lower	Upper
178	100		
176	19.2	15.8	23.6
179	15.8	12.0	18.0





#25

Fluoranthene-d10

Concen: 0.279 ng

RT: 19.20 min Scan# 1381

Delta R.T. 0.01 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS




Tot Ion:	212	Resp:	19564
Ion Ratio	Lower	Upper	
212	100		
106	1.8	1.4	2.0
104	1.0	0.8	1.2

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



Abundance Ion 212.00 (211.70 to 212.70): E
Ion 106.00 (105.70 to 106.70): E
Ion 104.00 (103.70 to 104.70): E



#26

Fluoranthene

Concen: 0.306 ng


RT: 19.23 min Scan# 1386

Delta R.T. -0.00 min



Lab File: BE100086.D


Acq: 19 Jun 2019 16:51

Tgt Ion:	202	Resp:	5769
Ion Ratio	Lower	Upper	
202	100		
101	5.9	5.0	7.4
203	17.8	13.7	20.5



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E





#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.35 min Scan# 1629

Delta R.T. 0.01 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS

Tot Ion	Ratio	Lower	Upper
240	100		
120	4.3	6.6	10.0#
236	28.1	23.8	35.6

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#28

Pyrene

Concen: 0.384 ng


RT: 19.59 min Scan# 1449

Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
202	100		
200	19.5	15.6	23.4
203	17.9	13.9	20.9






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E









#29
 Terphenyl-d14
 Concen: 0.340 ng
 RT: 19.80 min Scan# 1486
 Delta R.T. -0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Instrument :
 BNA_E
 ClientSampleId :
 PB120501BS

Tot Ion	Ratio	Lower	Upper
244	100		
212	38.2	29.8	44.8
122	7.2	6.1	9.1




Manual Integrations
 APPROVED


mohammad
 6/21/2019 8:20:30 AM



#30
 Benzo(a)anthracene
 Concen: 0.344 ng
 RT: 21.33 min Scan# 1627
 Delta R.T. -0.00 min
 Lab File: BE100086.D
 Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	23.0	34.4
229	20.5	16.4	24.6





#31

Chrysene

Concen: 0.368 ng

RT: 21.39 min Scan# 1632

Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E





ClientSampleId :

PB120501BS

Tot Ion:	228	Resp:	7422
Ion	Ratio	Lower	Upper
228	100		
226	29.7	23.8	35.8
229	20.8	16.3	24.5

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.302 ng




RT: 21.24 min Scan# 1620


Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion:	149	Resp:	4939
Ion	Ratio	Lower	Upper
149	100		
167	7.4	5.8	8.6
279	1.6	1.1	1.7





#33

Indeno(1,2,3-cd)pyrene

Concen: 0.502 ng

RT: 26.48 min Scan# 2928

Delta R.T. 0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E





ClientSampleId :

PB120501BS

Tot Ion	Ratio	Lower	Upper
276	100		
138	13.3	4.3	6.5#
277	23.9	19.4	29.0

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



#34

Perylene-d12

Concen: 0.400 ng




RT: 23.84 min Scan# 2193


Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.4	20.8	31.2
265	29.4	23.2	34.8









#35
Benzo(b)fluoranthene
Concen: 0.379 ng m
RT: 23.07 min Scan# 1977
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Instrument :
BNA_E
ClientSampleId :
PB120501BS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.6	18.4	27.6
125	10.6	6.4	9.6




Manual Integrations
APPROVED


mohammad
6/21/2019 8:20:30 AM



#36
Benzo(k)fluoranthene
Concen: 0.346 ng
RT: 23.12 min Scan# 1991
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.8	18.9	28.3
125	6.4	5.3	7.9









#37
Benzo(a)pyrene
Concen: 0.362 ng
RT: 23.73 min Scan# 2161
Delta R.T. -0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Instrument :
BNA_E
ClientSampleId :
PB120501BS

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.7	19.4	29.2
125	12.7	8.0	12.0




Manual Integrations
APPROVED


mohammad
6/21/2019 8:20:30 AM



#38
Dibenzo(a,h)anthracene
Concen: 0.446 ng
RT: 26.51 min Scan# 2935
Delta R.T. 0.00 min
Lab File: BE100086.D
Acq: 19 Jun 2019 16:51

Tgt Ion	Ratio	Lower	Upper
278	100		
139	11.0	9.0	13.6
279	26.1	21.4	32.0





#39

Benzo(a,h,i)perylene

Concen: 0.442 ng

RT: 27.29 min Scan# 3155

Delta R.T. -0.00 min

Lab File: BE100086.D

Acq: 19 Jun 2019 16:51

Instrument :

BNA_E


ClientSampleId :

PB120501BS

Tot Ion:	276	Resp:	9649
Ion Ratio	Lower	Upper	
276	100		
277	24.0	20.3	30.5
138	12.6	11.3	16.9

Manual Integrations
APPROVED

mohammad
6/21/2019 8:20:30 AM



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 277.00 (276.70 to 277.70): E
Ion 138.00 (137.70 to 138.70): E

