


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061919\
 Data File : BE100075.D
 Acq On : 19 Jun 2019 8:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 19 15:07:24 2019

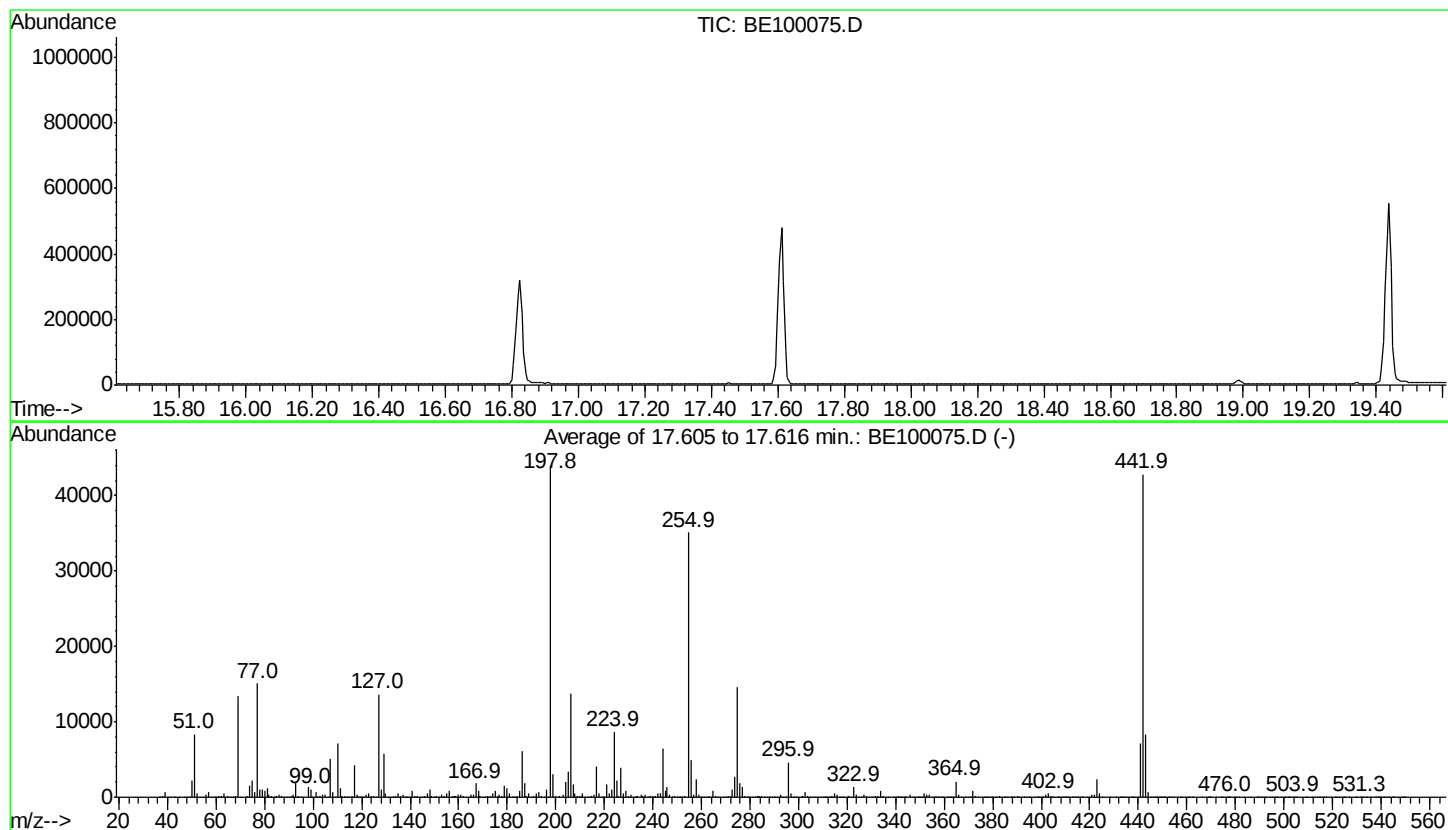

AutoFind: Scans 2556, 2557, 2558; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.0	8347	PASS
68	69	0.00	2	0.9	116	PASS
69	198	0.00	100	30.3	13339	PASS
70	69	0.00	2	0.4	56	PASS
127	198	10	80	30.9	13601	PASS
197	198	0.00	2	0.1	54	PASS
198	198	100	100	100.0	43971	PASS
199	198	5	9	6.9	3023	PASS
275	198	10	60	33.3	14663	PASS
365	198	1	100	4.6	2040	PASS
441	198	0.01	100	16.1	7072	PASS
442	198	50	100	97.3	42788	PASS
443	442	15	24	19.6	8381	PASS