


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061919\
 Data File : BE100084.D
 Acq On : 19 Jun 2019 15:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 19 15:07:24 2019

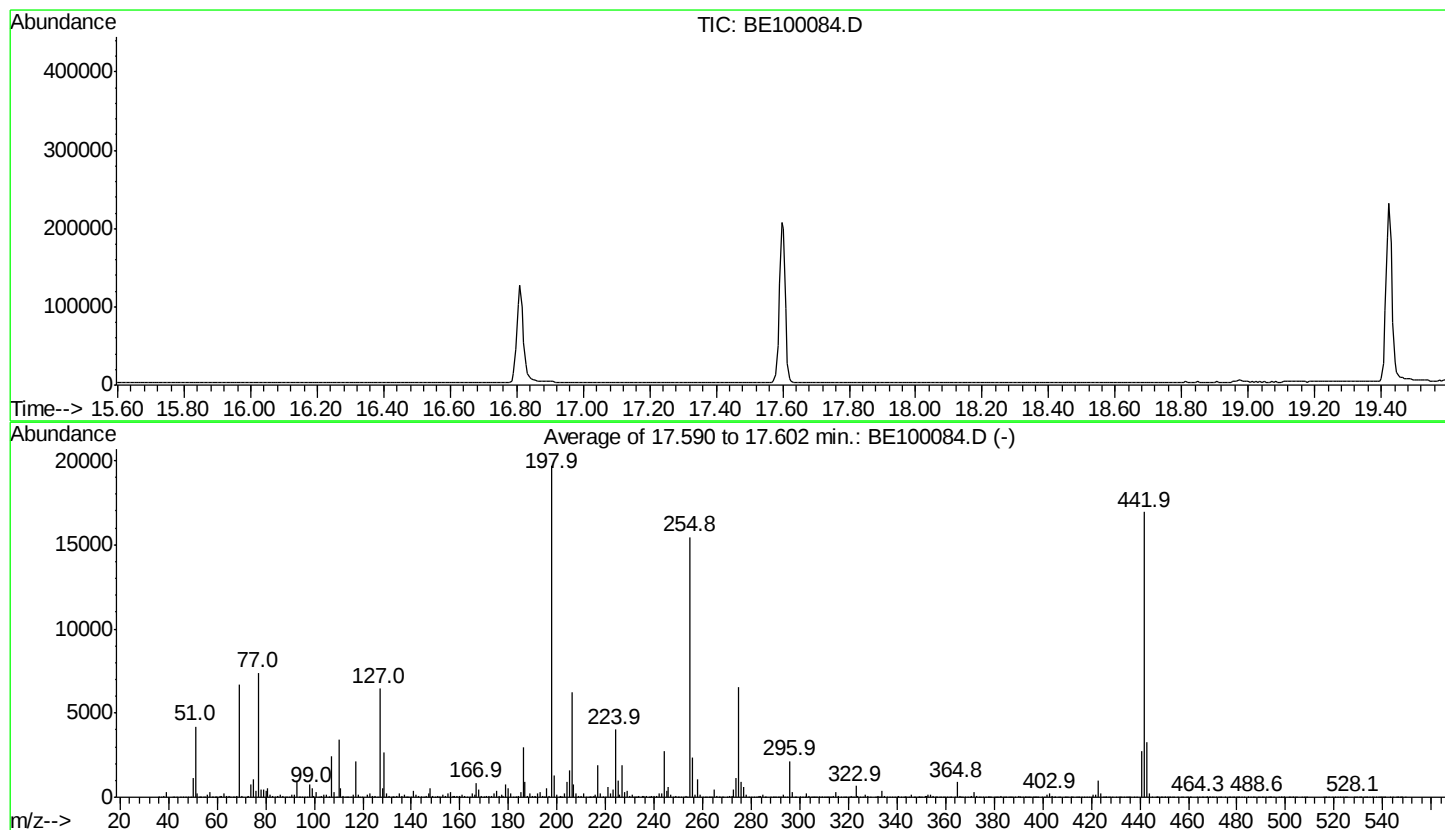

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	4186	PASS
68	69	0.00	2	1.3	88	PASS
69	198	0.00	100	34.0	6695	PASS
70	69	0.00	2	0.7	45	PASS
127	198	10	80	32.7	6442	PASS
197	198	0.00	2	0.2	43	PASS
198	198	100	100	100.0	19699	PASS
199	198	5	9	6.6	1305	PASS
275	198	10	60	33.3	6564	PASS
365	198	1	100	4.6	903	PASS
441	198	0.01	100	14.0	2758	PASS
442	198	50	100	86.0	16934	PASS
443	442	15	24	19.3	3274	PASS