


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062018\
 Data File : BE096826.D
 Acq On : 20 Jun 2018 9:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 20 15:45:14 2018

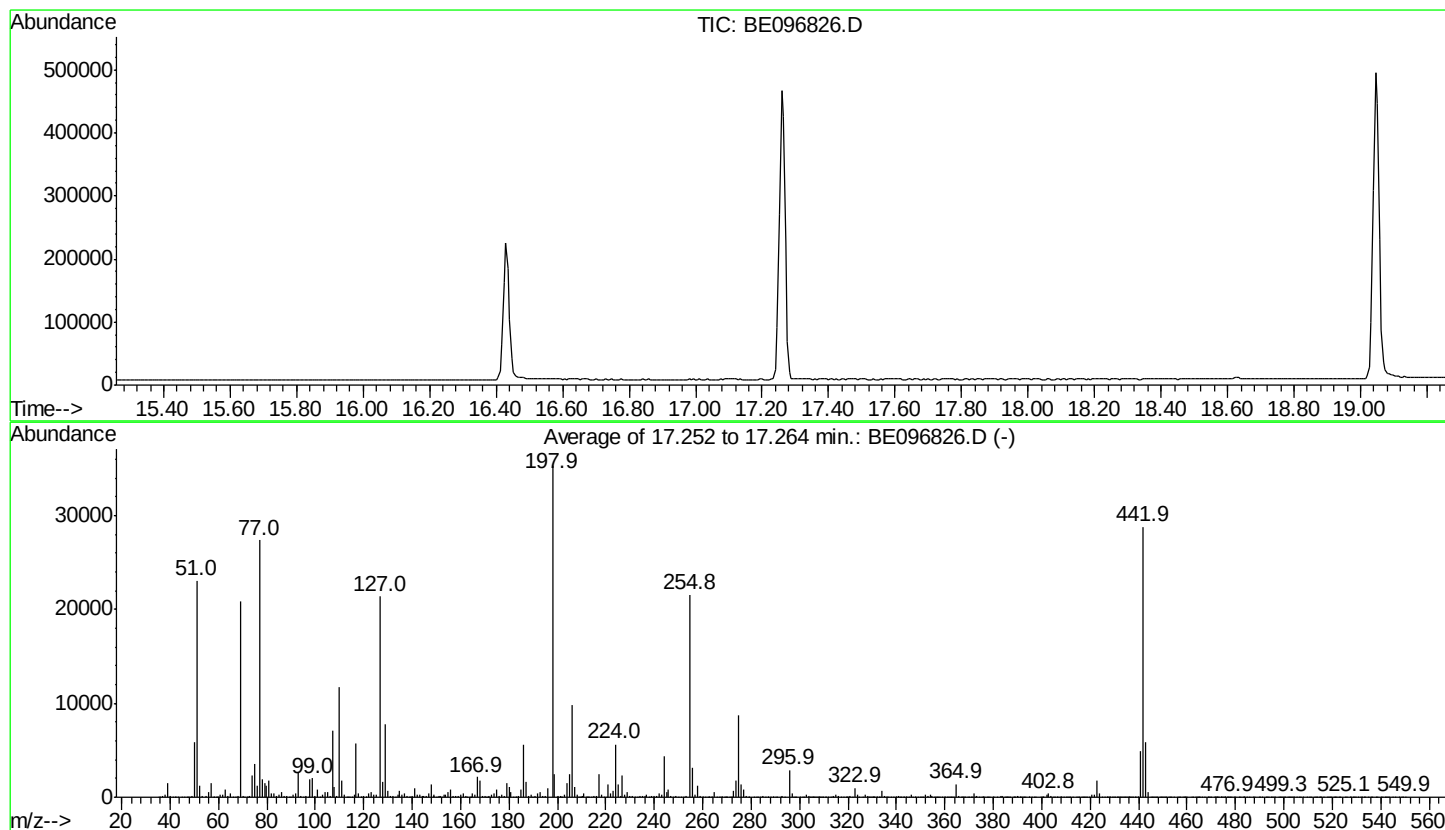

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.4	23119	PASS
68	69	0.00	2	0.6	132	PASS
69	198	0.00	100	59.2	20933	PASS
70	69	0.00	2	0.6	117	PASS
127	198	10	80	60.5	21383	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35344	PASS
199	198	5	9	7.0	2480	PASS
275	198	10	60	24.5	8673	PASS
365	198	1	100	3.9	1384	PASS
441	443	0.01	100	83.9	4930	PASS
442	198	50	100	81.5	28815	PASS
443	442	15	24	20.4	5874	PASS