
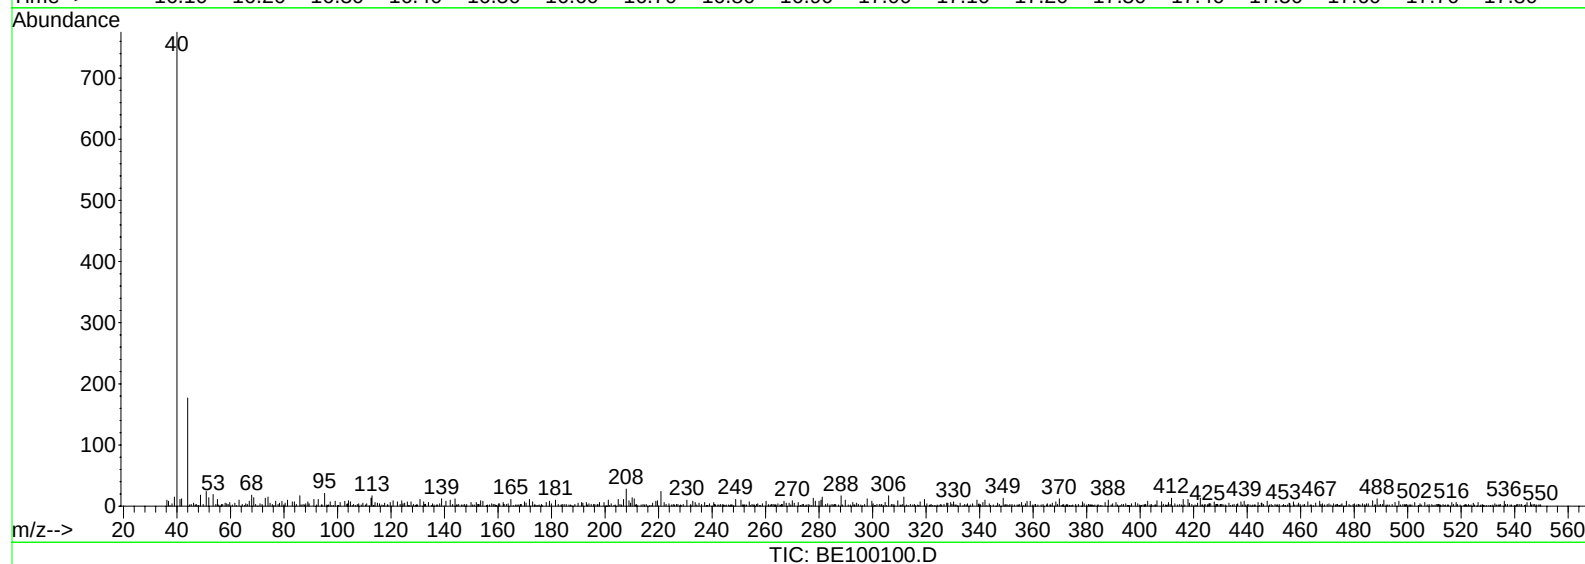


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062019\
 Data File : BE100100.D
 Acq On : 20 Jun 2019 9:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:24:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

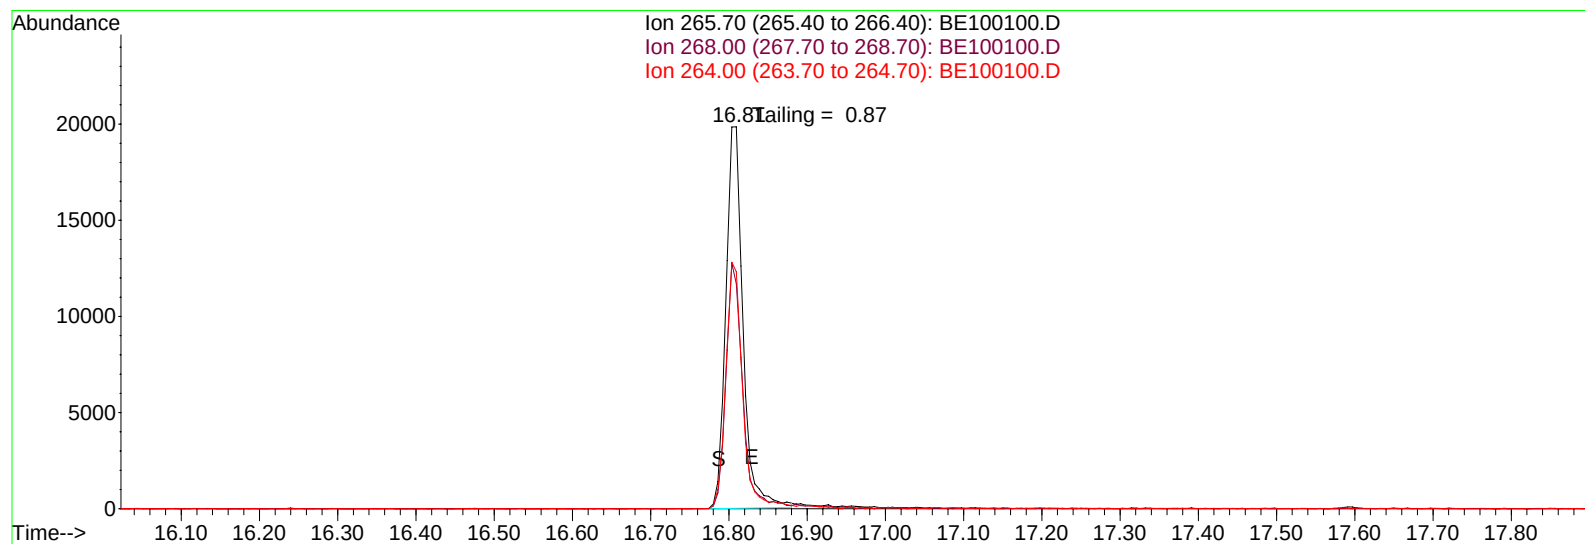

(69) Pentachlorophenol (C)



12.168min (+0.081) 93.51ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	55.56
264.00	65.00	66.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062019\
Data File : BE100100.D
Acq On : 20 Jun 2019 9:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:24:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

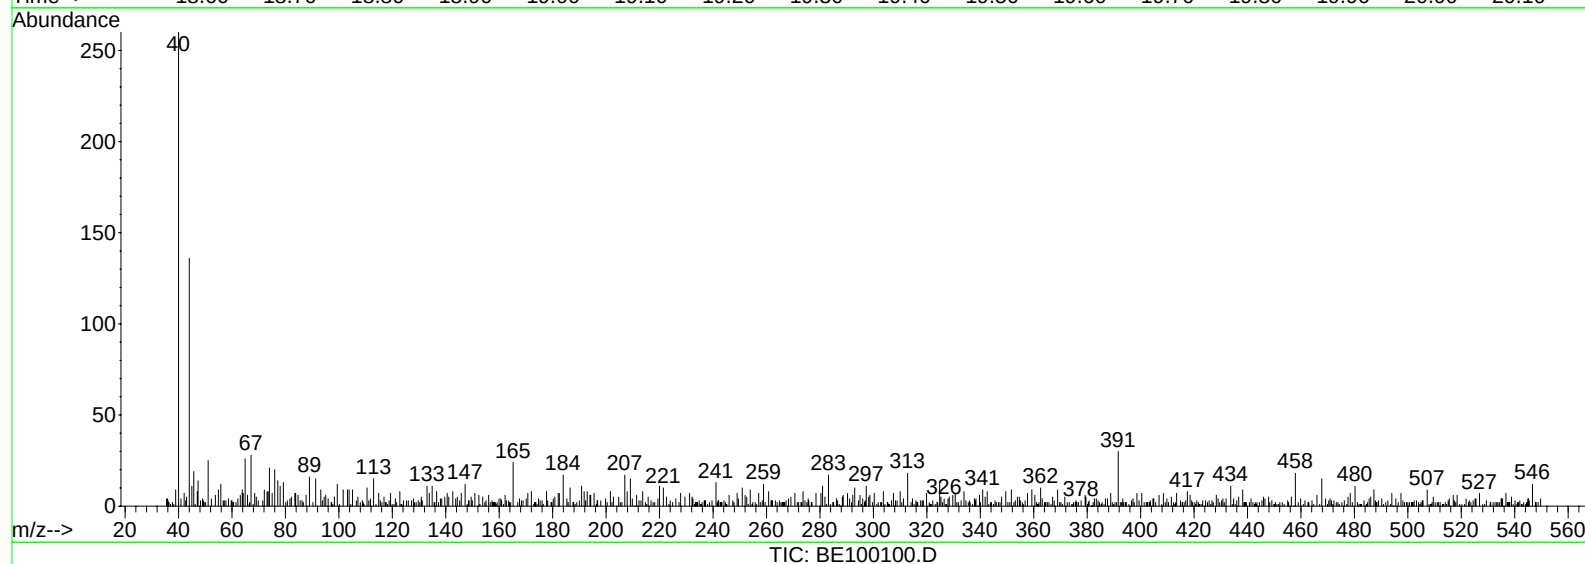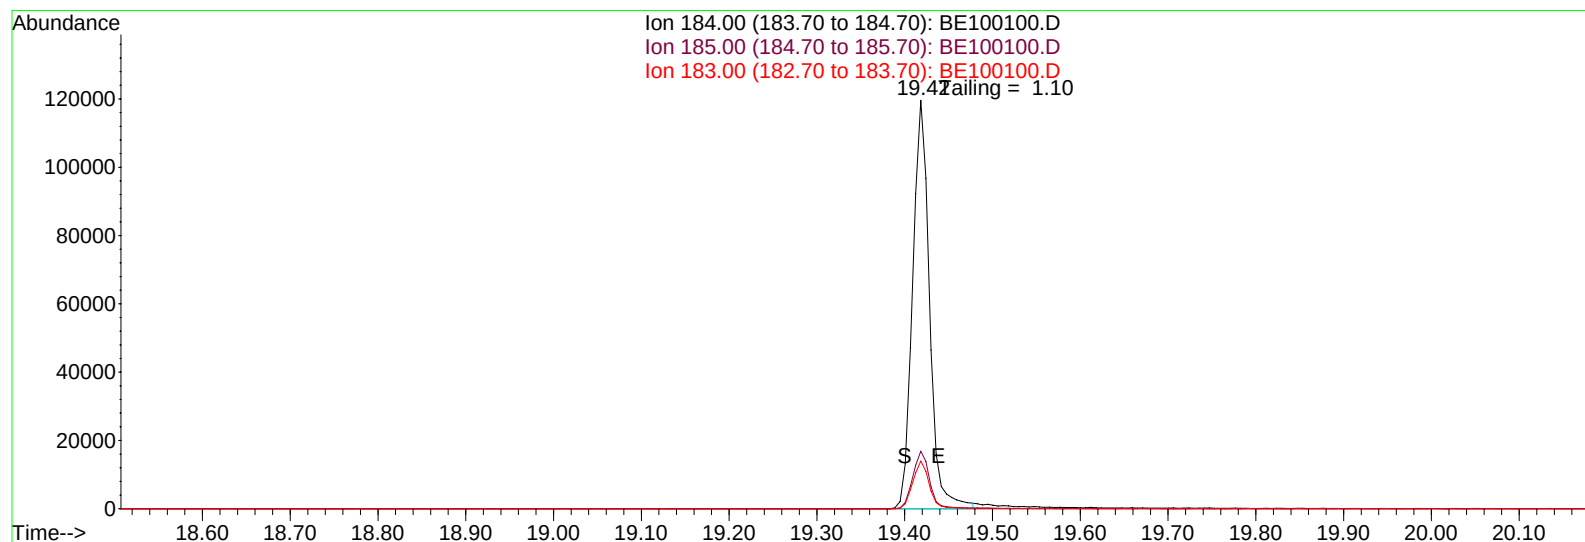

(76) Benzidine

14.495min (-0.096) 131.55ng

response 16

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	23.53#
183.00	12.20	0.00#
0.00	0.00	0.00