
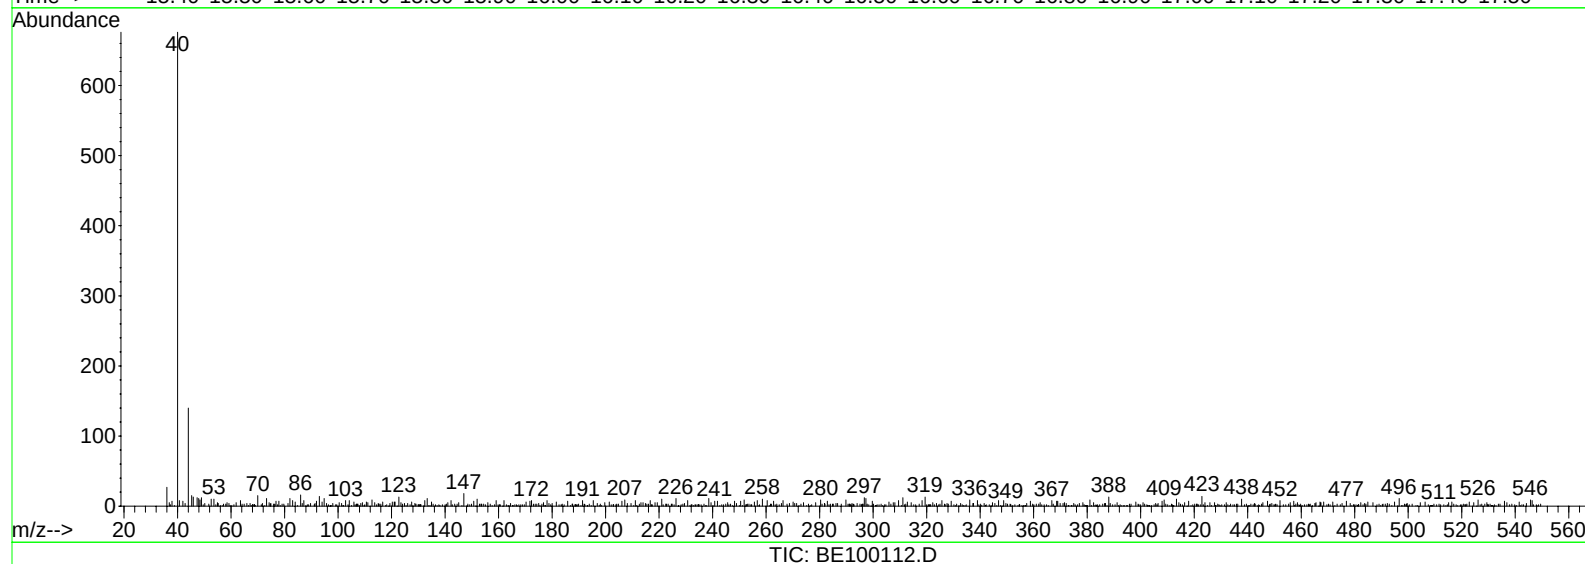


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062019\
Data File : BE100112.D
Acq On : 20 Jun 2019 18:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:37:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

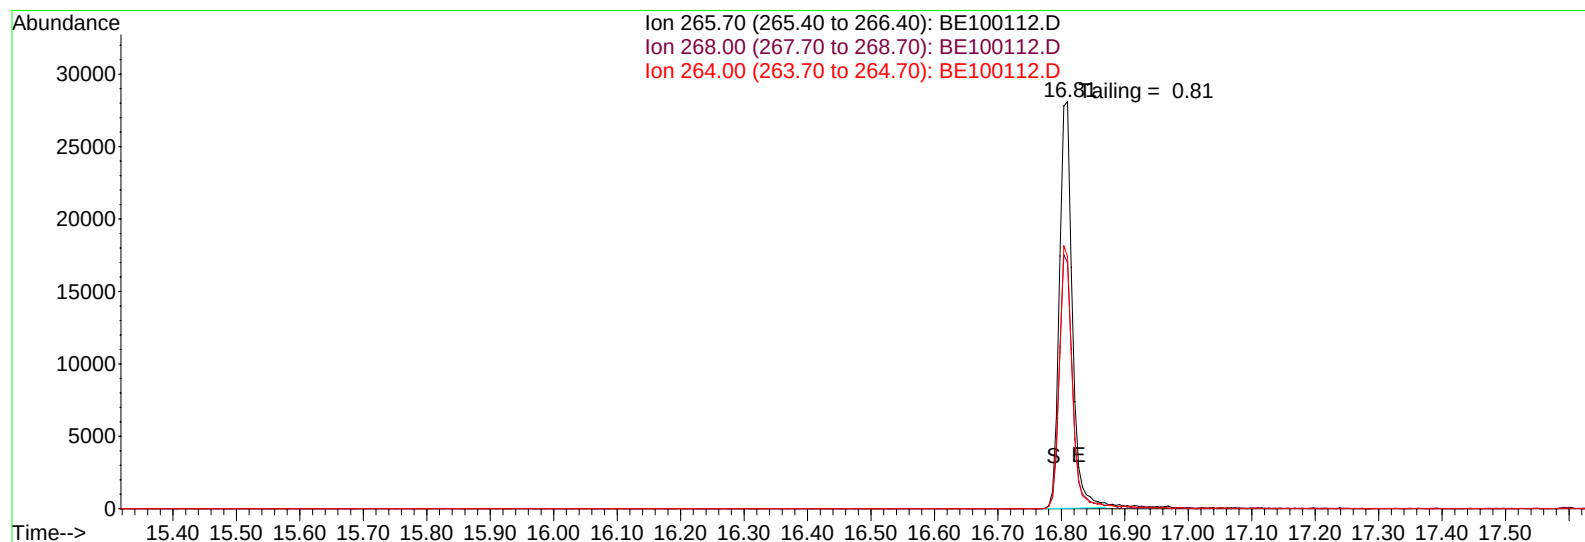

(69) Pentachlorophenol (C)



12.186min (+0.098) 408.79ng

response 17

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	58.33
264.00	65.00	25.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062019\
Data File : BE100112.D
Acq On : 20 Jun 2019 18:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 04:37:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

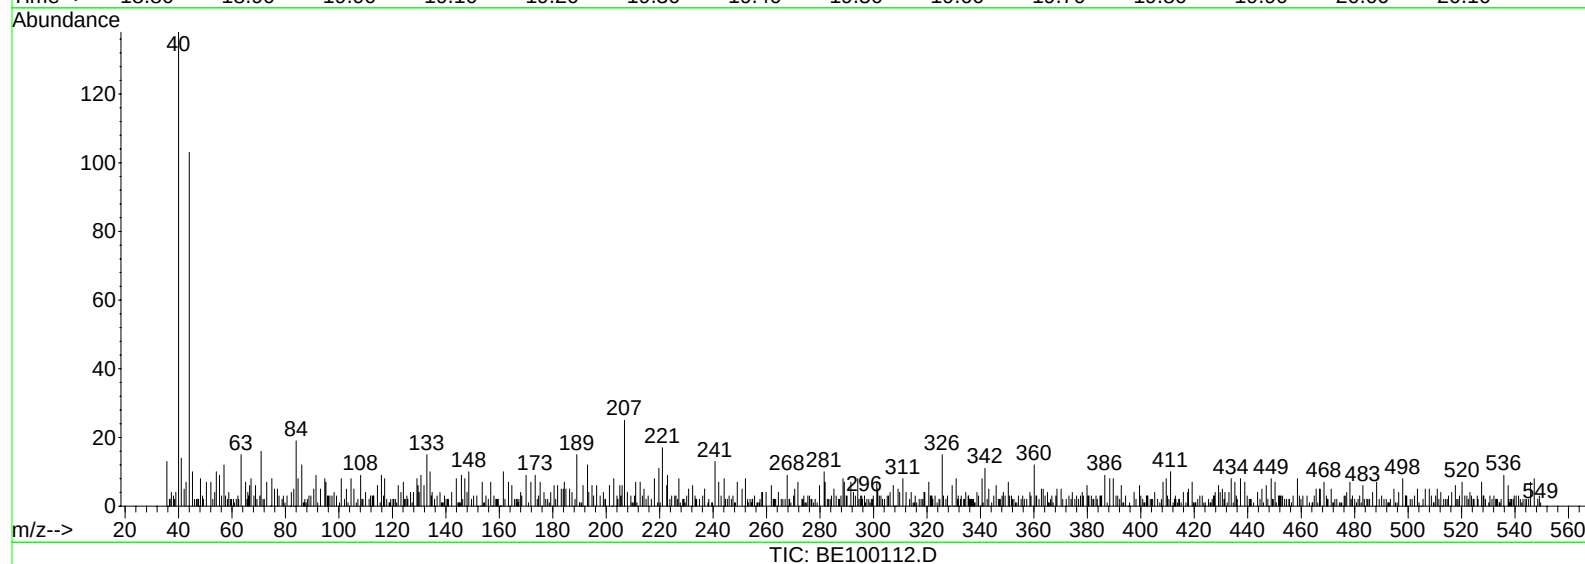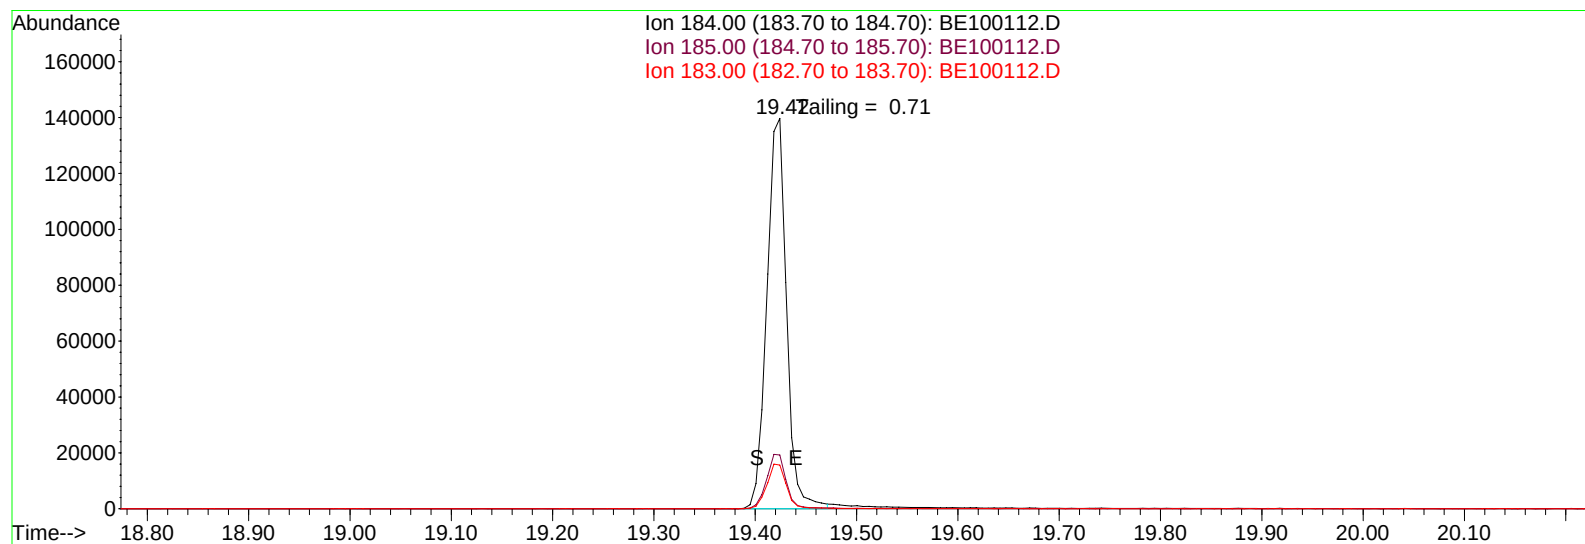

(76) Benzidine

14.659min (+0.069) 72.10ng

response 19

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	41.67#
183.00	12.20	41.67#
0.00	0.00	0.00