


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE062019\
Data File : BE100100.D
Acq On : 20 Jun 2019 9:37
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 15:07:24 2019

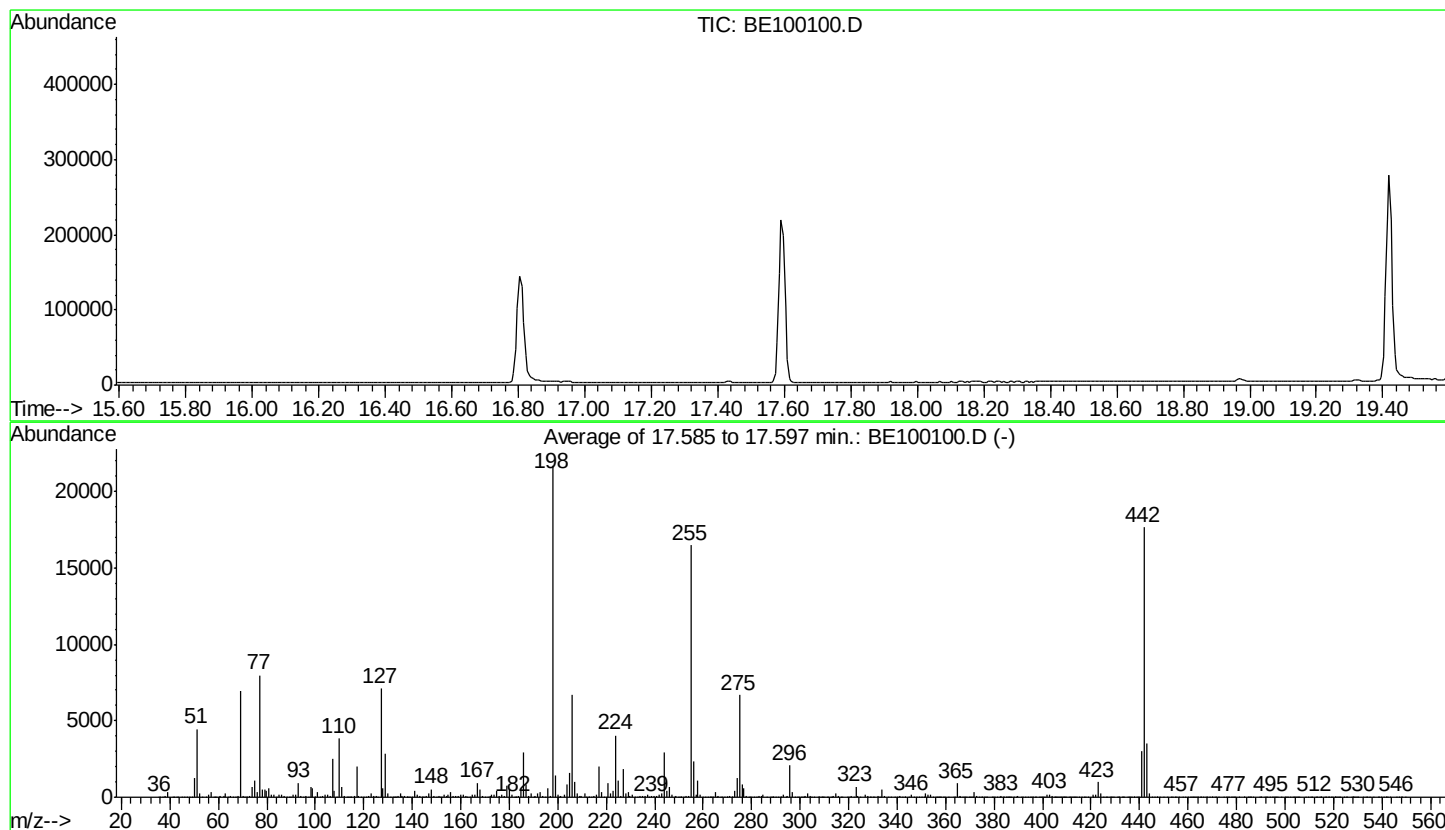

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.6	4464	PASS
68	69	0.00	2	1.8	127	PASS
69	198	0.00	100	32.2	6994	PASS
70	69	0.00	2	0.7	49	PASS
127	198	10	80	32.8	7109	PASS
197	198	0.00	2	0.3	58	PASS
198	198	100	100	100.0	21699	PASS
199	198	5	9	6.4	1390	PASS
275	198	10	60	30.8	6678	PASS
365	198	1	100	4.2	919	PASS
441	198	0.01	100	14.0	3031	PASS
442	198	50	100	81.4	17657	PASS
443	442	15	24	19.8	3492	PASS