
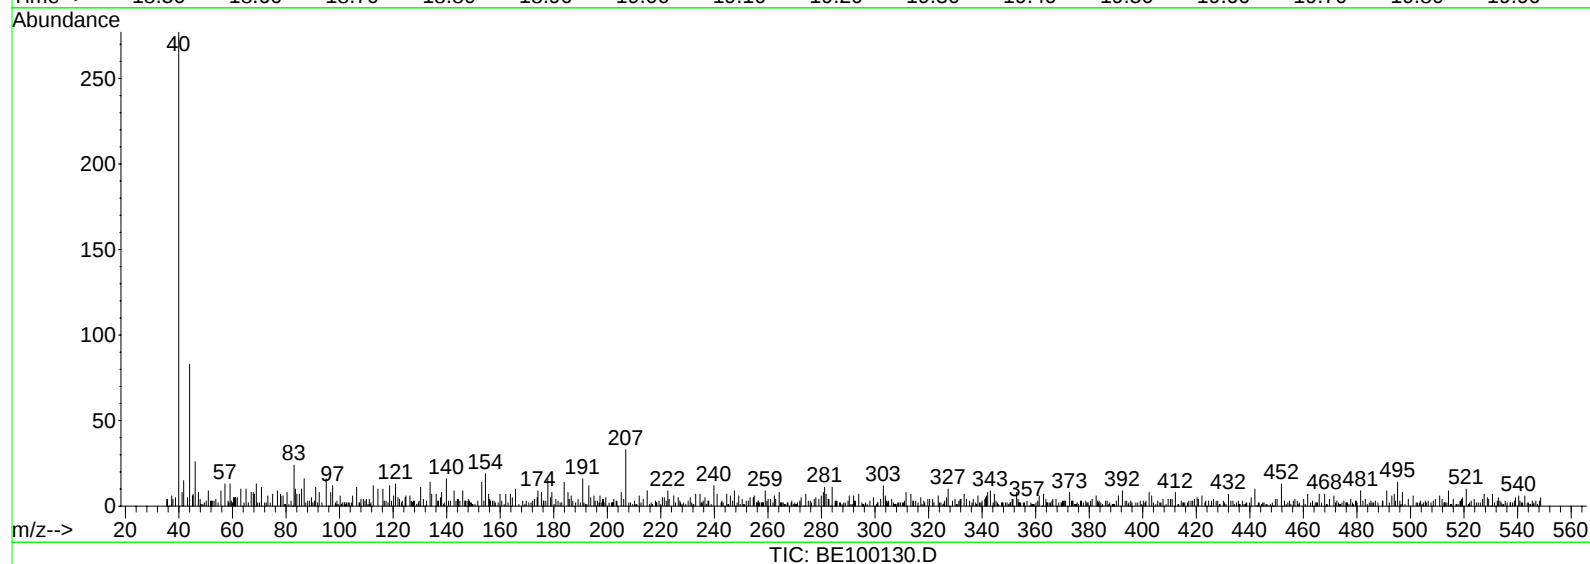


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062119\
 Data File : BE100130.D
 Acq On : 21 Jun 2019 7:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 03:12:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

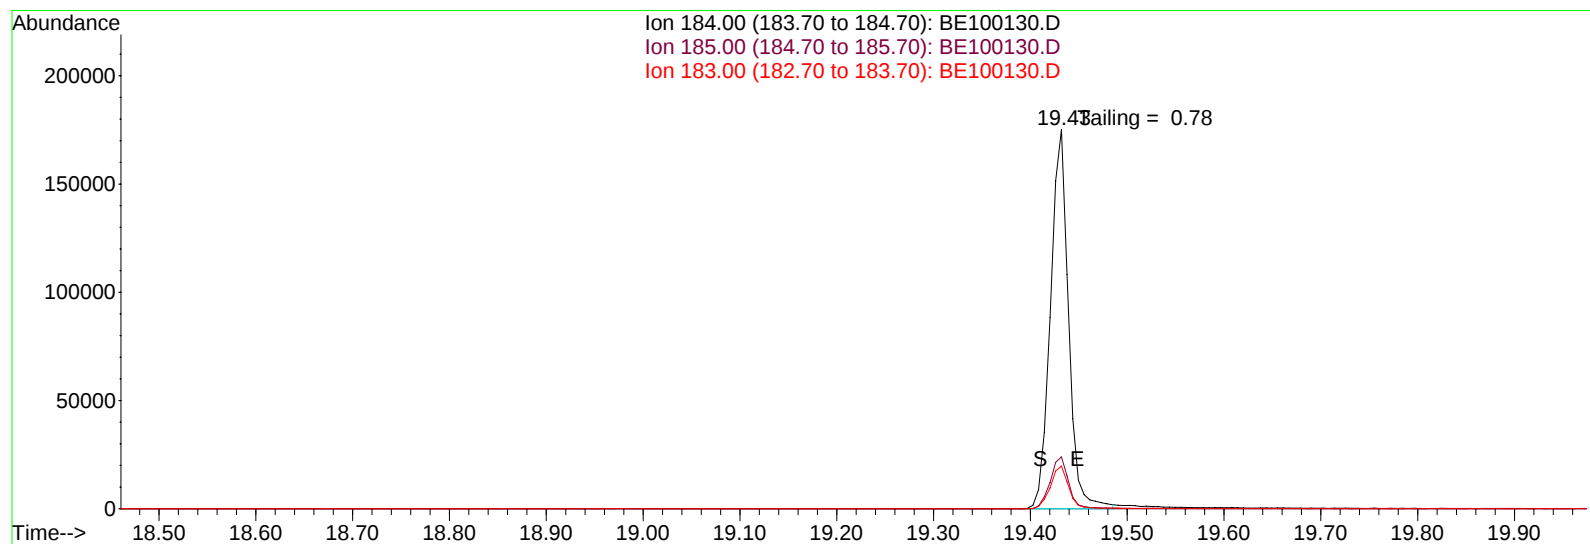

(76) Benzidine



14.679min (+0.089) 80.16ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	57.14#
183.00	12.20	14.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062119\
 Data File : BE100130.D
 Acq On : 21 Jun 2019 7:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 03:12:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

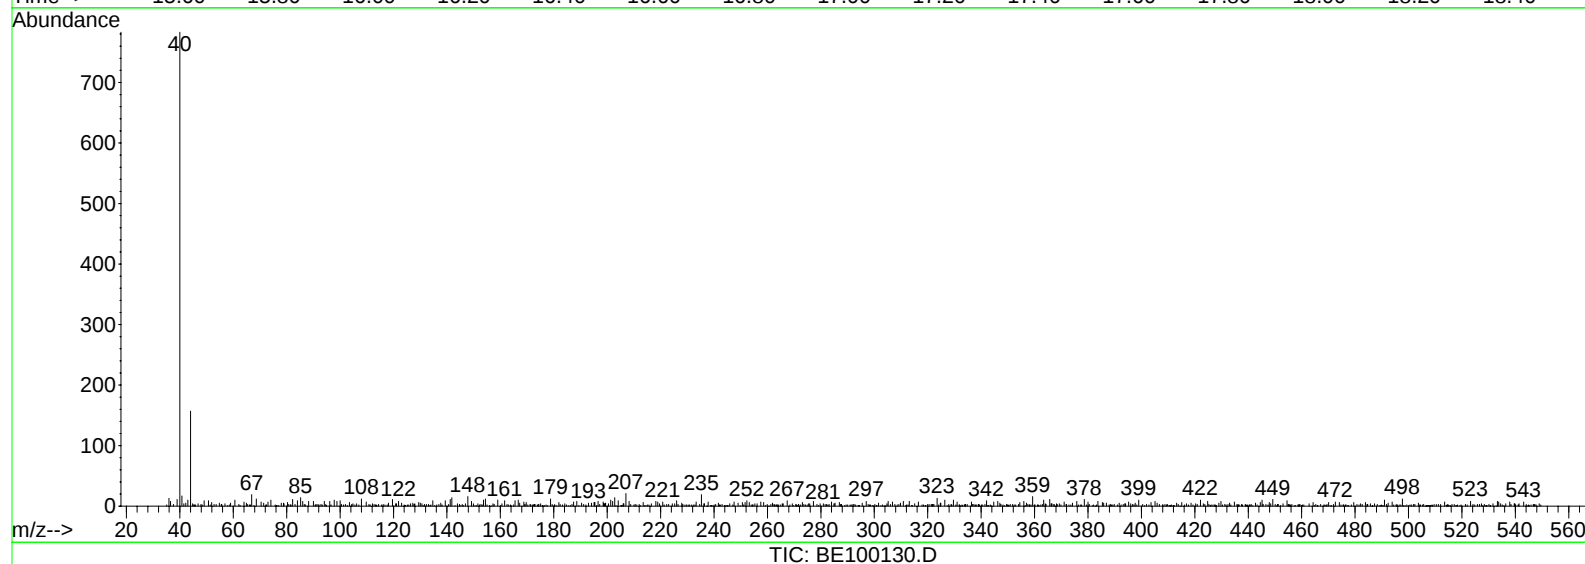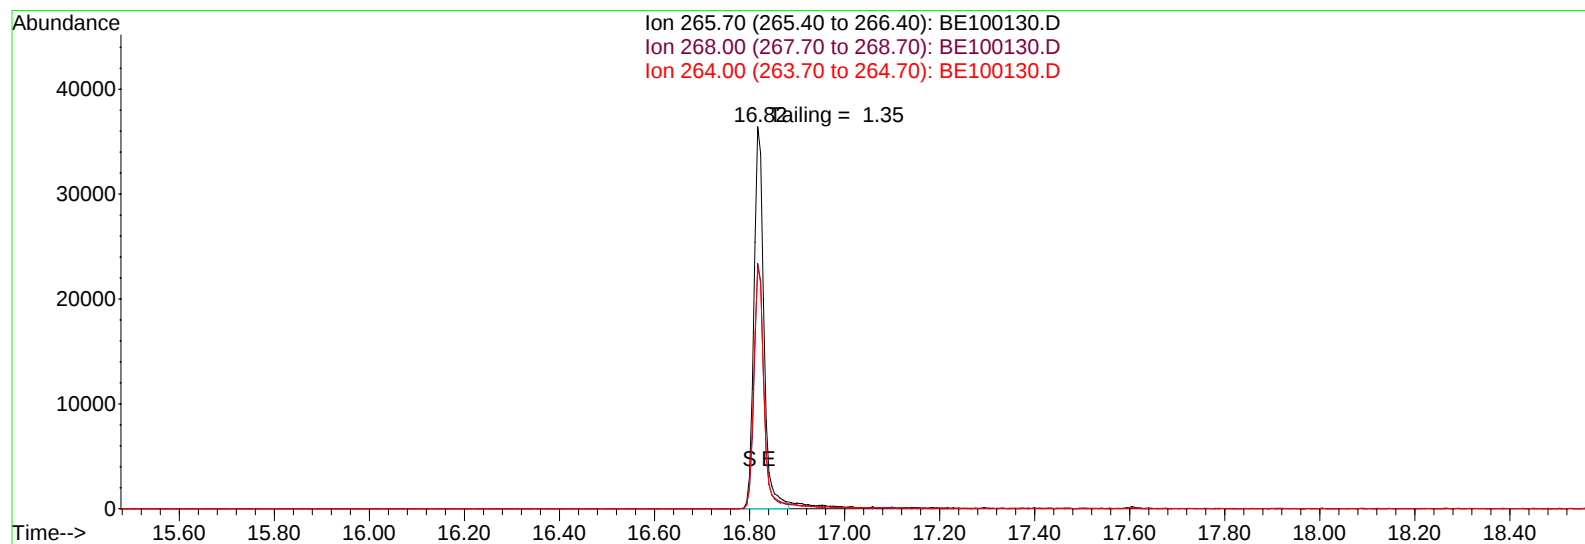

(69) Pentachlorophenol (C)

12.170min (+0.083) 42.94ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	25.00#
264.00	65.00	50.00#
0.00	0.00	0.00