

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062119\
 Data File : BE100150.D
 Acq On : 22 Jun 2019 1:34
 Operator : JU/SJ
 Sample : K3428-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EXT-013-SW161-061319

Manual Integrations
 APPROVED

mohammad
 6/25/2019 3:21:39 PM

Quant Time: Jun 22 03:28:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 19 15:07:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	726	0.40	ng	-0.02
7) Naphthalene-d8	10.52	136	2953	0.40	ng	-0.01
13) Acenaphthene-d10	14.40	164	2573	0.40	ng	-0.02
19) Phenanthrene-d10	17.15	188	7399	0.40	ng	-0.01
27) Chrysene-d12	21.34	240	9112	0.40	ng	0.00
34) Perylene-d12	23.83	264	11293	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.30	112	587	0.39	ng	0.00
5) Phenol-d6	6.90	99	863	0.42	ng	-0.03
8) Nitrobenzene-d5	8.90	82	859	0.30	ng	-0.01
11) 2-Methylnaphthalene-d10	12.14	152	160	0.03	ng	-0.02
14) 2,4,6-Tribromophenol	15.90	330	553	0.39	ng	-0.01
15) 2-Fluorobiphenyl	13.03	172	2688	0.27	ng	-0.02
25) Fluoranthene-d10	19.19	212	2084	0.02	ng	0.00
29) Terphenyl-d14	19.79	244	5160	0.28	ng	-0.02
Target Compounds						Qvalue
9) Naphthalene	10.58	128	9442	0.294	ng	99
12) 2-Methylnaphthalene	12.21	142	2468	0.468	ng	96
16) Acenaphthylene	14.12	152	12787	1.047	ng	98
17) Acenaphthene	14.47	154	1587	0.232	ng	93
18) Fluorene	15.45	166	6700	0.659	ng	# 85
23) Phenanthrene	17.19	178	128909	7.272	ng	99
24) Anthracene	17.28	178	11875	0.794	ng	98
26) Fluoranthene	19.22	202	188848	6.636	ng	98
28) Pyrene	19.58	202	240705	10.278	ng	96
30) Benzo(a)anthracene	21.33	228	133073	4.909	ng	94
31) Chrysene	21.38	228	164658	5.228	ng	97
32) Bis(2-ethylhexyl)phthalate	21.24	149	39967	1.563	ng	99
33) Indeno(1,2,3-cd)pyrene	26.47	276	81765	2.307	ng	# 98
35) Benzo(b)fluoranthene	23.07	252	158039	4.769	ng	# 98
36) Benzo(k)fluoranthene	23.11	252	53533m	1.420	ng	
37) Benzo(a)pyrene	23.72	252	118346m	3.700	ng	
38) Dibenzo(a,h)anthracene	26.48	278	22255	0.679	ng	# 90
39) Benzo(a,h,i)perylene	27.29	276	86565	2.541	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062119\
Data File : BE100150.D
Acq On : 22 Jun 2019 1:34
Operator : JU/SJ
Sample : K3428-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM

Quant Time: Jun 22 03:28:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE061919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 19 15:07:24 2019
Response via : Initial Calibration





#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 421
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
152	100		
150	143.2	99.8	149.8
115	72.0	51.3	76.9

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM




Abundance



Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E




Time-->



#4

2-Fluorophenol
Concen: 0.390 ng
RT: 5.30 min Scan# 211
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.5	22.0	33.0#
63	151.3	121.8	182.6




Abundance


Ion 112.00 (111.70 to 112.70): E


Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1



Time-->



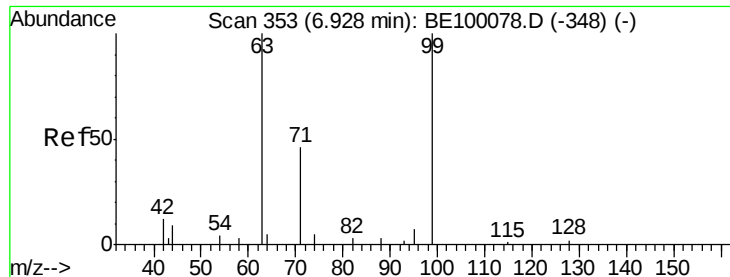

#5

Phenol-d6

Concen: 0.417 ng

RT: 6.90 min Scan# 350

Delta R.T. -0.03 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Instrument :

BNA_E





ClientSampleId :

EXT-013-SW161-061319

Tot Ion:	99	Resp:	863
Ion	Ratio	Lower	Upper
99	100		
42	16.3	0.0	0.0#
71	35.7	37.6	56.4#

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.52 min Scan# 643


Delta R.T. -0.01 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Tgt Ion:	136	Resp:	2953
Ion	Ratio	Lower	Upper
136	100		
137	14.2	11.6	17.4
54	31.8	33.9	50.9#
68	8.4	7.8	11.8



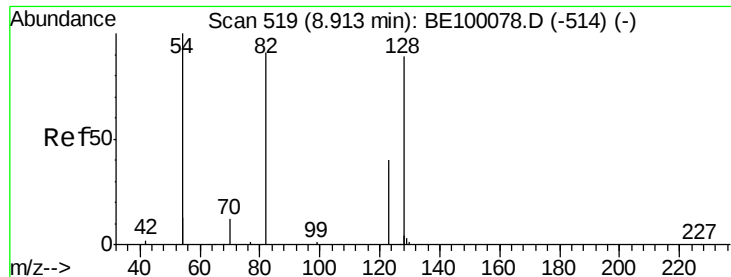

#8

Nitrobenzene-d5

Concen: 0.300 ng

RT: 8.90 min Scan# 518

Delta R.T. -0.01 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Instrument :

BNA_E


ClientSampleId :

EXT-013-SW161-061319




Tot Ion:	82	Resp:	859
Ion	Ratio	Lower	Upper
82	100		
128	174.2	128.0	192.0
54	169.7	143.4	215.0

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



Abundance Ion 82.00 (81.70 to 82.70): BE1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE1



#9

Naphthalene

Concen: 0.294 ng

RT: 10.58 min Scan# 647




Delta R.T. -0.01 min


Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Tgt Ion:	128	Resp:	9442
Ion	Ratio	Lower	Upper
128	100		
129	3.6	3.1	4.7
127	4.0	3.4	5.2

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E









#11
2-Methylnaphthalene-d10
Concen: 0.028 ng
RT: 12.14 min Scan# 758
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion:152 Resp: 160
Ion Ratio Lower Upper
152 100
151 21.9 16.3 24.5




Manual Integrations
APPROVED


mohammad
6/25/2019 3:21:39 PM



#12
2-Methylnaphthalene
Concen: 0.468 ng
RT: 12.21 min Scan# 763
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion:142 Resp: 2468
Ion Ratio Lower Upper
142 100
141 94.0 74.1 111.1
115 45.6 40.9 61.3



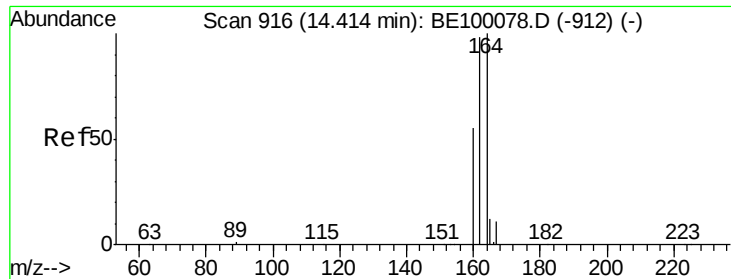


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.40 min Scan# 915
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
164	100		
162	99.9	78.2	117.2
160	50.8	45.6	68.4

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM




Abundance



Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E




Time-->



#14
2,4,6-Tribromophenol
Concen: 0.389 ng
RT: 15.90 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
330	100		
332	94.0	73.3	109.9
141	114.8	22.2	33.2#




Abundance


Ion 330.00 (329.70 to 330.70): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



Time-->



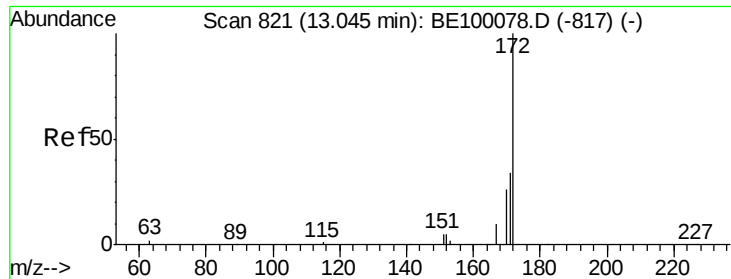





#15
2-Fluorobiphenyl
Concen: 0.266 ng
RT: 13.03 min Scan# 820
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
172	100		
171	34.9	29.8	44.8
170	24.5	23.2	34.8




Manual Integrations
APPROVED


mohammad
6/25/2019 3:21:39 PM



#16
Acenaphthylene
Concen: 1.047 ng
RT: 14.12 min Scan# 896
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.2	15.9	23.9
153	14.3	10.1	15.1





#17

Acenaphthene

Concen: 0.232 ng

RT: 14.47 min Scan# 920

Delta R.T. -0.00 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Instrument :

BNA_E


ClientSampleId :

EXT-013-SW161-061319




Tot Ion:	154	Resp:	1587
Ion Ratio	Lower	Upper	
154	100		
153	130.2	95.5	143.3
152	67.4	54.9	82.3

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#18

Fluorene

Concen: 0.659 ng


RT: 15.45 min Scan# 987

Delta R.T. -0.01 min



Lab File: BE100150.D




Acq: 22 Jun 2019 1:34

Tgt Ion:	166	Resp:	6700
Ion Ratio	Lower	Upper	
166	100		
165	113.4	79.8	119.8
167	22.3	10.2	15.4#



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.15 min Scan# 1114

Delta R.T. -0.01 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Tot Ion	Ratio	Resp	Lower	Upper
188	100	7399		
94	0.0	0.0	0.0	
80	8.0	6.3	9.5	

Instrument :





BNA_E

ClientSampleId :

EXT-013-SW161-061319

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



#23

Phenanthrene

Concen: 7.272 ng


RT: 17.19 min Scan# 1117


Delta R.T. -0.01 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	128909		
176	19.8	15.9	23.9	
179	15.7	13.1	19.7	









#24
 Anthracene
 Concen: 0.794 ng
 RT: 17.28 min Scan# 1124
 Delta R.T. -0.01 min
 Lab File: BE100150.D
 Acq: 22 Jun 2019 1:34

Instrument :
 BNA_E
 ClientSampleId :
 EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.8	23.6
179	14.4	12.0	18.0




Manual Integrations
 APPROVED


mohammad
 6/25/2019 3:21:39 PM



#25
 Fluoranthene-d10
 Concen: 0.020 ng
 RT: 19.19 min Scan# 1379
 Delta R.T. -0.00 min
 Lab File: BE100150.D
 Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
212	100		
106	1.5	1.4	2.0
104	2.7	0.8	1.2#






#26
Fluoranthene
Concen: 6.636 ng
RT: 19.22 min Scan# 1384
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319


Tot Ion	Ratio	Lower	Upper
202	100		
101	5.8	5.0	7.4
203	18.0	13.7	20.5

Manual Integrations
APPROVED



mohammad
6/25/2019 3:21:39 PM



Abundance Ion 202.00 (201.70 to 202.70): E
200000
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E




Time-->





#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.34 min Scan# 1627
Delta R.T. -0.00 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34


Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.2	6.6	10.0#
236	31.4	23.8	35.6

Abundance Ion 240.00 (239.70 to 240.70): E
10000
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



Time-->









#28
Pvrene
Concen: 10.278 ng
RT: 19.58 min Scan# 1447
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion:	202	Resp:	240705
Ion Ratio	Lower	Upper	
202	100		
200	19.7	15.6	23.4
203	20.7	13.9	20.9




Manual Integrations
APPROVED


mohammad
6/25/2019 3:21:39 PM



#29
Terphenyl-d14
Concen: 0.283 ng
RT: 19.79 min Scan# 1483
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion:	244	Resp:	5160
Ion Ratio	Lower	Upper	
244	100		
212	42.4	29.8	44.8
122	7.1	6.1	9.1









#30
Benzo(a)anthracene
Concen: 4.909 ng
RT: 21.33 min Scan# 1626
Delta R.T. -0.00 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.8	23.0	34.4
229	23.7	16.4	24.6




Manual Integrations
APPROVED


mohammad
6/25/2019 3:21:39 PM



#31
Chrysene
Concen: 5.228 ng
RT: 21.38 min Scan# 1630
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.1	23.8	35.8
229	22.4	16.3	24.5






#32
Bis(2-ethylhexyl)phthalate
Concen: 1.563 ng
RT: 21.24 min Scan# 1619
Delta R.T. -0.00 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319




Tot Ion	Ratio	Lower	Upper
149	100		
167	7.5	5.8	8.6
279	1.5	1.1	1.7

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM






Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E




#33
Indeno(1,2,3-cd)pyrene
Concen: 2.307 ng
RT: 26.47 min Scan# 2923
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
276	100		
138	9.2	4.3	6.5#
277	24.0	19.4	29.0

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E









#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.83 min Scan# 2189
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
264	100		
260	28.8	20.8	31.2
265	43.5	23.2	34.8#




Manual Integrations
APPROVED


mohammad
6/25/2019 3:21:39 PM



#35
Benzo(b)fluoranthene
Concen: 4.769 ng
RT: 23.07 min Scan# 1974
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	18.4	27.6
125	5.5	6.4	9.6#





#36

Benzo(k)fluoranthene

Concen: 1.420 ng m

RT: 23.11 min Scan# 1987

Delta R.T. -0.01 min

Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Instrument :

BNA_E


ClientSampleId :

EXT-013-SW161-061319




Tot Ion:	252	Resp:	53533
Ion Ratio	Lower	Upper	
252	100		
253	24.2	18.9	28.3
125	5.8	5.3	7.9

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E



#37

Benzo(a)pyrene

Concen: 3.700 ng m

RT: 23.72 min Scan# 2157




Delta R.T. -0.01 min


Lab File: BE100150.D

Acq: 22 Jun 2019 1:34

Tgt Ion:	252	Resp:	118346
Ion Ratio	Lower	Upper	
252	100		
253	23.4	19.4	29.2
125	5.7	8.0	12.0#

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E









#38
Dibenzo(a,h)anthracene
Concen: 0.679 ng
RT: 26.48 min Scan# 2927
Delta R.T. -0.02 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Instrument :
BNA_E
ClientSampleId :
EXT-013-SW161-061319

Tot Ion	Ratio	Lower	Upper
278	100		
139	11.0	9.0	13.6
279	33.6	21.4	32.0

Manual Integrations
APPROVED

mohammad
6/25/2019 3:21:39 PM



#39
Benzo(g,h,i)perylene
Concen: 2.541 ng
RT: 27.29 min Scan# 3153
Delta R.T. -0.01 min
Lab File: BE100150.D
Acq: 22 Jun 2019 1:34

Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.1	20.3	30.5
138	10.1	11.3	16.9

