


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062119\
Data File : BE100130.D
Acq On : 21 Jun 2019 7:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 15:07:24 2019

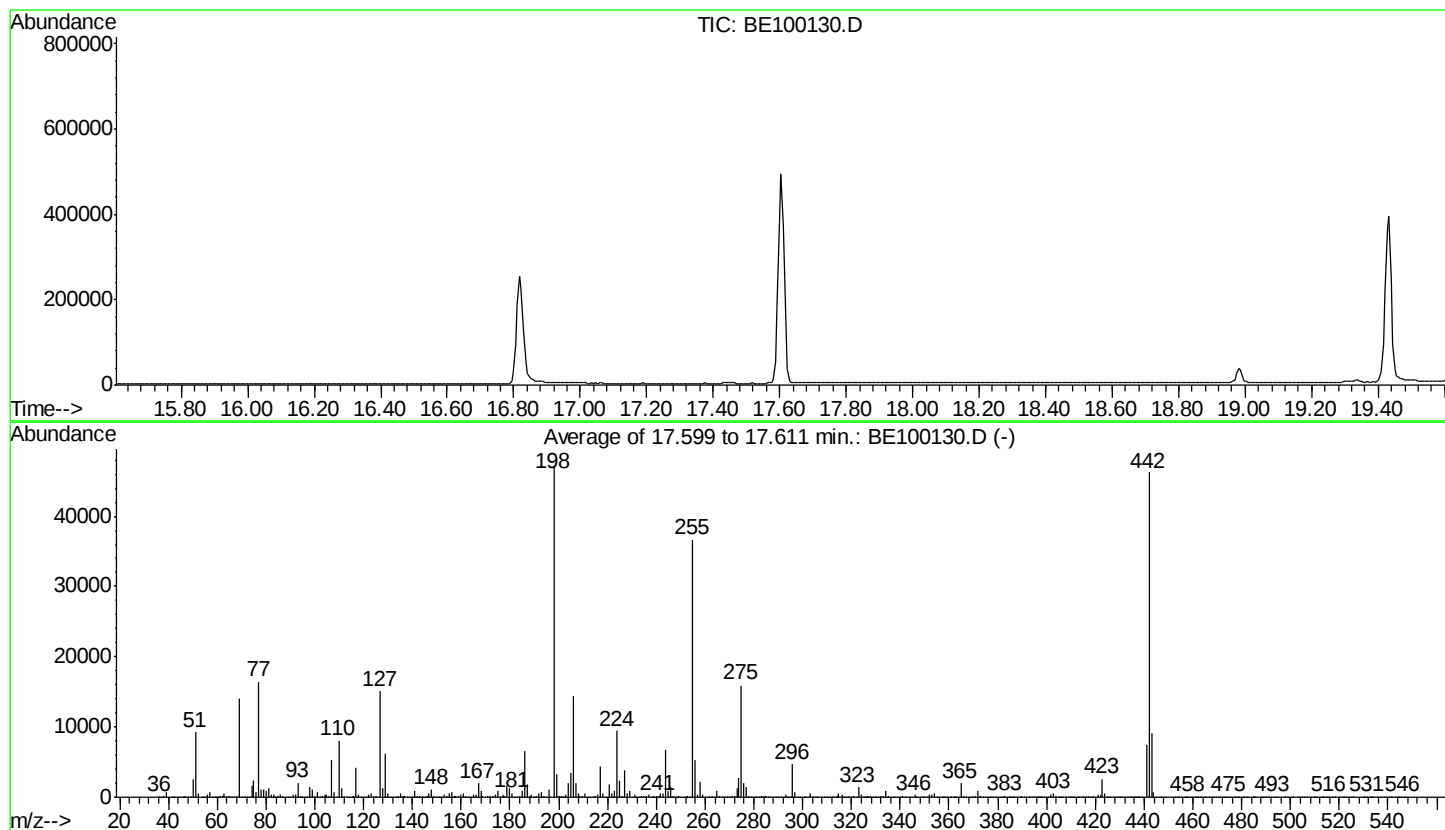

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	9262	PASS
68	69	0.00	2	1.5	214	PASS
69	198	0.00	100	29.9	14095	PASS
70	69	0.00	2	0.6	78	PASS
127	198	10	80	32.0	15091	PASS
197	198	0.00	2	0.1	52	PASS
198	198	100	100	100.0	47216	PASS
199	198	5	9	6.9	3279	PASS
275	198	10	60	33.6	15875	PASS
365	198	1	100	4.1	1936	PASS
441	198	0.01	100	15.7	7423	PASS
442	198	50	100	98.2	46378	PASS
443	442	15	24	19.8	9185	PASS