


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE062119\
 Data File : BE100140.D
 Acq On : 21 Jun 2019 17:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 19 15:07:24 2019

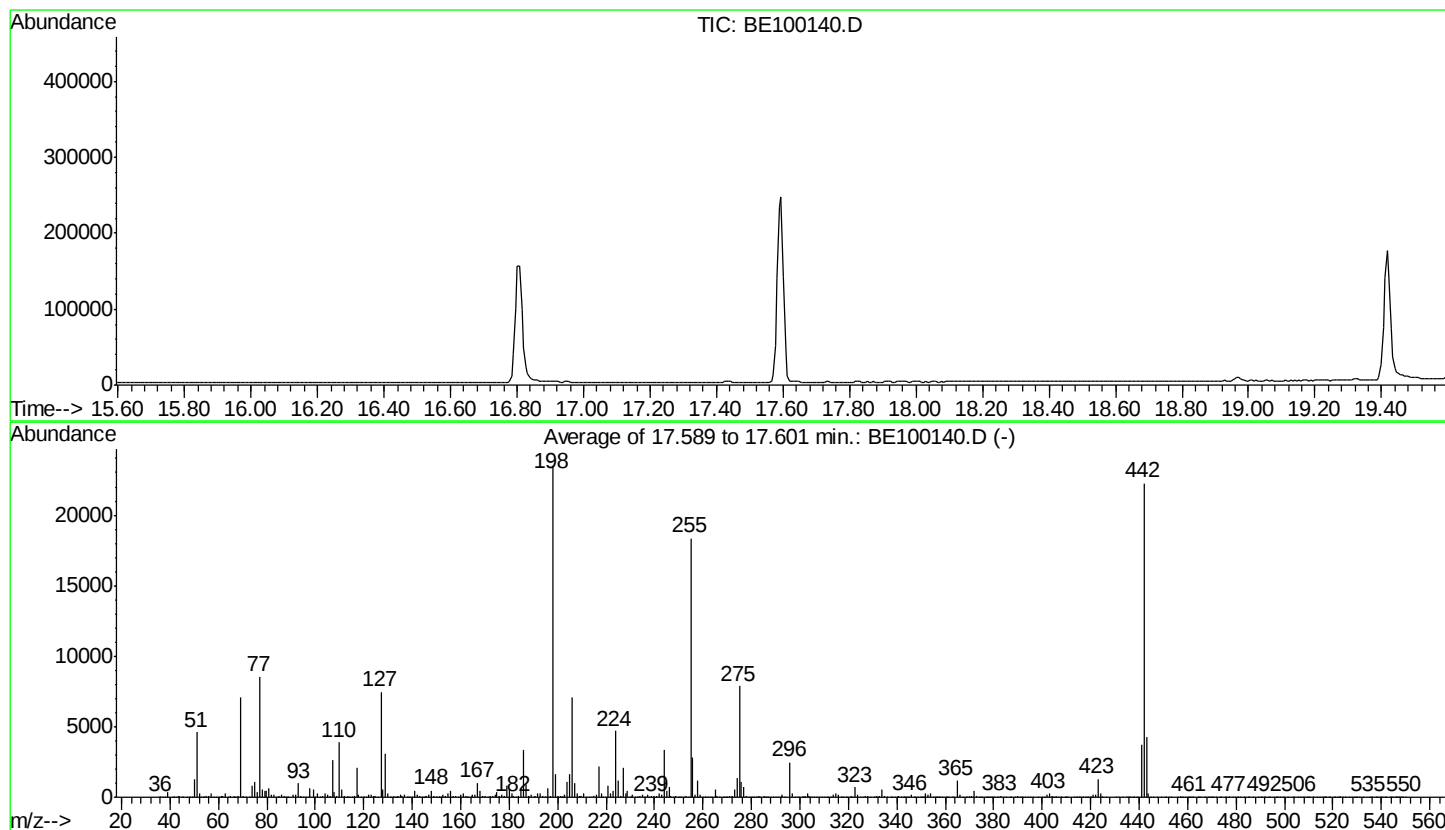

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.5	4593	PASS
68	69	0.00	2	1.2	82	PASS
69	198	0.00	100	30.1	7076	PASS
70	69	0.00	2	0.7	52	PASS
127	198	10	80	31.8	7470	PASS
197	198	0.00	2	0.3	59	PASS
198	198	100	100	100.0	23500	PASS
199	198	5	9	6.8	1595	PASS
275	198	10	60	33.5	7882	PASS
365	198	1	100	4.9	1148	PASS
441	198	0.01	100	15.7	3686	PASS
442	198	50	100	94.7	22245	PASS
443	442	15	24	19.0	4236	PASS