
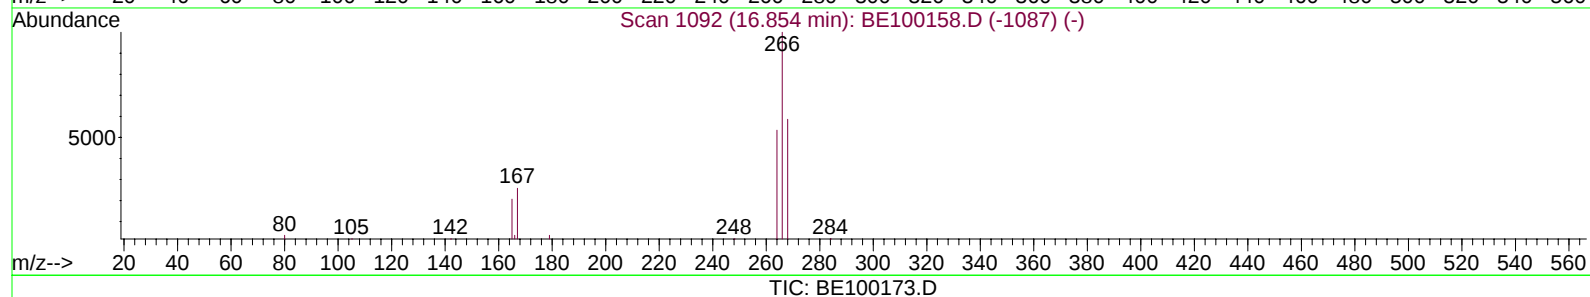
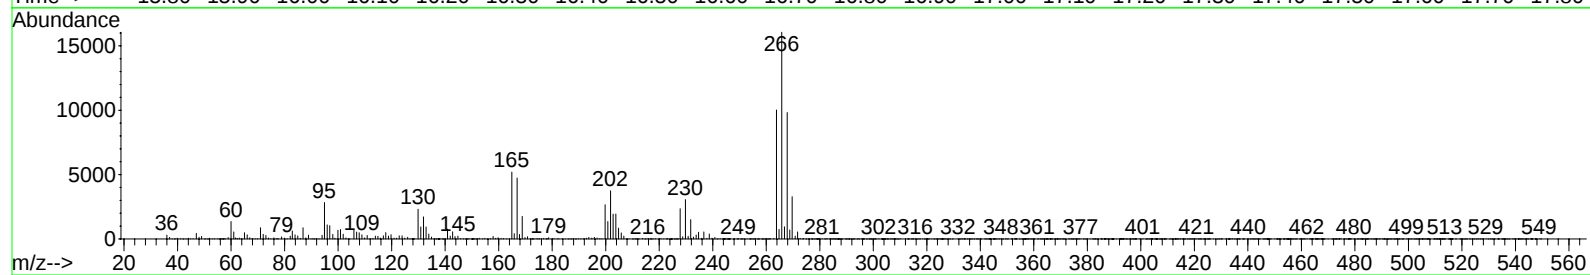


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062519\
Data File : BE100173.D
Acq On : 25 Jun 2019 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 12:14:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:47:20 2019
Response via : Initial Calibration

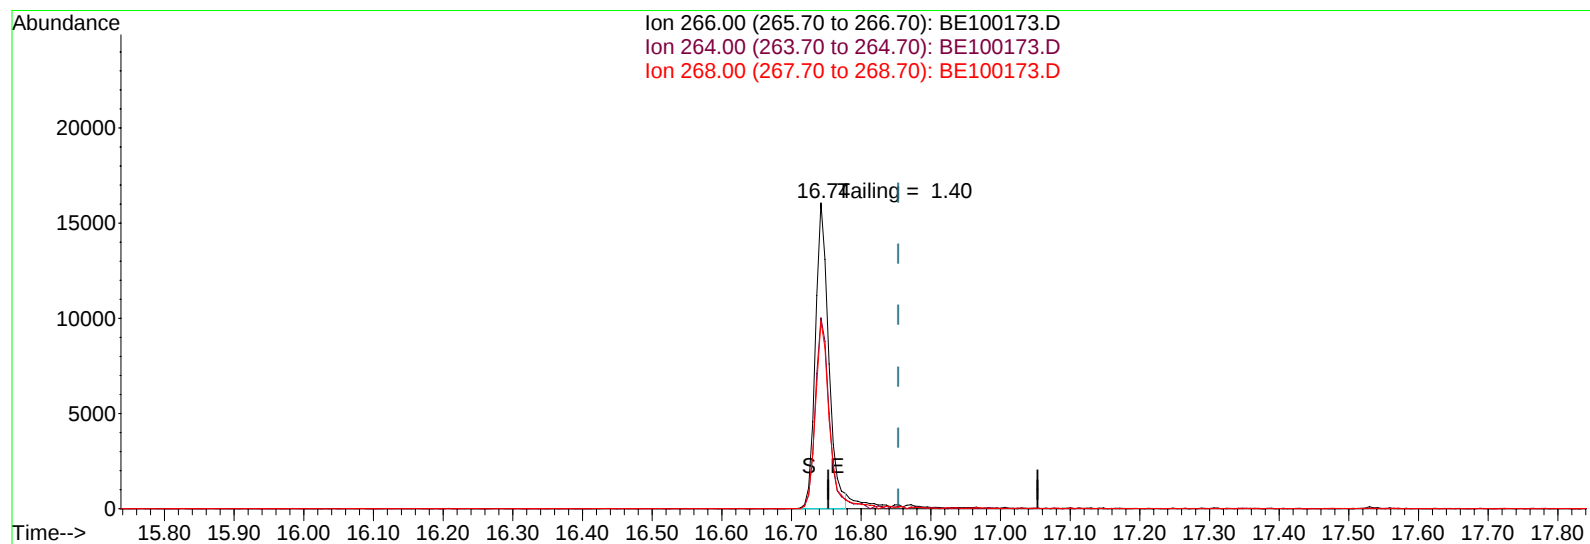

TIC: BE100173.D

(22) Pentachlorophenol

16.742min (-0.111) 5774.02ng

response 15917

Ion	Exp%	Act%
266.00	100	100
264.00	73.10	62.42
268.00	76.90	61.15#
0.00	0.00	0.00