


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE062519\
Data File : BE100173.D
Acq On : 25 Jun 2019 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 25 15:40:27 2019

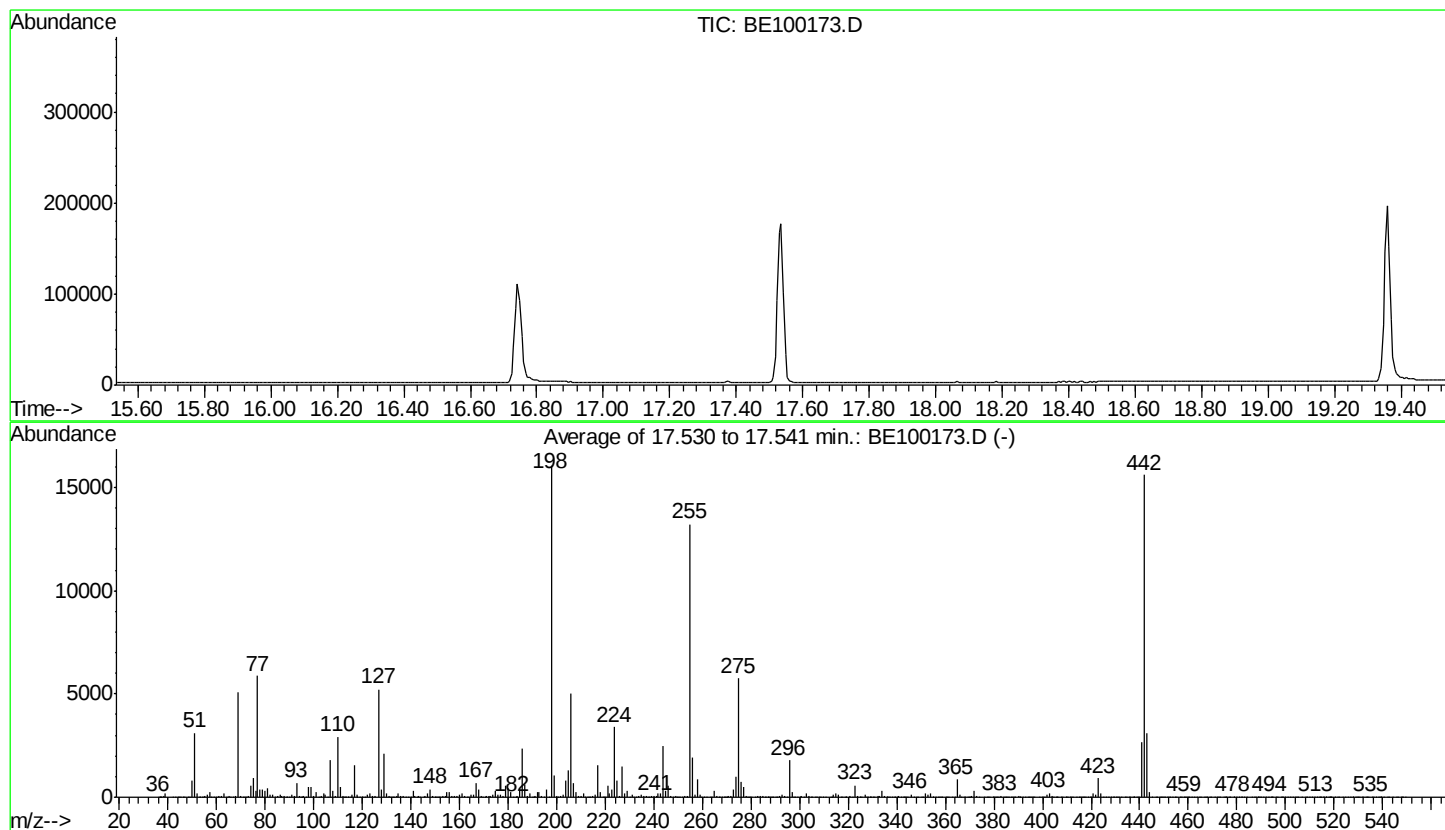

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.5	3126	PASS
68	69	0.00	2	1.1	55	PASS
69	198	0.00	100	31.6	5076	PASS
70	69	0.00	2	0.7	36	PASS
127	198	10	80	32.6	5233	PASS
197	198	0.00	2	0.2	30	PASS
198	198	100	100	100.0	16057	PASS
199	198	5	9	6.6	1066	PASS
275	198	10	60	35.8	5743	PASS
365	198	1	100	5.3	854	PASS
441	198	0.01	100	16.6	2662	PASS
442	198	50	100	97.2	15605	PASS
443	442	15	24	19.9	3106	PASS