


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE062618\
 Data File : BE096842.D
 Acq On : 26 Jun 2018 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 20 15:45:14 2018

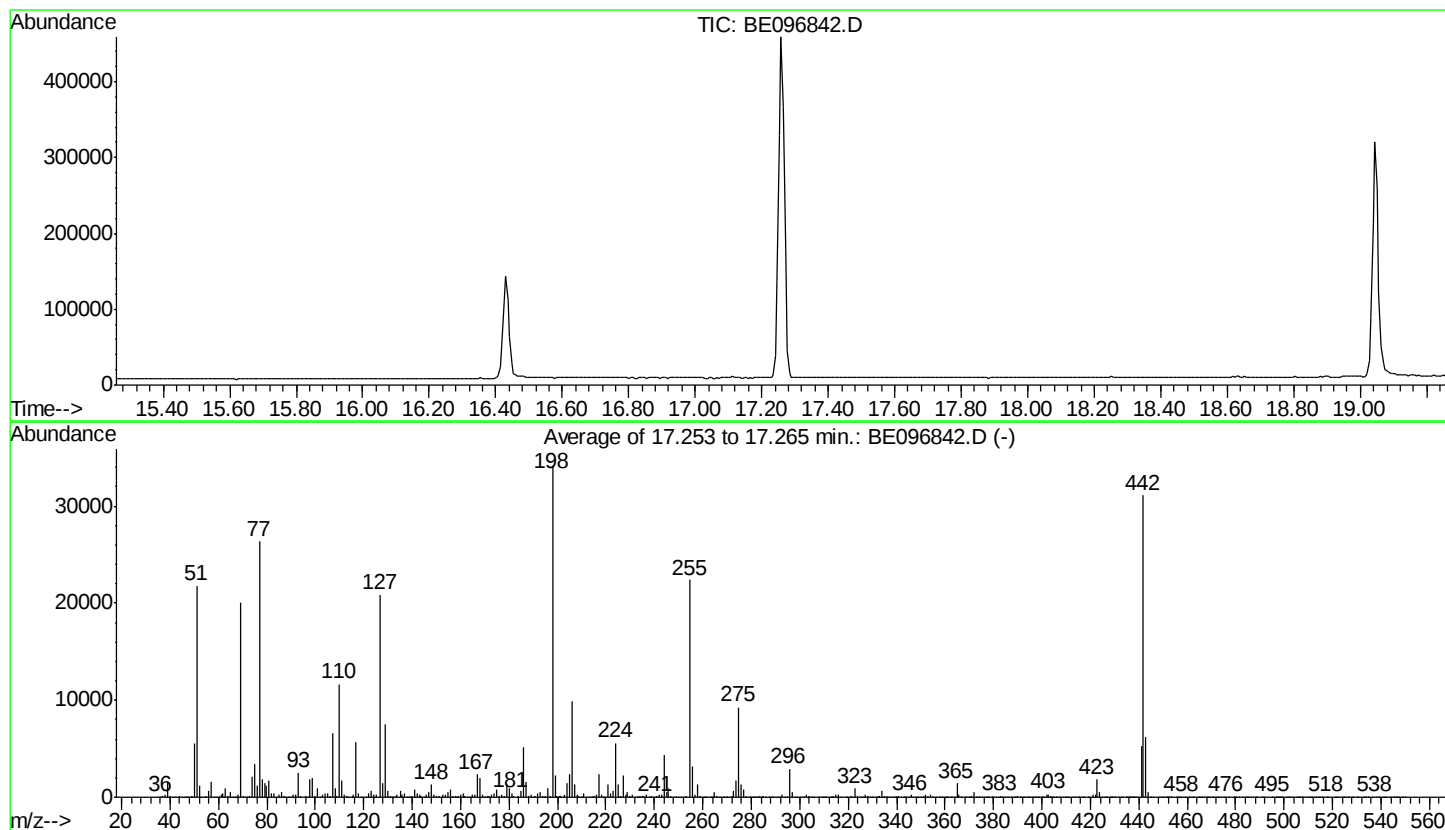

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.7	21771	PASS
68	69	0.00	2	1.2	248	PASS
69	198	0.00	100	58.8	20104	PASS
70	69	0.00	2	0.5	97	PASS
127	198	10	80	61.0	20848	PASS
197	198	0.00	2	0.4	129	PASS
198	198	100	100	100.0	34169	PASS
199	198	5	9	6.7	2296	PASS
275	198	10	60	27.2	9285	PASS
365	198	1	100	4.1	1393	PASS
441	443	0.01	100	84.0	5239	PASS
442	198	50	100	90.9	31072	PASS
443	442	15	24	20.1	6238	PASS