
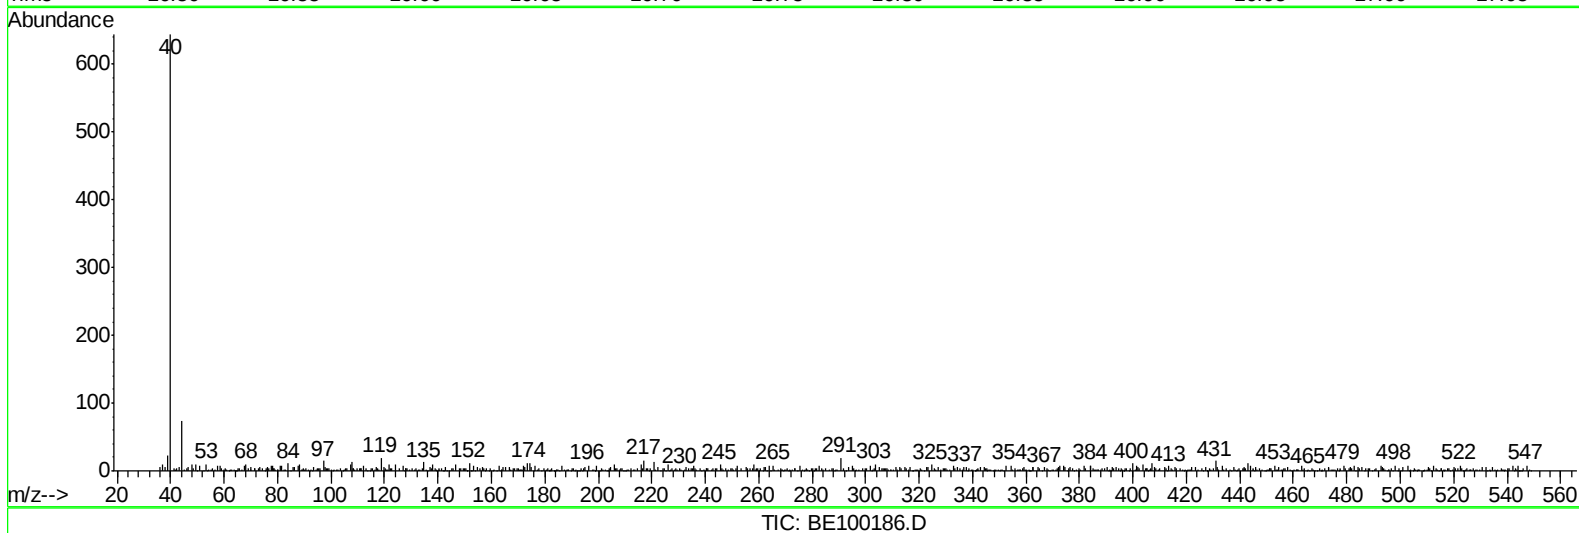


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062619\
Data File : BE100186.D
Acq On : 26 Jun 2019 8:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 03:29:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

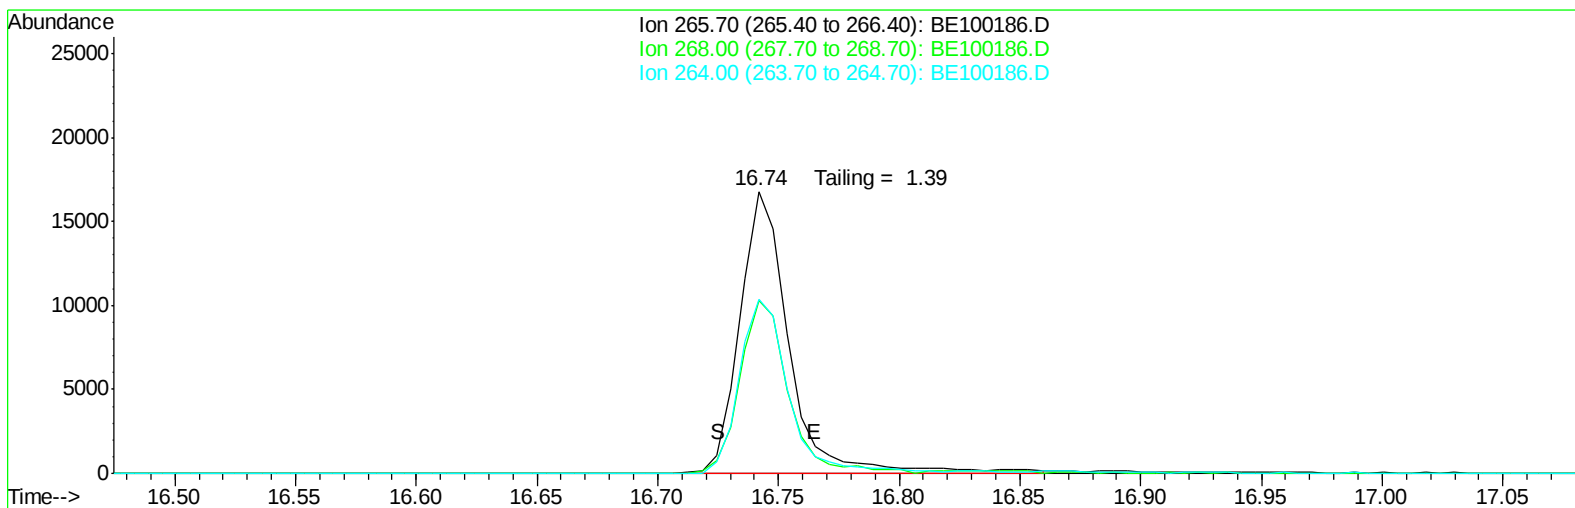

(69) Pentachlorophenol (C)



12.165min (+0.078) 75.15ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	70.00
264.00	65.00	70.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062619\
Data File : BE100186.D
Acq On : 26 Jun 2019 8:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 03:29:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

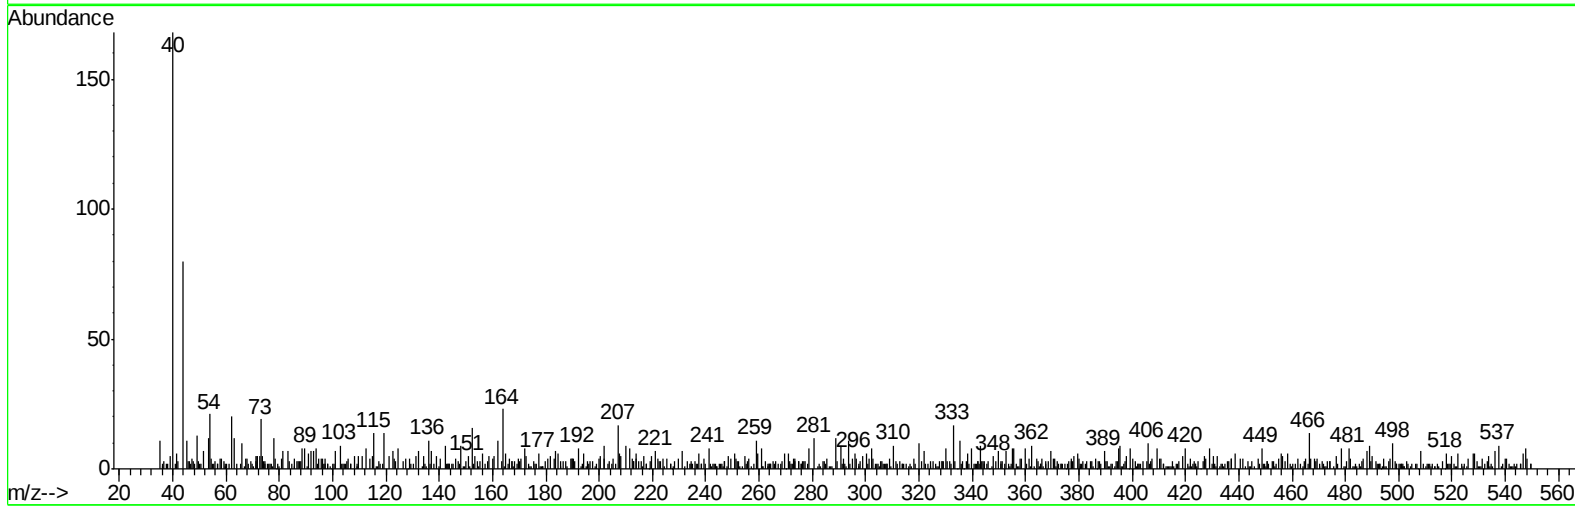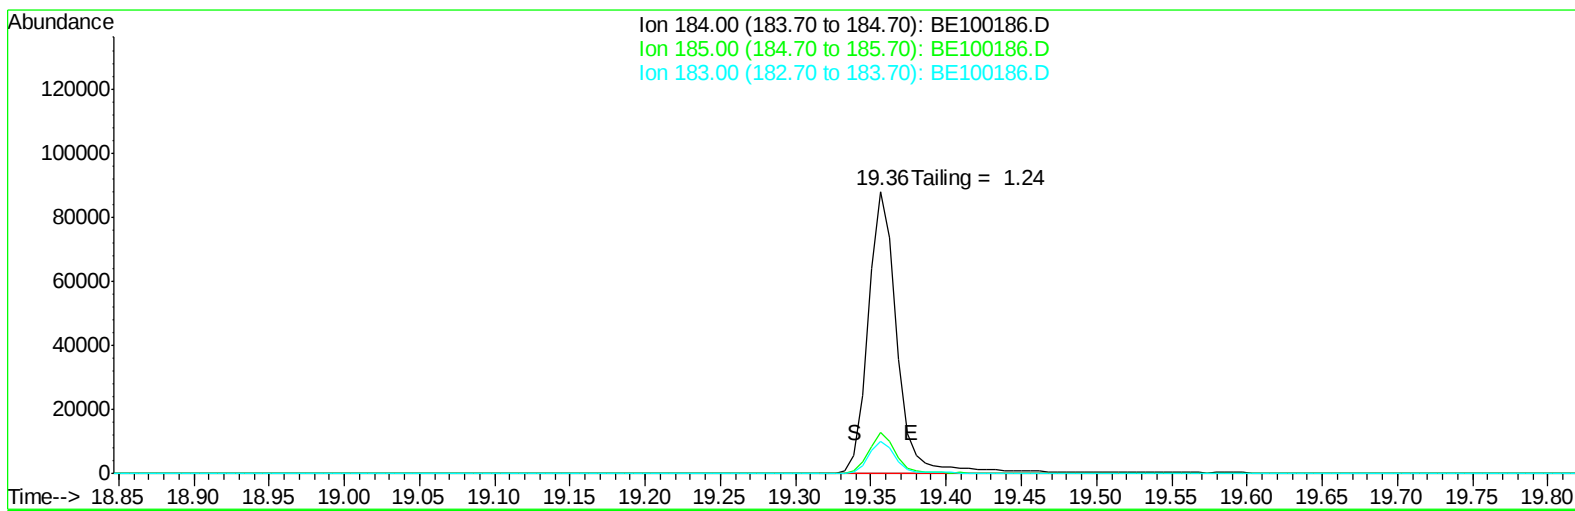

TIC: BE100186.D

(76) Benzidine

14.586min (-0.005) 61.66ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	76.92#
183.00	12.20	84.62#
0.00	0.00	0.00