

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062619\
 Data File : BE100193.D
 Acq On : 26 Jun 2019 13:54
 Operator : JU/SJ
 Sample : PB120737BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB120737BL

Quant Time: Jun 27 05:05:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 15:40:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	531	0.40	ng	0.00
7) Naphthalene-d8	10.51	136	1640	0.40	ng	0.04
13) Acenaphthene-d10	14.36	164	1308	0.40	ng	0.01
19) Phenanthrene-d10	17.11	188	4009	0.40	ng	0.01
27) Chrysene-d12	21.28	240	5969	0.40	ng	0.00
34) Perylene-d12	23.73	264	7092	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.24	112	394	0.33	ng	0.00
5) Phenol-d6	6.89	99	117	0.07	ng	0.01
8) Nitrobenzene-d5	8.94	82	214	0.13	ng	0.09
11) 2-Methylnaphthalene-d10	12.14	152	839	0.27	ng	0.06
14) 2,4,6-Tribromophenol	15.94	330	62	0.08	ng	0.09
15) 2-Fluorobiphenyl	13.03	172	1442	0.27	ng	0.06
25) Fluoranthene-d10	19.14	212	16993	0.29	ng	0.00
29) Terphenyl-d14	19.74	244	3568	0.30	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062619\
Data File : BE100193.D
Acq On : 26 Jun 2019 13:54
Operator : JU/SJ
Sample : PB120737BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB120737BL

Quant Time: Jun 27 05:05:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 25 15:40:27 2019
Response via : Initial Calibration

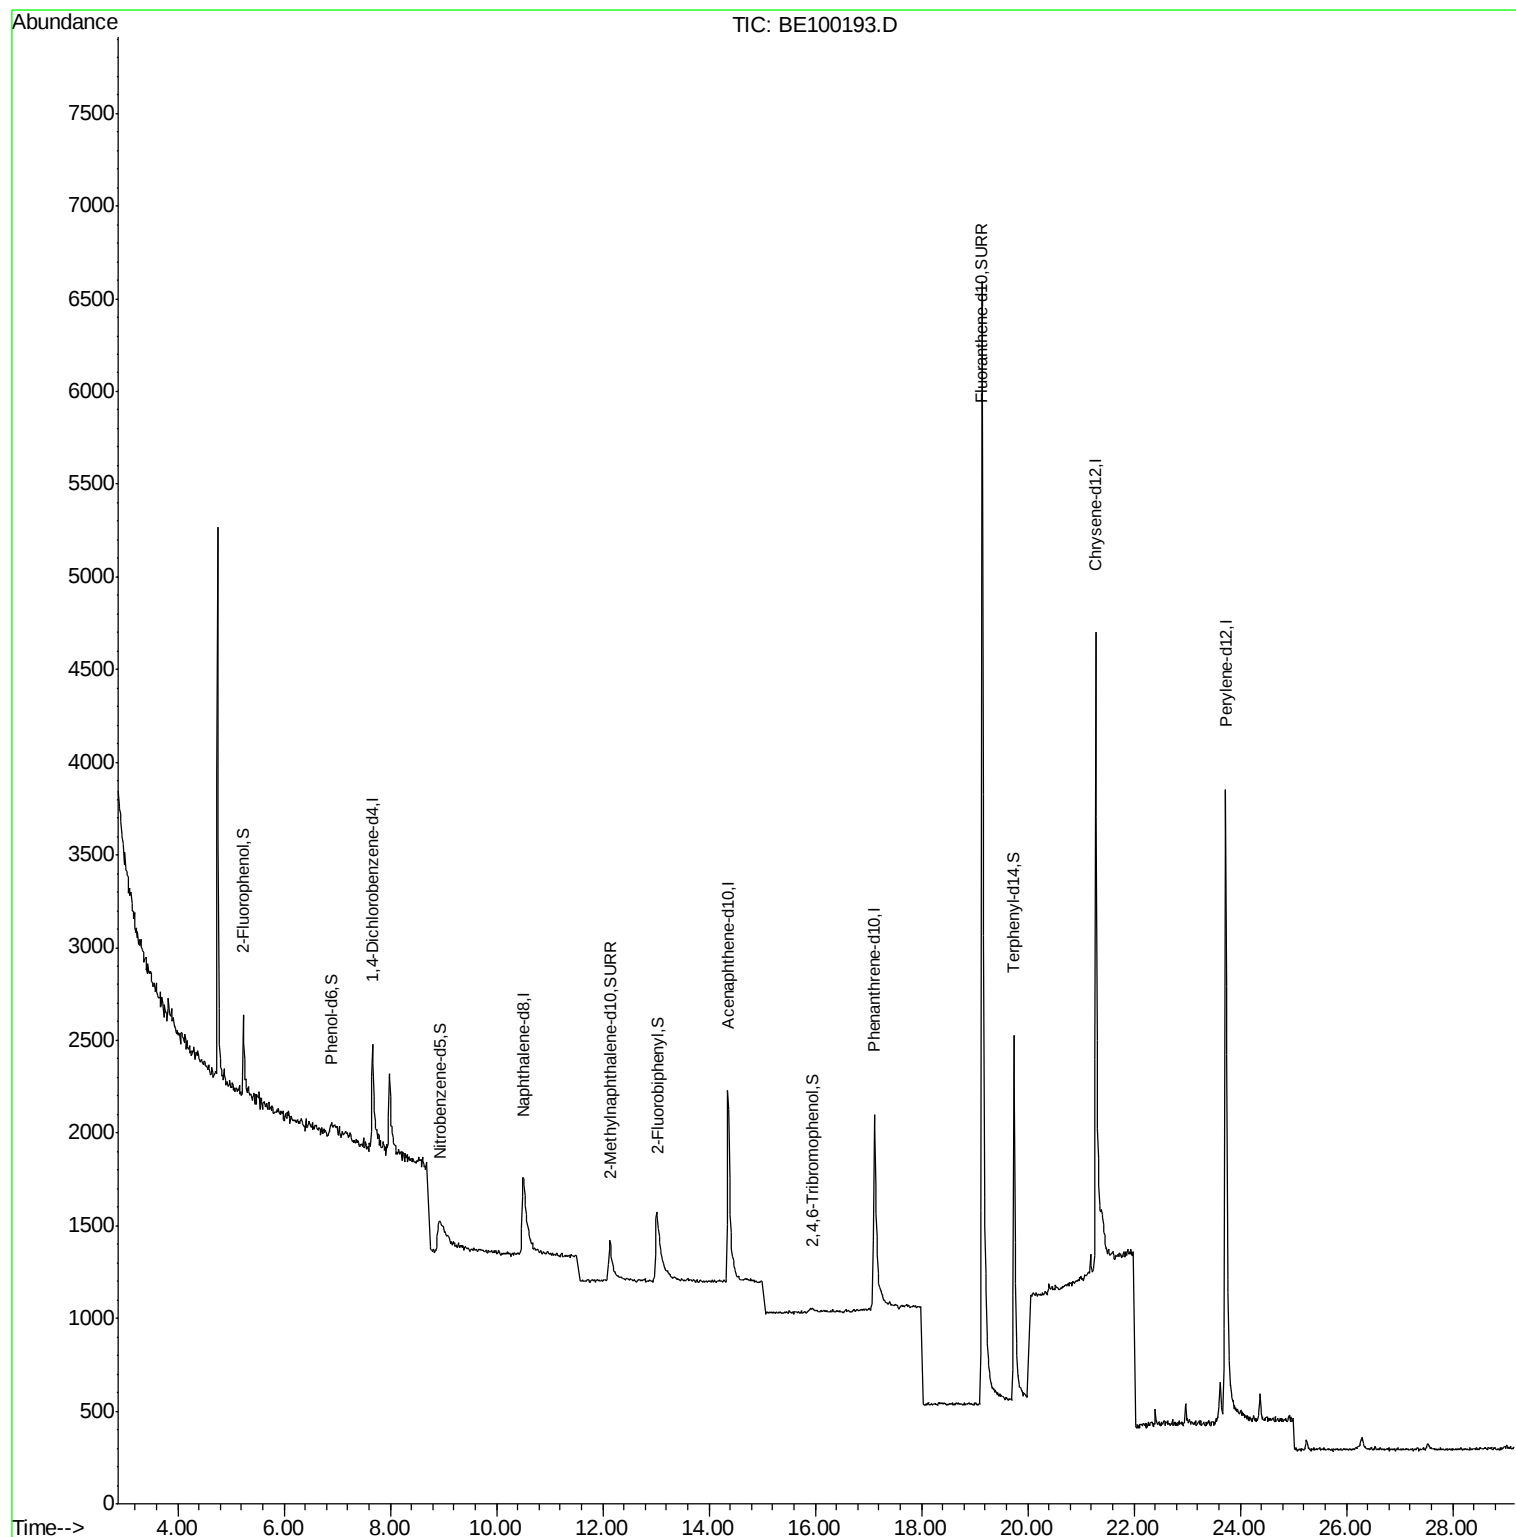




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.67 min Scan# 417
Delta R.T. 0.00 min
Lab File: BE100193.D
Acq: 26 Jun 2019 13:54

Instrument :
BNA_E
ClientSampleId :
PB120737BL

Tot Ion:152 Resp: 531
Ion Ratio Lower Upper
152 100
150 133.0 113.4 170.2
115 70.6 55.8 83.6

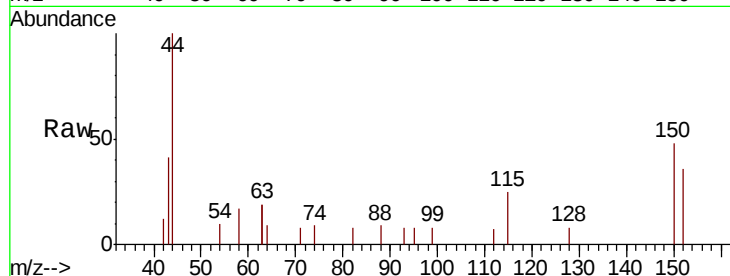


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

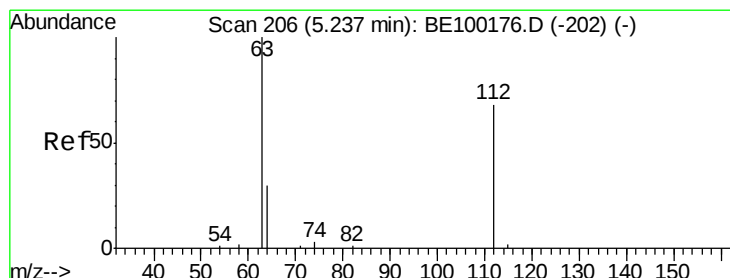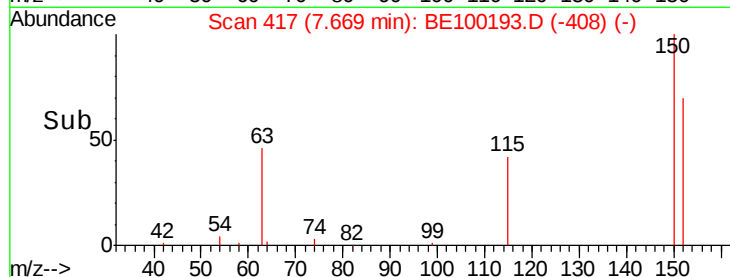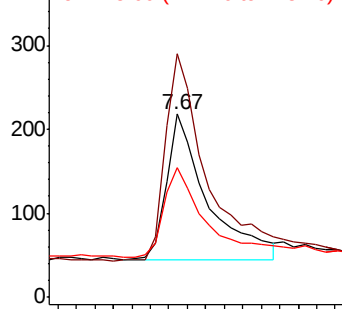



#4


2-Fluorophenol
Concen: 0.334 ng
RT: 5.24 min Scan# 206
Delta R.T. 0.00 min
Lab File: BE100193.D
Acq: 26 Jun 2019 13:54

Tgt Ion:112 Resp: 394
Ion Ratio Lower Upper
112 100
64 53.3 40.7 61.1
63 127.7 93.2 139.8

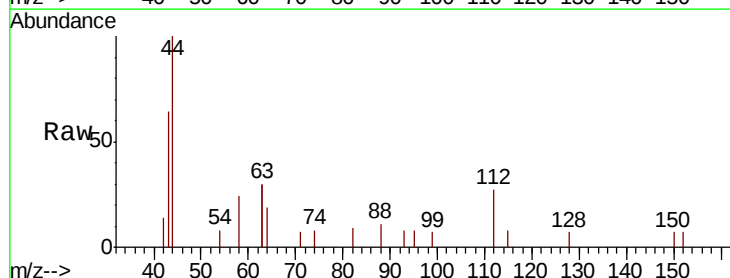

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE1
Ion 63.00 (62.70 to 63.70): BE1

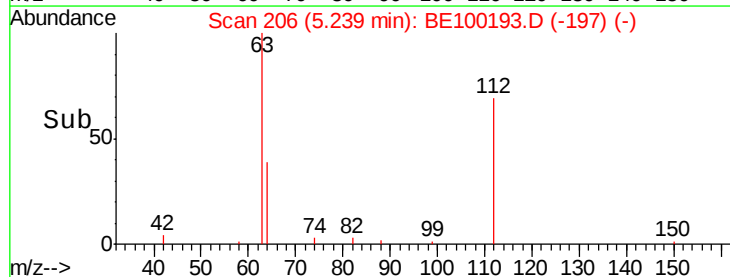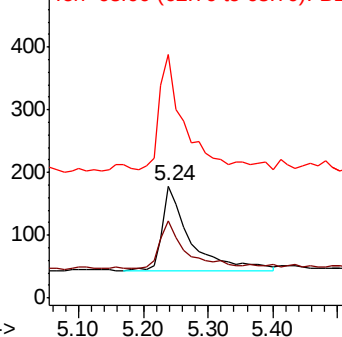

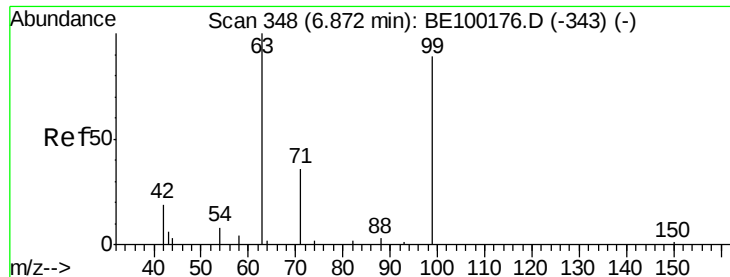

#5

Phenol-d6

Concen: 0.072 ng

RT: 6.89 min Scan# 349

Delta R.T. 0.01 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Instrument :

BNA_E

ClientSampleId :

PB120737BL


Tot Ion: 99 Resp: 117

Ion Ratio Lower Upper




99 100

42 34.2 10.4 15.6#

71 42.7 32.4 48.6

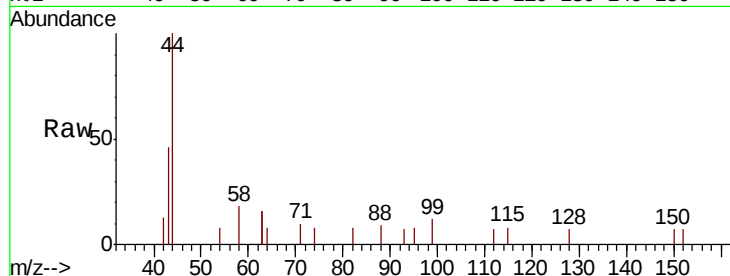

Abundance Ion 99.00 (98.70 to 99.70): BE1
Ion 42.00 (41.70 to 42.70): BE1
Ion 71.00 (70.70 to 71.70): BE1

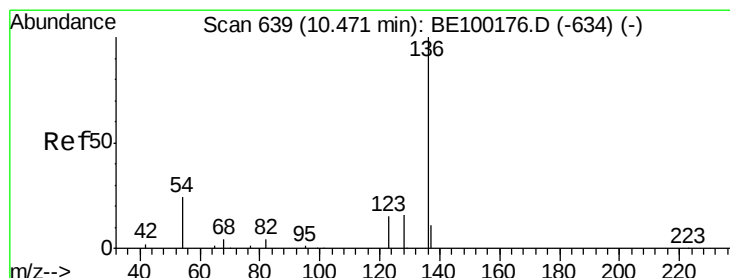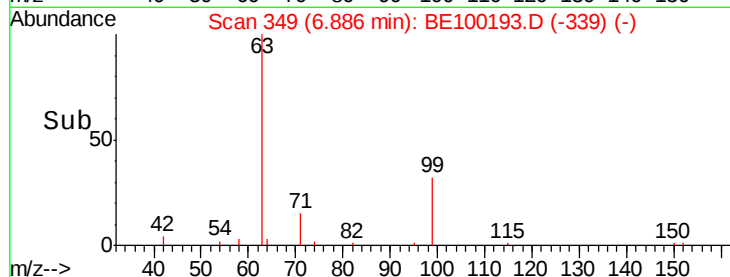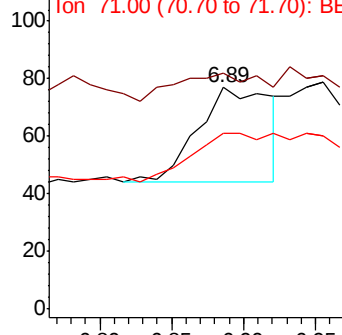

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.51 min Scan# 642

Delta R.T. 0.04 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Tgt Ion: 136 Resp: 1640


Ion Ratio Lower Upper

136 100



137 25.3 13.8 20.8#


54 70.5 35.4 53.2#

68 17.8 8.8 13.2#

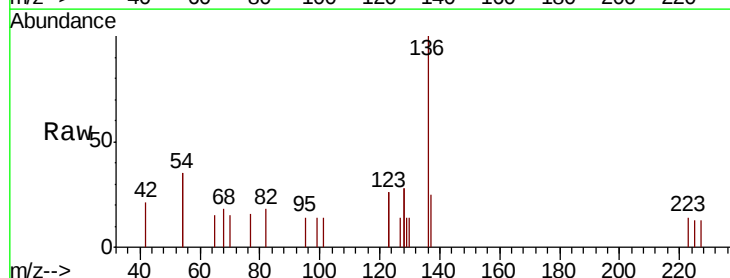

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE1
Ion 68.00 (67.70 to 68.70): BE1

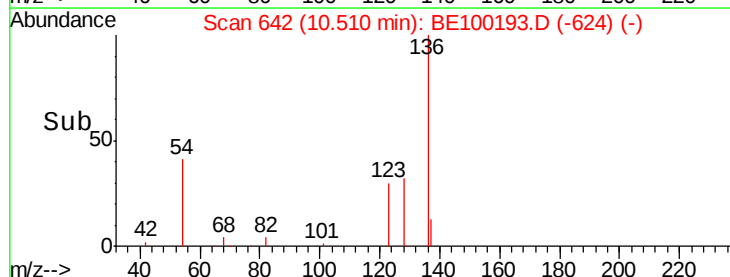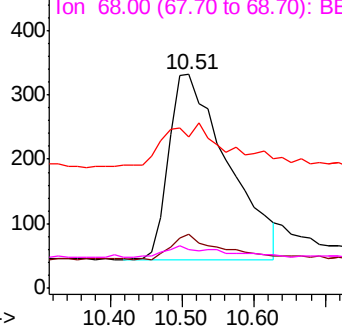

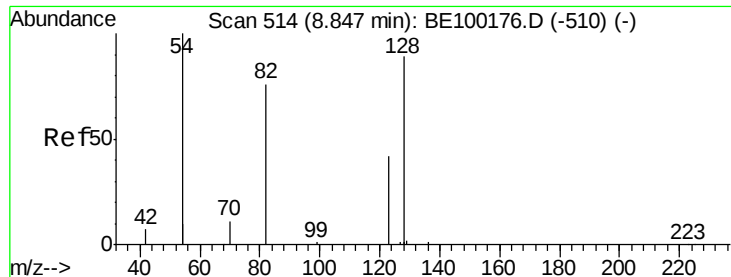

#8

Nitrobenzene-d5

Concen: 0.131 ng

RT: 8.94 min Scan# 521

Delta R.T. 0.09 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Instrument :

BNA_E

ClientSampleId :

PB120737BL


Tot Ion: 82 Resp: 214

Ion Ratio Lower Upper

82 100

128 270.5 144.6 217.0#




54 277.3 163.0 244.6#

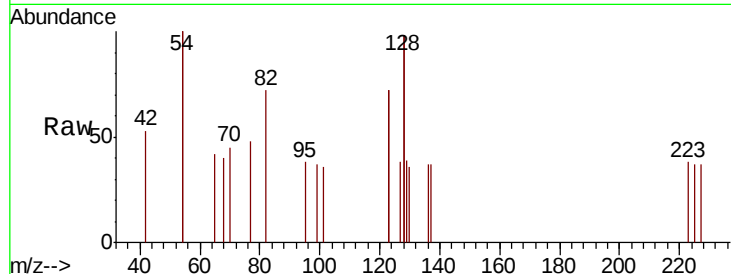

Abundance Ion 82.00 (81.70 to 82.70): BE1

Ion 128.00 (127.70 to 128.70): BE1

Ion 54.00 (53.70 to 54.70): BE1

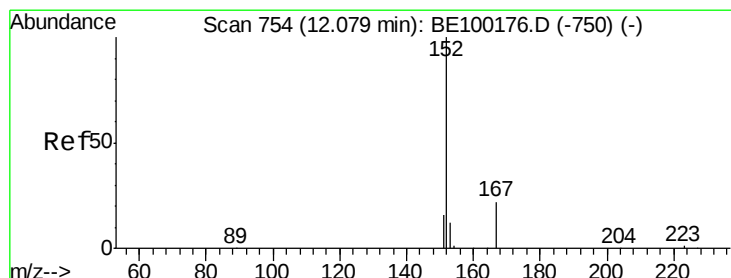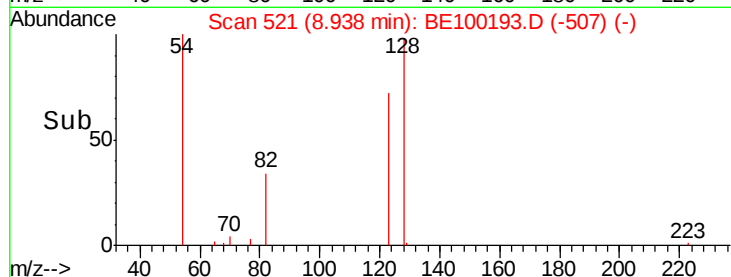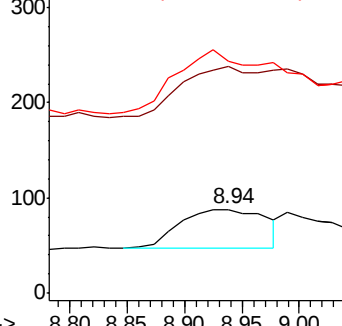

#11

2-Methylnaphthalene-d10

Concen: 0.273 ng

RT: 12.14 min Scan# 758

Delta R.T. 0.06 min

Lab File: BE100193.D


Acq: 26 Jun 2019 13:54

Tgt Ion: 152 Resp: 839

Ion Ratio Lower Upper



152 100


151 19.8 16.3 24.5

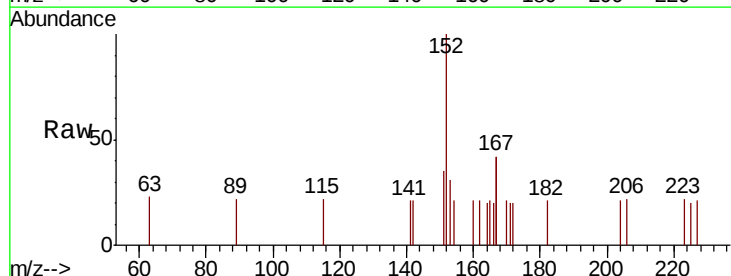

Abundance Ion 152.00 (151.70 to 152.70): BE1

Ion 151.00 (150.70 to 151.70): BE1

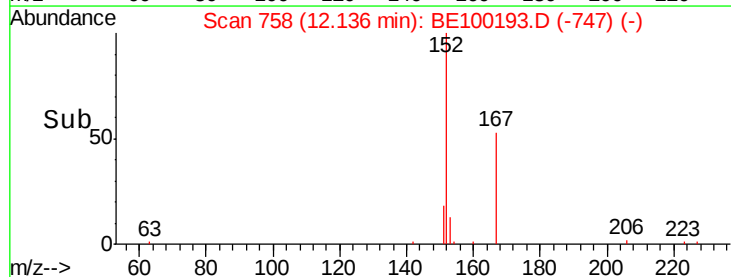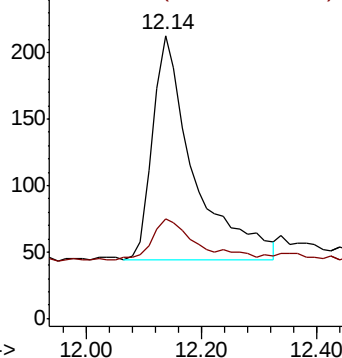

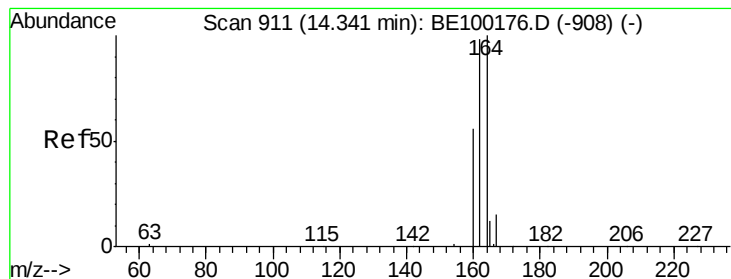

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.36 min Scan# 912

Delta R.T. 0.01 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Instrument :

BNA_E

ClientSampleId :

PB120737BL


Tot Ion:164 Resp: 1308

Ion Ratio Lower Upper

164 100

162 99.5 78.6 118.0




160 65.8 46.9 70.3

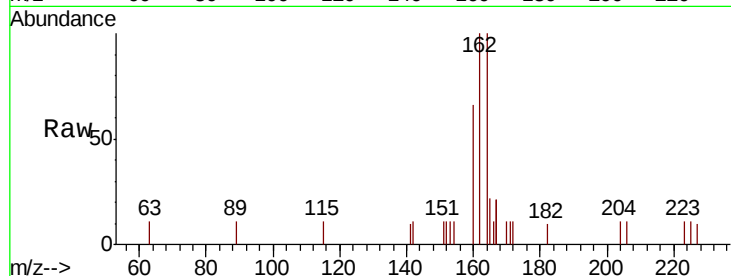

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

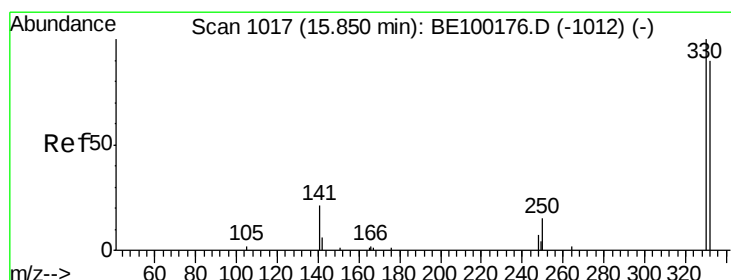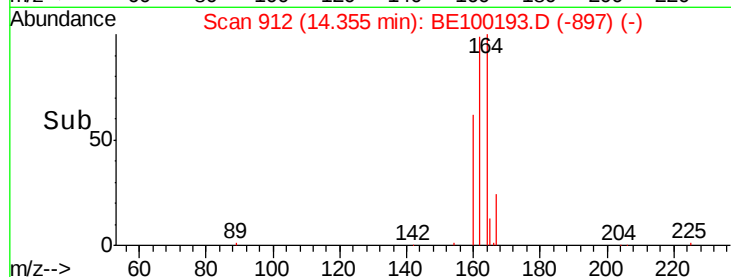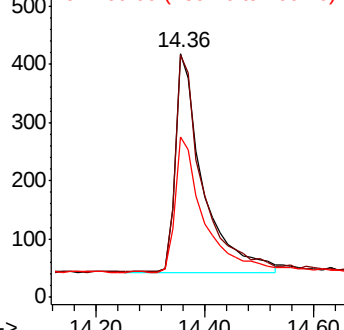

#14

2,4,6-Tribromophenol

Concen: 0.082 ng

RT: 15.94 min Scan# 1024

Delta R.T. 0.09 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54


Tgt Ion:330 Resp: 62

Ion Ratio Lower Upper

330 100

332 106.5 77.7 116.5



141 0.0 18.9 28.3#

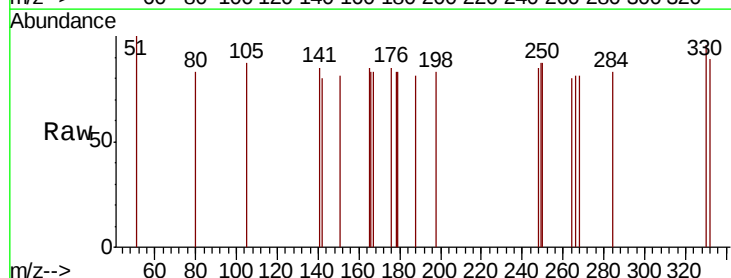


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



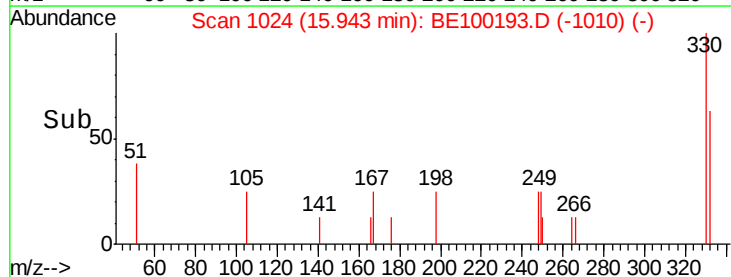
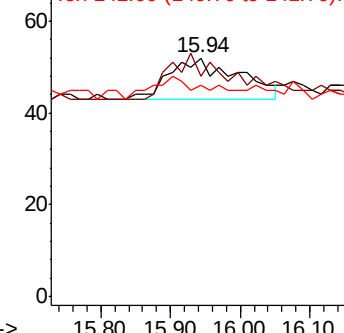


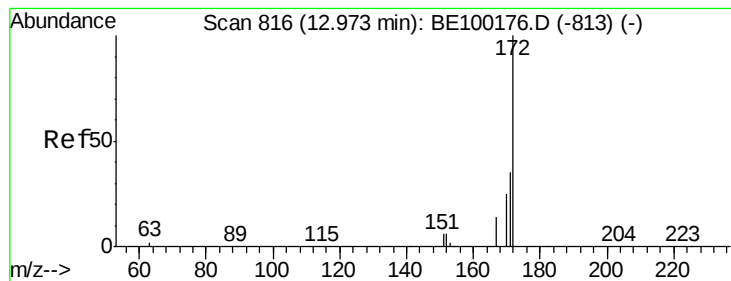

#15
2-Fluorobiphenyl
Concen: 0.275 ng
RT: 13.03 min Scan# 820
Delta R.T. 0.06 min
Lab File: BE100193.D
Acq: 26 Jun 2019 13:54




Instrument :
BNA_E
ClientSampleId :
PB120737BL


Tot Ion:172 Resp: 1442
Ion Ratio Lower Upper
172 100
171 45.0 31.0 46.4
170 38.2 23.9 35.9#

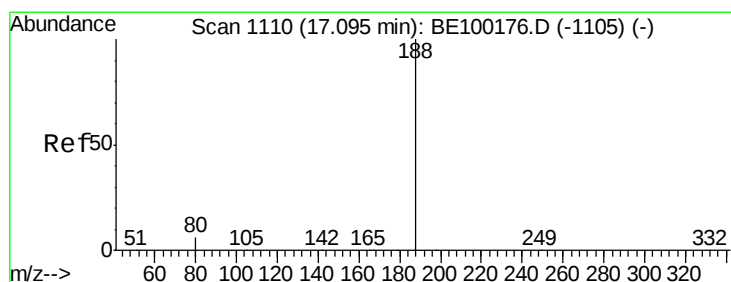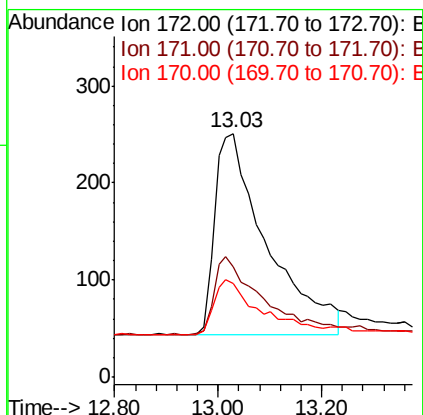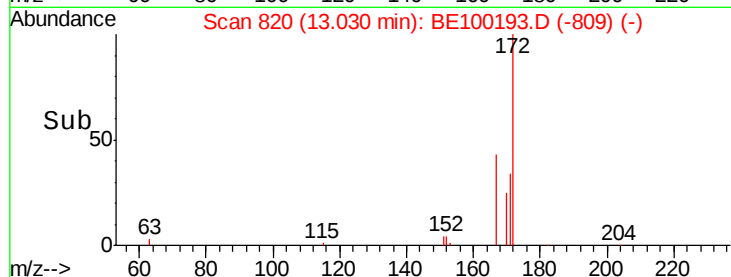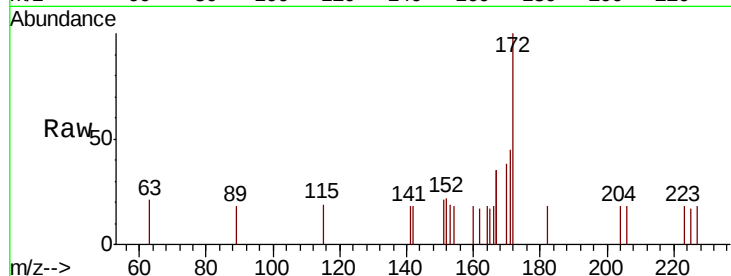

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.11 min Scan# 1111
Delta R.T. 0.01 min
Lab File: BE100193.D
Acq: 26 Jun 2019 13:54

Tgt Ion:188 Resp: 4009
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.1 6.4 9.6#

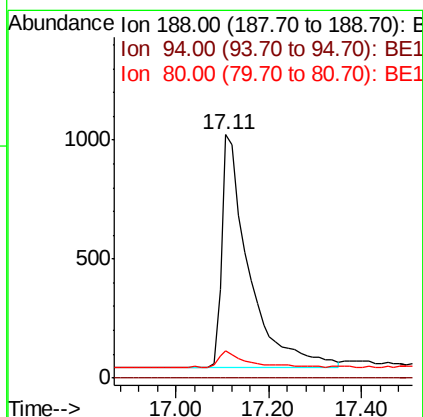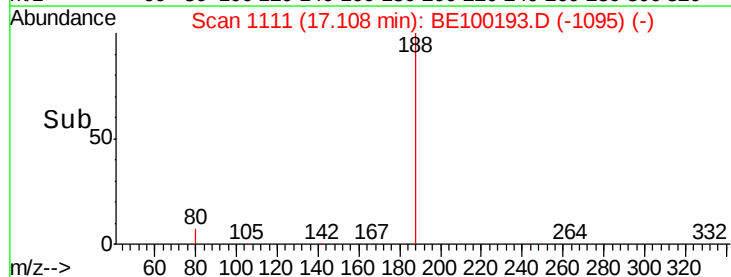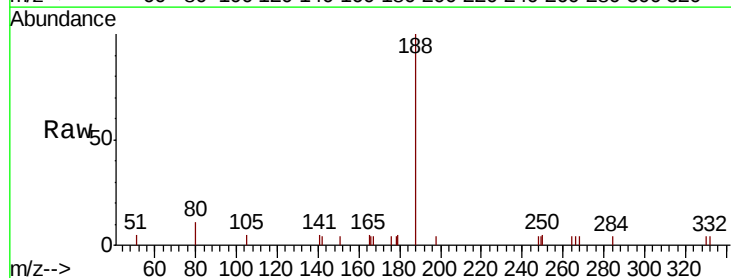

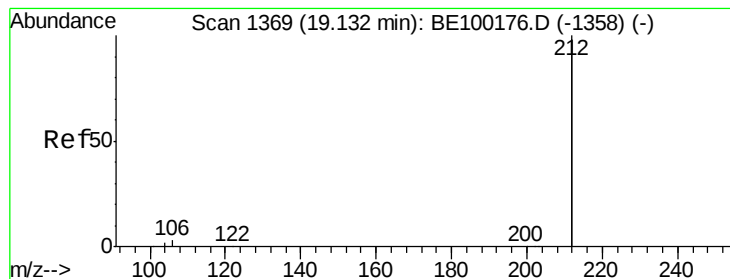

#25

Fluoranthene-d10

Concen: 0.294 ng

RT: 19.14 min Scan# 1370

Delta R.T. 0.01 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Instrument :

BNA_E

ClientSampleId :

PB120737BL


Tot Ion:212 Resp: 16993

Ion Ratio Lower Upper

212 100

106 1.3 1.3 1.9




104 0.9 0.7 1.1

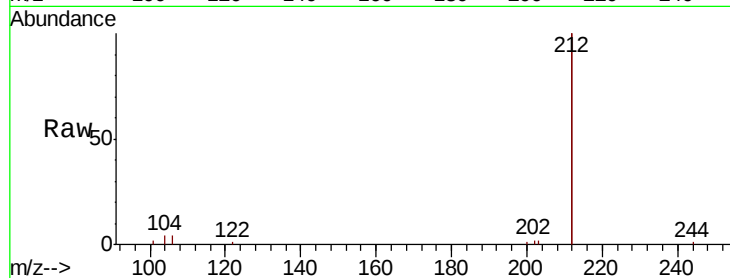

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

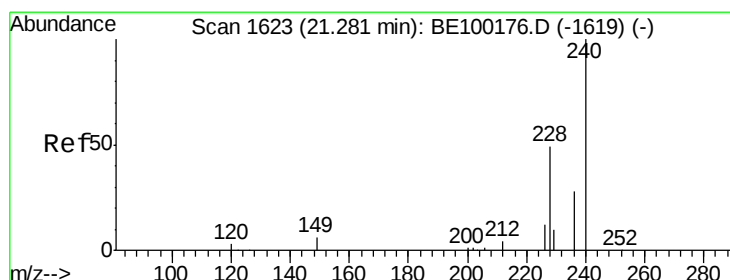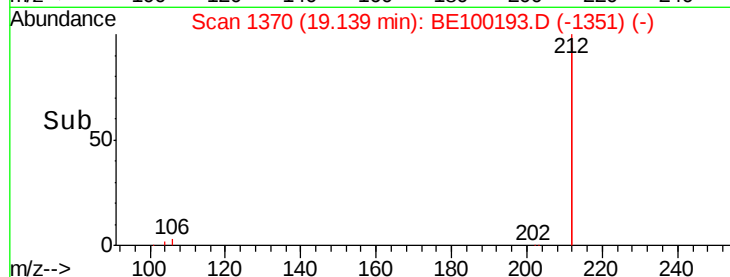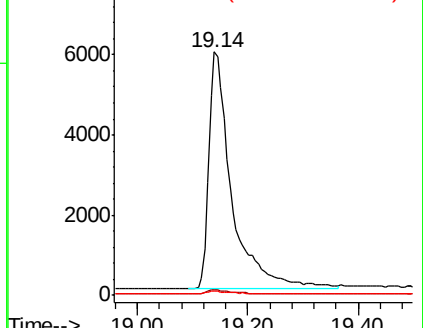

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.28 min Scan# 1623

Delta R.T. 0.00 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54


Tgt Ion:240 Resp: 5969

Ion Ratio Lower Upper

240 100

120 6.4 4.1 6.1#



236 28.5 23.0 34.6

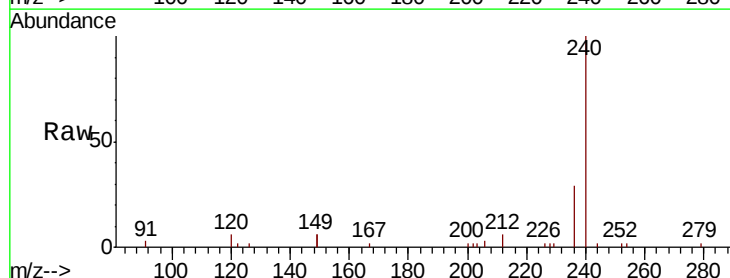


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

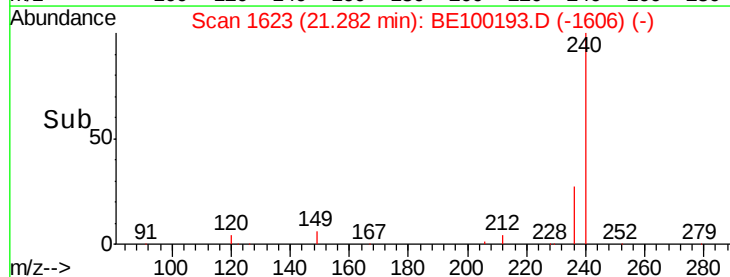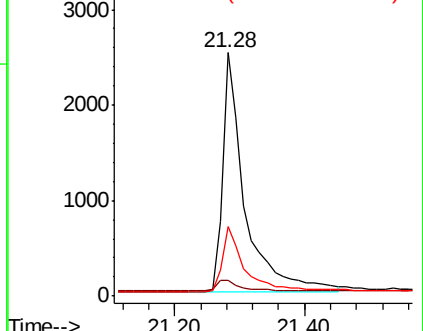

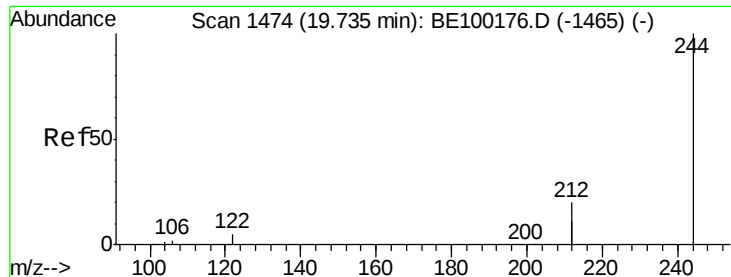

#29

Terphenyl-d14

Concen: 0.304 ng

RT: 19.74 min Scan# 1475

Delta R.T. 0.01 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54

Instrument :

BNA_E

ClientSampleId :

PB120737BL


Tot Ion:244 Resp: 3568

Ion Ratio Lower Upper

244 100

212 43.2 30.7 46.1




122 8.1 5.8 8.6

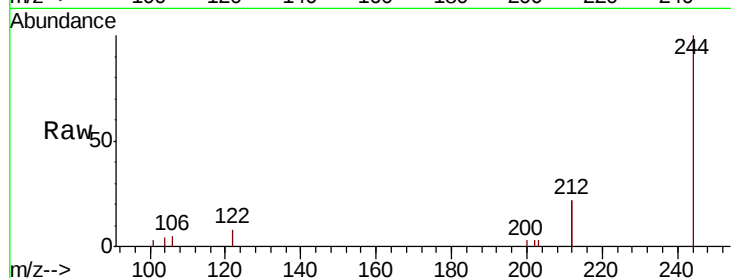

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

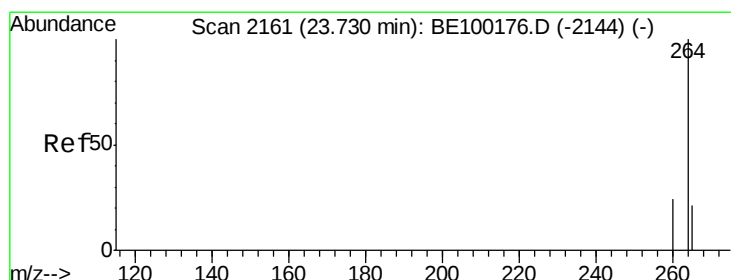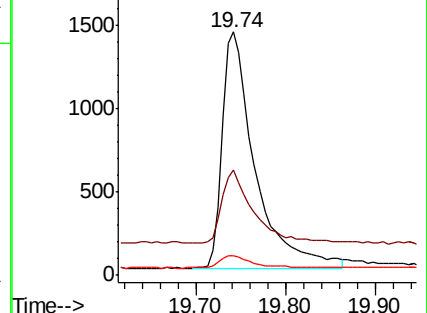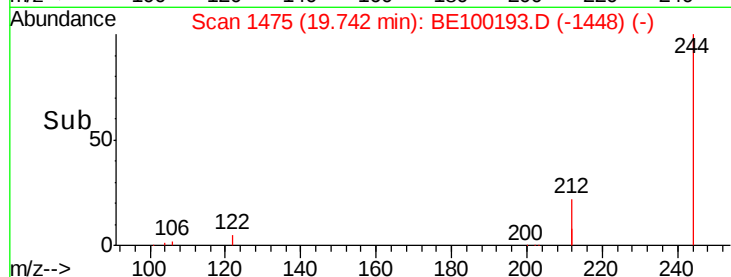

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.73 min Scan# 2161

Delta R.T. -0.00 min

Lab File: BE100193.D

Acq: 26 Jun 2019 13:54


Tgt Ion:264 Resp: 7092

Ion Ratio Lower Upper

264 100

260 26.5 20.4 30.6

265 26.6 22.5 33.7

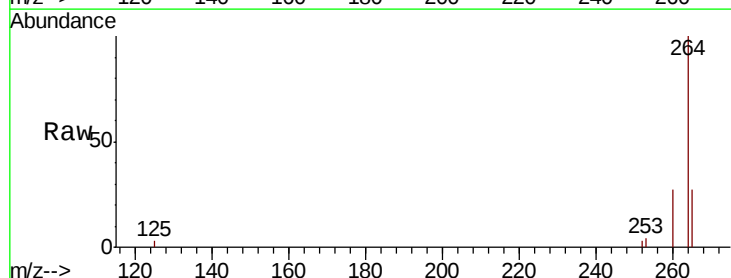

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

