


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE062619\
 Data File : BE100186.D
 Acq On : 26 Jun 2019 8:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 25 15:40:27 2019

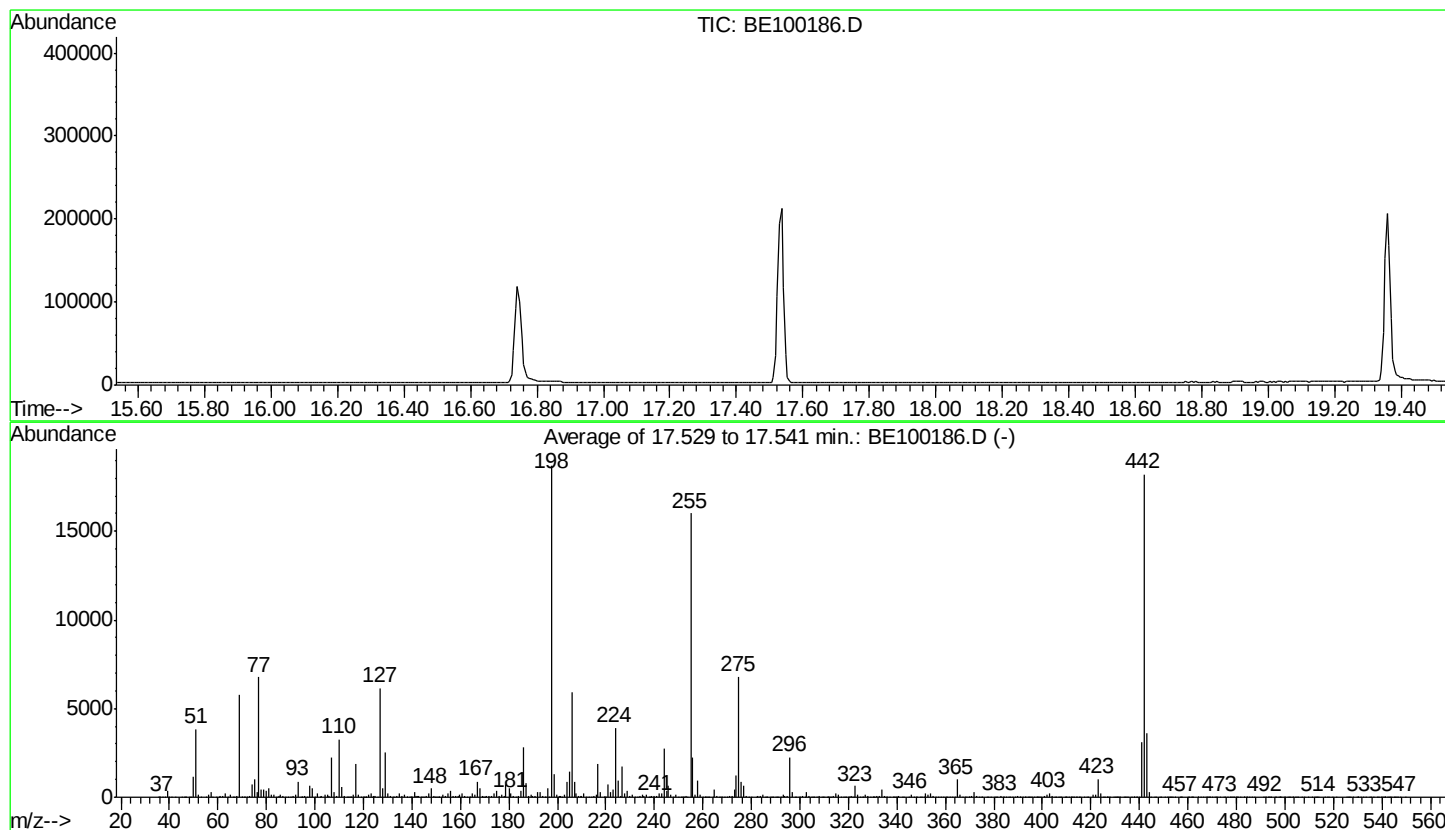

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	3840	PASS
68	69	0.00	2	1.1	64	PASS
69	198	0.00	100	31.1	5809	PASS
70	69	0.00	2	0.3	18	PASS
127	198	10	80	33.0	6171	PASS
197	198	0.00	2	0.2	38	PASS
198	198	100	100	100.0	18704	PASS
199	198	5	9	6.9	1296	PASS
275	198	10	60	36.3	6798	PASS
365	198	1	100	5.3	995	PASS
441	198	0.01	100	16.6	3110	PASS
442	198	50	100	97.3	18198	PASS
443	442	15	24	19.7	3590	PASS