


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062819\
 Data File : BE100225.D
 Acq On : 28 Jun 2019 8:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

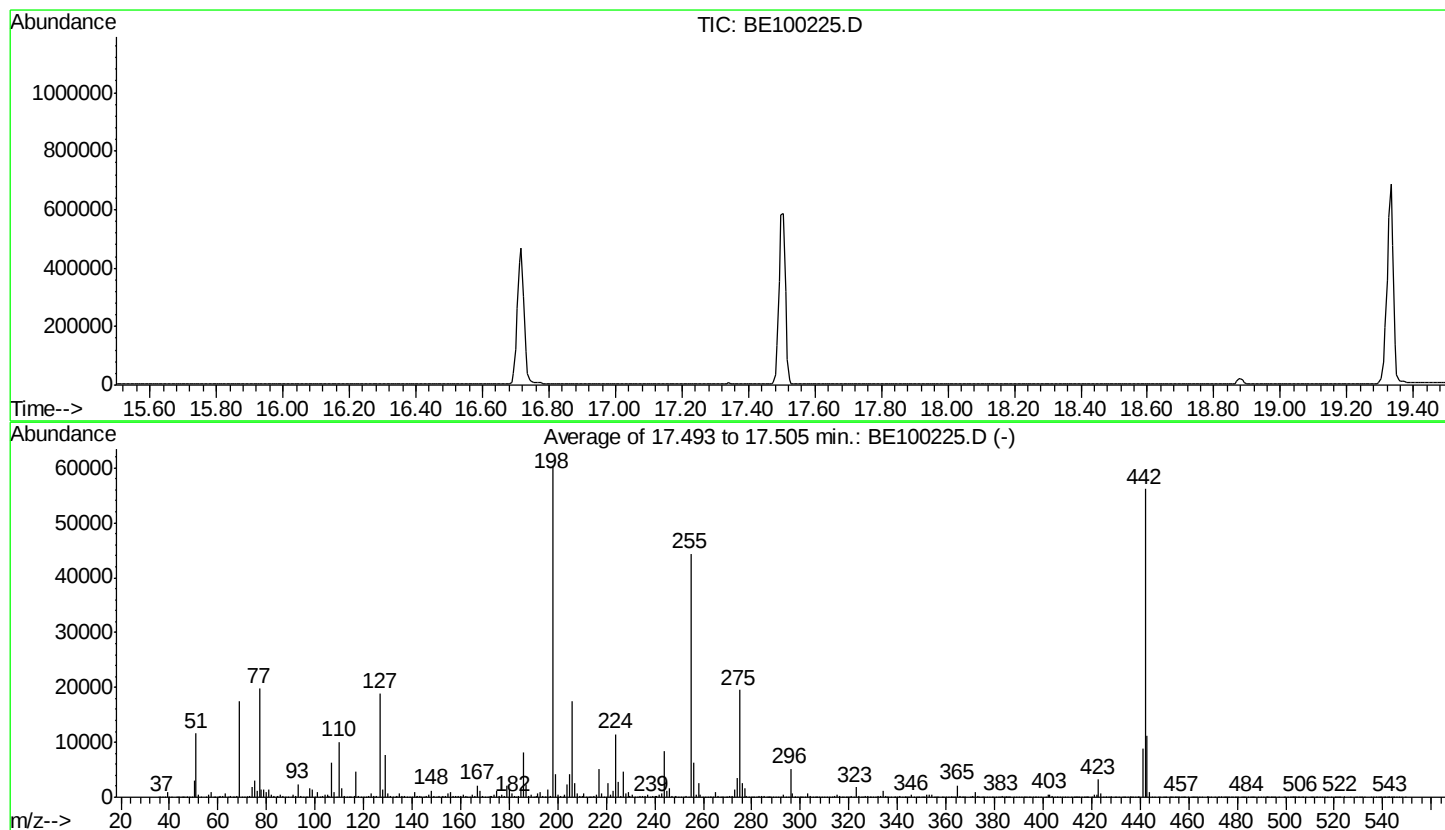

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.1	11554	PASS
68	69	0.00	2	1.8	314	PASS
69	198	0.00	100	29.0	17492	PASS
70	69	0.00	2	0.5	96	PASS
127	198	10	80	31.2	18820	PASS
197	198	0.00	2	0.3	152	PASS
198	198	100	100	100.0	60410	PASS
199	198	5	9	6.9	4193	PASS
275	198	10	60	32.3	19518	PASS
365	198	1	100	3.6	2172	PASS
441	198	0.01	100	14.8	8956	PASS
442	198	50	100	92.9	56127	PASS
443	442	15	24	19.8	11124	PASS