


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062819\
 Data File : BE100239.D
 Acq On : 28 Jun 2019 17:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

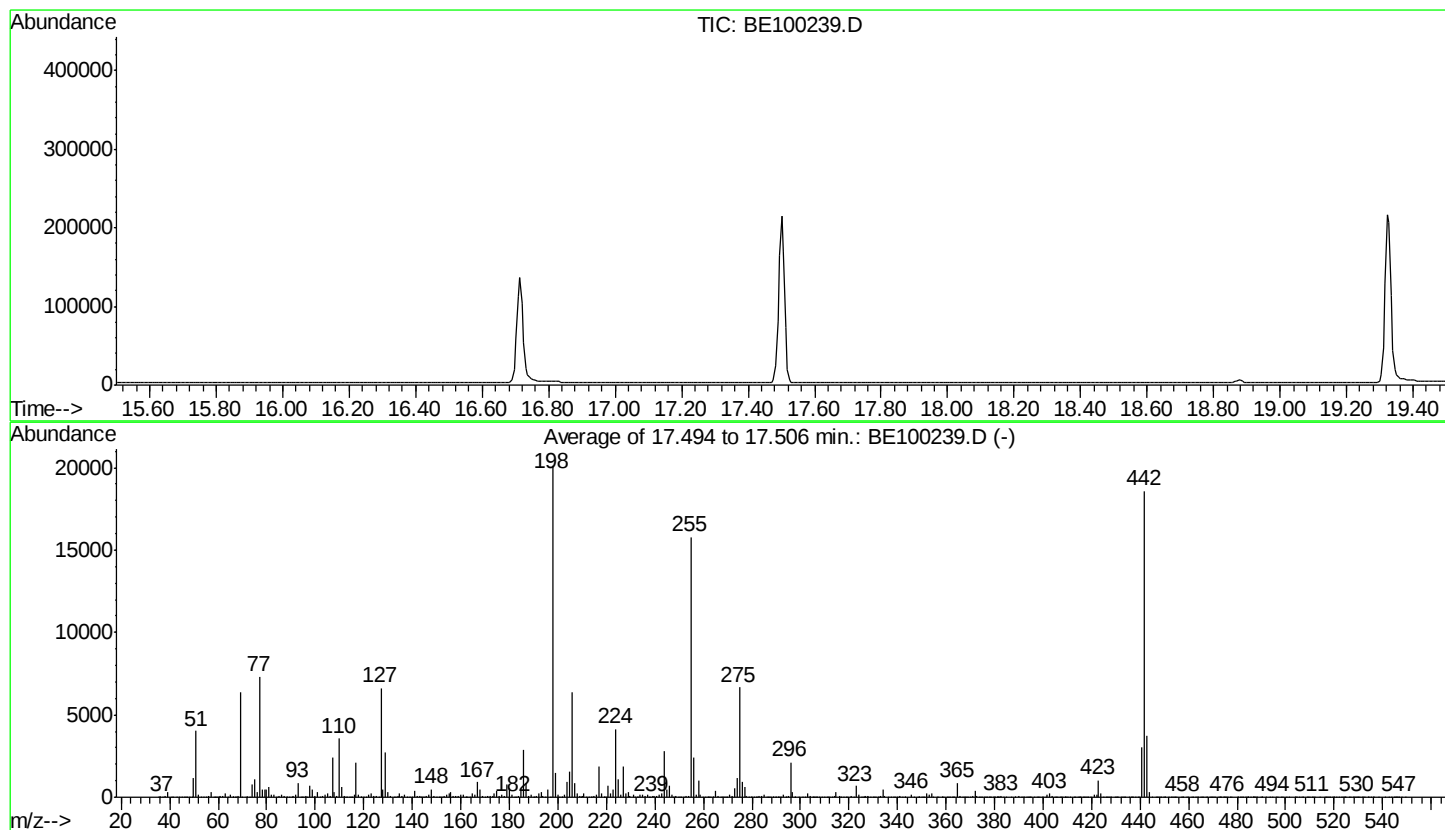

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.9	4012	PASS
68	69	0.00	2	1.7	106	PASS
69	198	0.00	100	31.5	6343	PASS
70	69	0.00	2	0.3	22	PASS
127	198	10	80	32.9	6616	PASS
197	198	0.00	2	0.1	18	PASS
198	198	100	100	100.0	20122	PASS
199	198	5	9	7.3	1465	PASS
275	198	10	60	33.0	6647	PASS
365	198	1	100	4.4	876	PASS
441	198	0.01	100	15.2	3050	PASS
442	198	50	100	92.4	18600	PASS
443	442	15	24	19.9	3707	PASS