
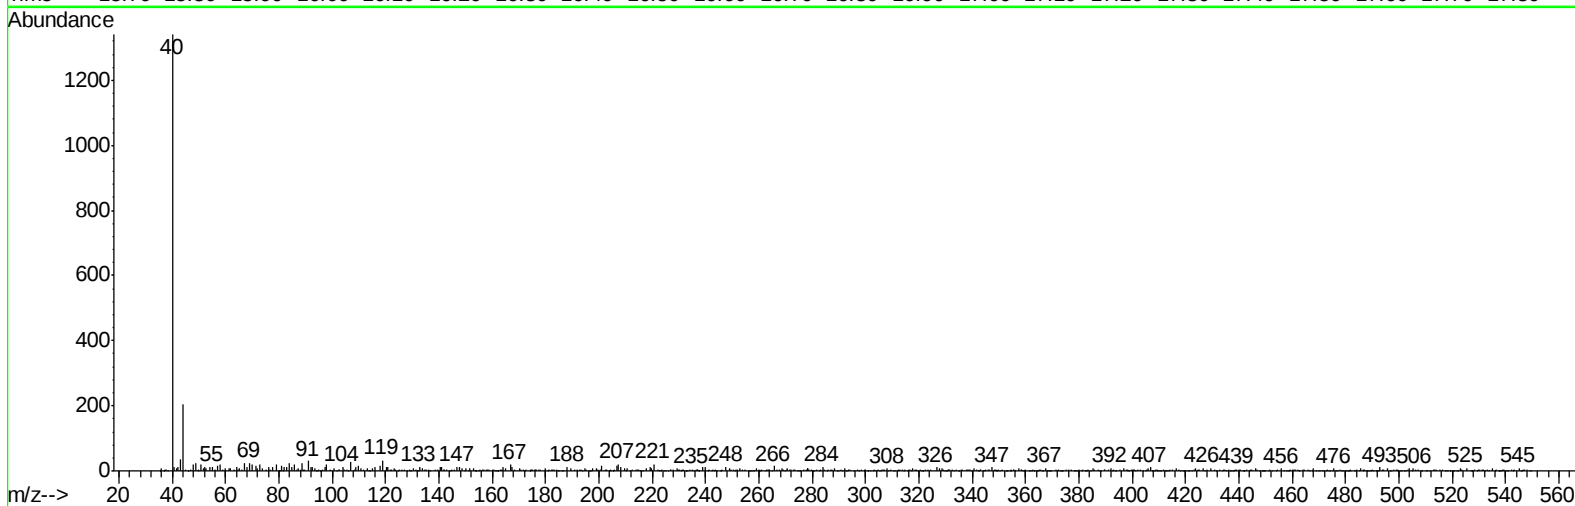


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070119\
 Data File : BE100258.D
 Acq On : 1 Jul 2019 10:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 09:14:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

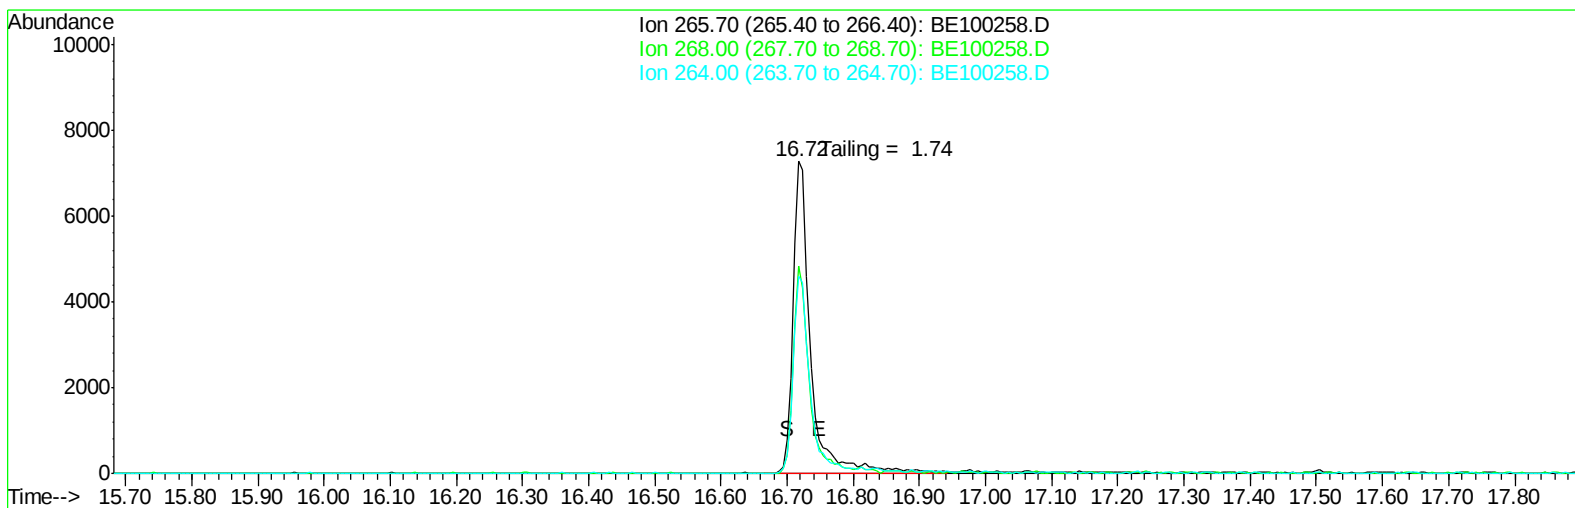

TIC: BE100258.D

(69) Pentachlorophenol (C)



12.129min (+0.042) 195.38ng

response 13

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	57.14
264.00	65.00	57.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070119\
Data File : BE100258.D
Acq On : 1 Jul 2019 10:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 09:14:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

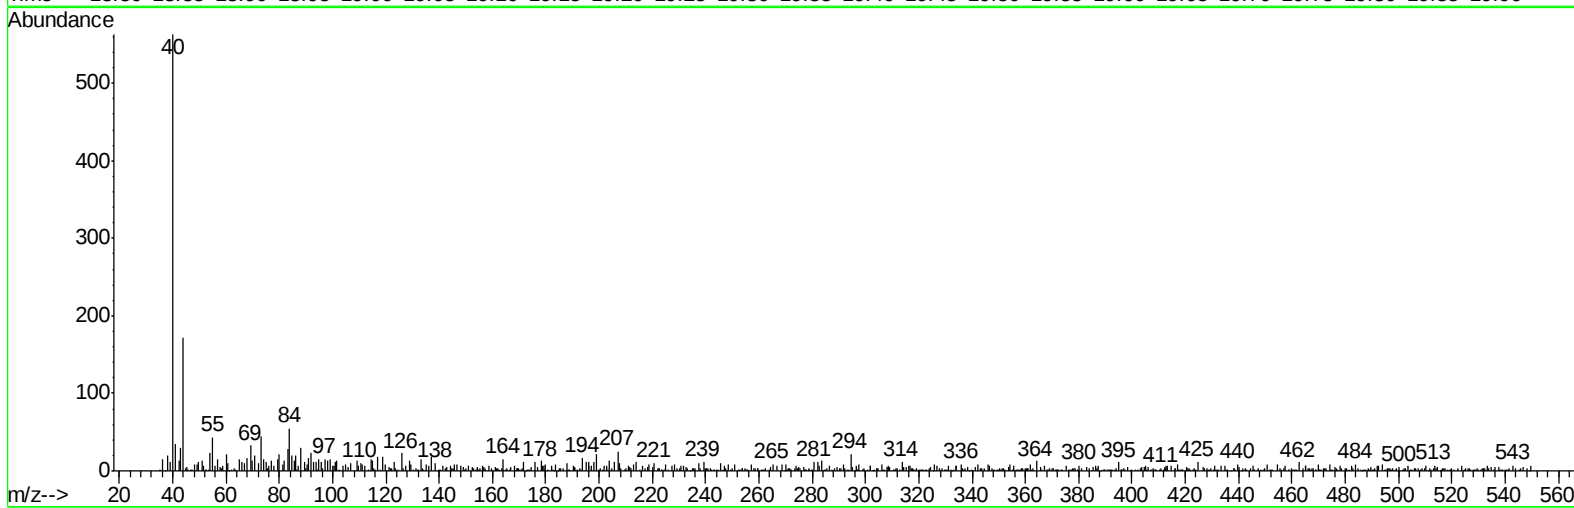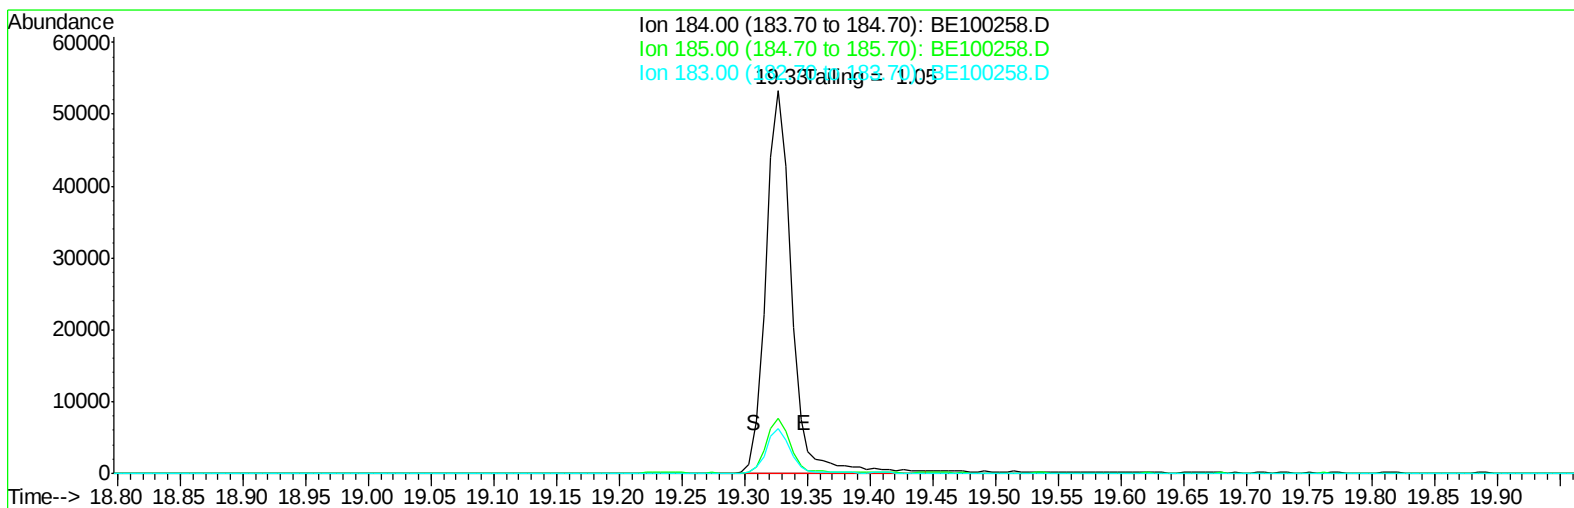

(76) Benzidine

14.550min (-0.040) 91.61ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	87.50#
183.00	12.20	100.00#
0.00	0.00	0.00