


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070119\
 Data File : BE100277.D
 Acq On : 1 Jul 2019 23:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

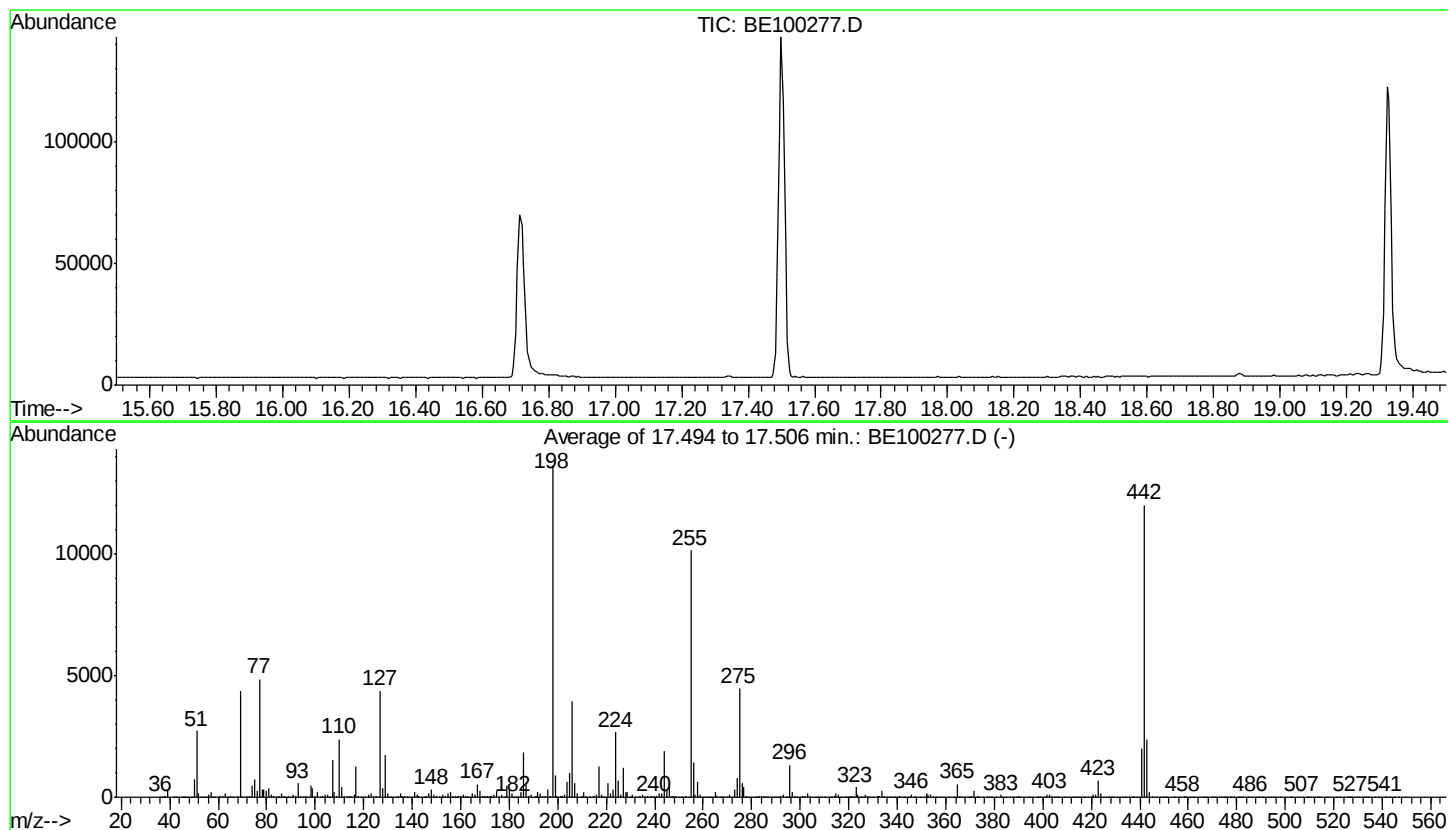

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.0	2720	PASS
68	69	0.00	2	1.5	64	PASS
69	198	0.00	100	31.9	4347	PASS
70	69	0.00	2	0.9	37	PASS
127	198	10	80	32.1	4367	PASS
197	198	0.00	2	0.3	46	PASS
198	198	100	100	100.0	13620	PASS
199	198	5	9	6.5	879	PASS
275	198	10	60	32.8	4462	PASS
365	198	1	100	4.0	550	PASS
441	198	0.01	100	14.7	2003	PASS
442	198	50	100	88.1	12003	PASS
443	442	15	24	19.7	2361	PASS