


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE070219\
Data File : BE100303.D
Acq On : 2 Jul 2019 15:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 14:06:53 2019

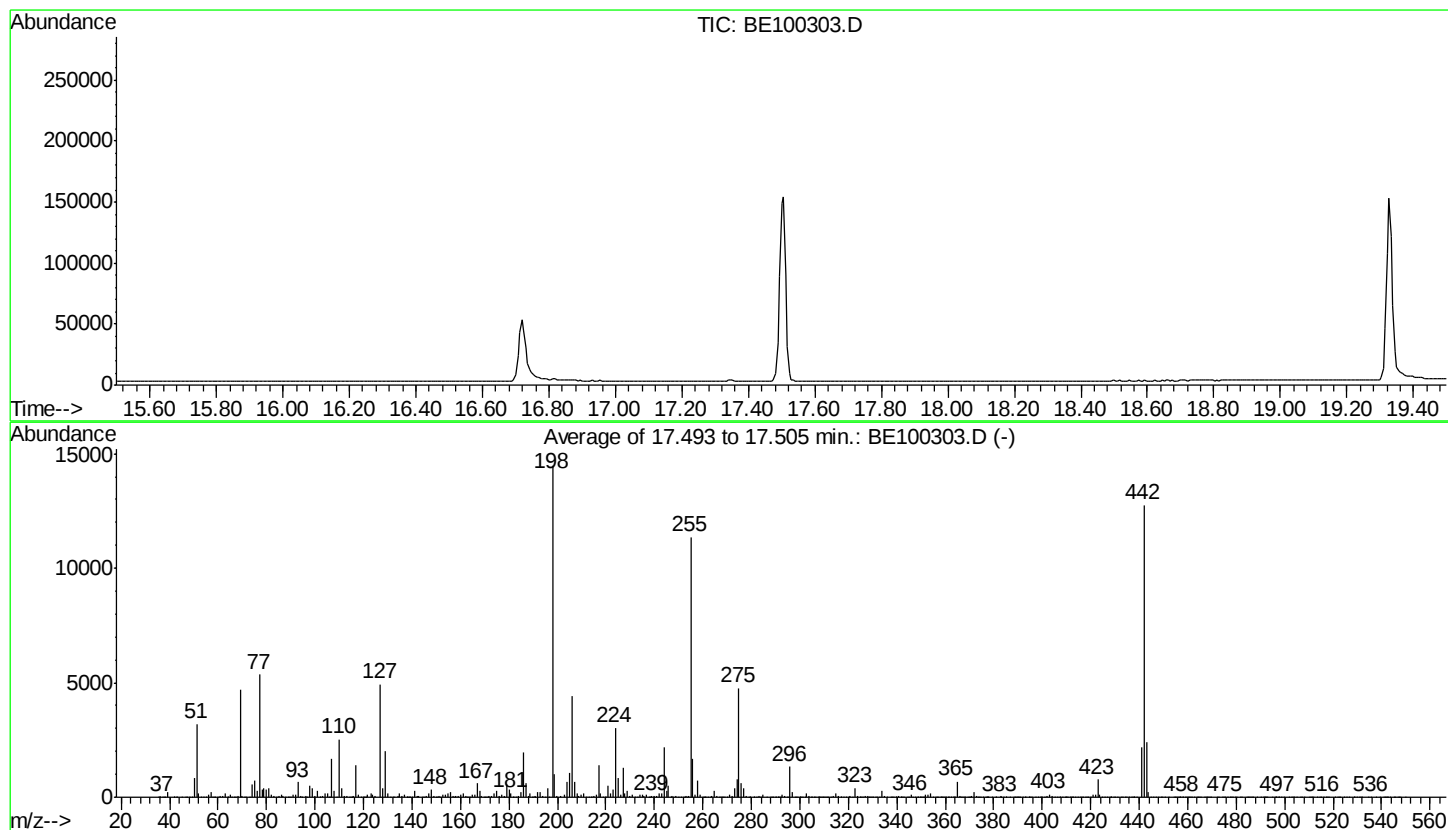

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	3200	PASS
68	69	0.00	2	1.6	77	PASS
69	198	0.00	100	32.6	4716	PASS
70	69	0.00	2	0.6	30	PASS
127	198	10	80	34.2	4944	PASS
197	198	0.00	2	0.2	26	PASS
198	198	100	100	100.0	14477	PASS
199	198	5	9	6.9	1006	PASS
275	198	10	60	33.0	4779	PASS
365	198	1	100	4.7	680	PASS
441	198	0.01	100	15.1	2185	PASS
442	198	50	100	88.1	12756	PASS
443	442	15	24	18.7	2391	PASS