


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070319\
 Data File : BE100322.D
 Acq On : 3 Jul 2019 11:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

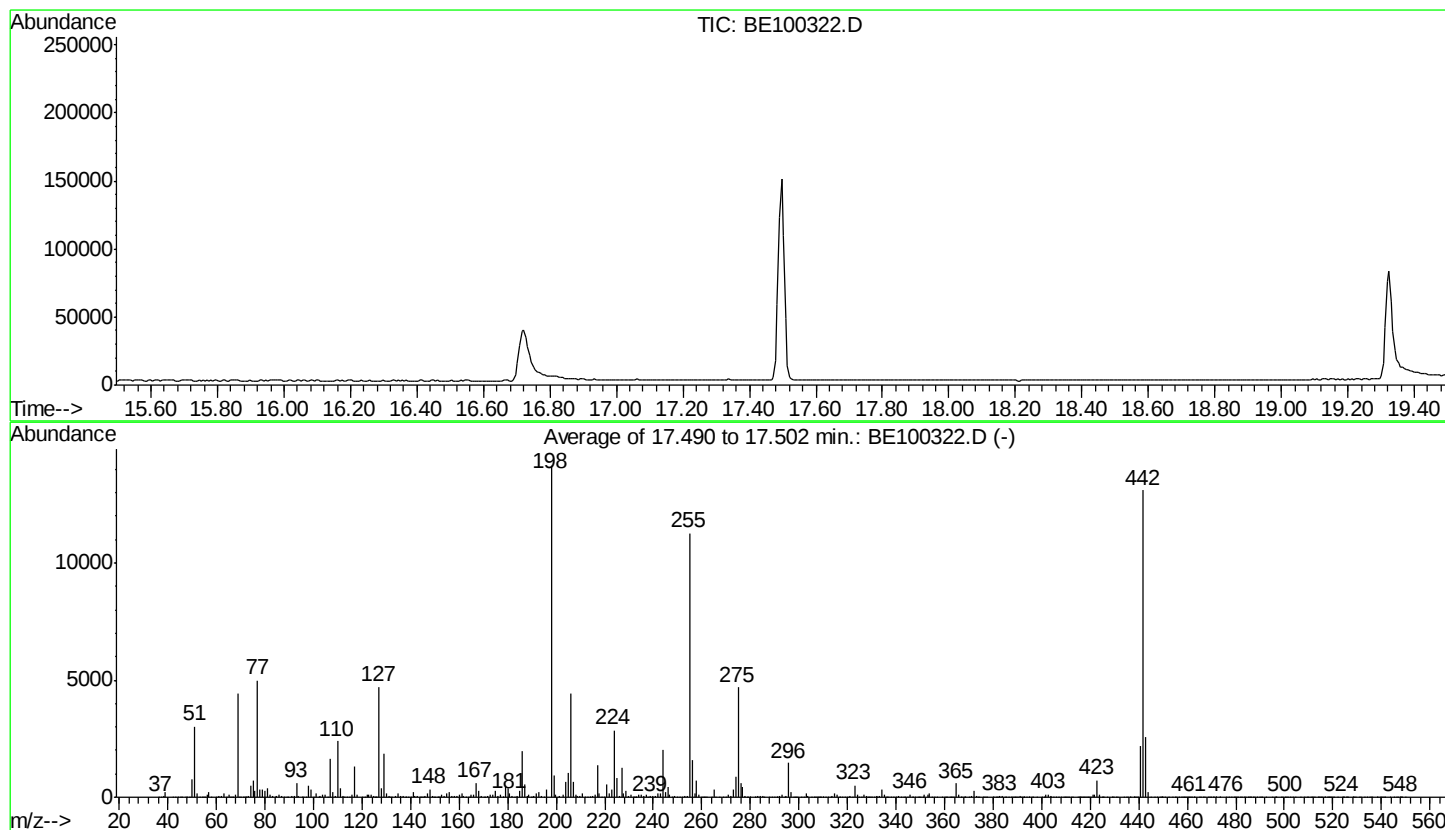

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	3021	PASS
68	69	0.00	2	1.9	84	PASS
69	198	0.00	100	31.3	4426	PASS
70	69	0.00	2	0.3	14	PASS
127	198	10	80	33.4	4724	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14153	PASS
199	198	5	9	6.6	940	PASS
275	198	10	60	33.1	4683	PASS
365	198	1	100	4.2	595	PASS
441	198	0.01	100	15.6	2202	PASS
442	198	50	100	92.6	13112	PASS
443	442	15	24	19.5	2558	PASS