


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070319\
 Data File : BE100332.D
 Acq On : 3 Jul 2019 17:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

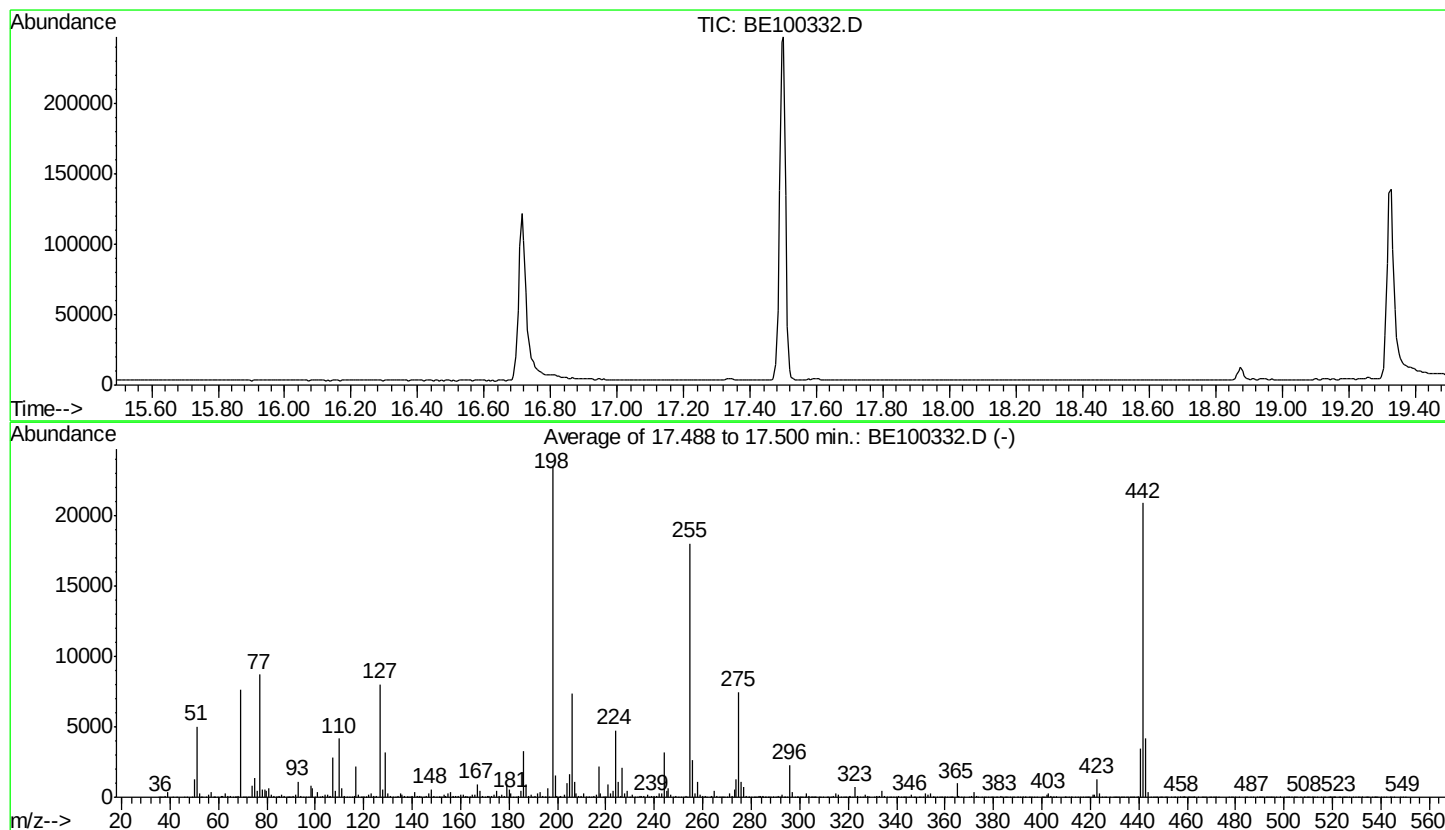

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	5039	PASS
68	69	0.00	2	1.8	135	PASS
69	198	0.00	100	32.4	7632	PASS
70	69	0.00	2	0.6	44	PASS
127	198	10	80	34.0	8006	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23555	PASS
199	198	5	9	6.7	1575	PASS
275	198	10	60	31.7	7463	PASS
365	198	1	100	4.1	959	PASS
441	198	0.01	100	14.6	3439	PASS
442	198	50	100	88.7	20890	PASS
443	442	15	24	19.9	4158	PASS