

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 09 05:32:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

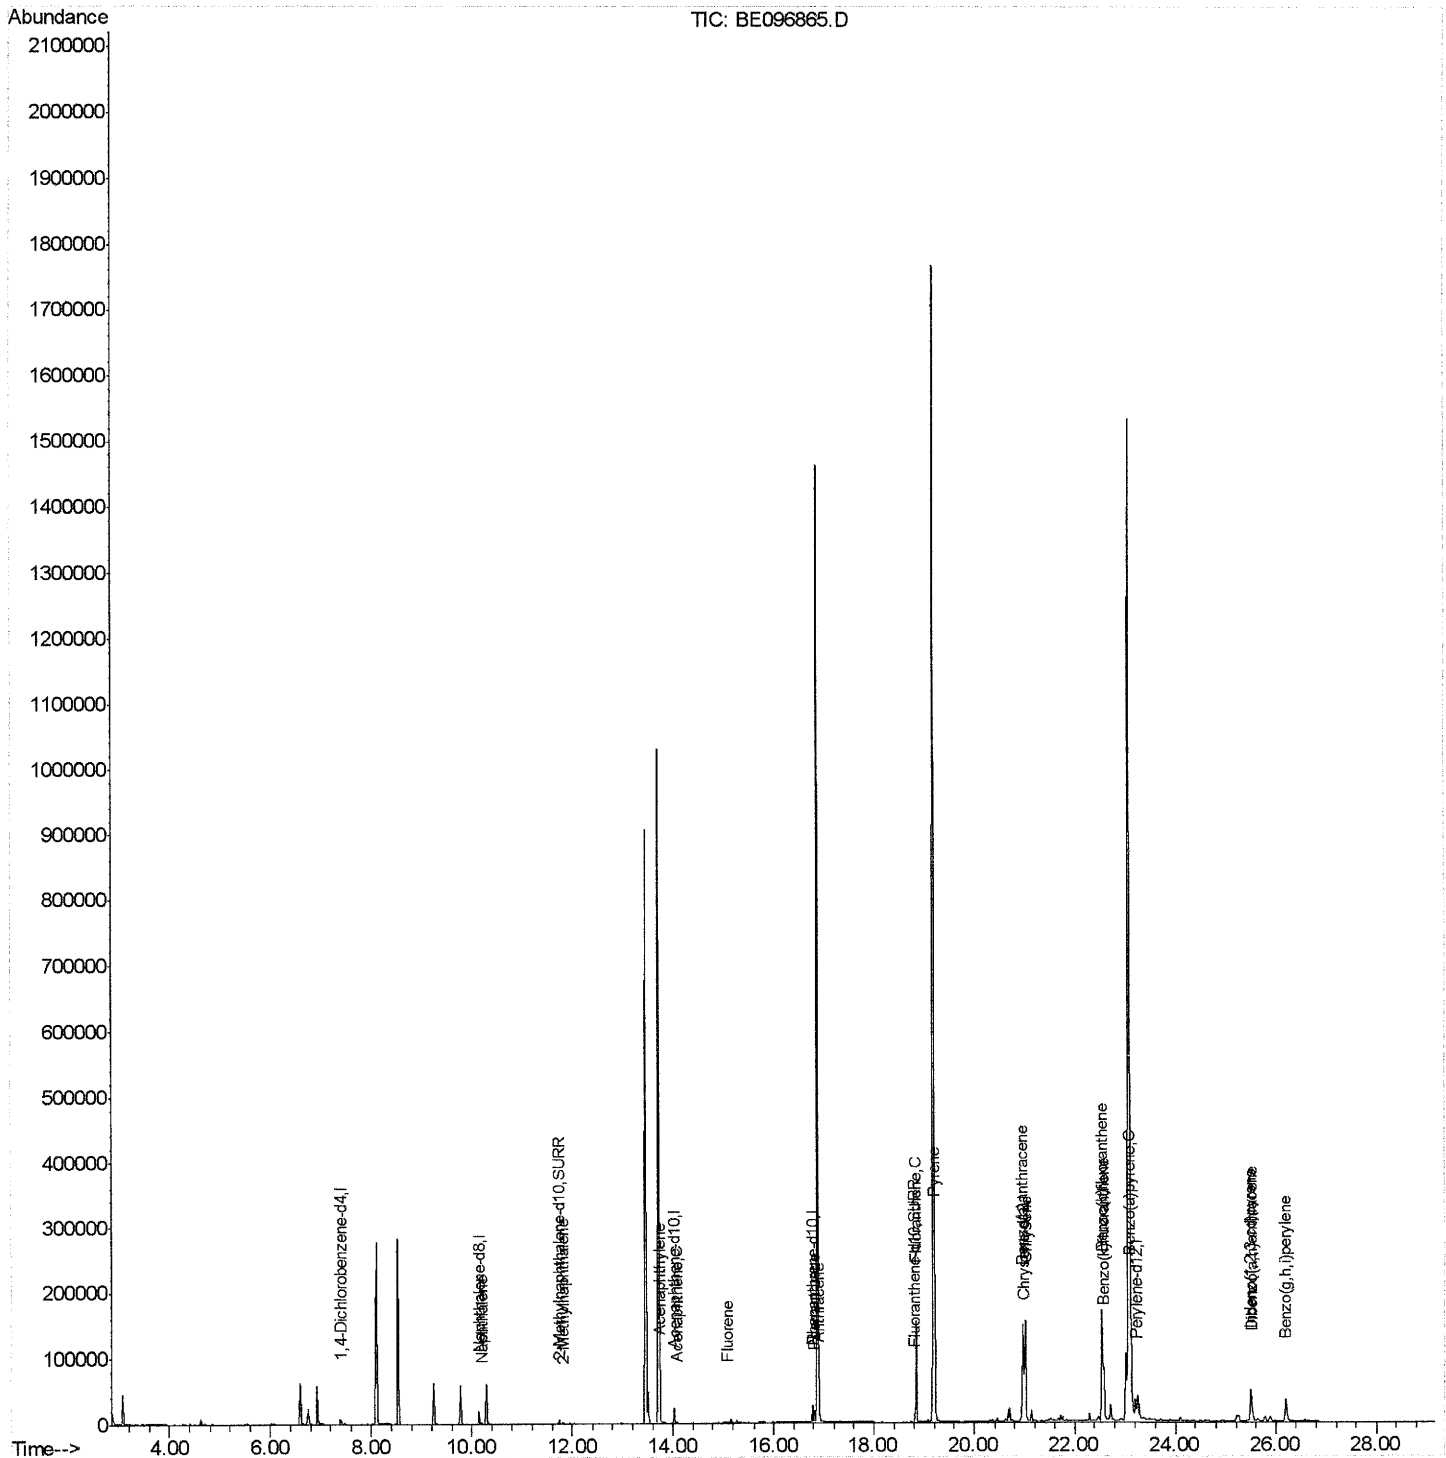

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

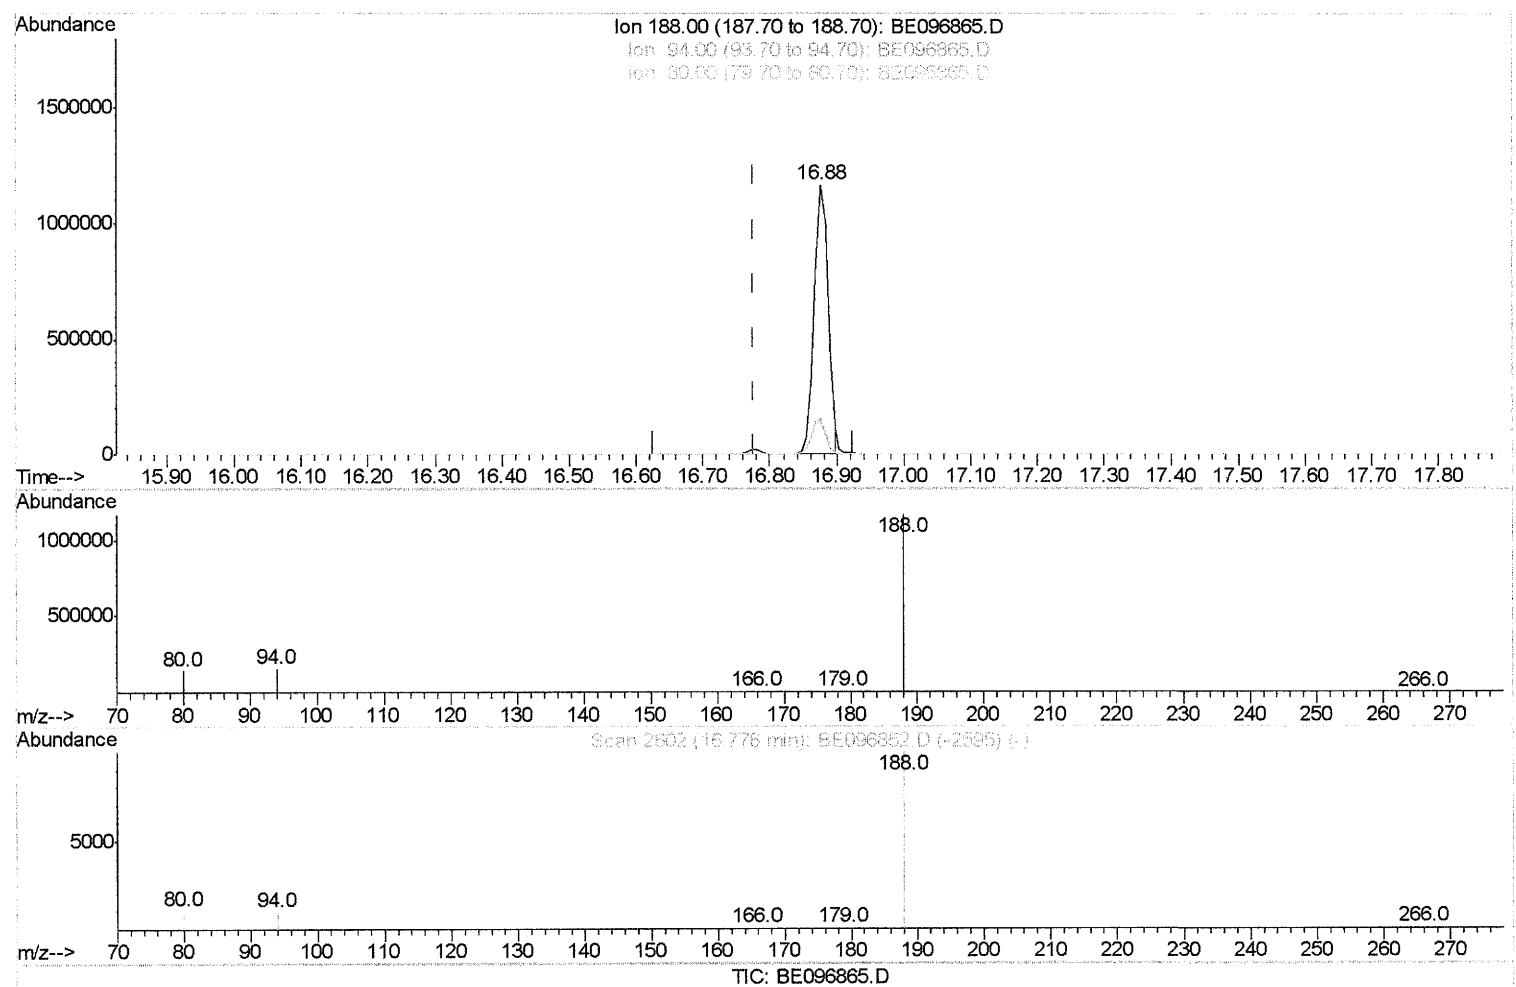

(10) Phenanthrene-d10 (I)
 16.875min (+0.099) 0.40ng/ul
 response 1653983

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.26#
80.00	11.80	12.12
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

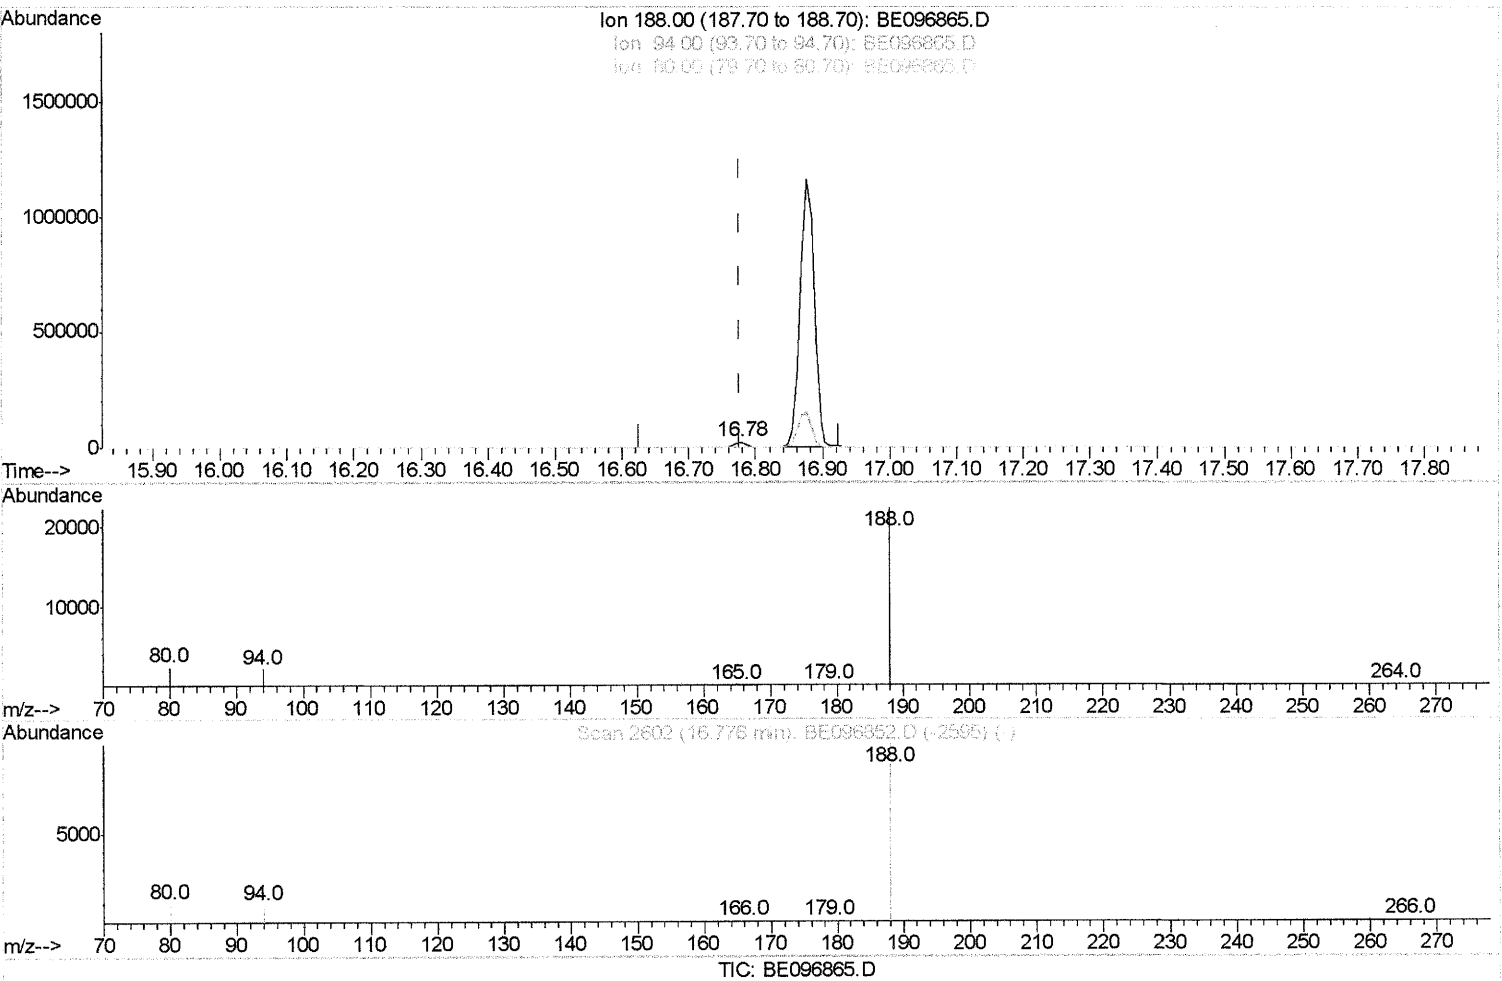

(10) Phenanthrene-d10 (I)

16.777min (+0.001) 0.40ng/ul m

SJ 7/11/18

response 30858

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.64
80.00	11.80	10.73
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
Data File : BE096865.D
Acq On : 6 Jul 2018 22:27
Operator : SJ/JU
Sample : J3721-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F1H24

Manual Integrations
APPROVED

Sohil
7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 06 16:55:25 2018
Response via : Initial Calibration

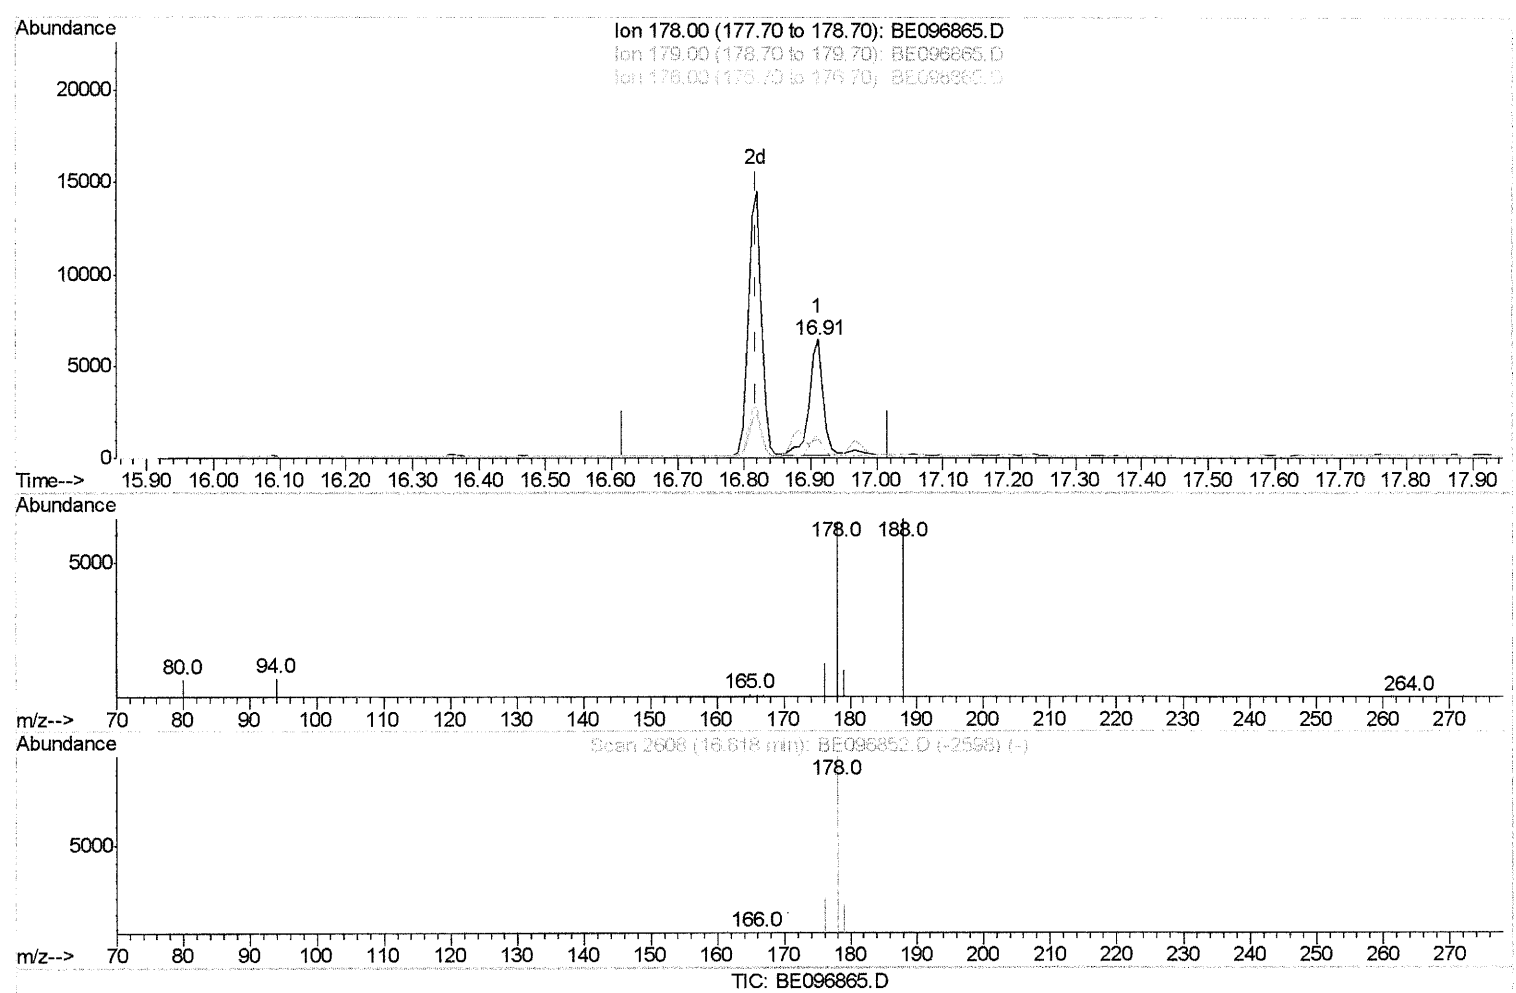

(12) Phenanthrene

16.910min (+0.092) 0.12ng/ul

response 9550

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.35#
176.00	17.00	19.99
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

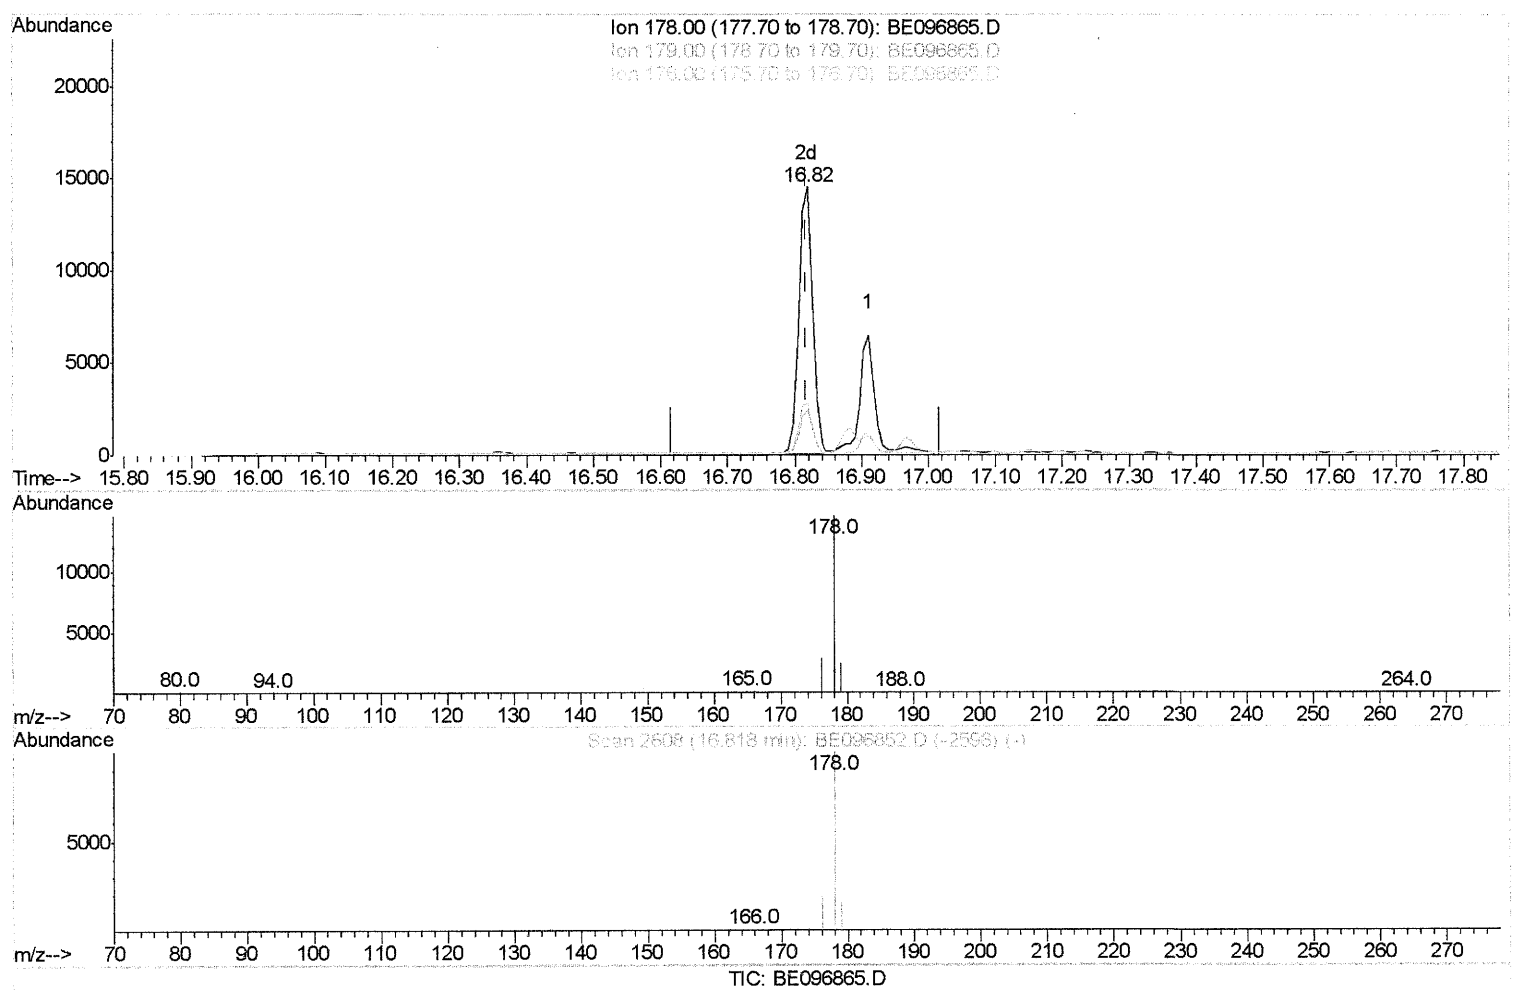

(12) Phenanthrene

16.819min (+0.001) 0.25ng/ul m

SJ 7/11/18

response 20228

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.73#
176.00	17.00	19.41
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

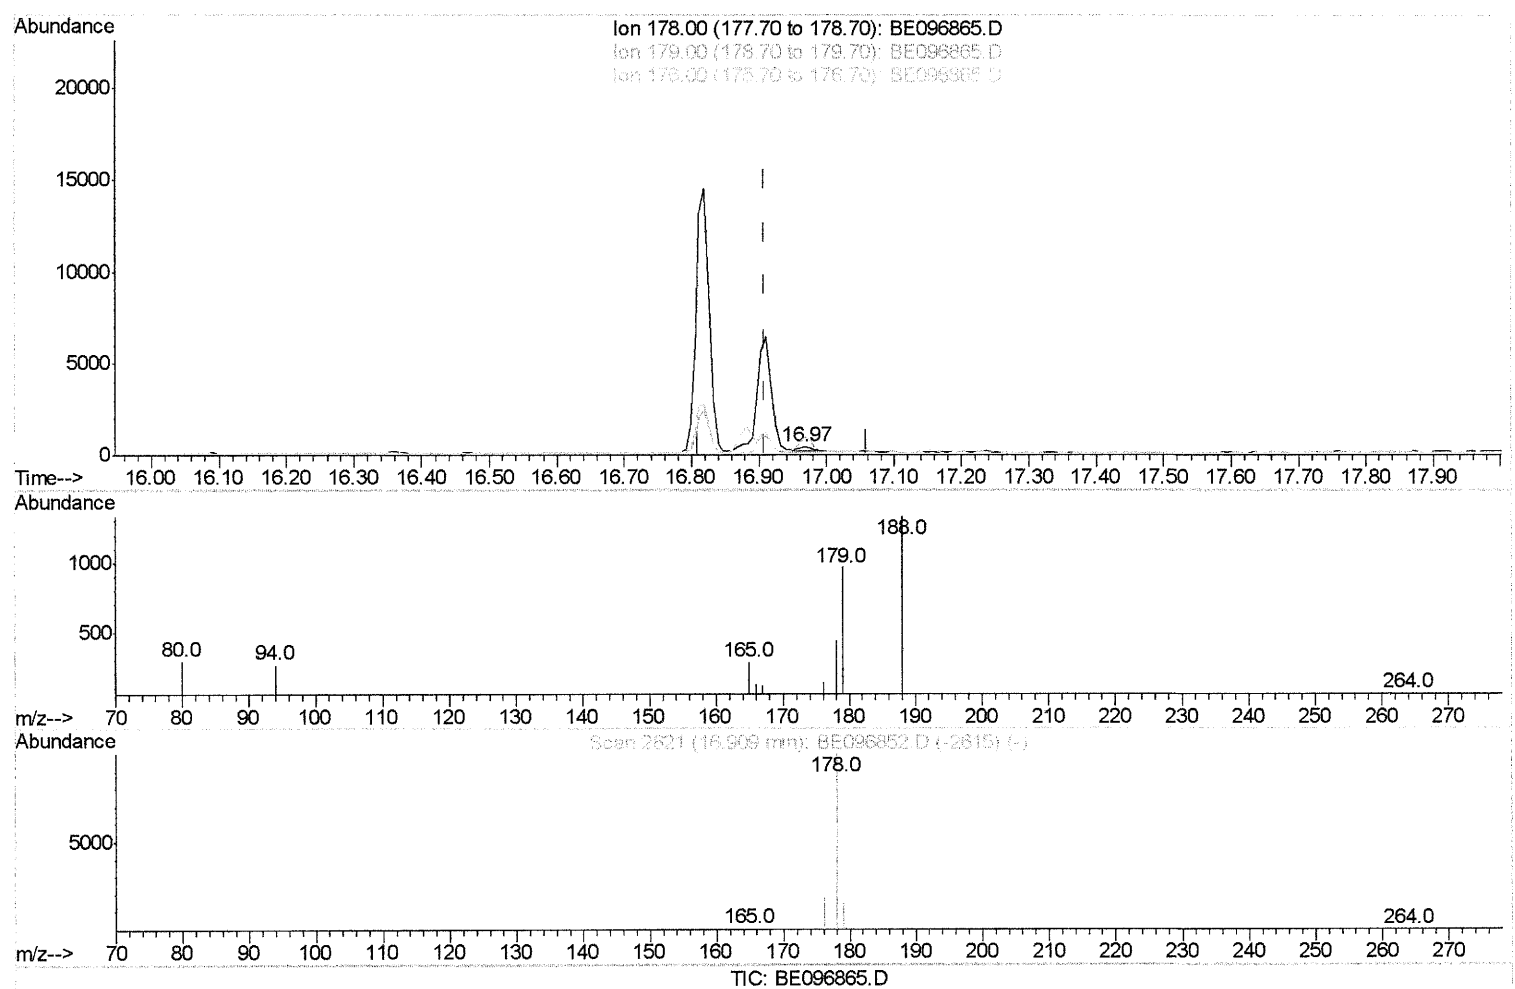

(13) Anthracene

16.967min (+0.057) 0.01ng/ul

response 505

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	219.32#
176.00	18.40	30.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

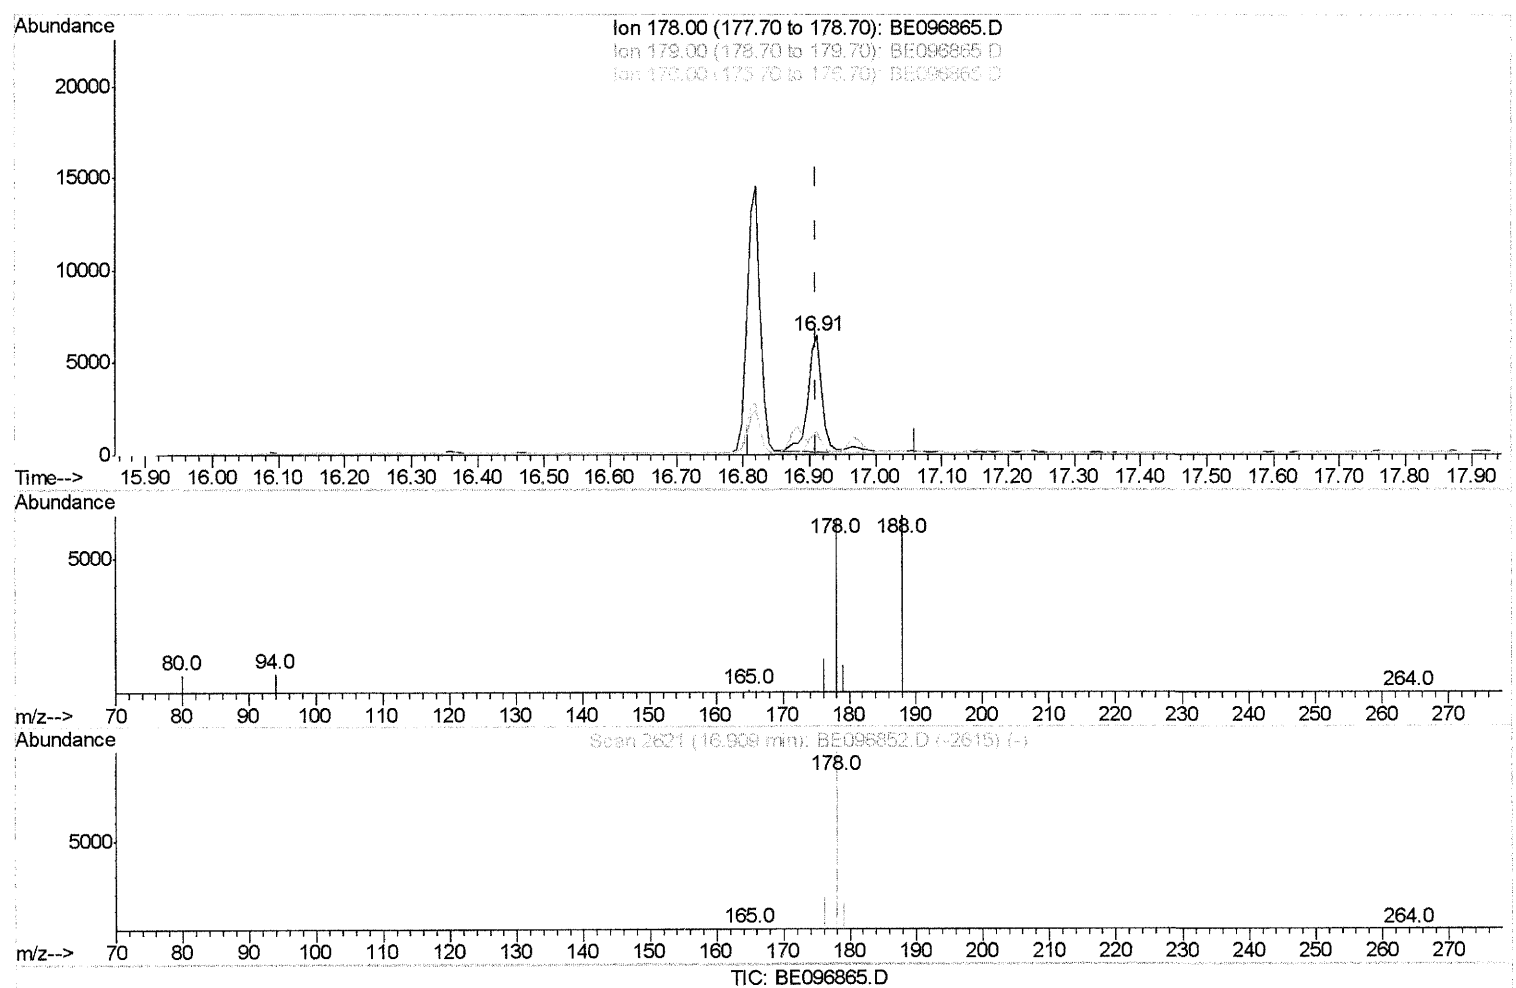

(13) Anthracene

16.910min (+0.001) 0.14ng/ul m

SJ 7/11/18

response 9336

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	16.35#
176.00	18.40	19.99
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

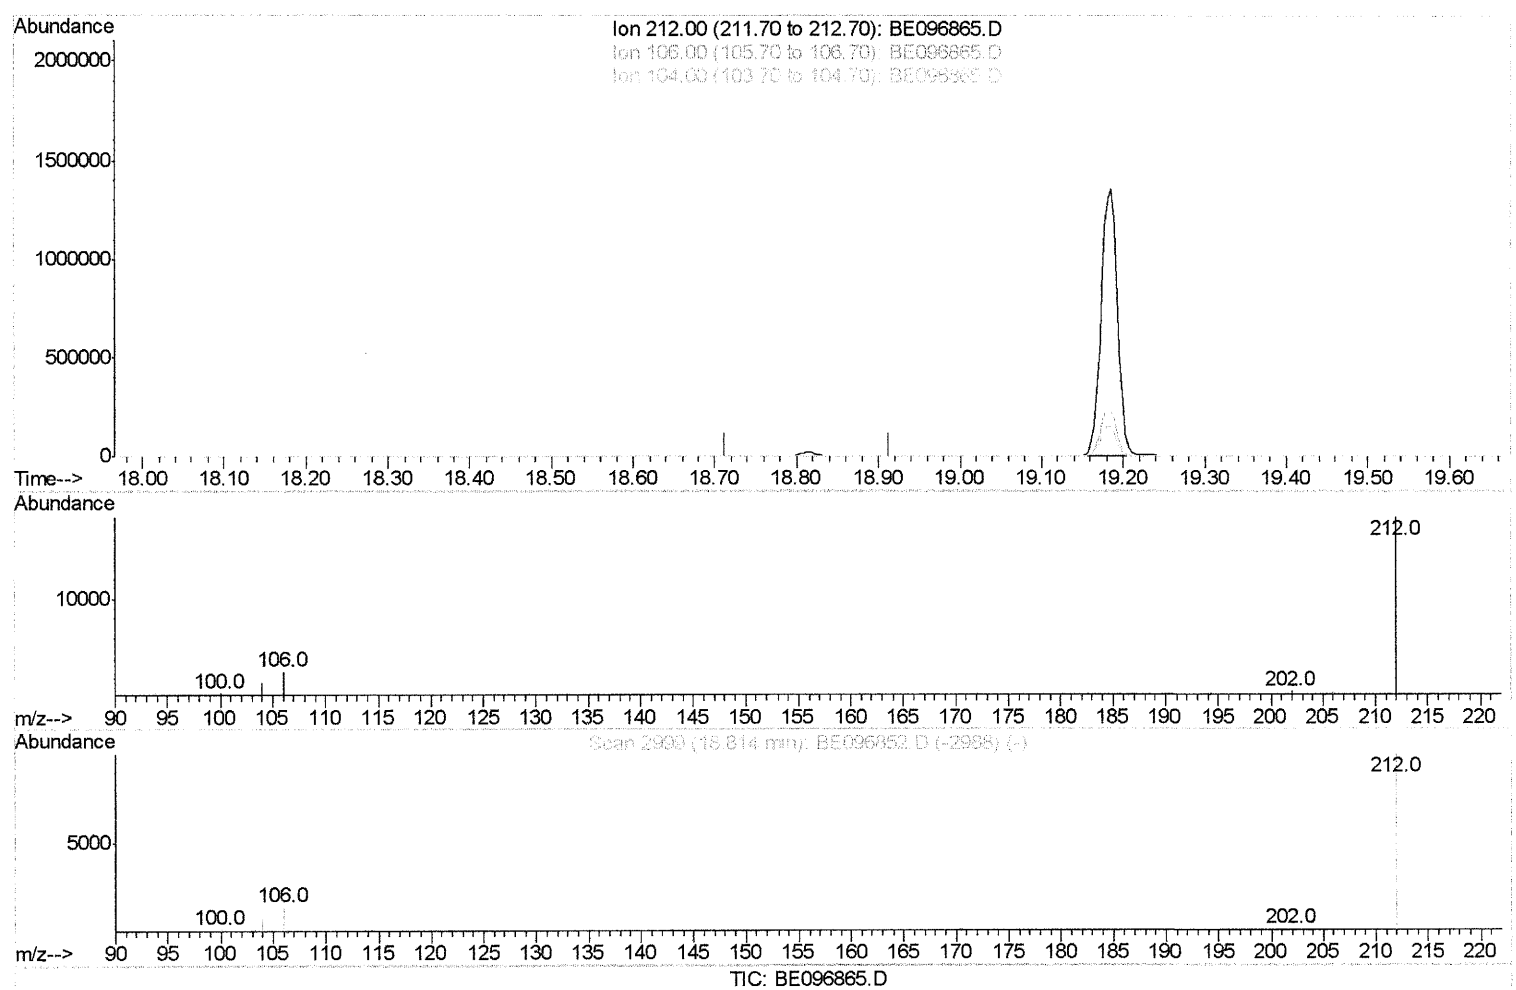

(14) Fluoranthene-d10 (SURR)

18.814min (-18.814) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

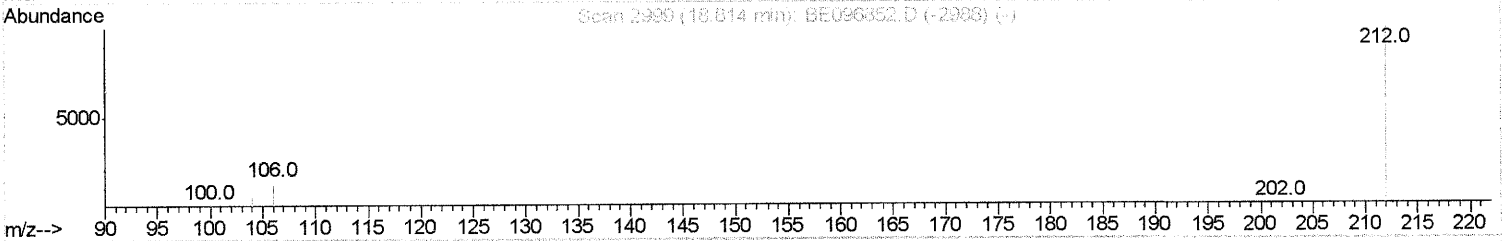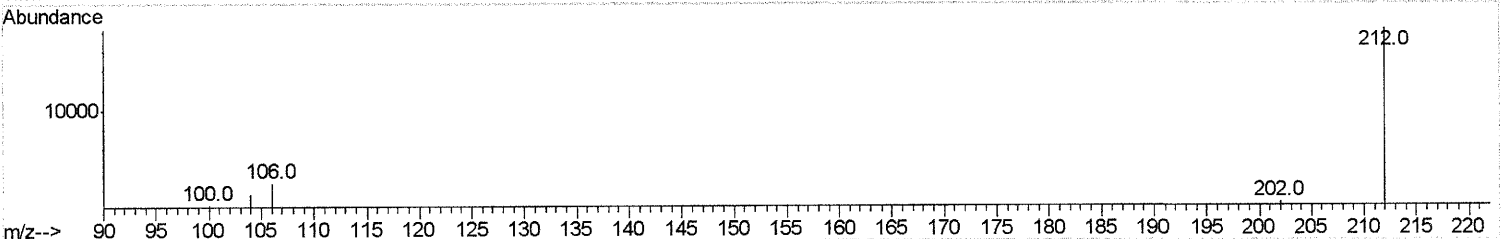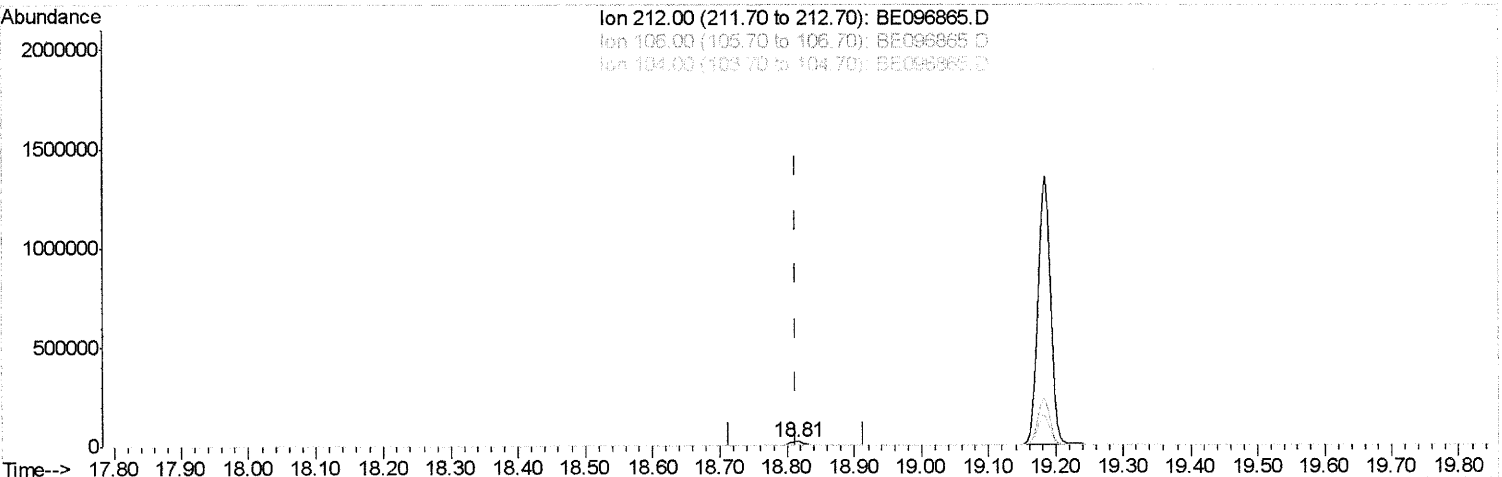

TIC: BE096865.D

(14) Fluoranthene-d10 (SURR)

18.814min (+0.000) 0.31ng/ul m

SJ 7/11/18

response 23889

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

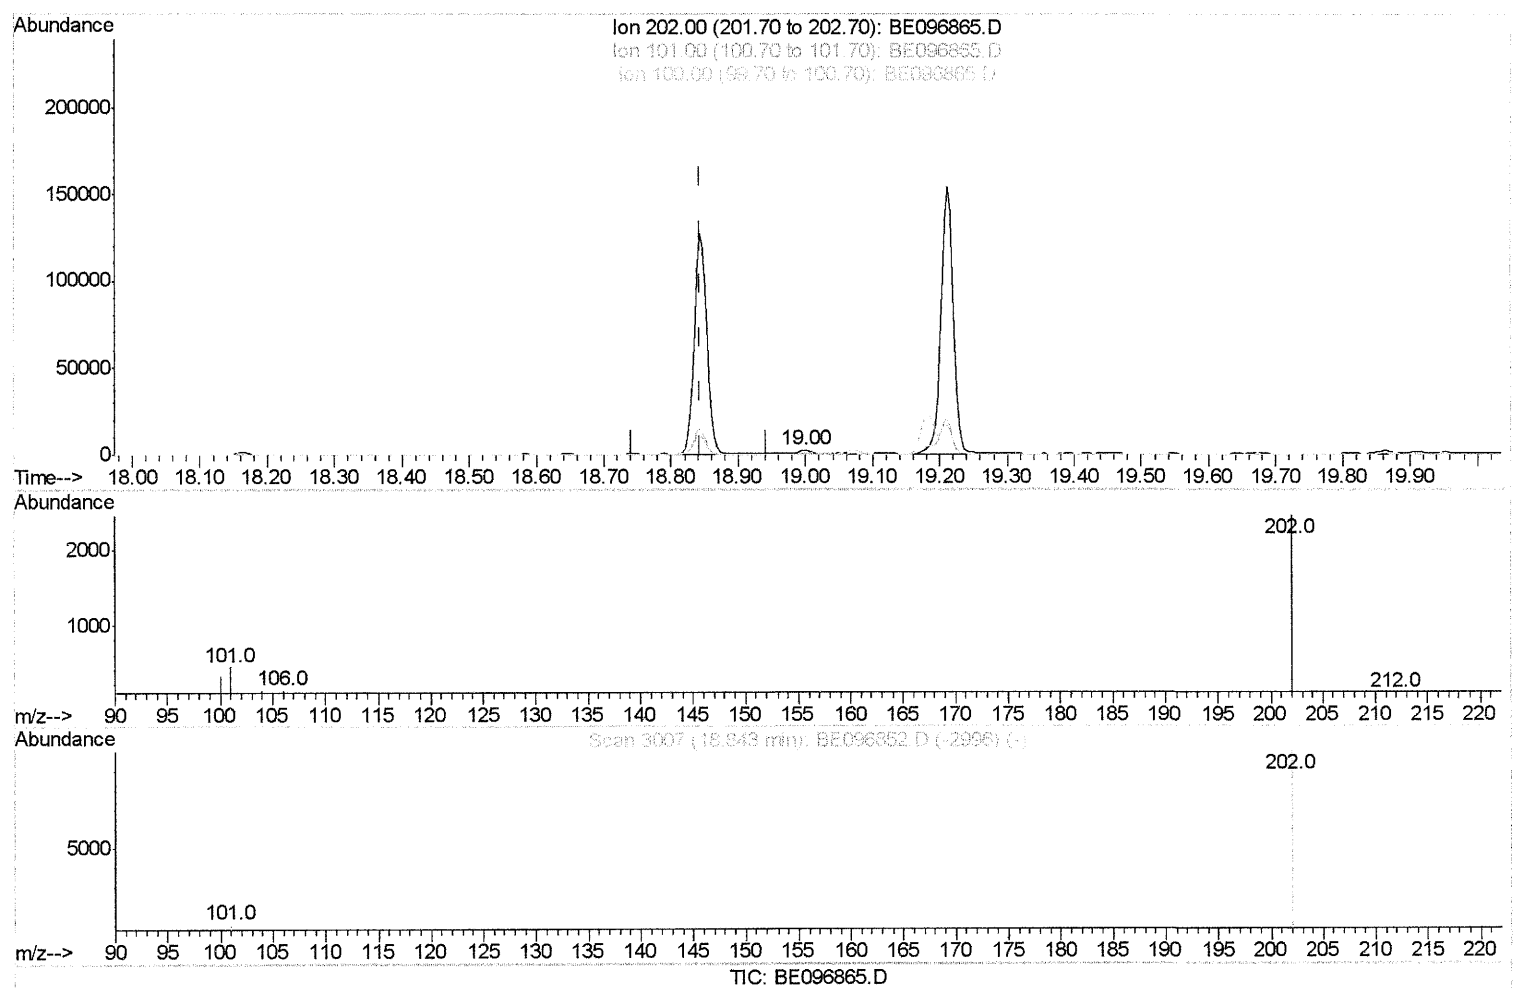

(15) Fluoranthene (C)

18.996min (+0.154) 0.03ng/ul

response 2689

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	17.97
100.00	19.50	12.81
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

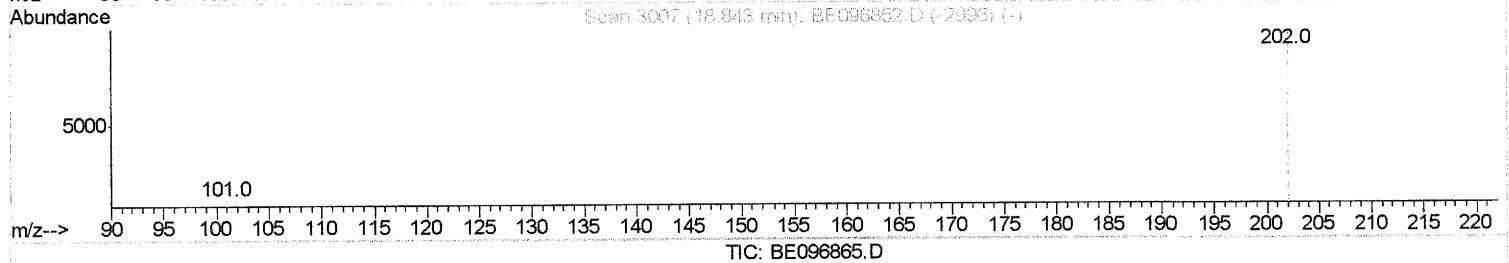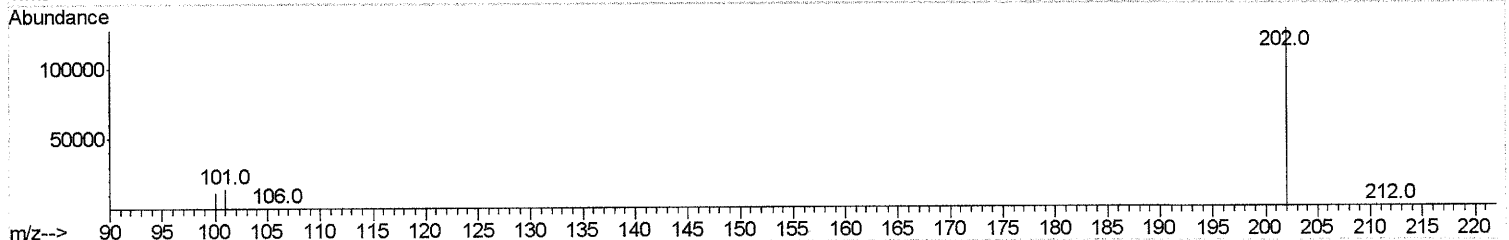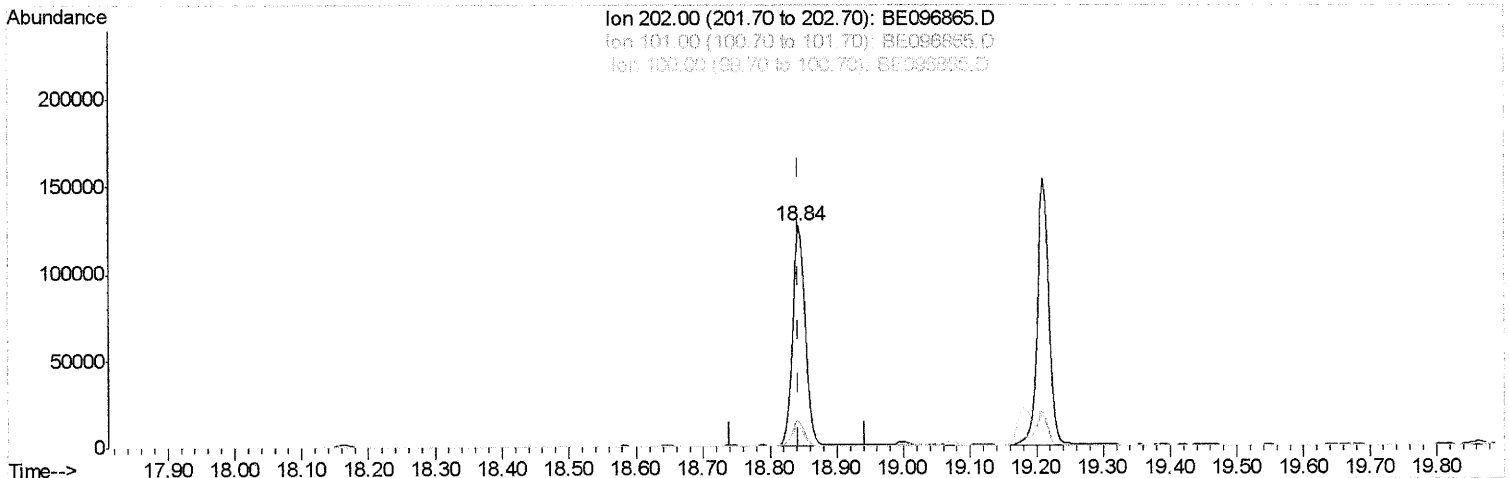

(15) Fluoranthene (C)

18.843min (+0.000) 1.92ng/ul m

SJ 7/11/18

response 162683

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	11.33
100.00	19.50	8.79
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

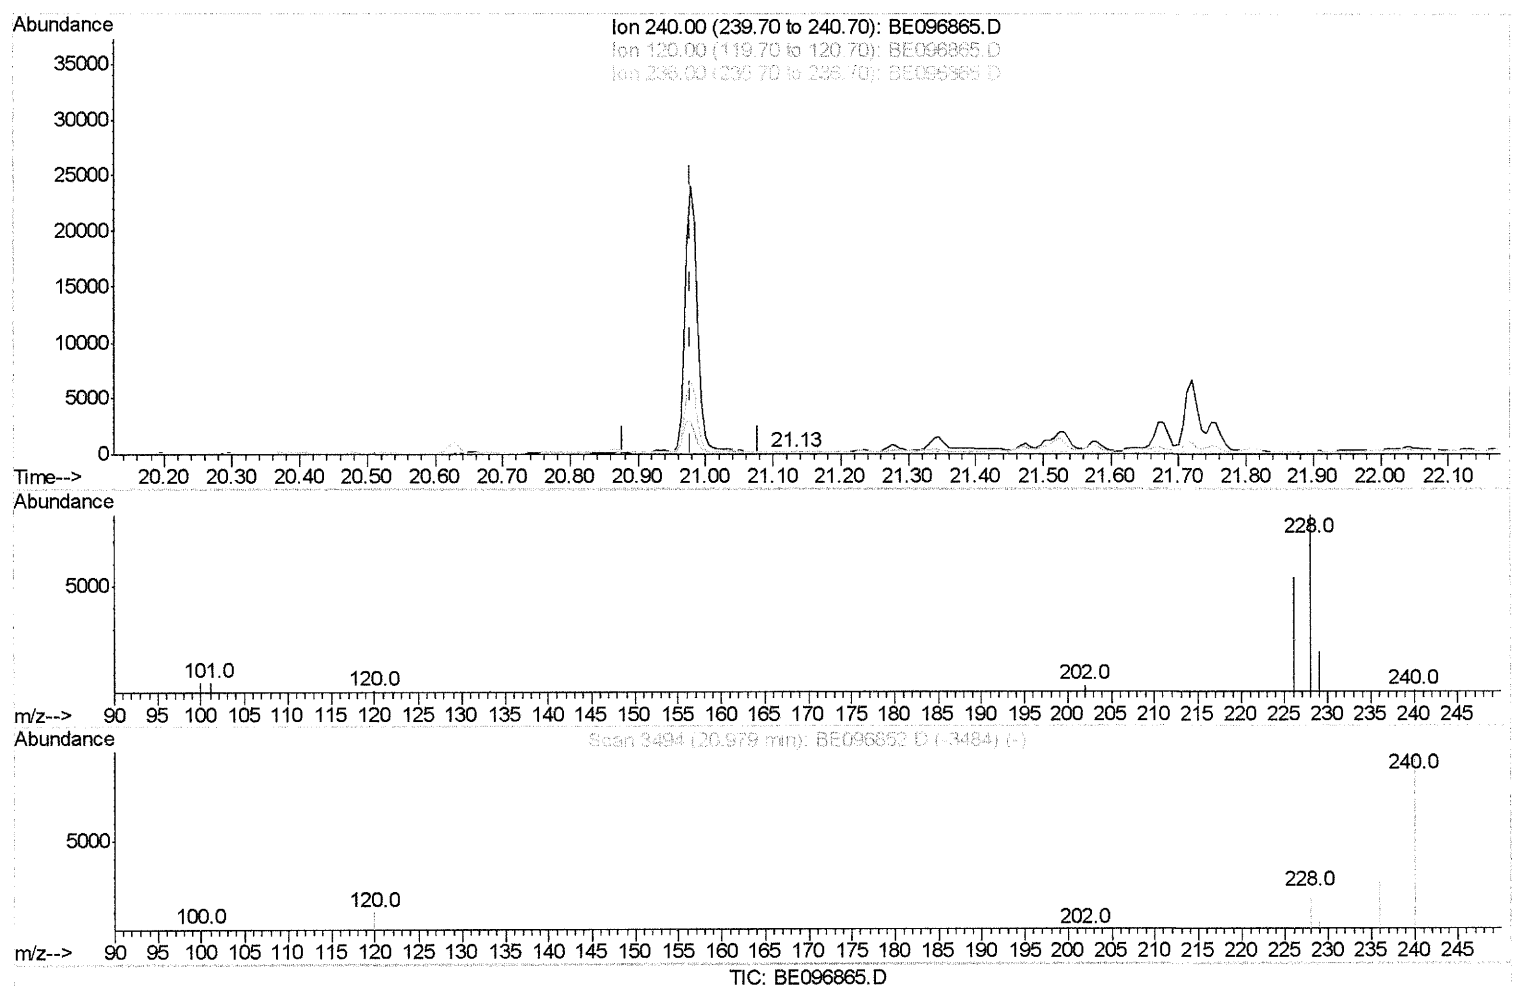

(16) Chrysene-d12 (I)

21.132min (+0.153) 0.40ng/ul

response 34

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	101.52#
236.00	34.90	70.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 03:30:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

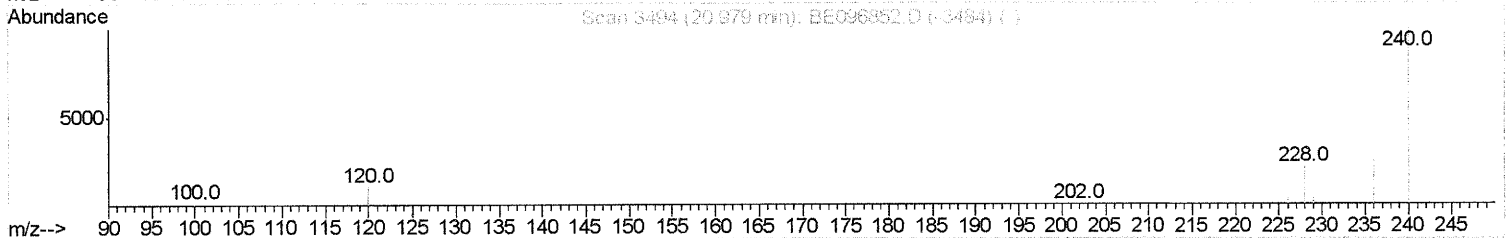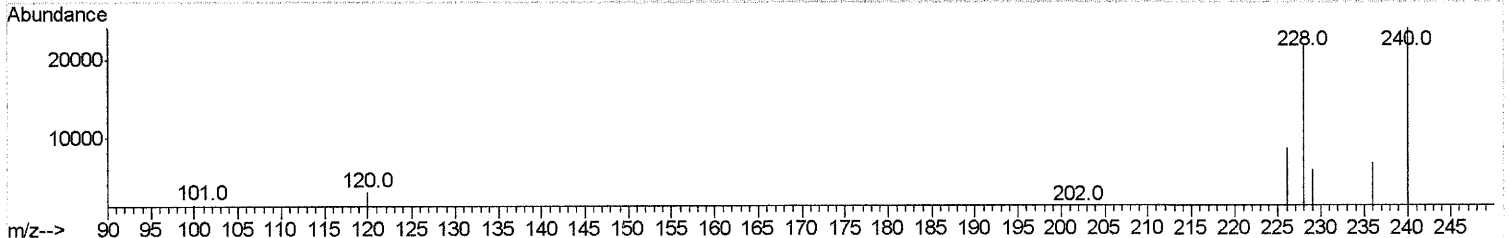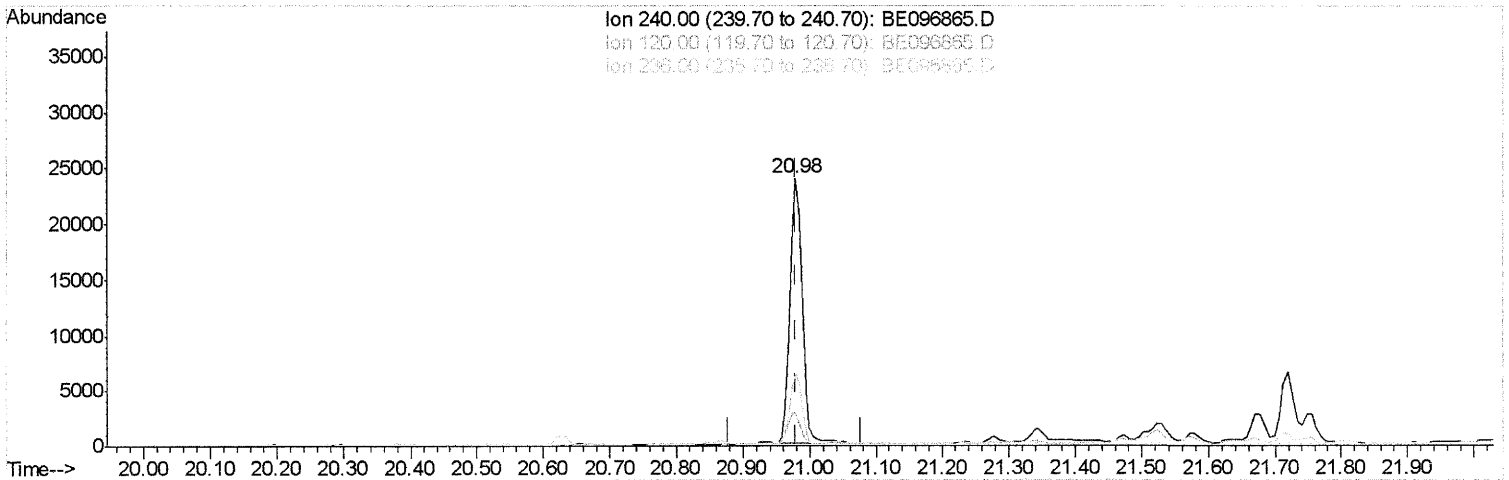

(16) Chrysene-d12 (I)

20.978min (-0.001) 0.40ng/ul m

SJ 7/11/18

response 30068

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.28#
236.00	34.90	27.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

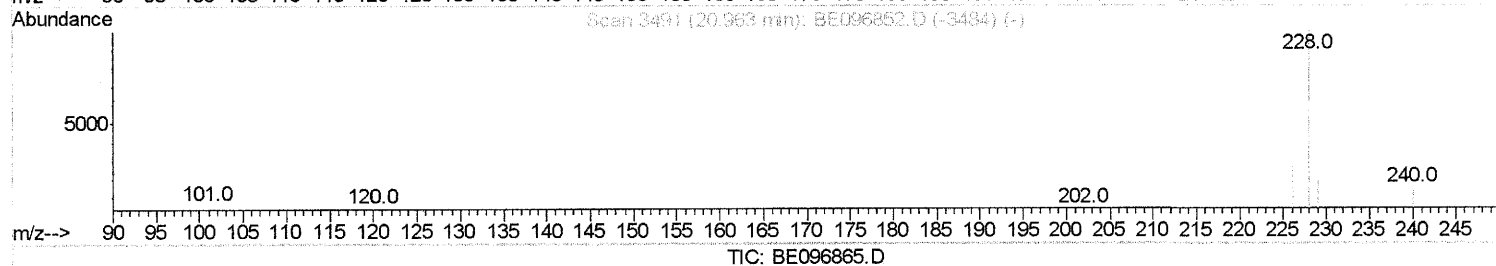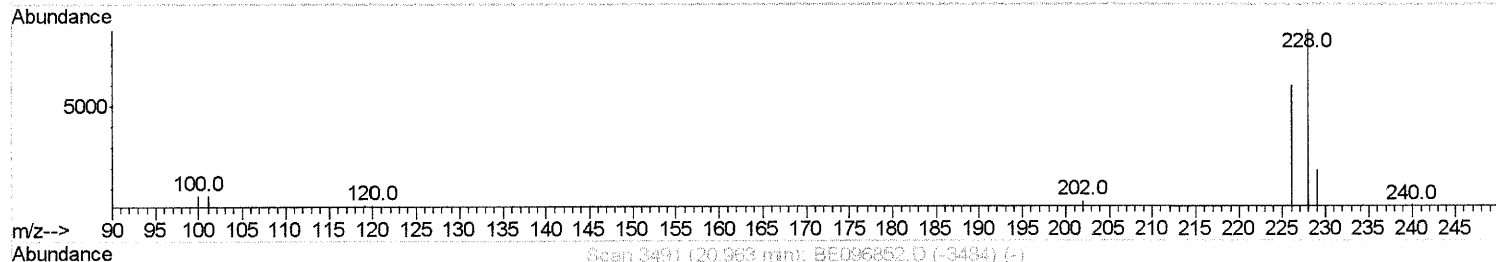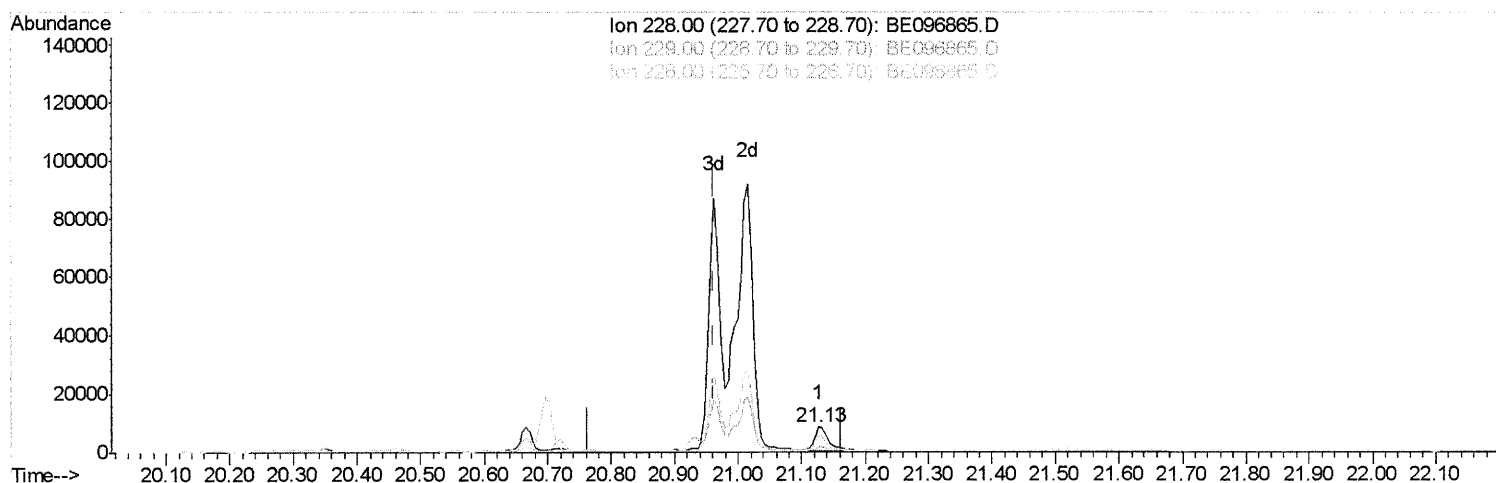

(18) Benzo(a)anthracene

21.127min (+0.164) 0.17ng/ul

response 12119

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	22.05#
226.00	21.30	68.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

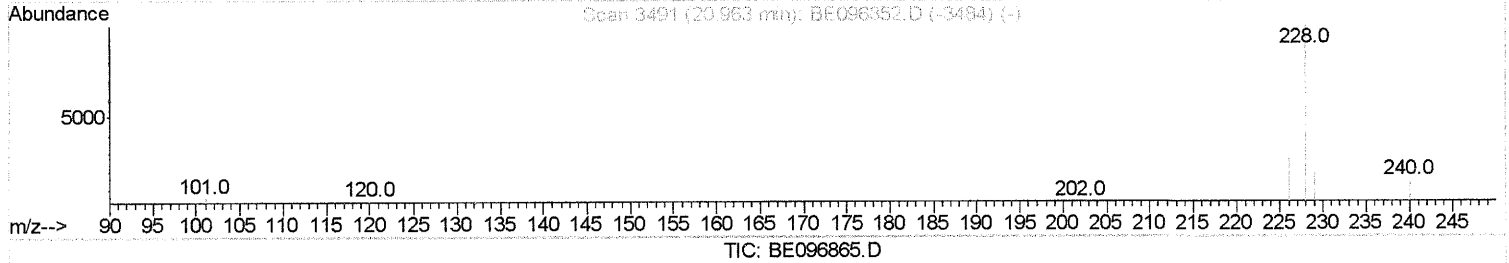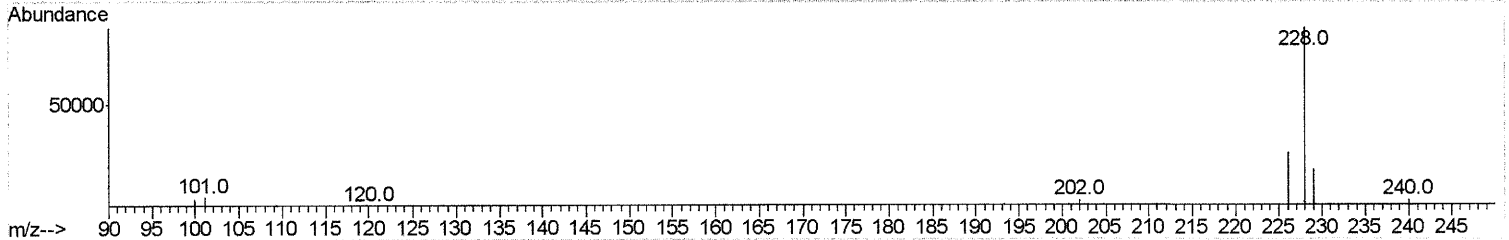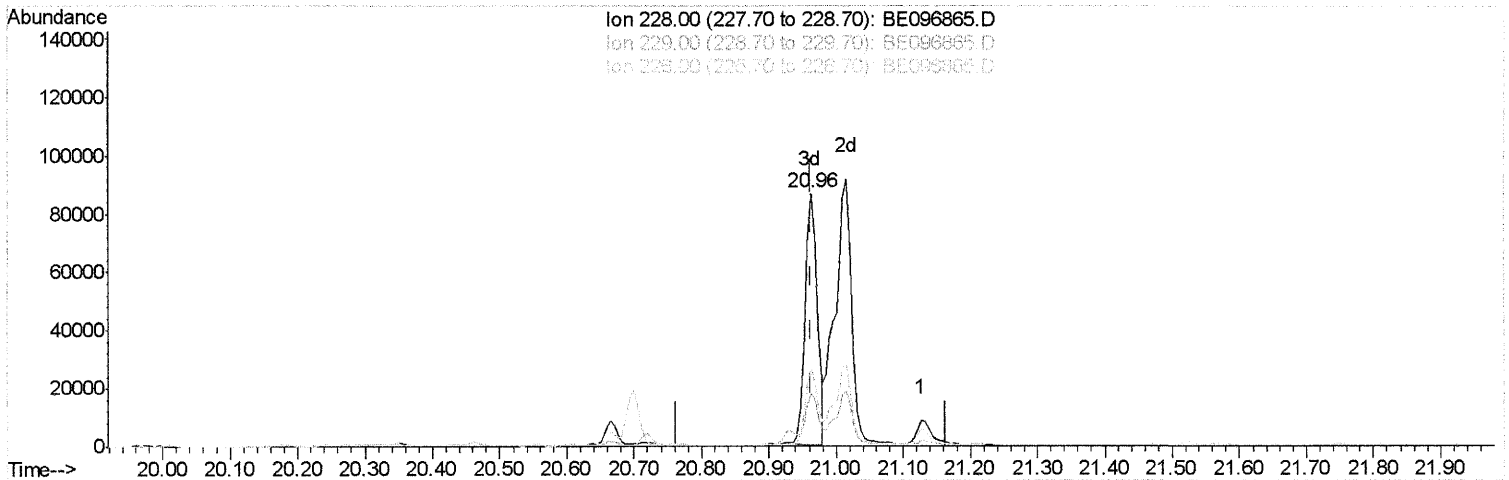

(18) Benzo(a)anthracene

20.962min (-0.001) 1.52ng/ul m

SJ 7/11/18

response 108016

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.95#
226.00	21.30	30.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

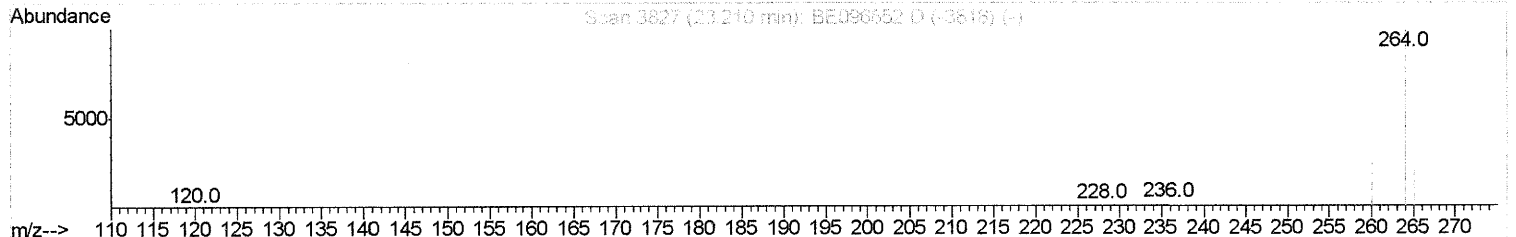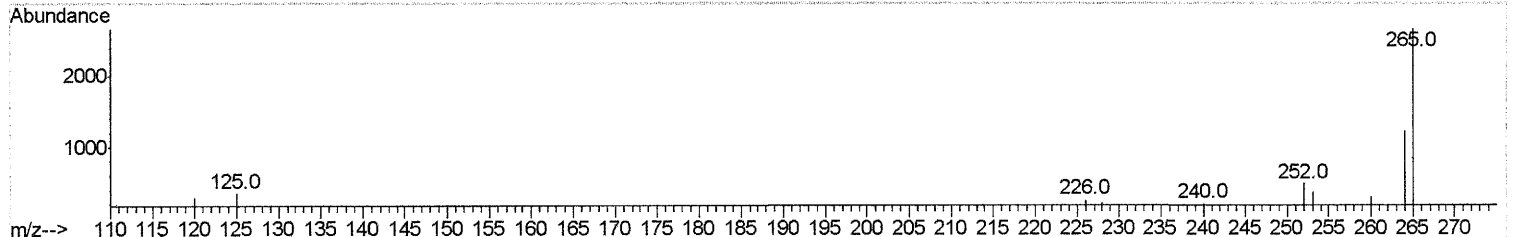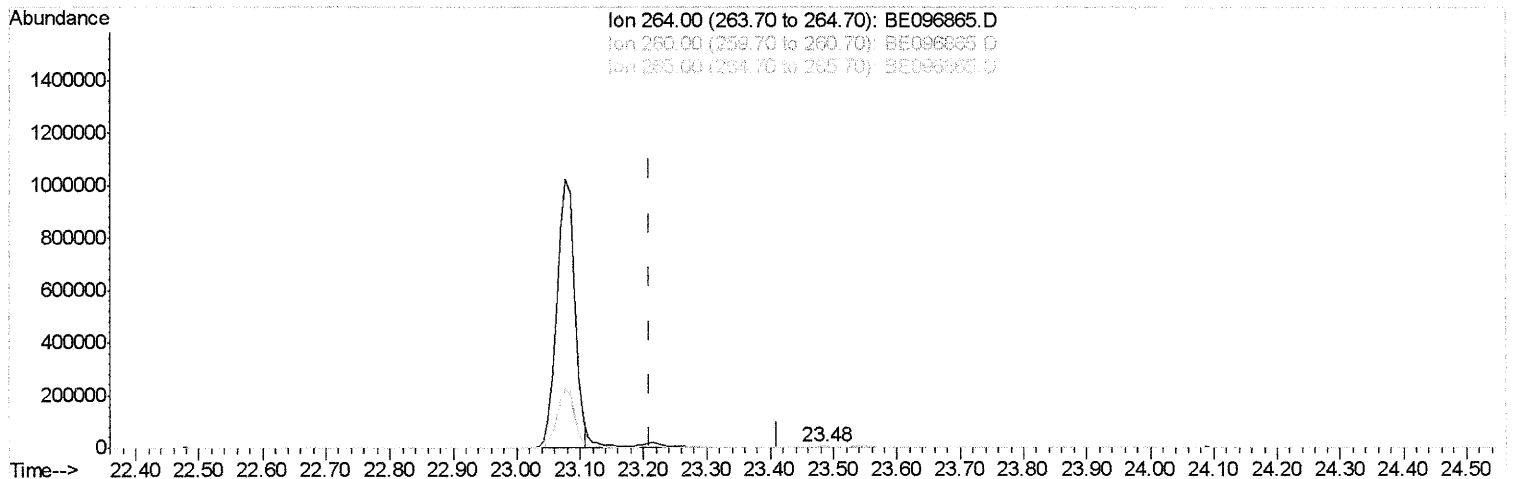

TIC: BE096865.D

(20) Perylene-d12 (I)

23.485min (+0.274) 0.40ng/ul

response 370

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.86#
265.00	103.50	218.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:22:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

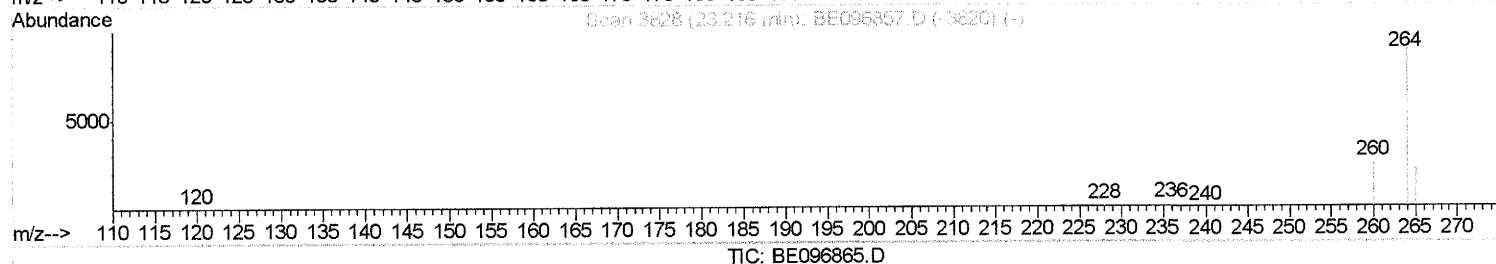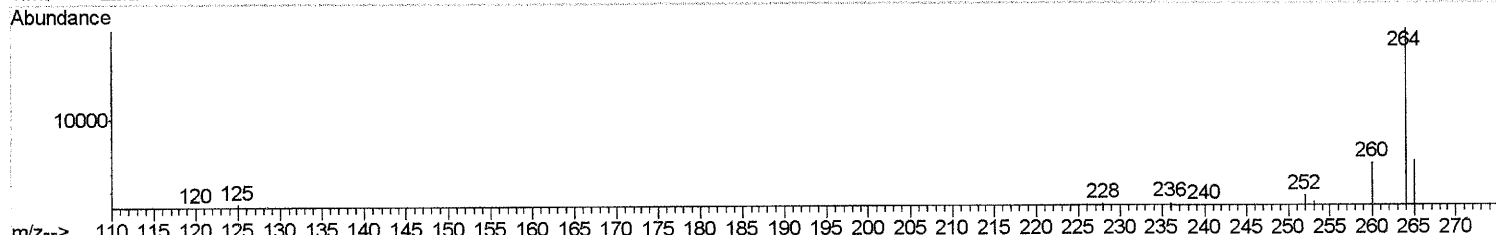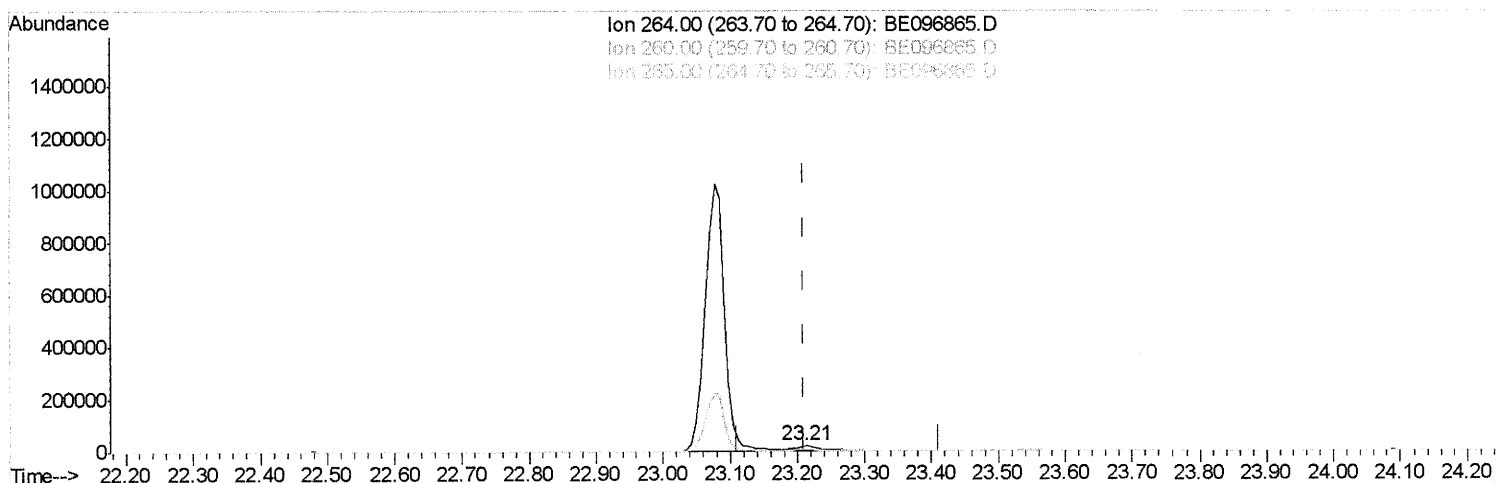

(20) Perylene-d12 (I)

23.210min (-0.000) 0.40ng/ul m

SJ 7/11/18

response 27303

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.08
265.00	103.50	26.39#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

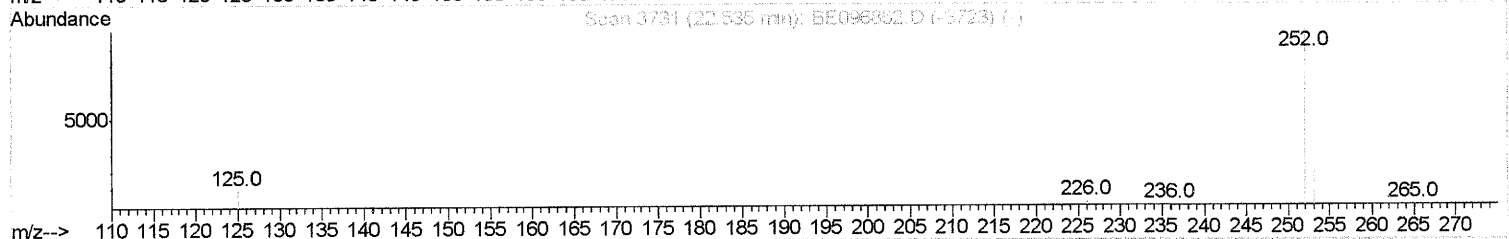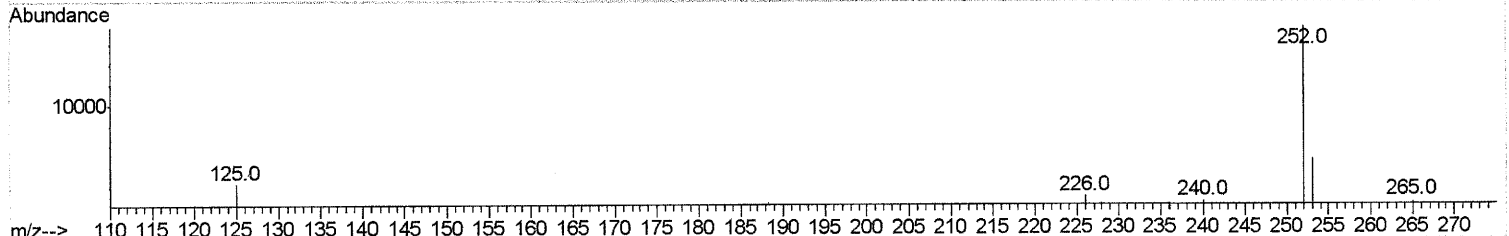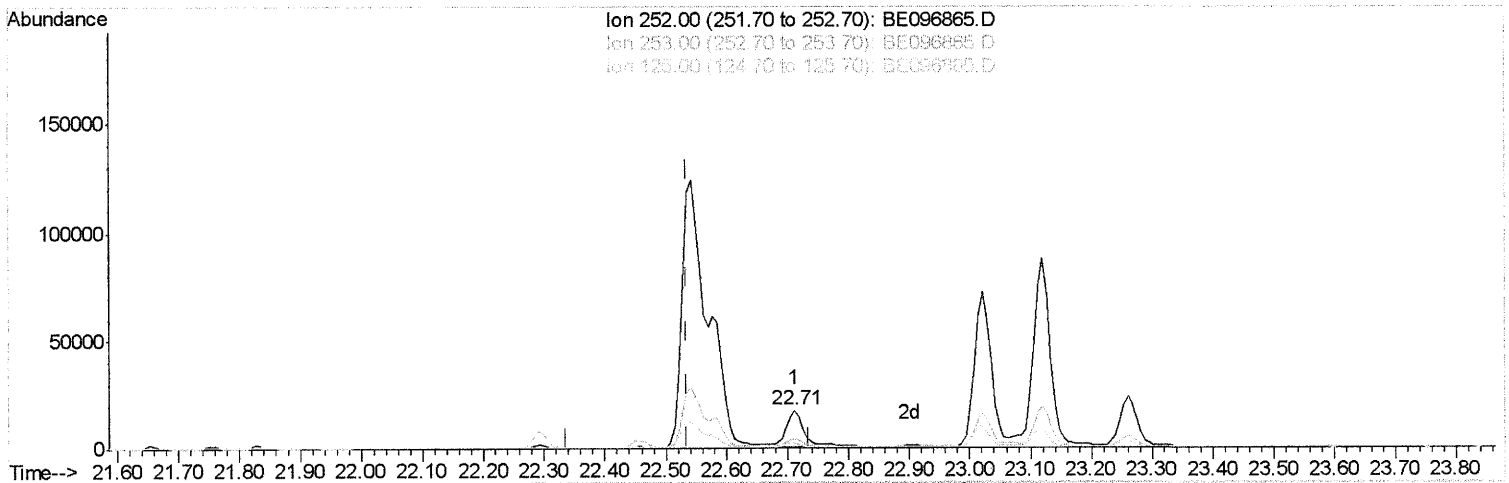

TIC: BE096865.D

(21) Benzo(b)fluoranthene
 22.711min (+0.176) 0.36ng/ui
 response 34727

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.18
125.00	17.50	13.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

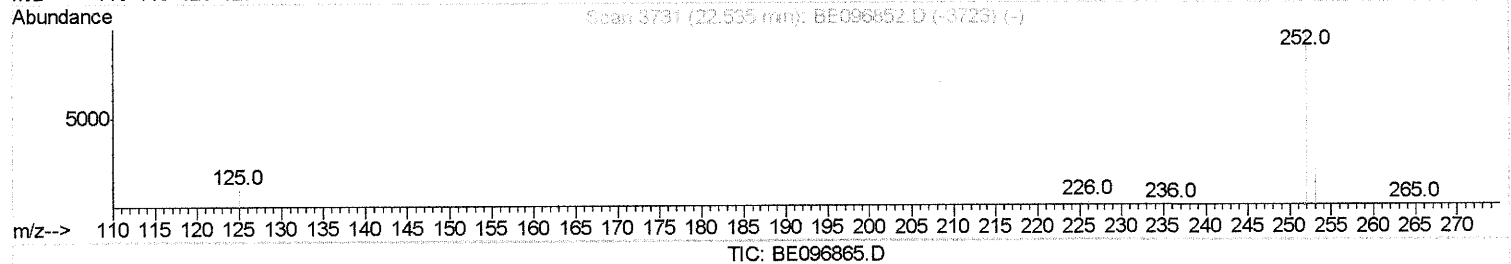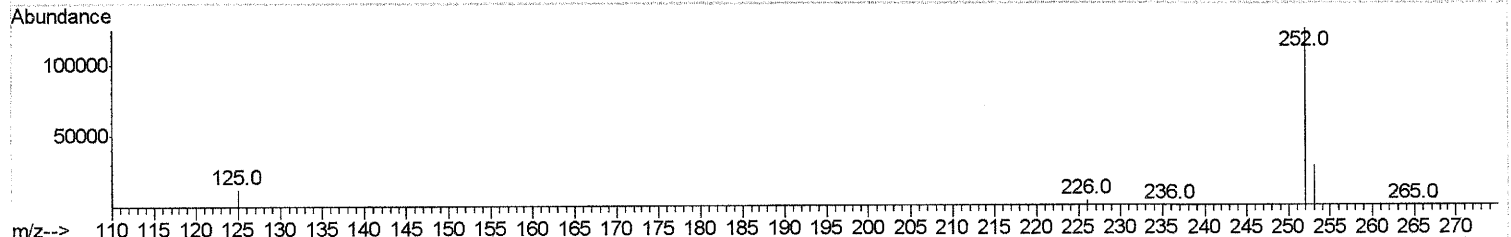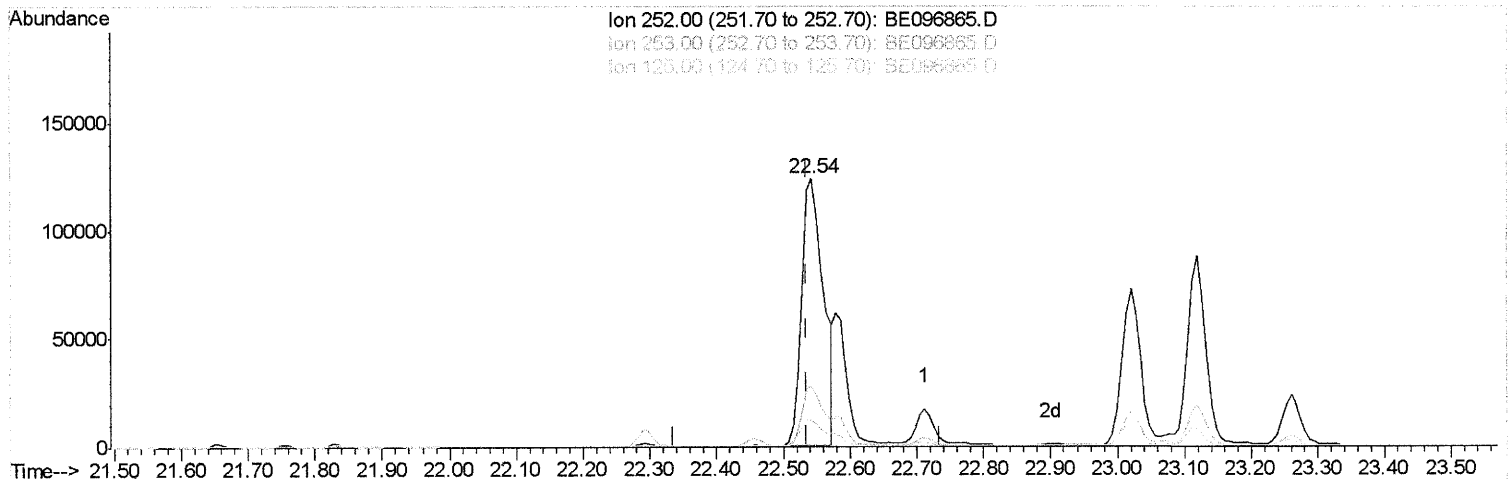

(21) Benzo(b)fluoranthene

22.542min (+0.007) 2.95ng/ul m

SJ 7/11/18

response 283837

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.79
125.00	17.50	9.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

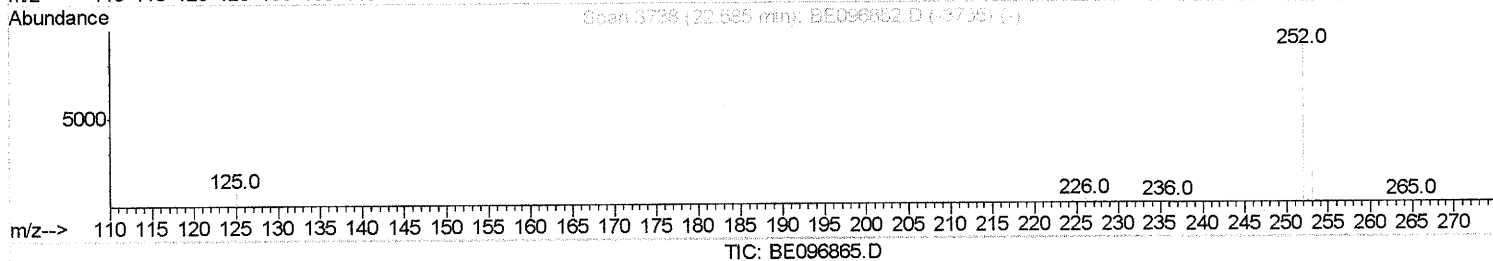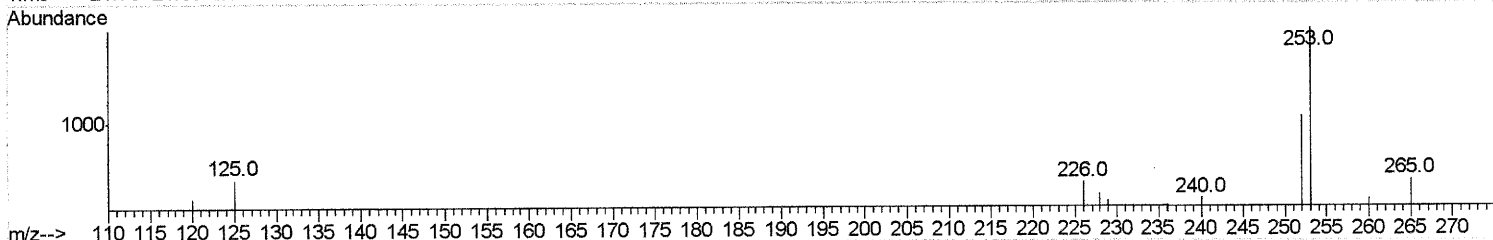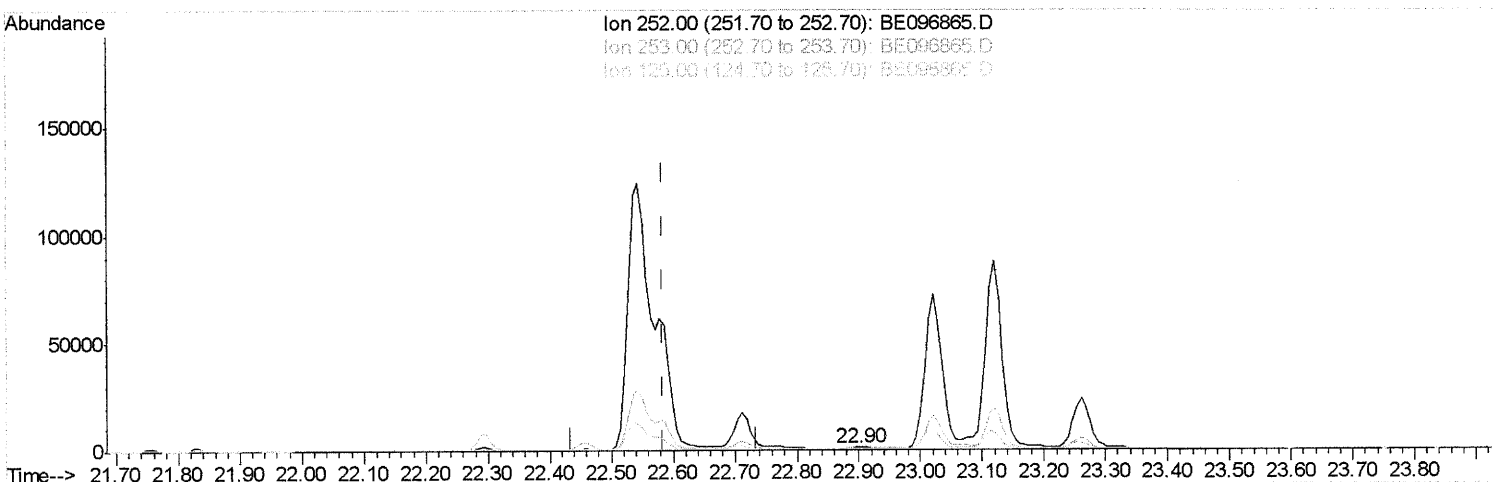

(22) Benzo(k)fluoranthene

22.901min (+0.316) 0.01ng/ul

response 1099

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	186.66#
125.00	17.10	39.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

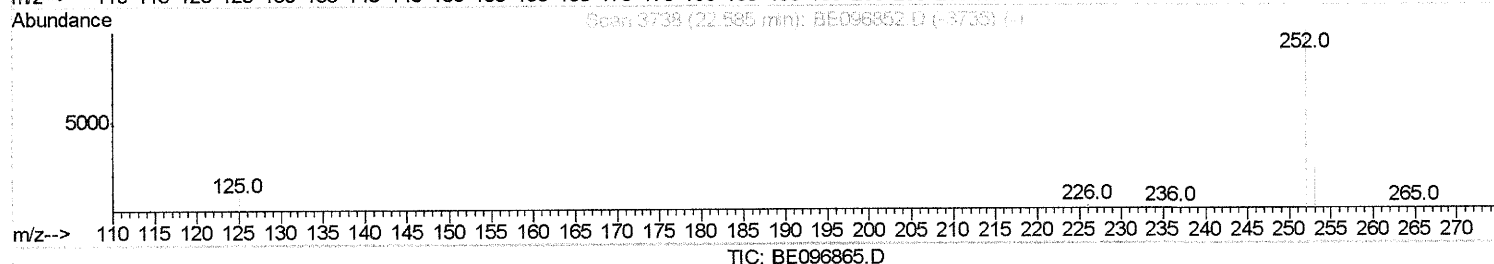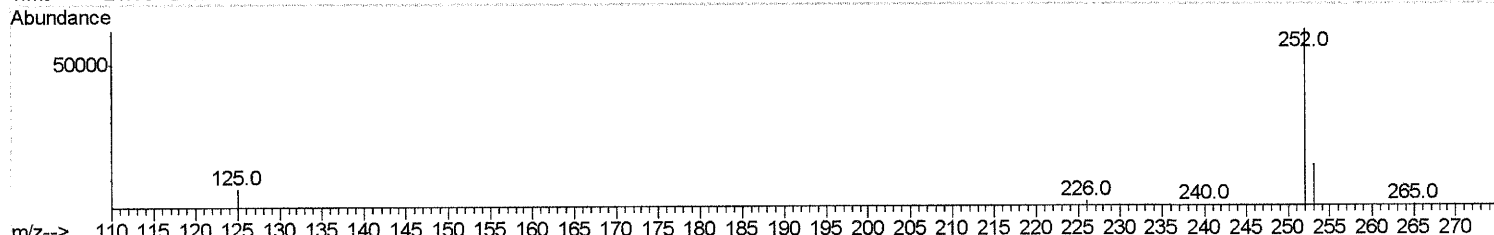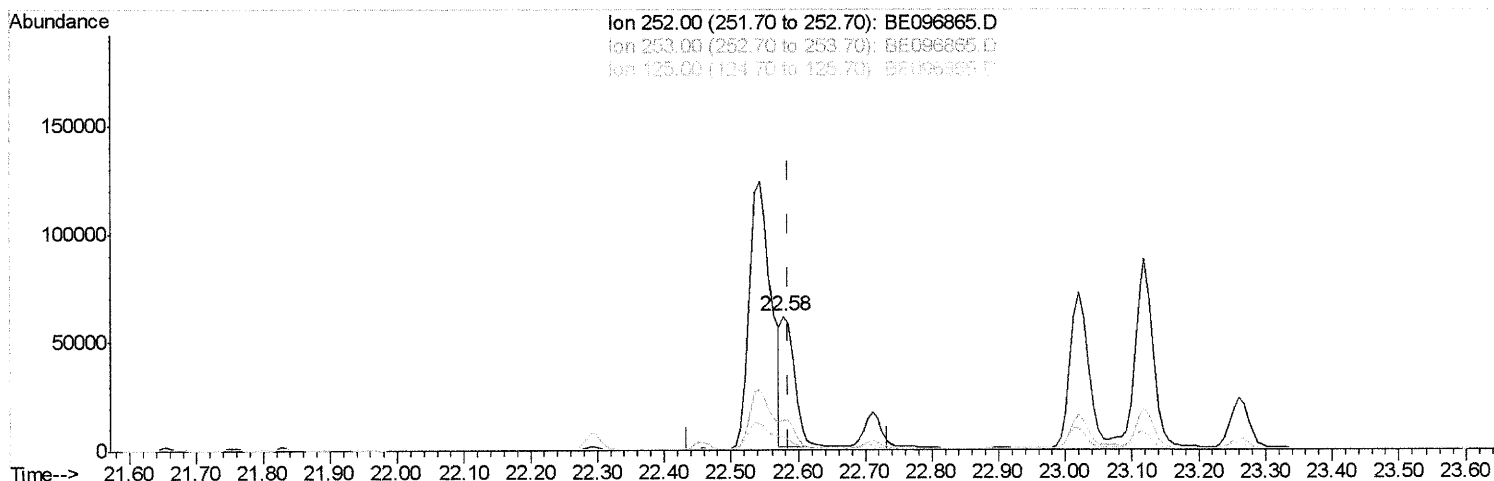

(22) Benzo(k)fluoranthene

22.577min (-0.007) 0.78ng/ul m

SJ 7/11/18

response 81830

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.21#
125.00	17.10	10.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

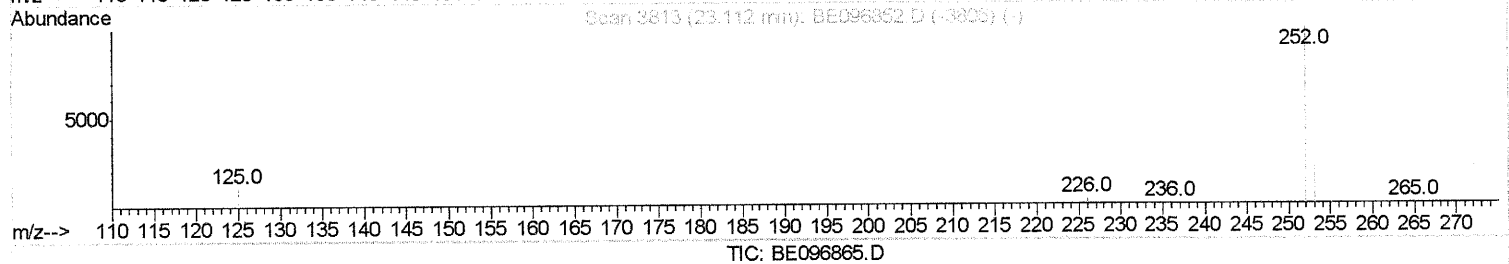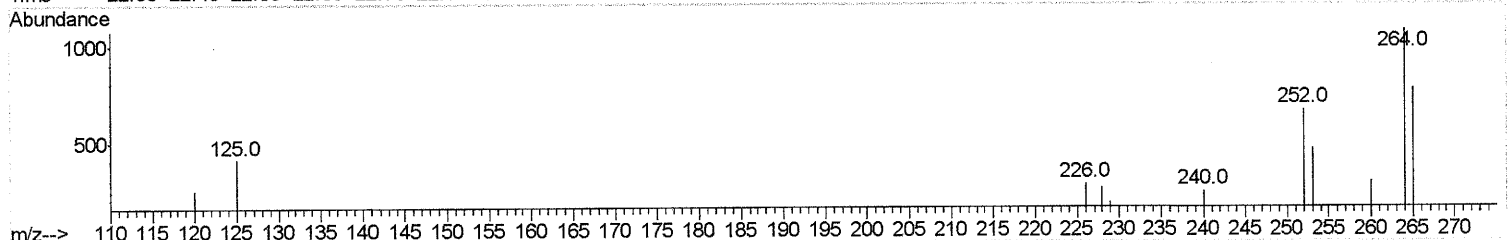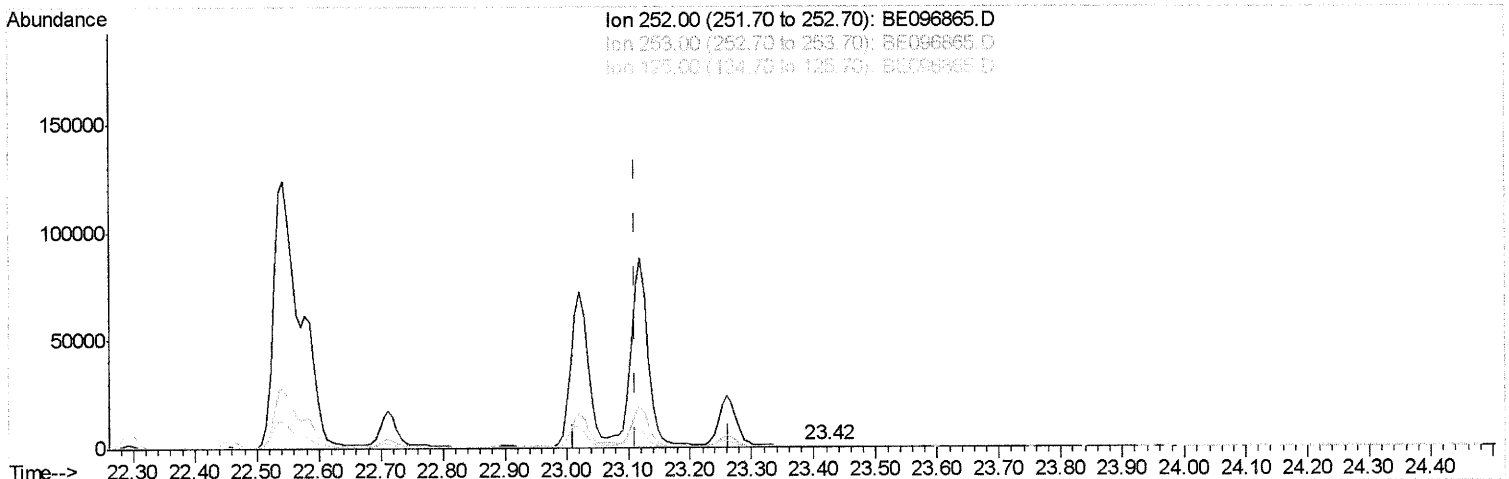

(23) Benzo(a)pyrene (C)

23.421min (+0.309) 0.01ng/ul

response 718

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	69.08#
125.00	22.60	62.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

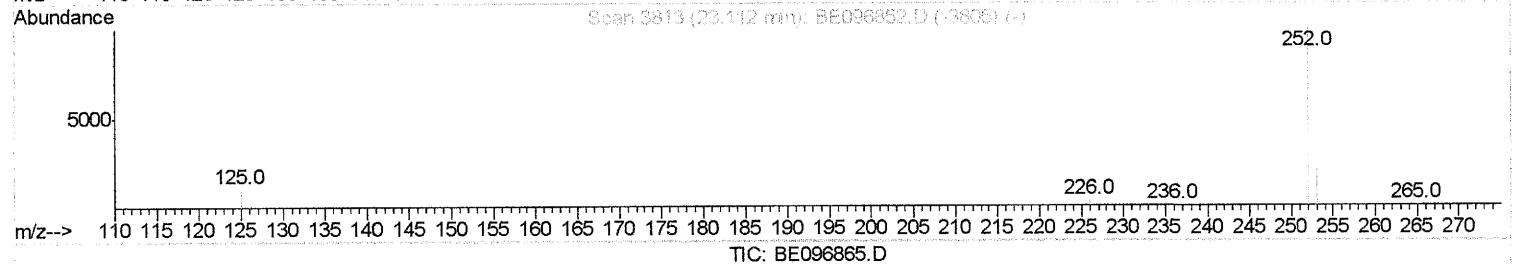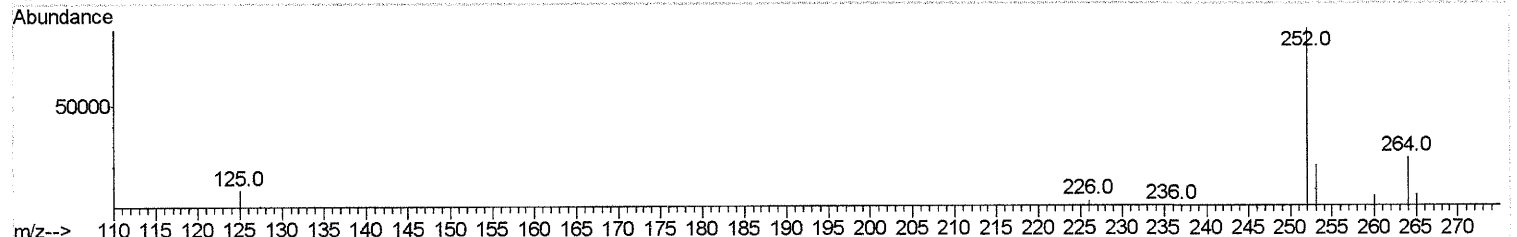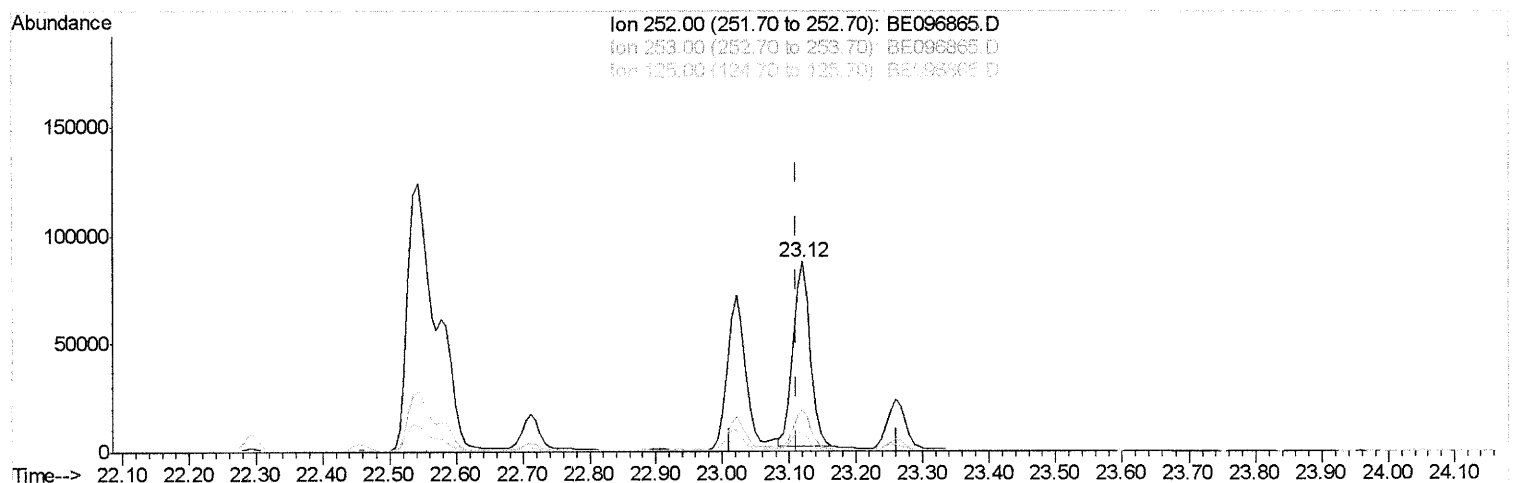

(23) Benzo(a)pyrene (C)

23.119min (+0.007) 1.90ng/ul m

SJ 7/11/18

response 154279

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.79#
125.00	22.60	9.67#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

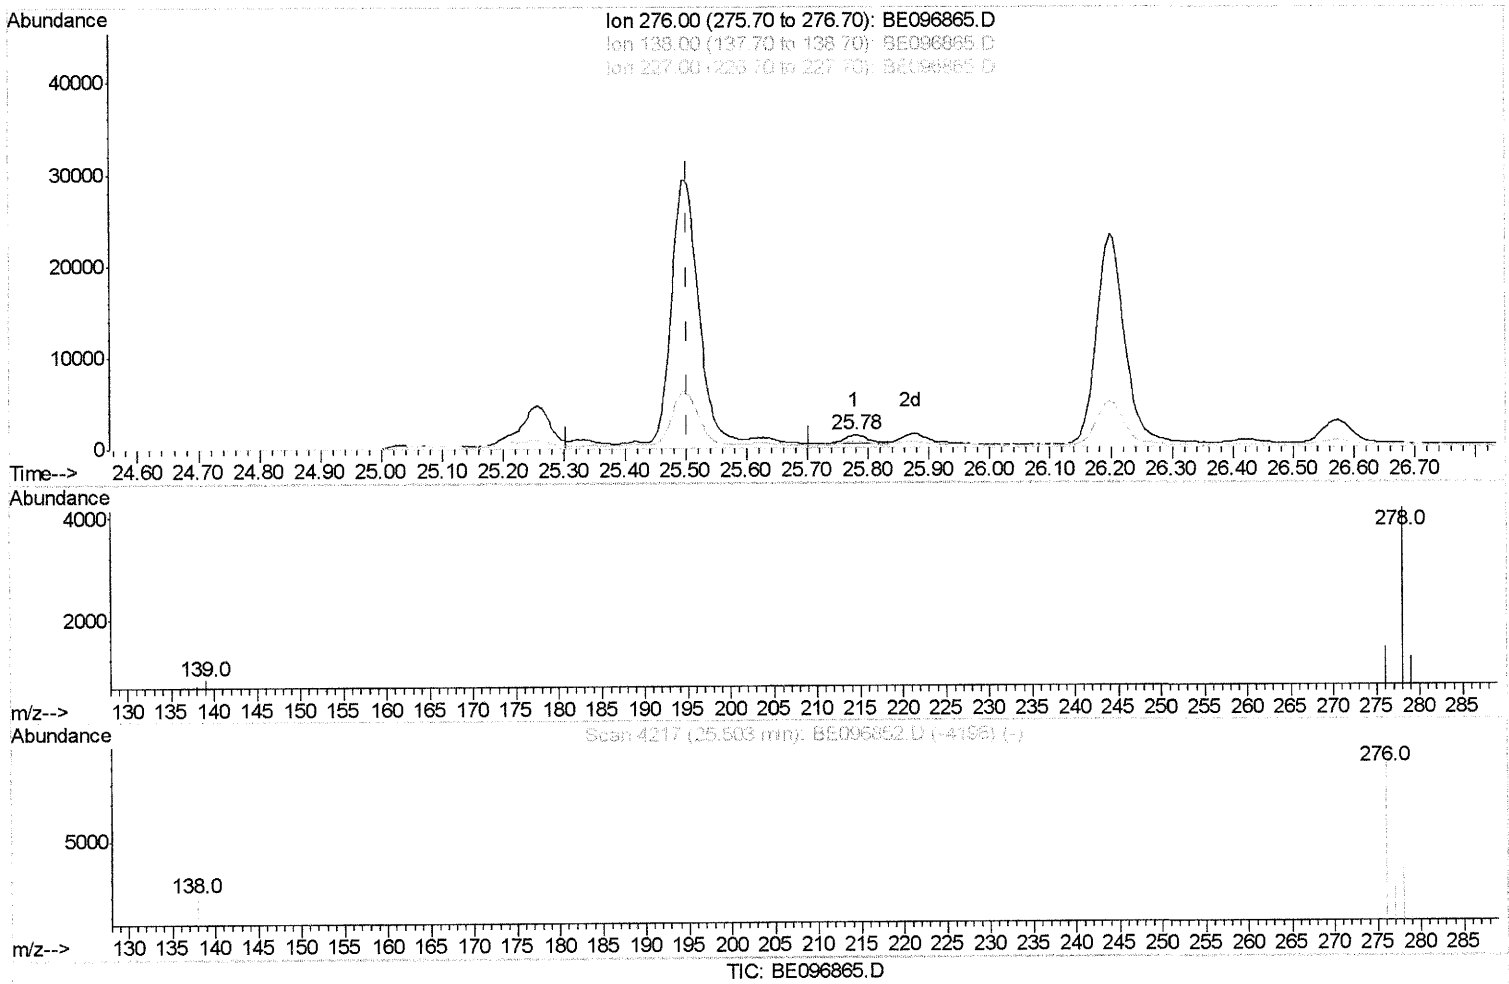

(24) Indeno(1,2,3-cd)pyrene

25.777min (+0.274) 0.03ng/ul

response 2924

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	54.17#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

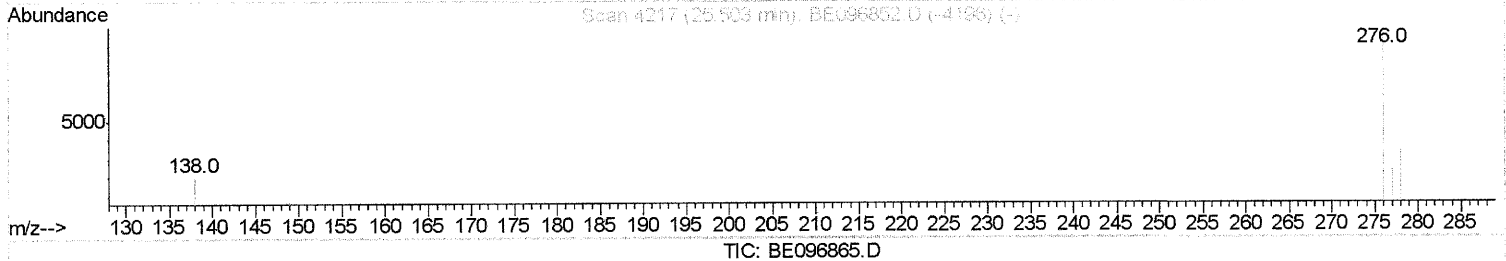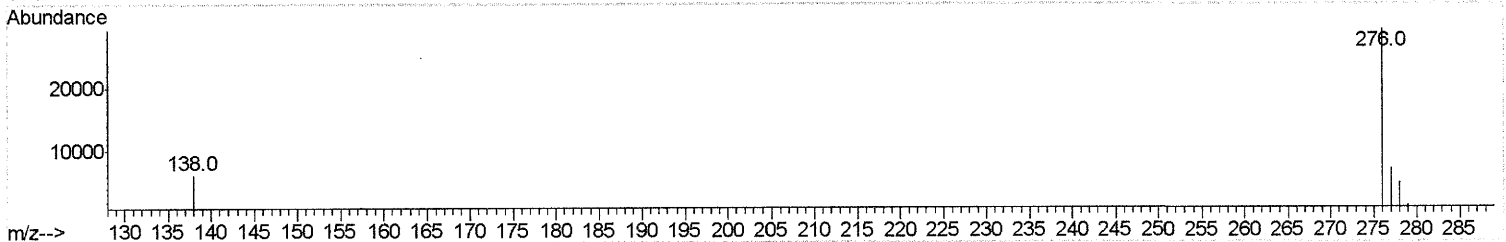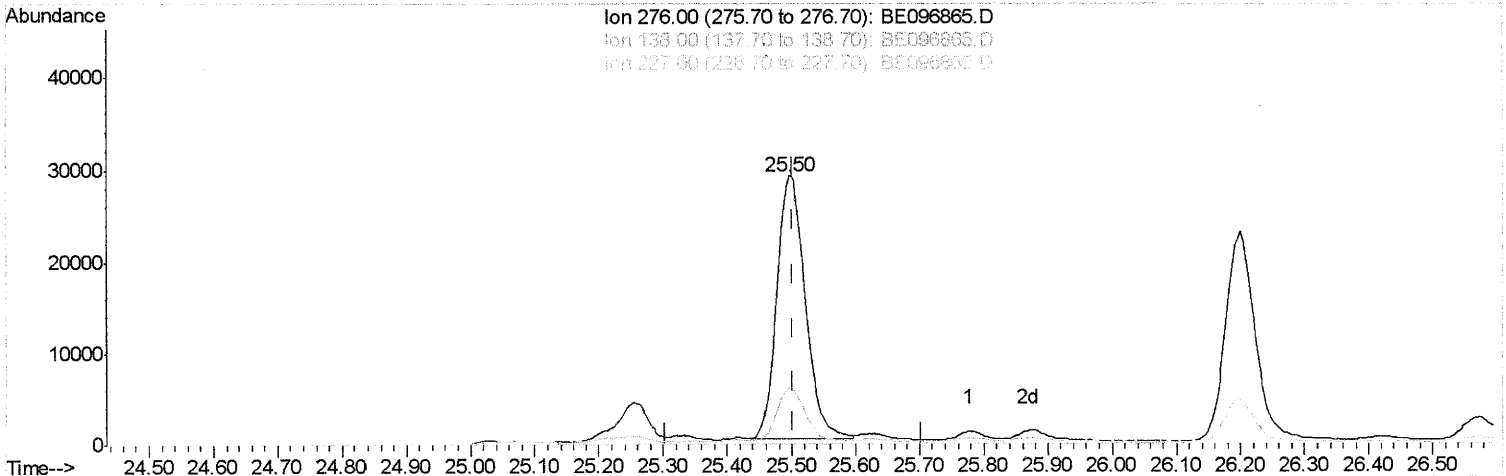

TIC: BE096865.D

(24) Indeno(1,2,3-cd)pyrene

25.496min (-0.008) 1.05ng/ul m

SJ 7/11/18

response 88457

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	1.79#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

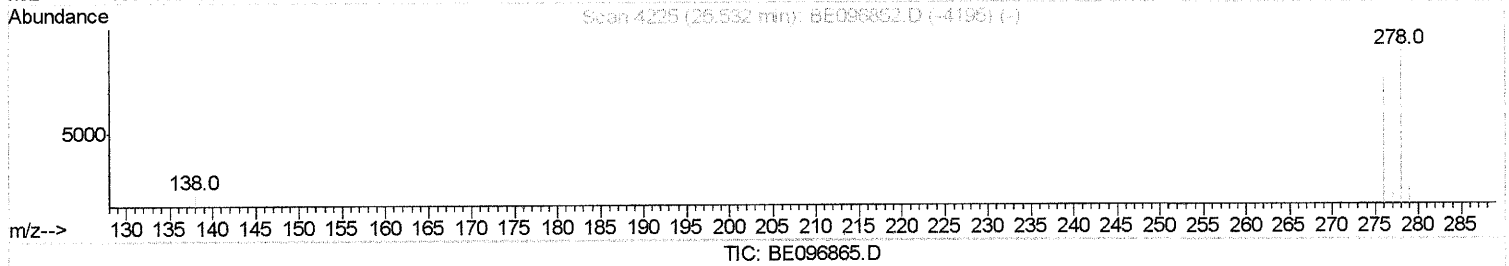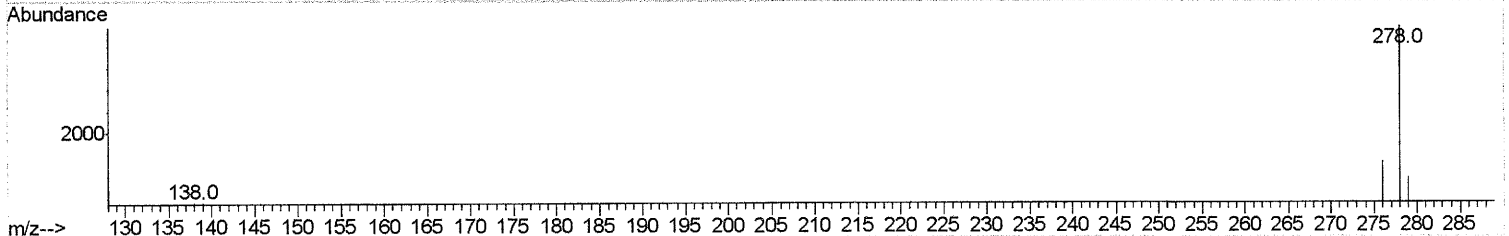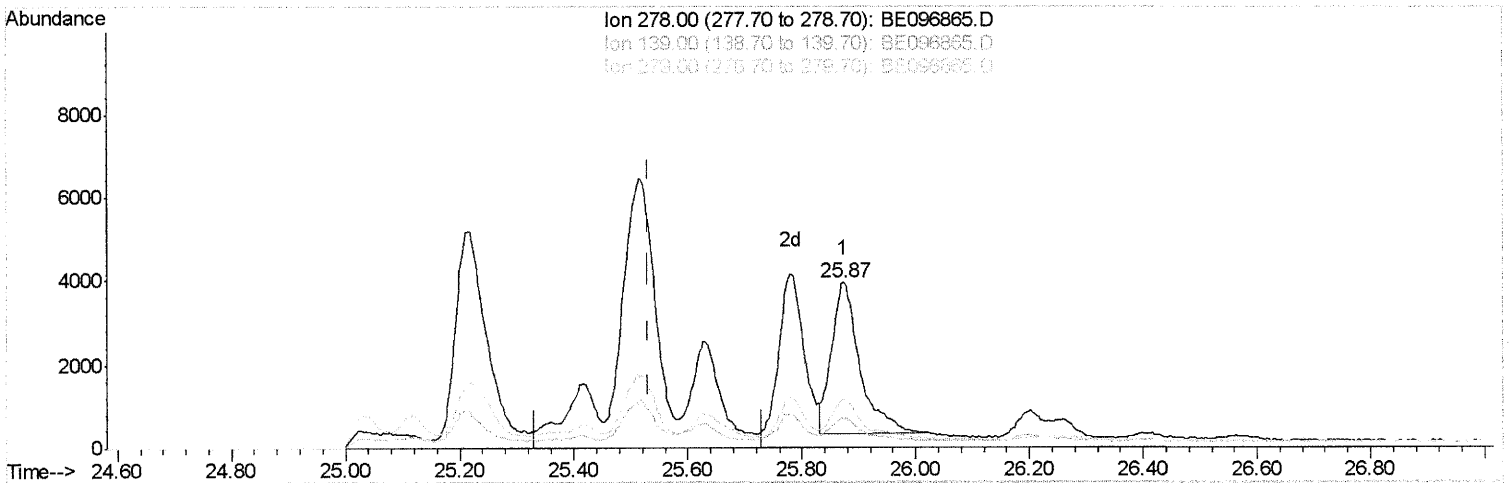

TIC: BE096865.D

(25) Dibenzo(a,h)anthracene

25.874min (+0.342) 0.19ng/ul

response 12734

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	18.00
279.00	32.40	29.76
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

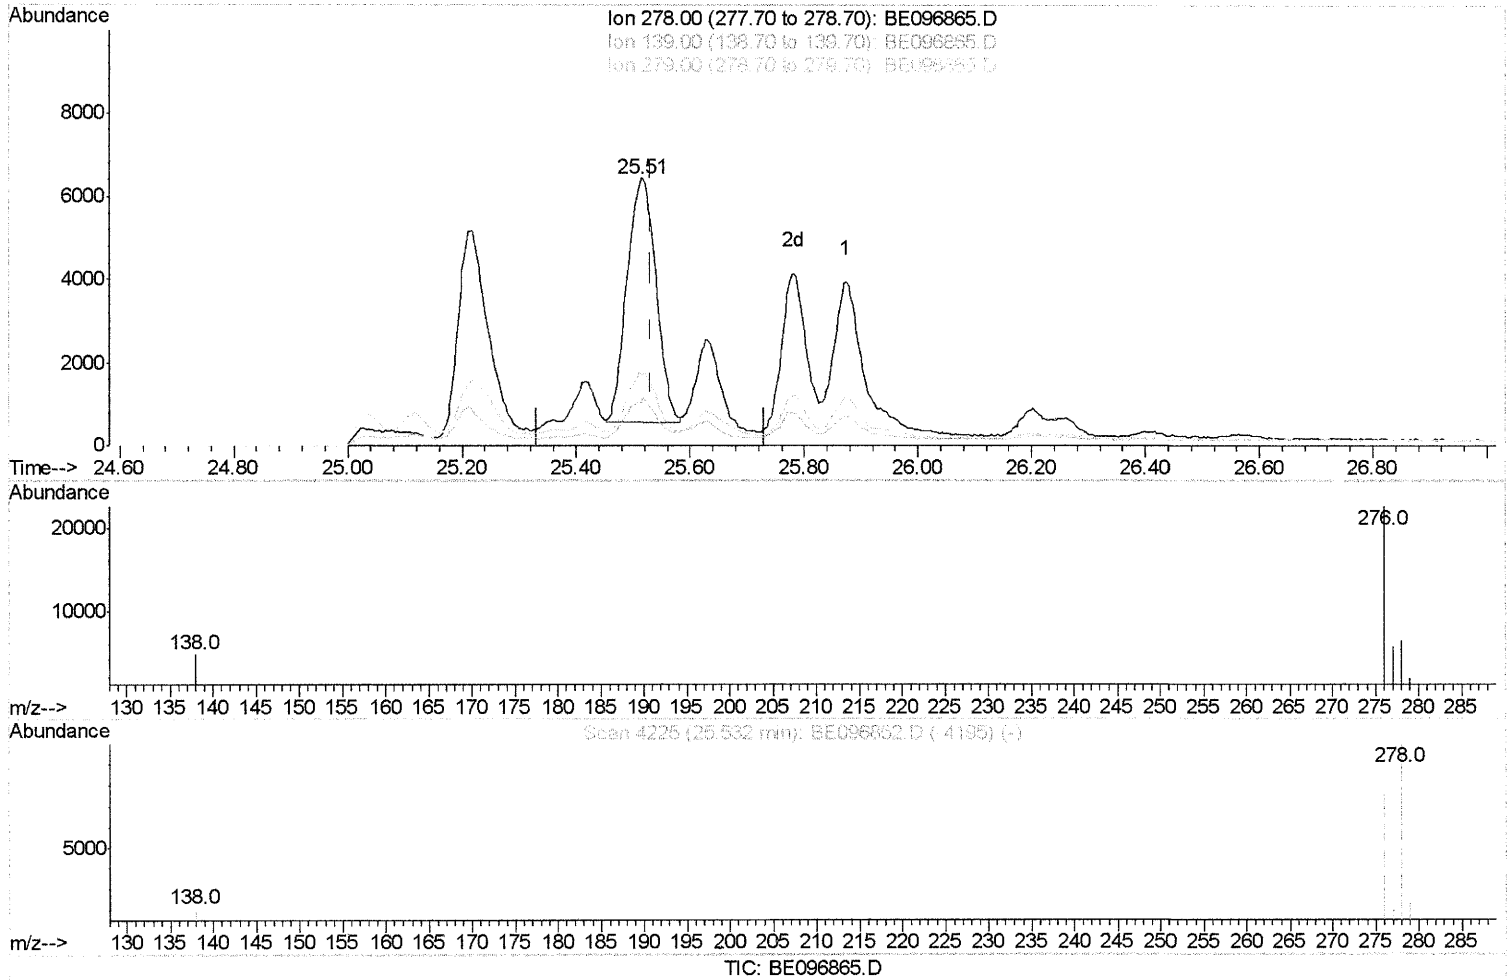

(25) Dibenzo(a,h)anthracene

25.514min (-0.018) 0.31ng/ul m

SJ 7/11/18

response 20585

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	16.52#
279.00	32.40	27.40
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

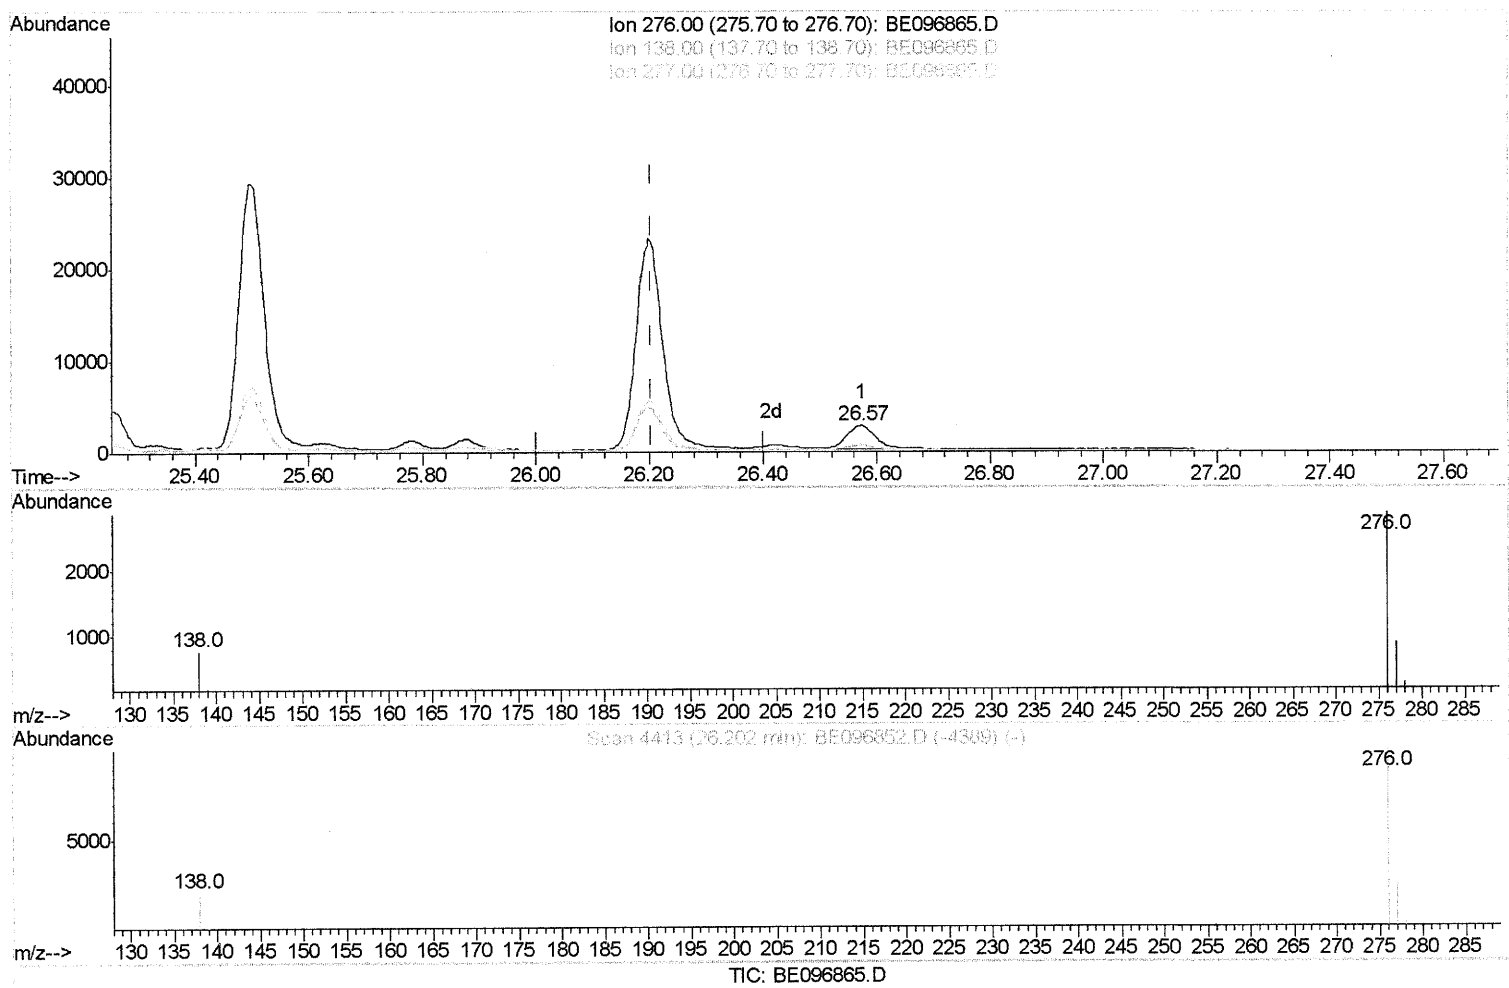

(26) Benzo(g,h,i)perylene
 26.573min (+0.370) 0.11ng/ul
 response 9186

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	26.71
277.00	25.60	30.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096865.D
 Acq On : 6 Jul 2018 22:27
 Operator : SJ/JU
 Sample : J3721-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H24

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:11 PM

Quant Time: Jul 07 05:18:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

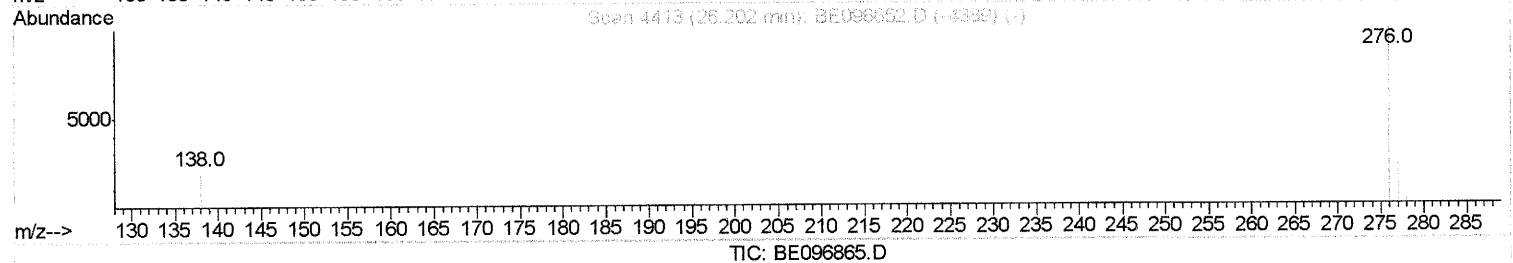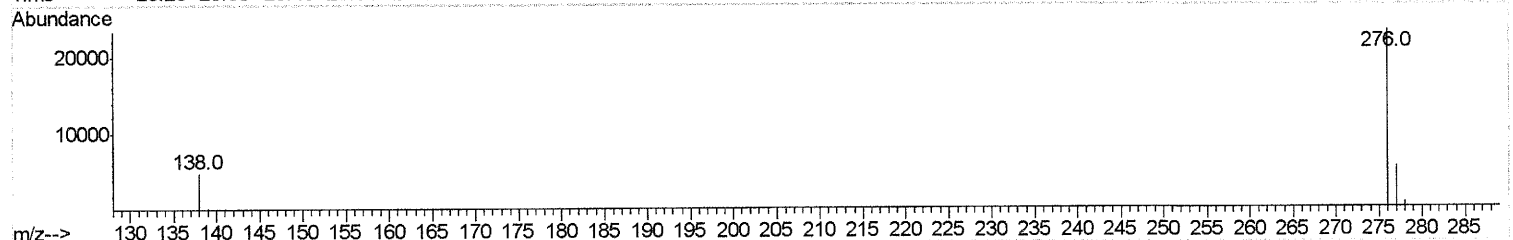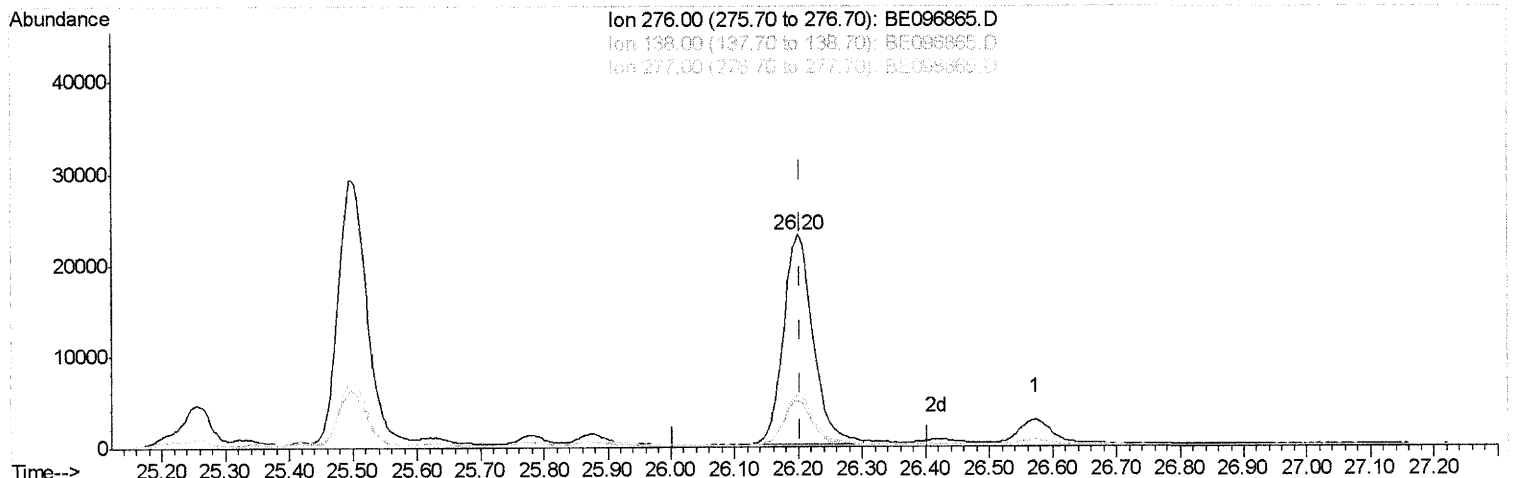

(26) Benzo(g,h,i)perylene

26.198min (-0.004) 0.91ng/ul m

SJ 7/11/18

response 74509

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	21.21#
277.00	25.60	24.28
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
Client Sampled :
F1H24

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
Data File : BE096865.D
Acq On : 6 Jul 2018 22:27
Operator : SJ/JU
Sample : J3721-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
7/9/2018 4:14:11 PM

Quant Time: Jul 09 05:32:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 06 16:55:25 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	3786	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	19840	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	12742	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	30858m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	30068m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	27303m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.74	152	9138	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	23889m	0.31	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.19	128	3071	0.064	ng/ul#	95
5) 2-Methylnaphthalene	11.81	142	806	0.025	ng/ul	99
7) Acenaphthylene	13.75	152	8158	0.156	ng/ul	97
8) Acenaphthene	14.09	153	1455	0.034	ng/ul#	93
9) Fluorene	15.08	166	1743	0.039	ng/ul	90
12) Phenanthrene	16.82	178	20228m	0.254	ng/ul	
13) Anthracene	16.91	178	9336m	0.138	ng/ul	
15) Fluoranthene	18.84	202	162683m	1.920	ng/ul	
17) Pyrene	19.21	202	195040	1.976	ng/ul#	80
18) Benzo(a)anthracene	20.96	228	108016m	1.523	ng/ul	
19) Chrysene	21.02	228	159200	1.733	ng/ul	98
21) Benzo(b)fluoranthene	22.54	252	283837m	3.809	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	81830m	1.006	ng/ul	
23) Benzo(a)pyrene	23.12	252	154279m	2.448	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.50	276	88457m	1.352	ng/ul	
25) Dibenzo(a,h)anthracene	25.51	278	20585m	0.396	ng/ul	
26) Benzo(a,h,i)perylene	26.20	276	74509m	1.173	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed