

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 09 05:43:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

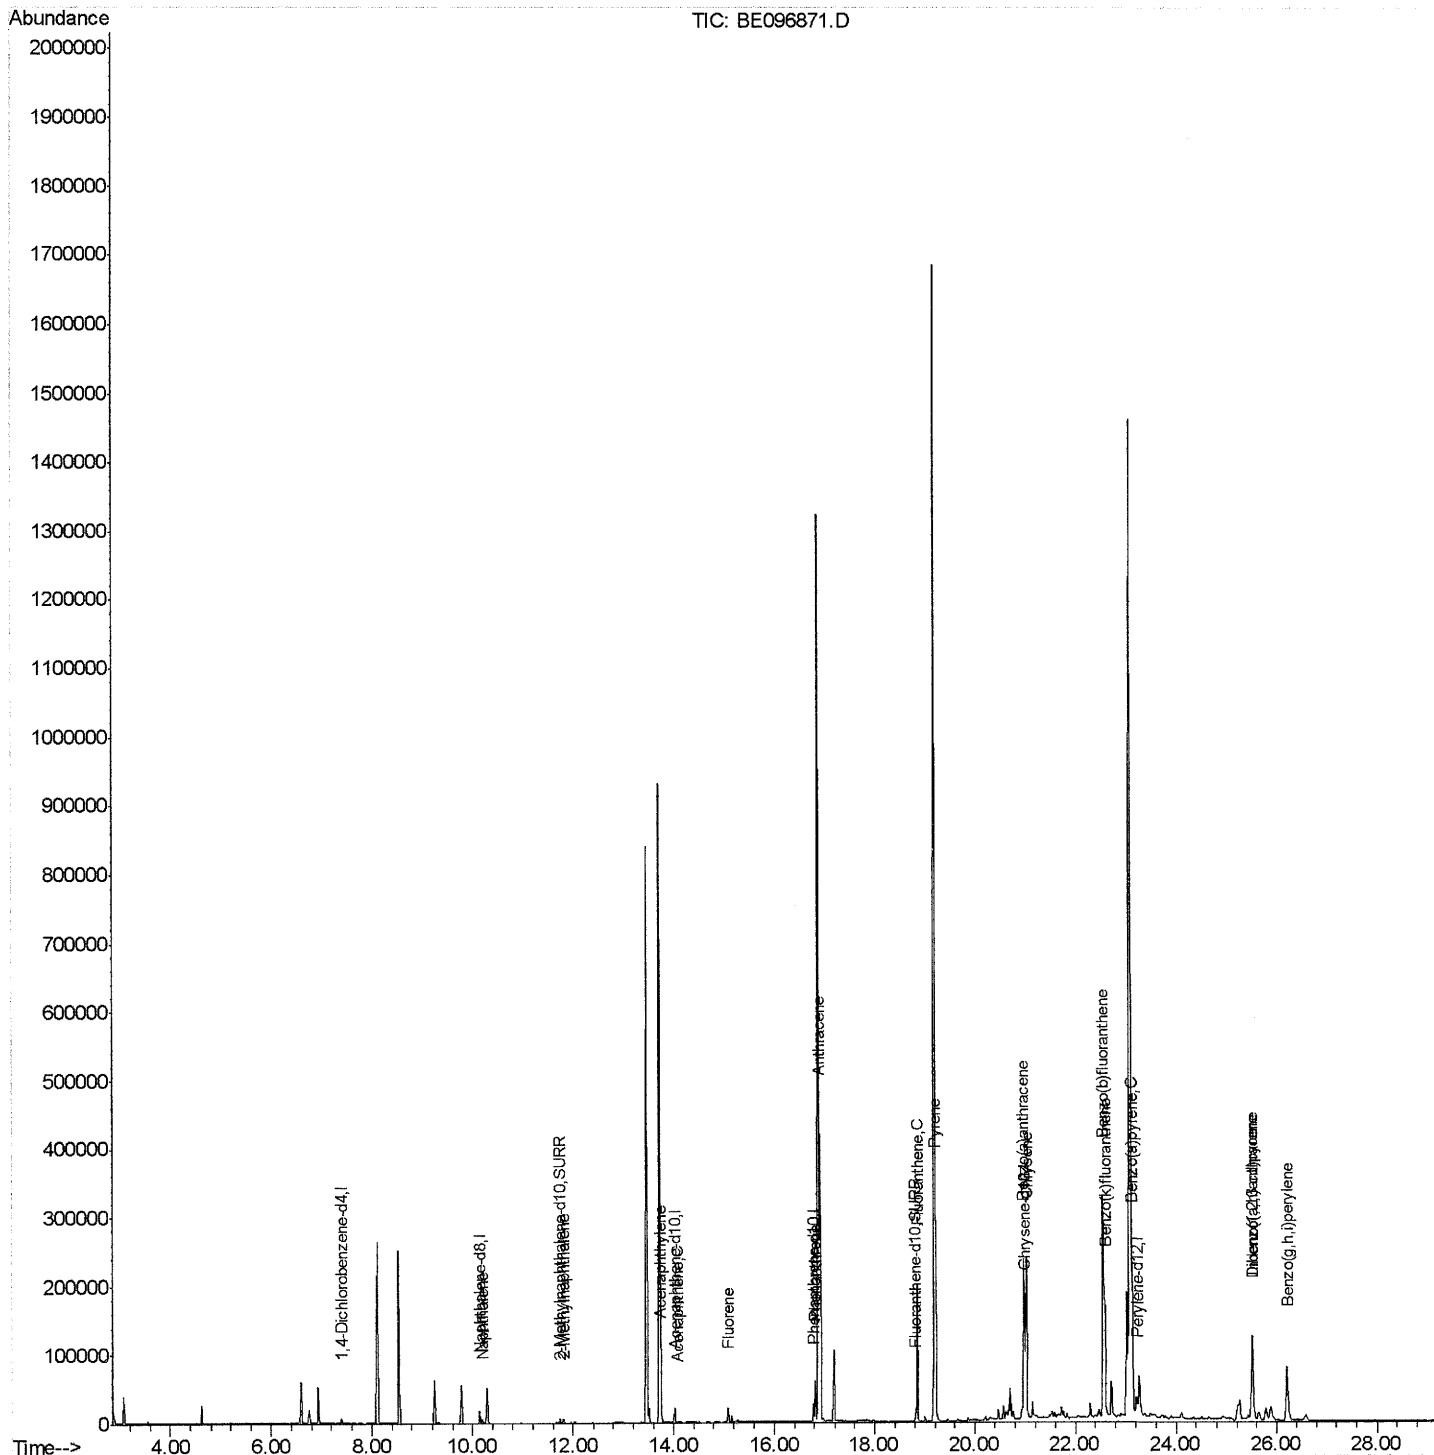

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 03:26:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

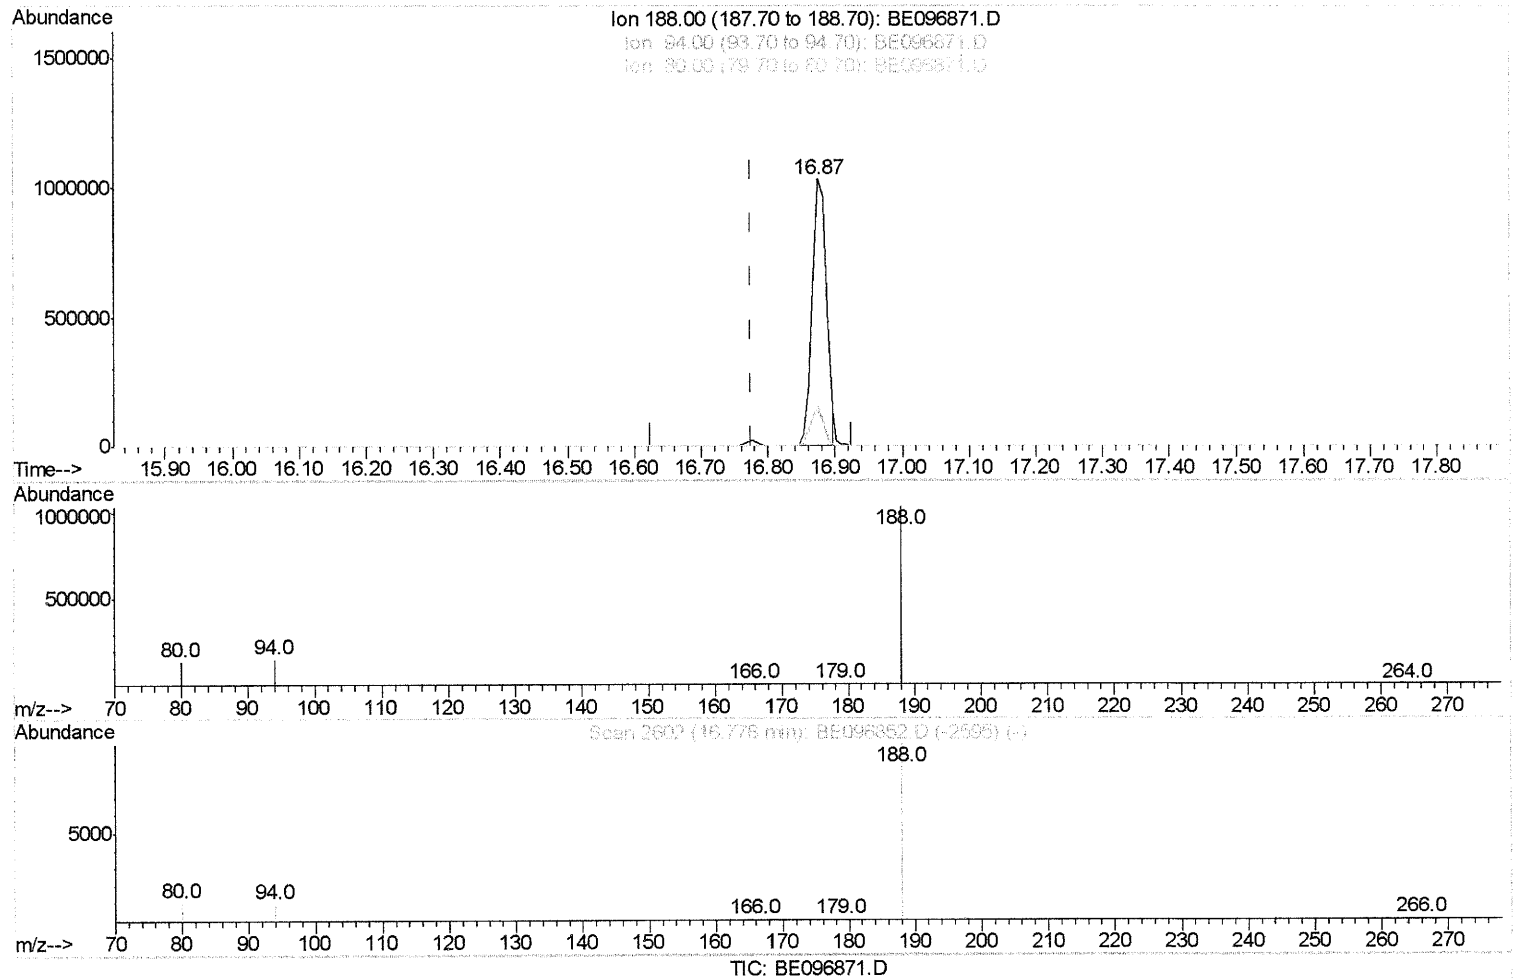

(10) Phenanthrene-d10 (I)
 16.874min (+0.098) 0.40ng/ul
 response 1495480

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.39#
80.00	11.80	13.24
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 03:26:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

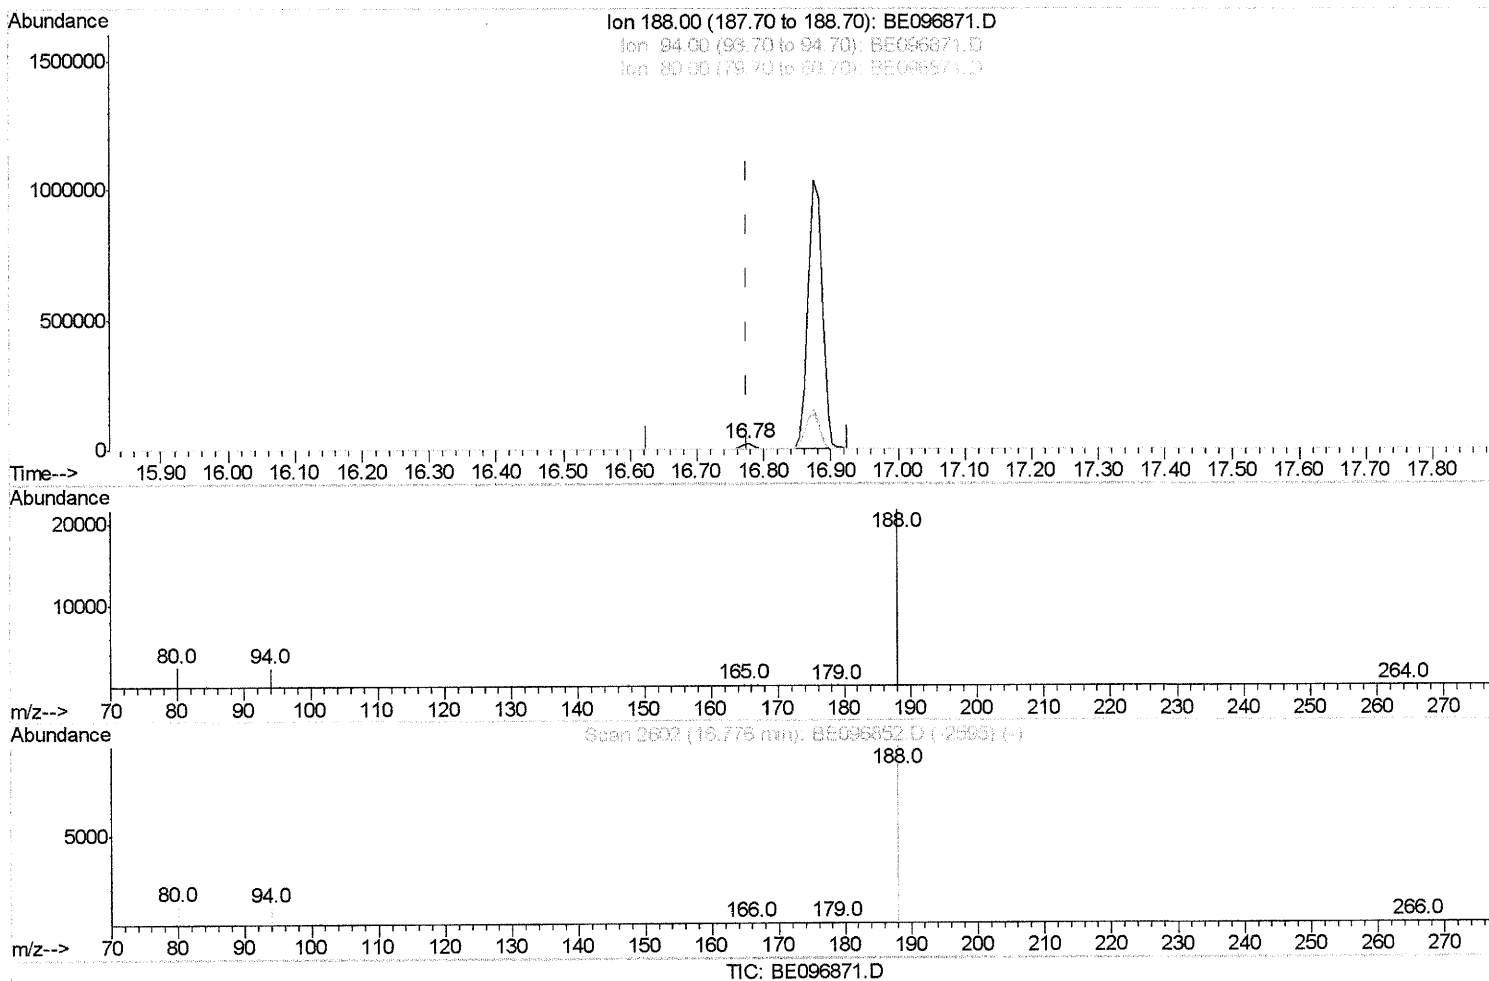

(10) Phenanthrene-d10 (I)

16.775min (-0.000) 0.40ng/ul m

SJ 7/11/18

response 28818

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.62
80.00	11.80	11.42
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 03:26:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

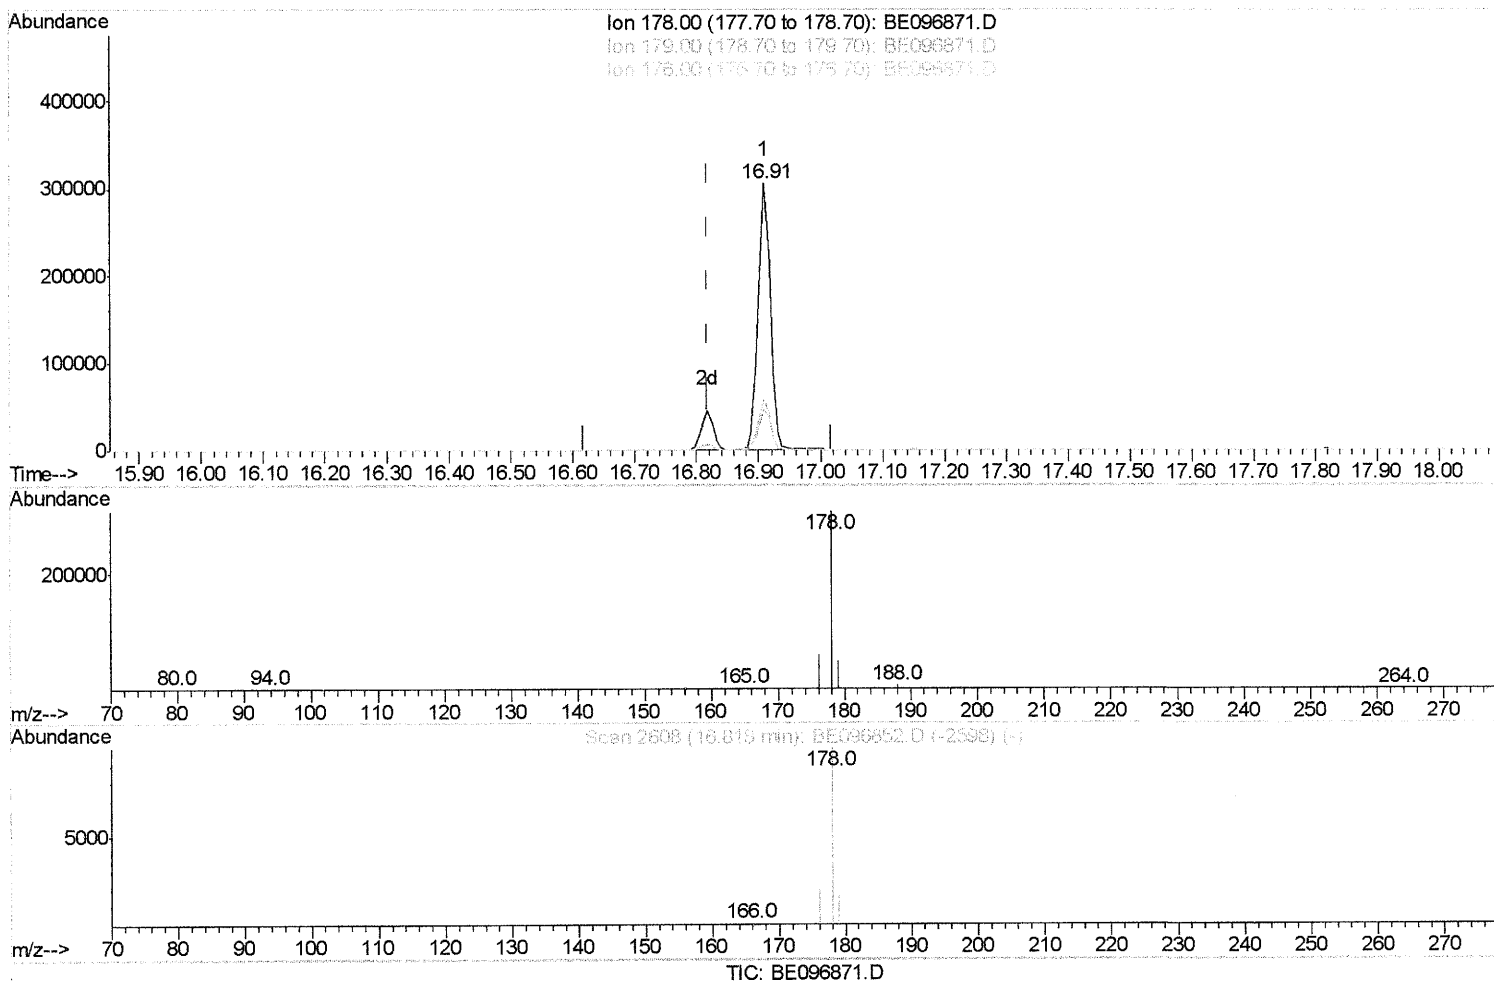

(12) Phenanthrene

16.909min (+0.091) 5.64ng/ul

response 419373

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.56#
176.00	17.00	19.05
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 03:26:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

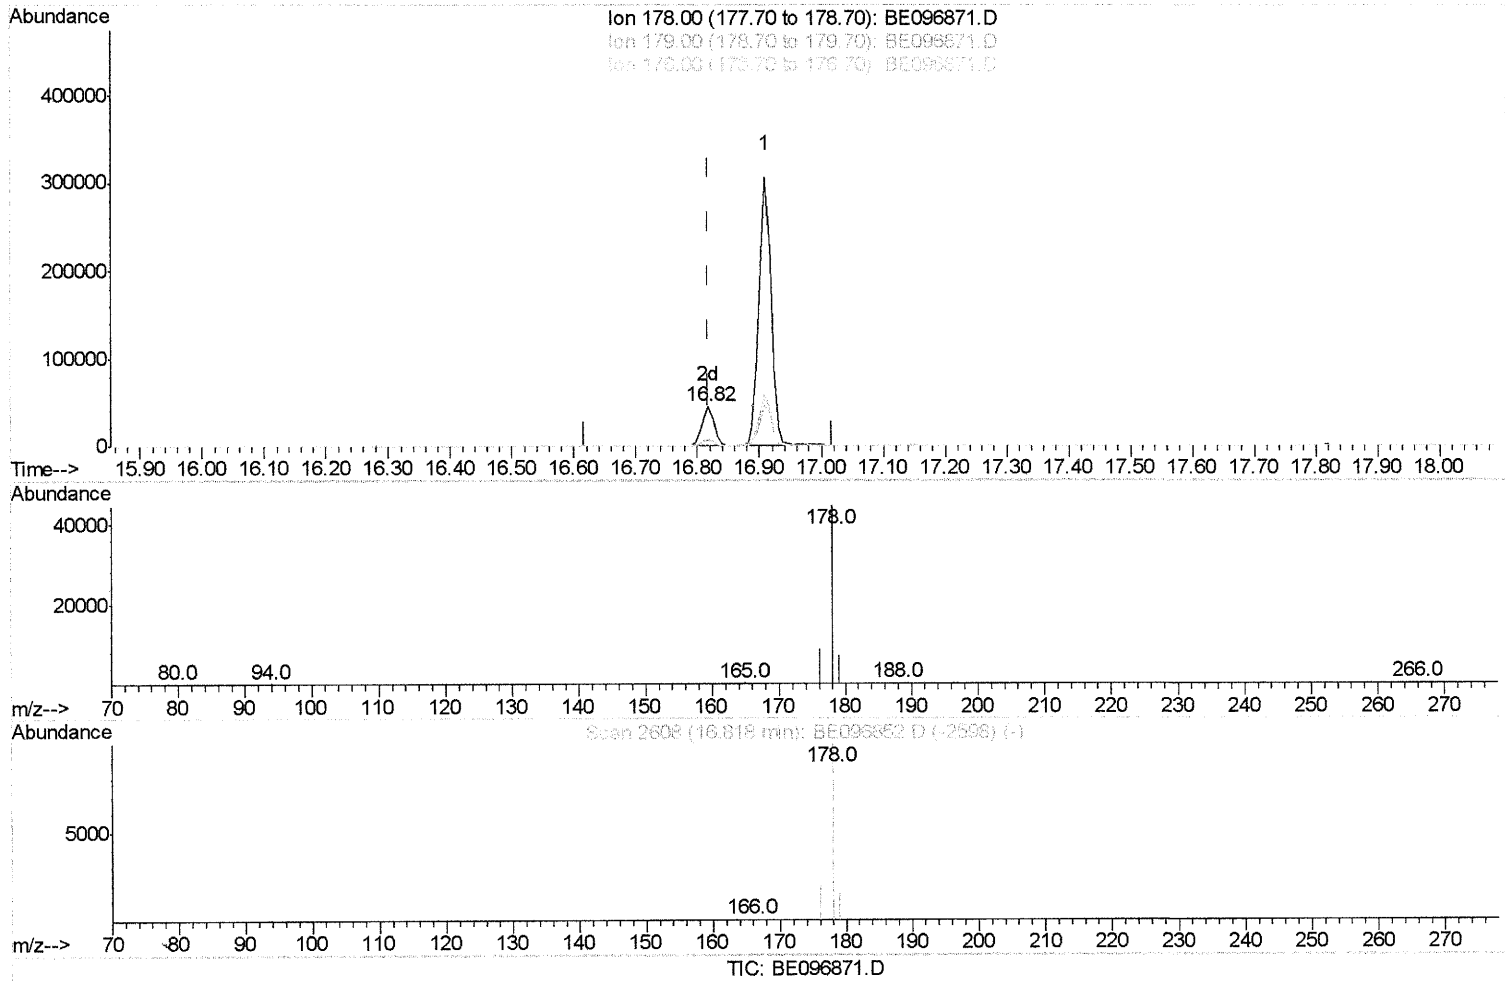

(12) Phenanthrene

16.818min (-0.000) 0.82ng/ul m

response 60835

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.93#
176.00	17.00	19.47
0.00	0.00	0.00

SJ 7/11/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

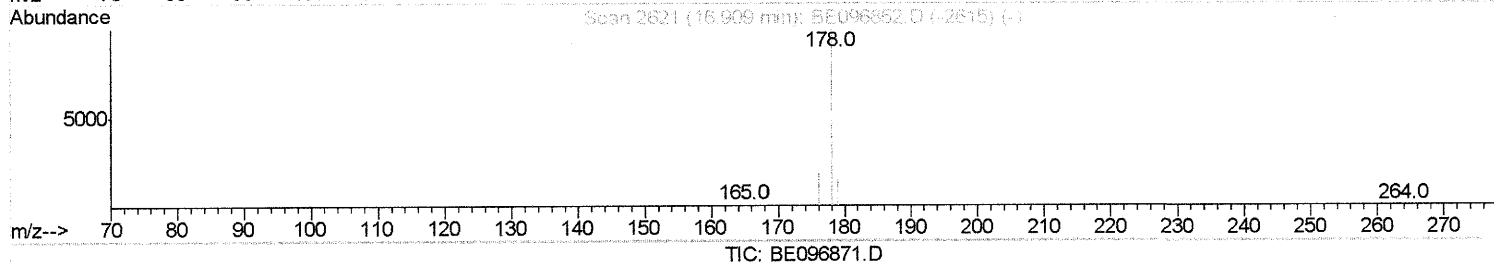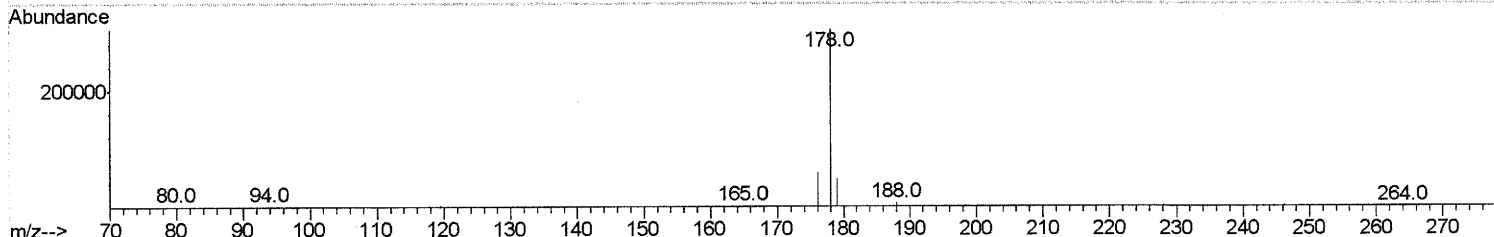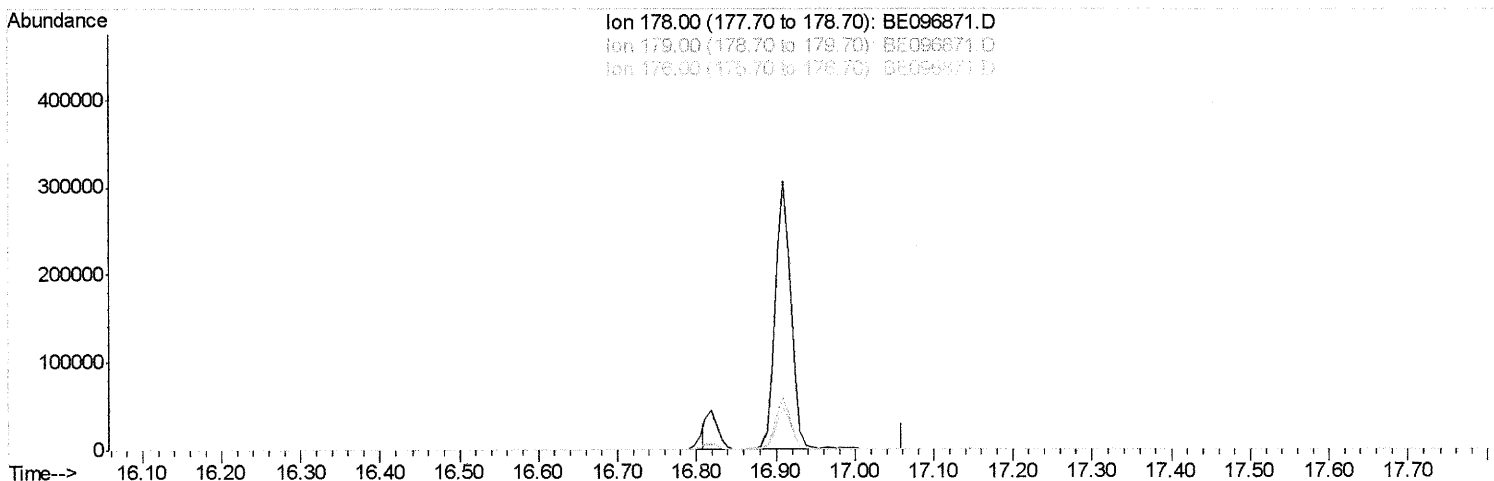

(13) Anthracene

16.909min (-16.909) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	22.60	0.00#
176.00	18.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

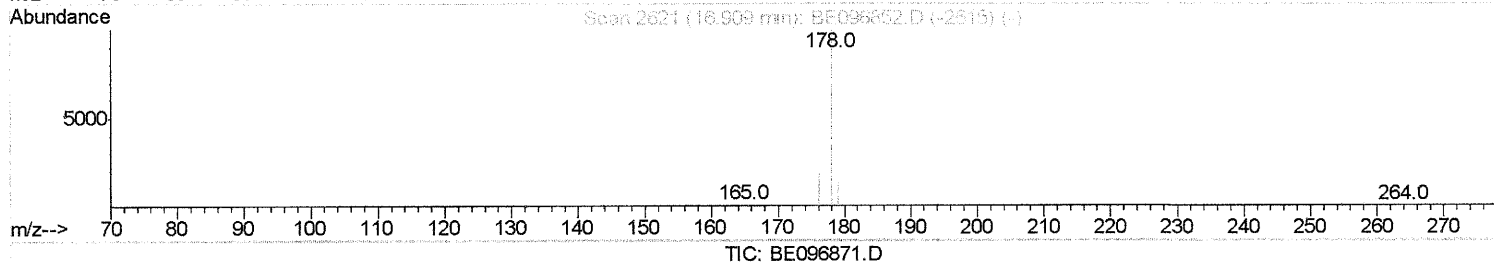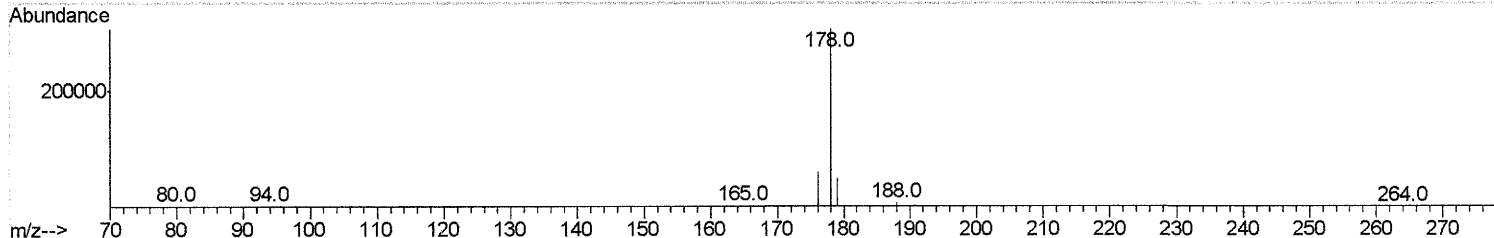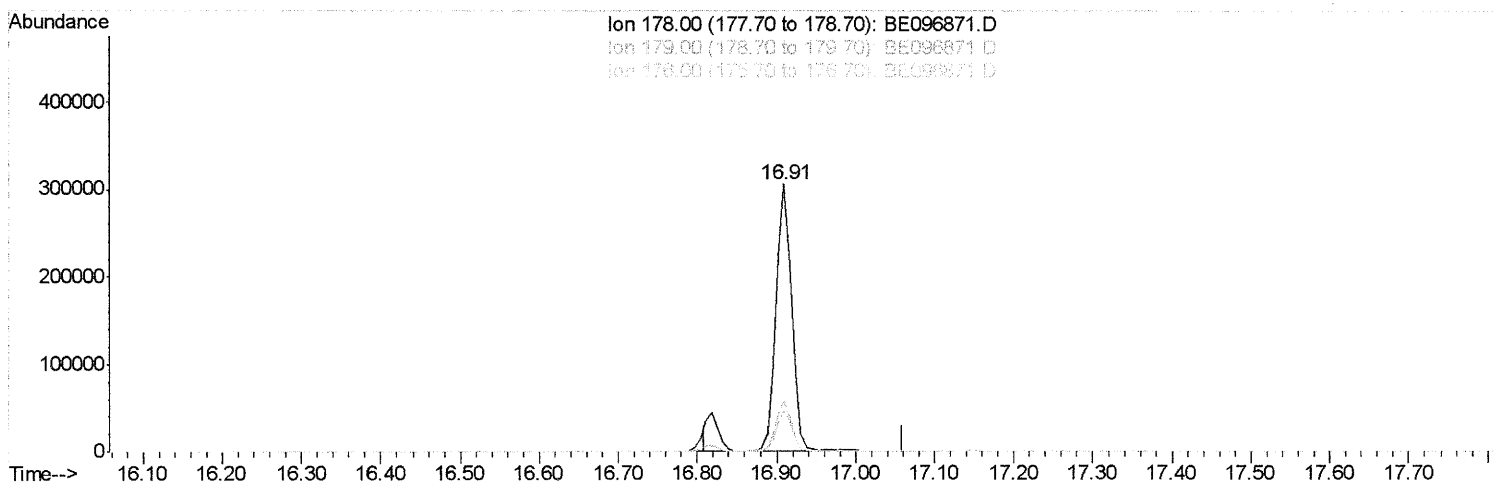

(13) Anthracene

16.909min (-0.000) 6.56ng/ul m

SJ 7/11/18

response 413925

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	15.56#
176.00	18.40	19.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

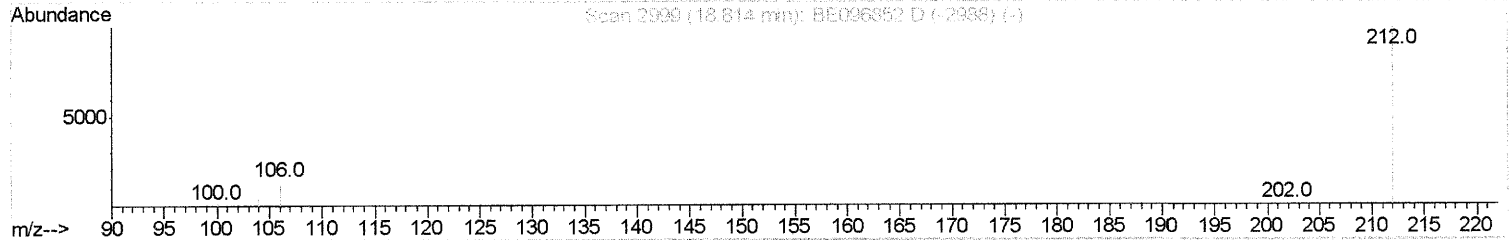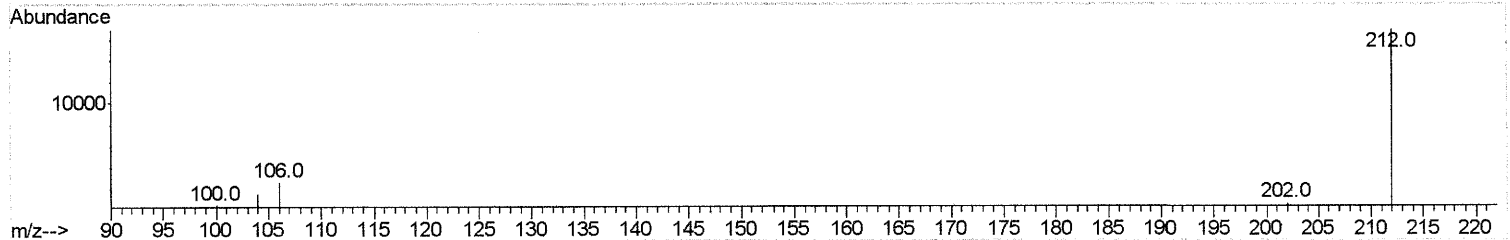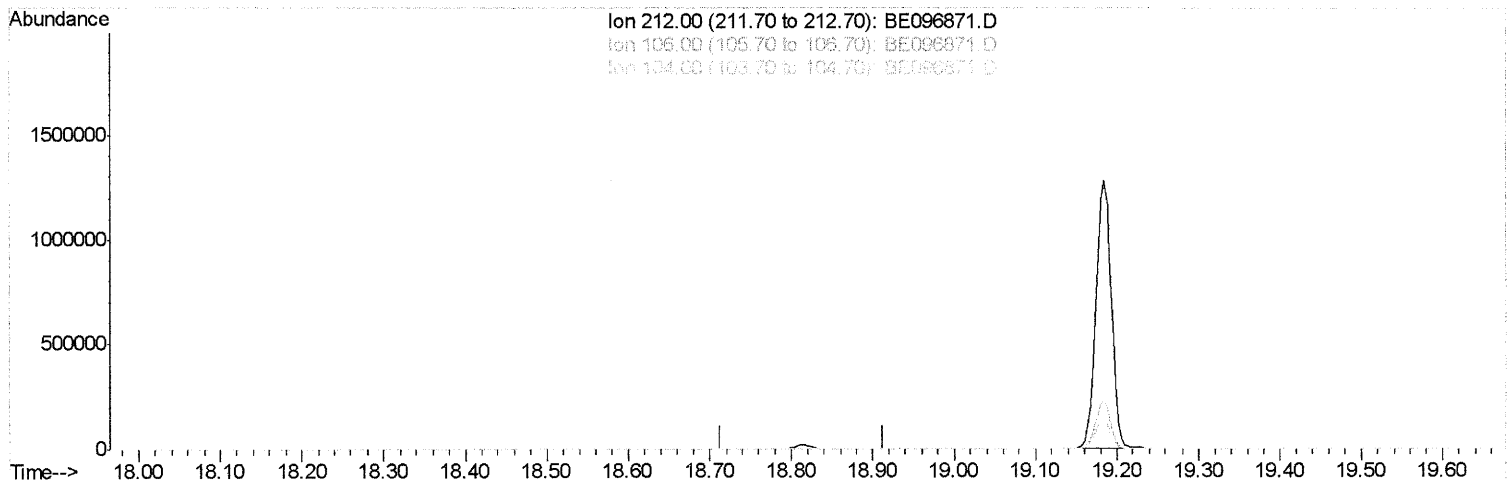

TIC: BE096871.D

(14) Fluoranthene-d10 (SURR)

18.814min (-18.814) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

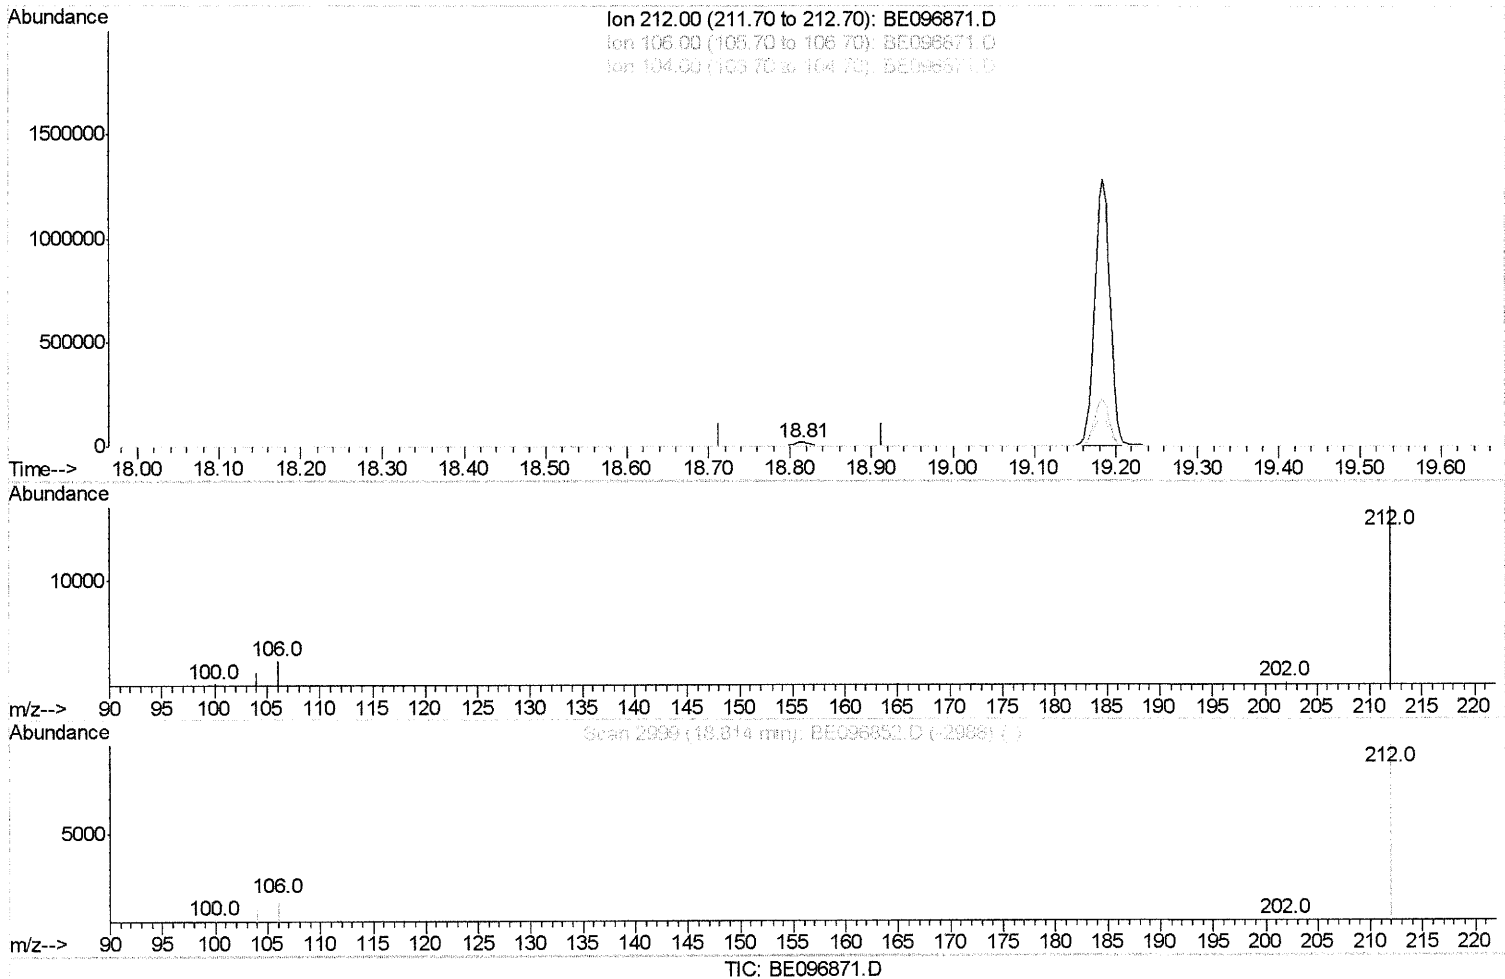

(14) Fluoranthene-d10 (SURR)

18.813min (-0.001) 0.31ng/ul m

SJ 7/11/18

response 22063

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

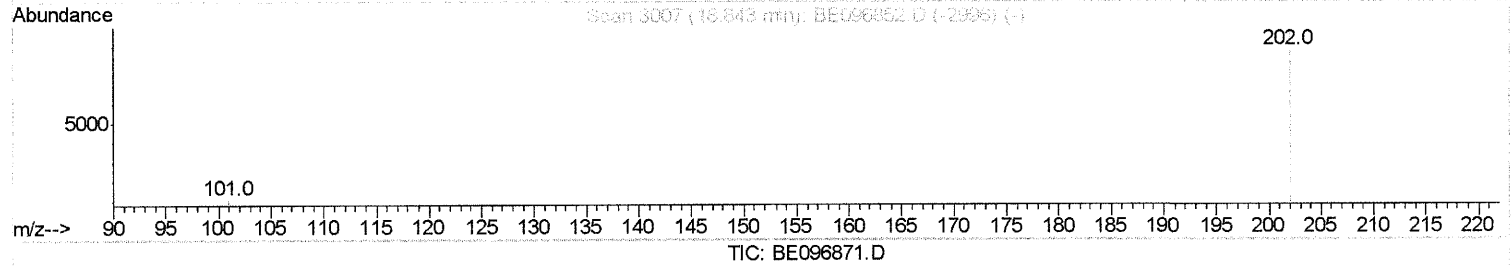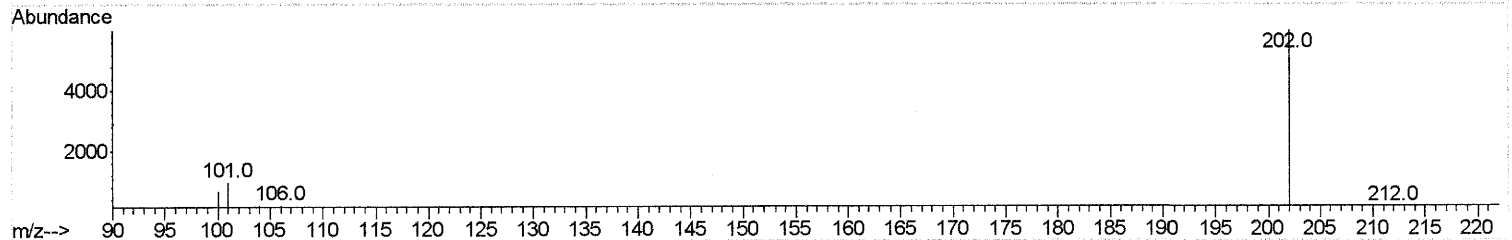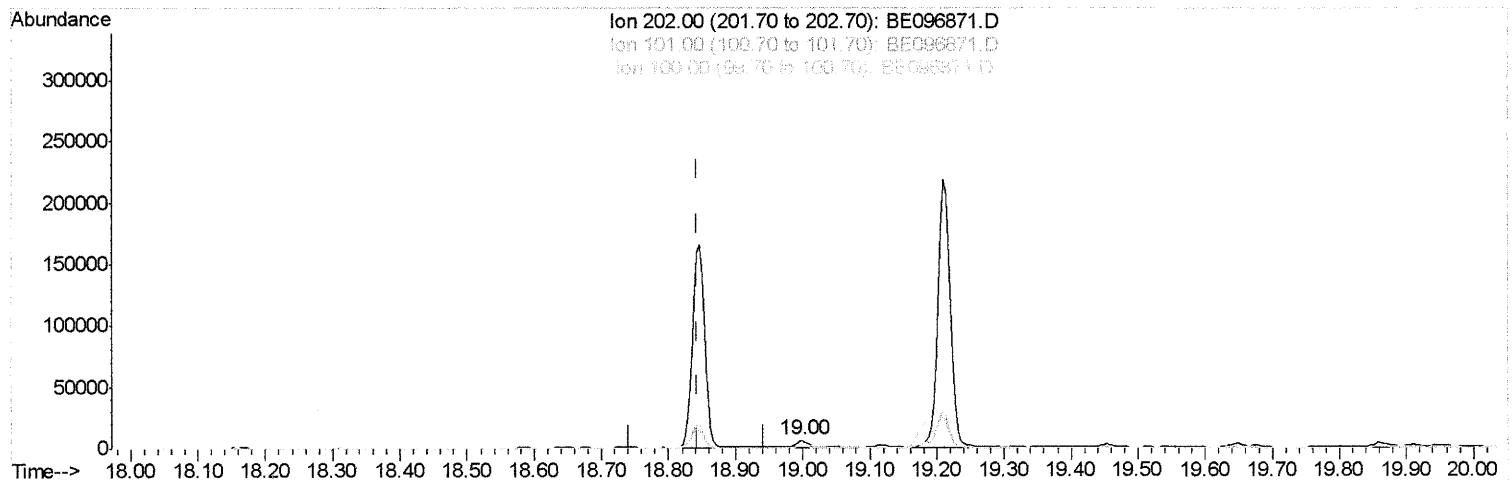

(15) Fluoranthene (C)

18.999min (+0.156) 0.09ng/ul

response 7275

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	16.19
100.00	19.50	11.07
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

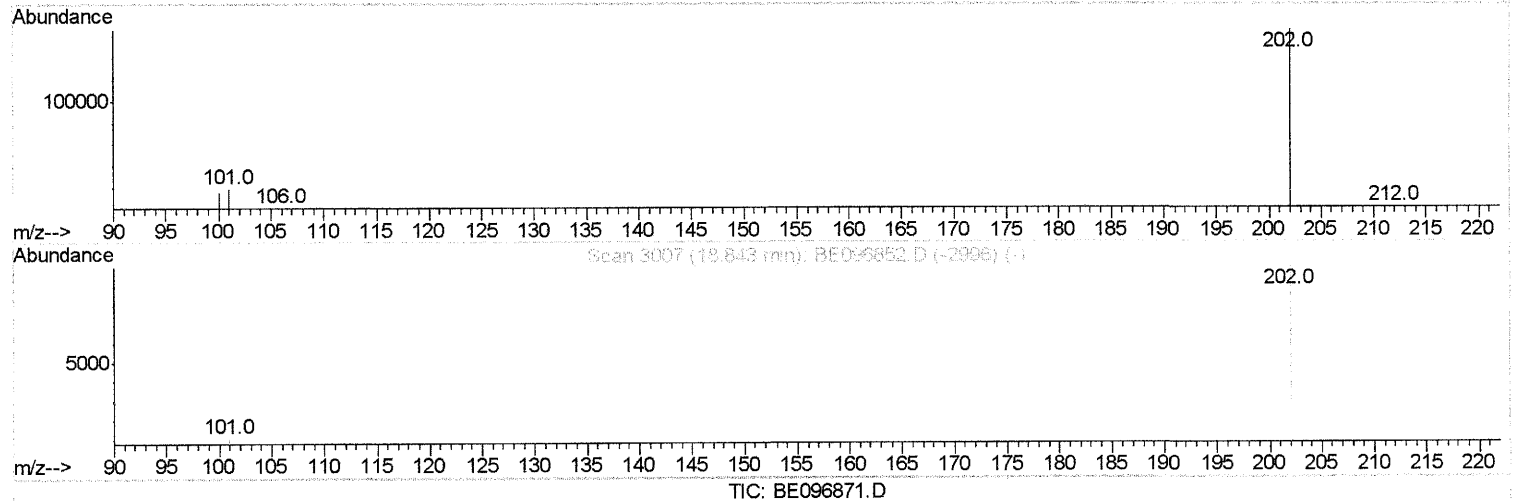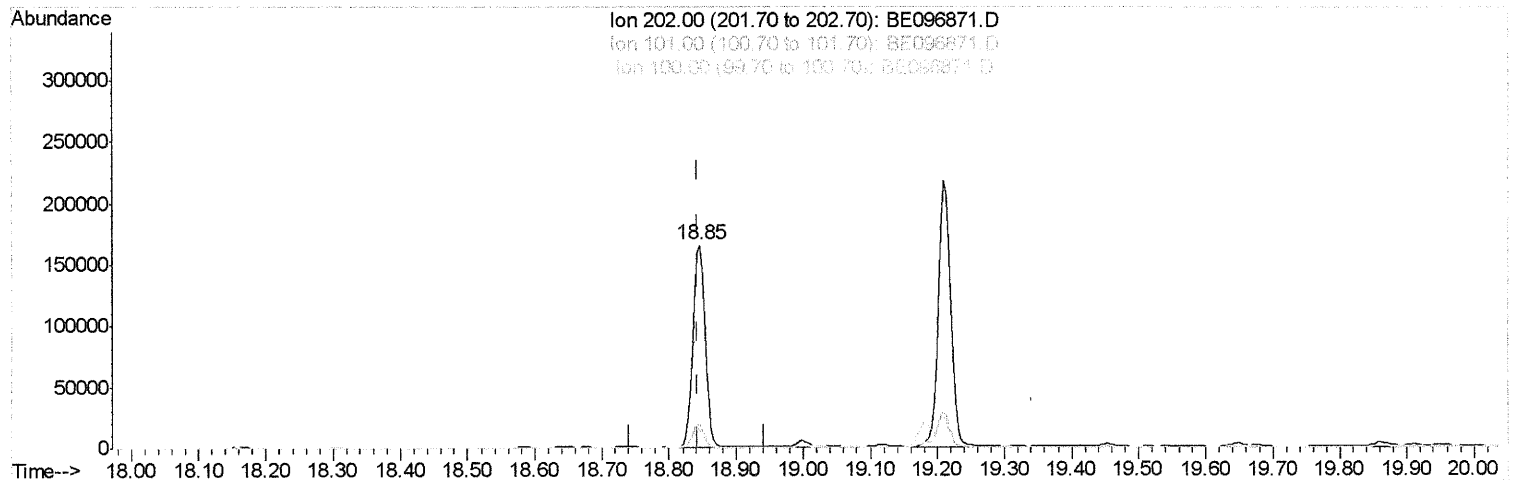

(15) Fluoranthene (C)

18.845min (+0.003) 2.65ng/ul m

SJ 7/11/18

response 209418

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	11.38
100.00	19.50	8.82
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

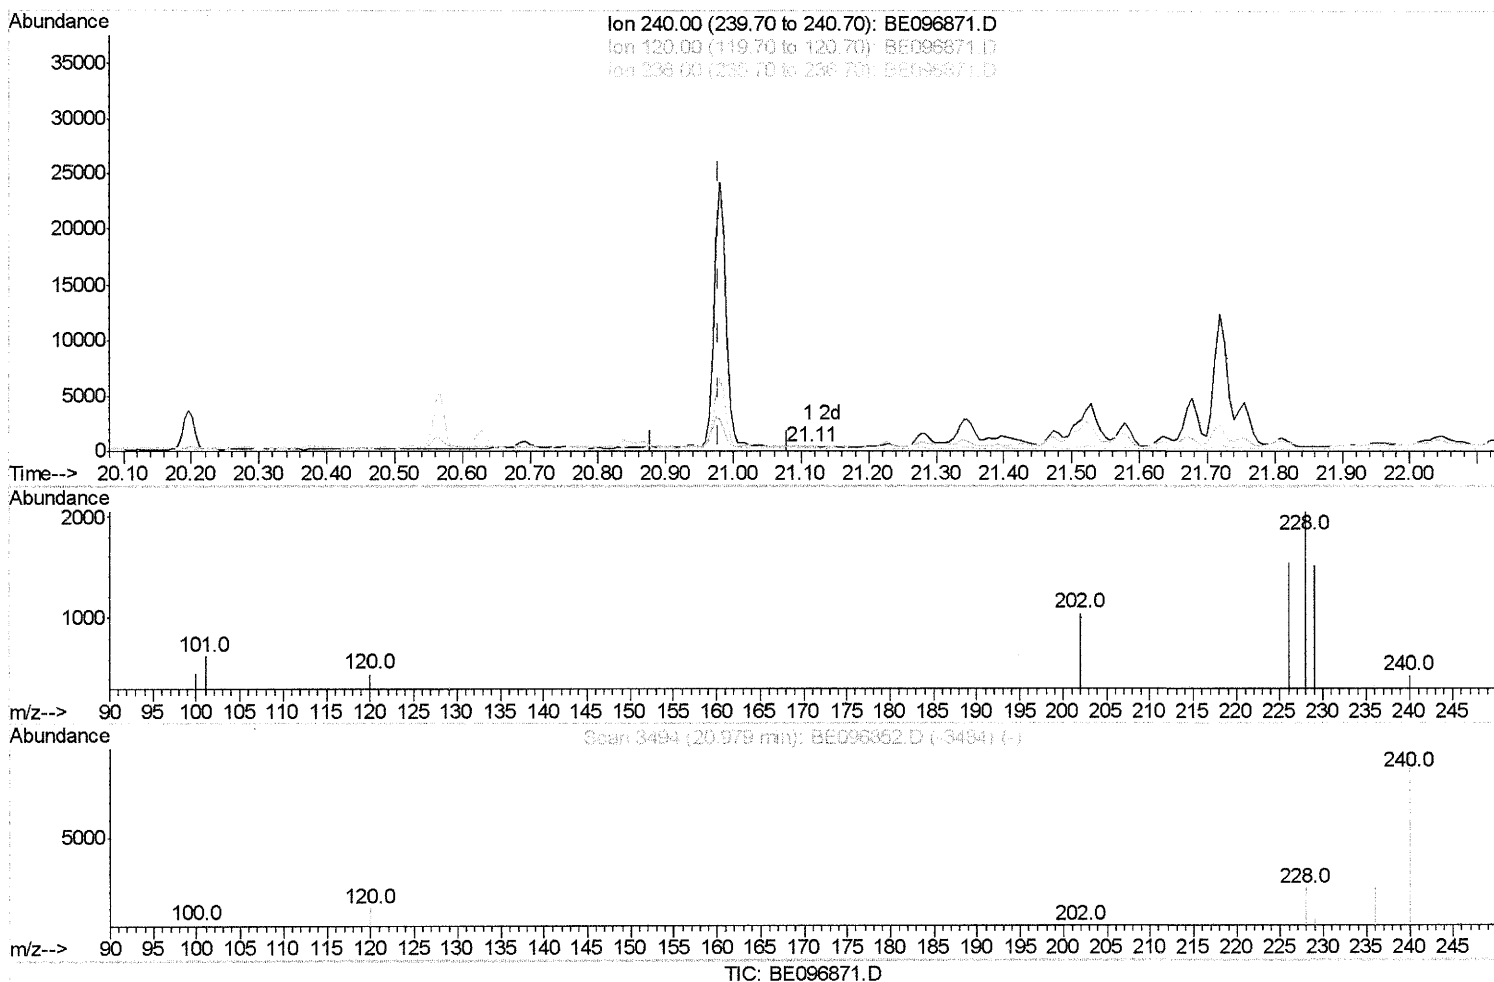

(16) Chrysene-d12 (I)

21.113min (+0.134) 0.40ng/ul

response 103

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	105.58#
236.00	34.90	72.09#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

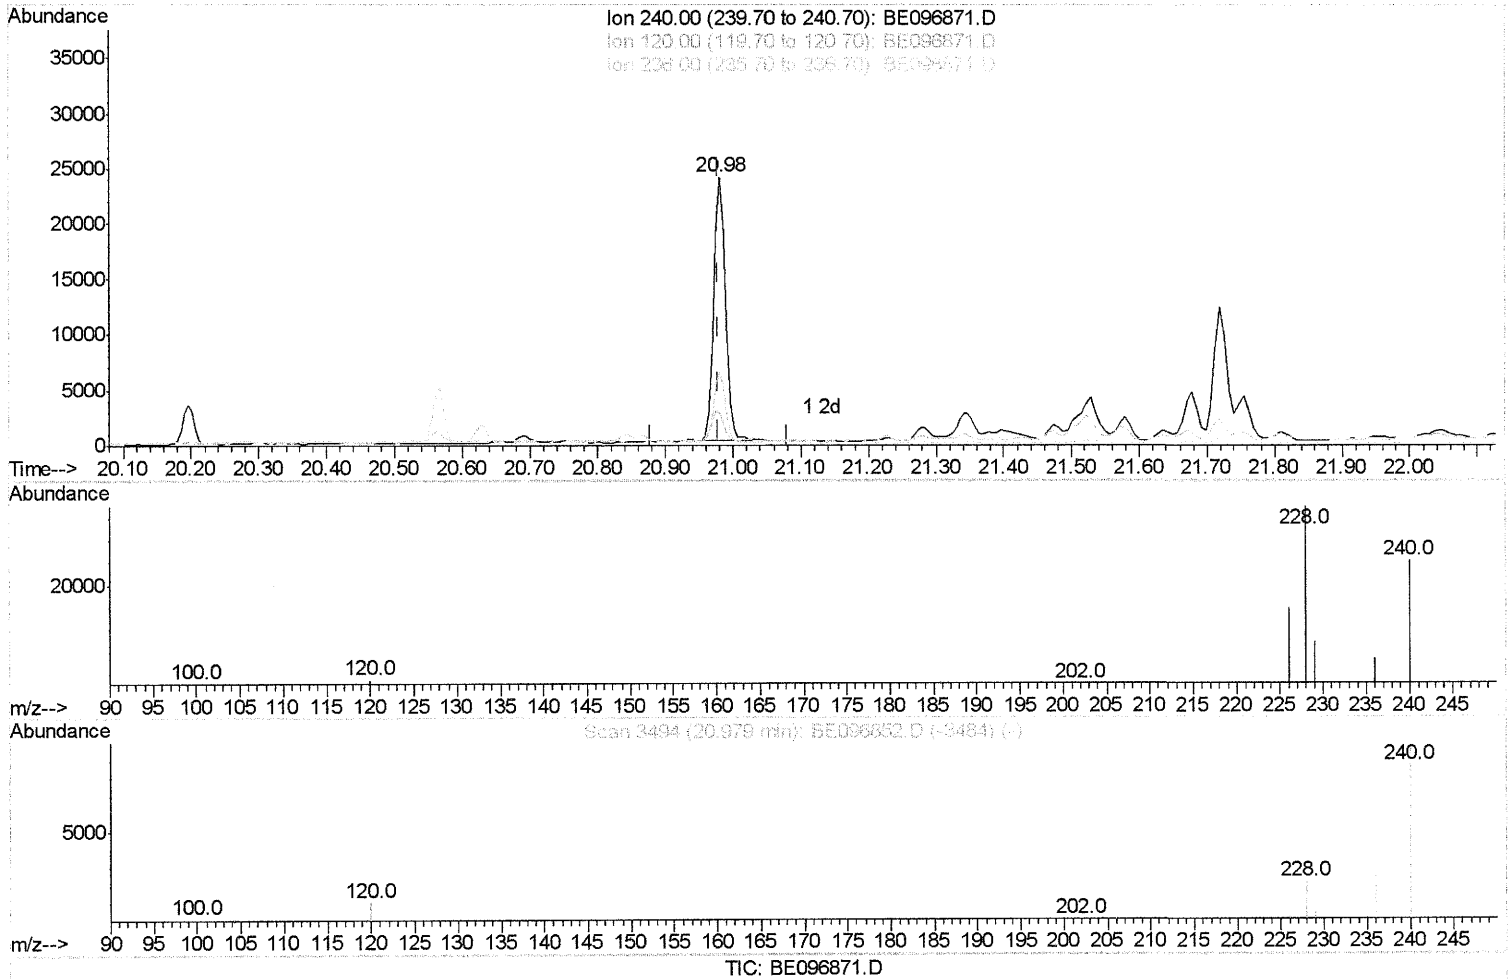

(16) Chrysene-d12 (I)

20.980min (+0.001) 0.40ng/ul m

SJ 7/11/18

response 28348

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.24#
236.00	34.90	27.18#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

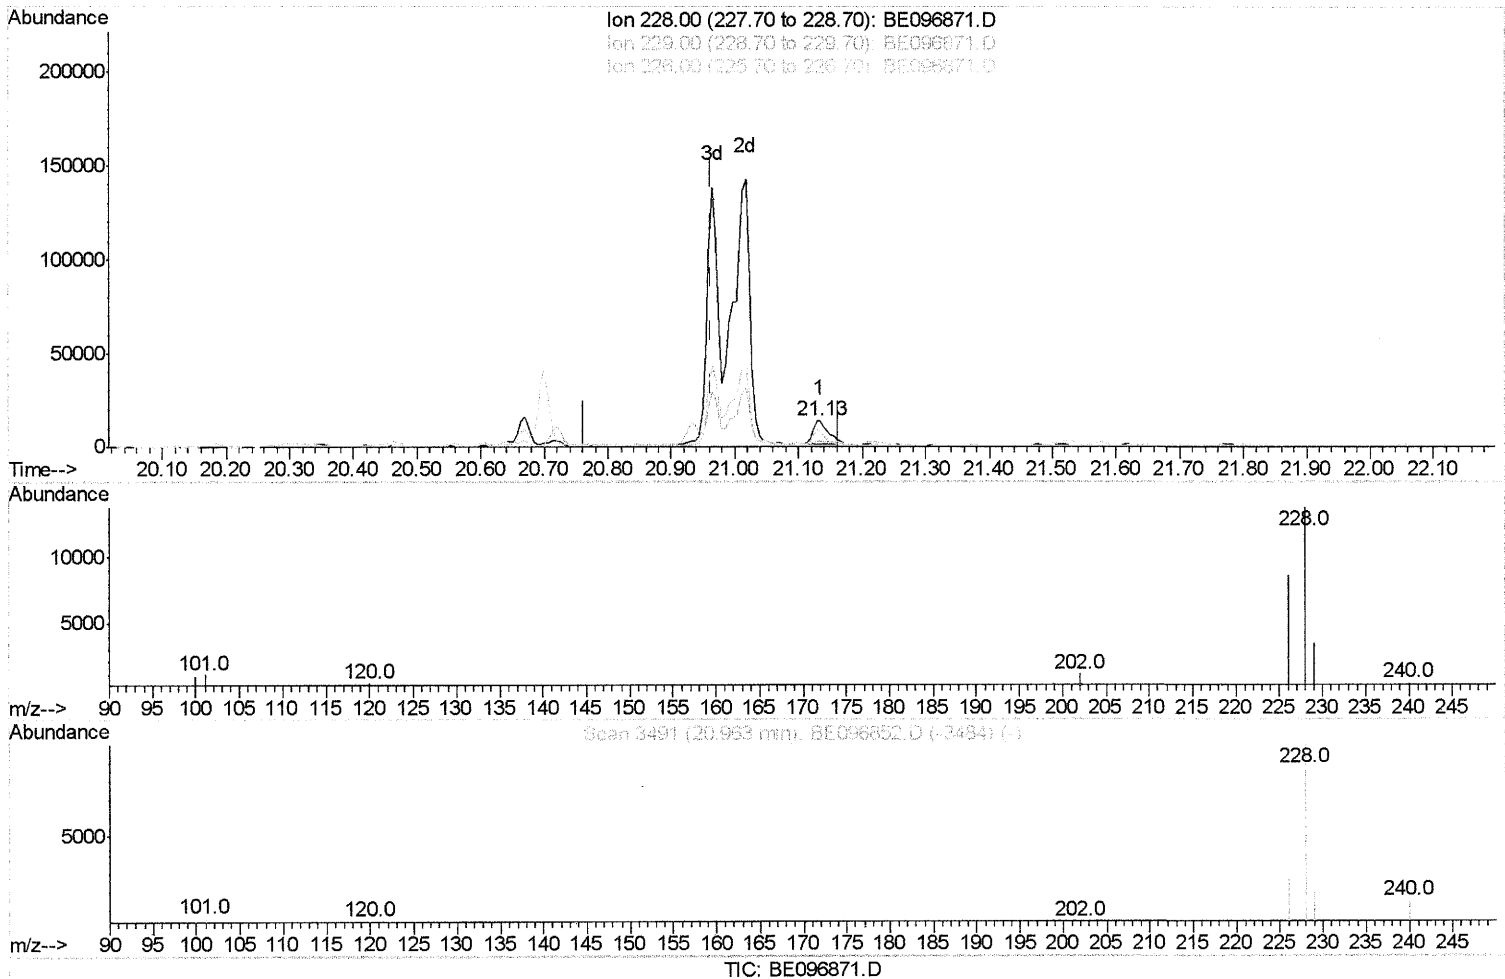

(18) Benzo(a)anthracene
 21.134min (+0.171) 0.32ng/ul
 response 21529

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	25.15
226.00	21.30	62.24#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:43:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

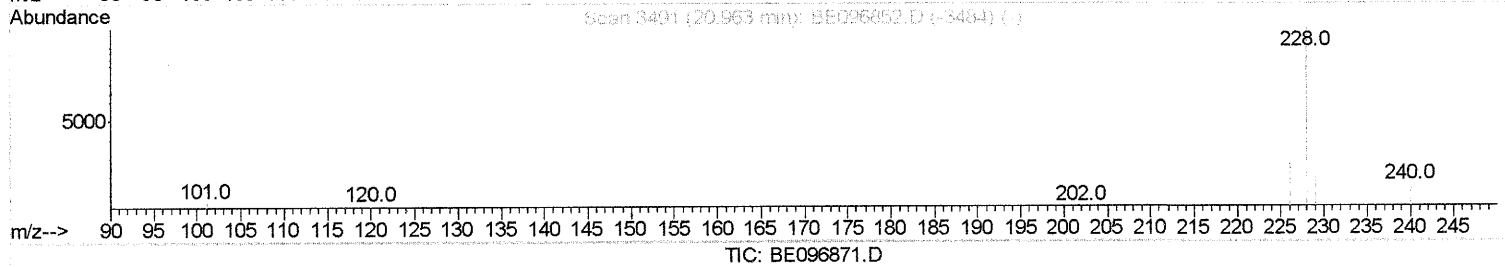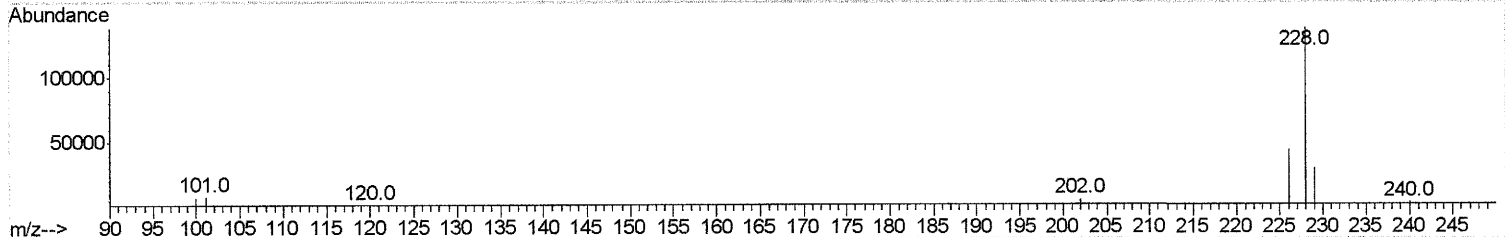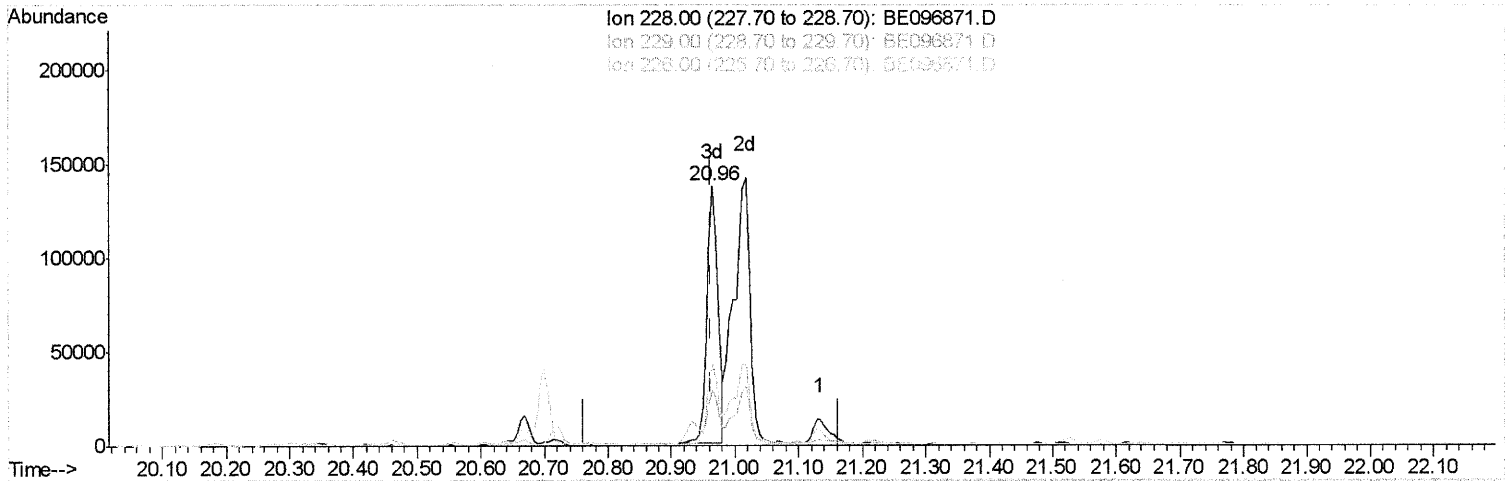

(18) Benzo(a)anthracene

20.964min (+0.001) 2.50ng/ul m

SJ 7/11/18

response 167292

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	21.50#
226.00	21.30	31.26#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:45:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

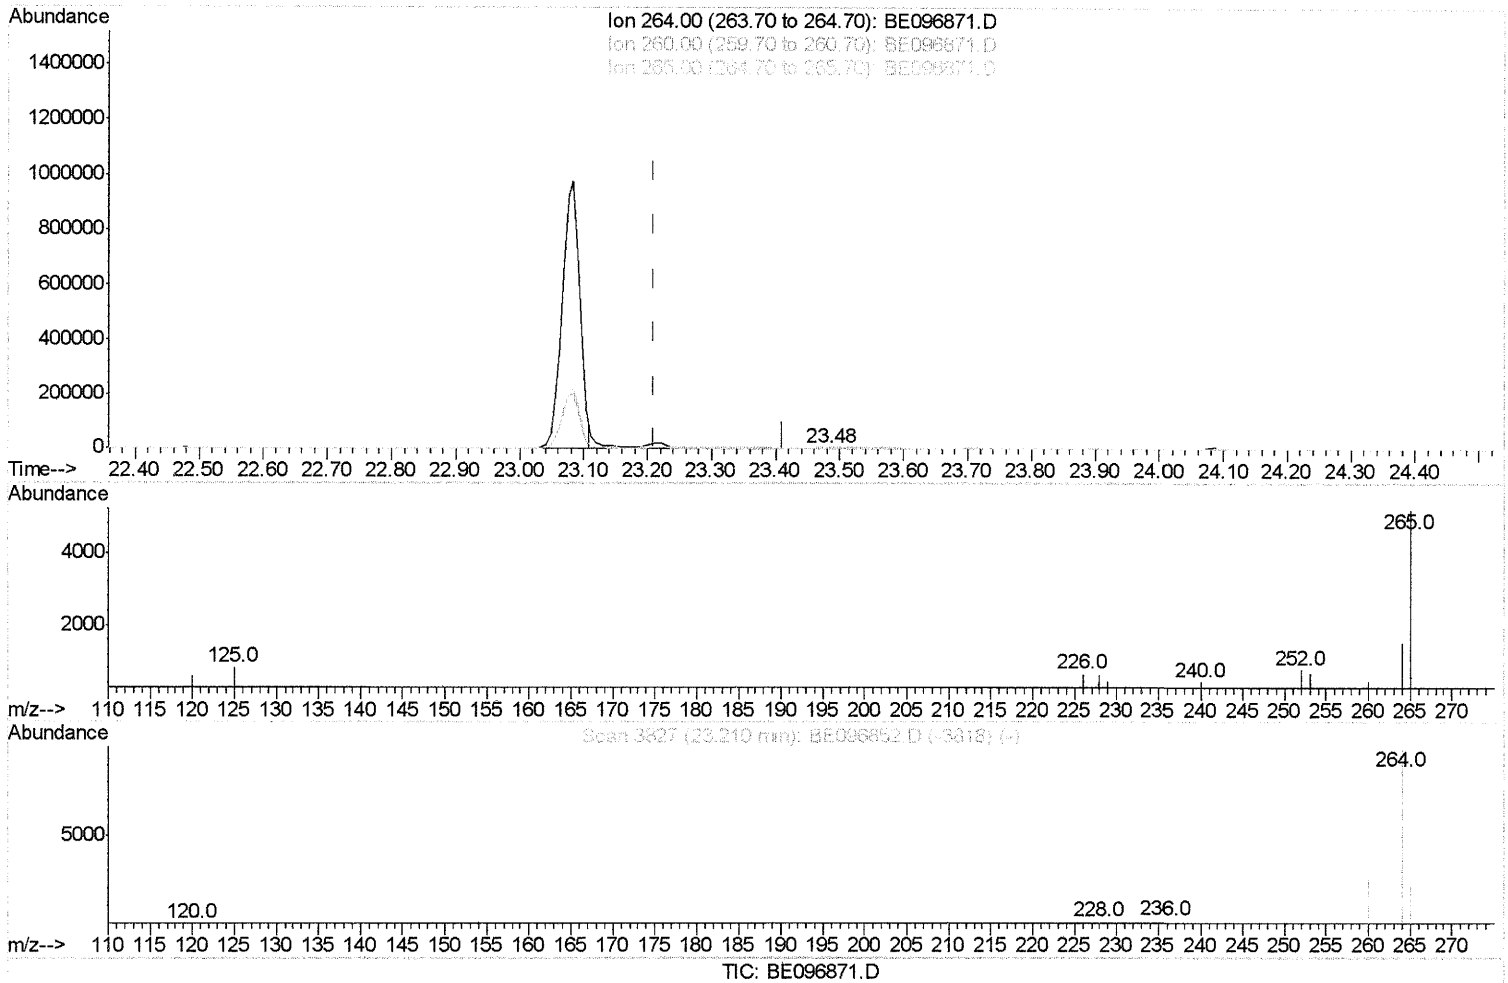

(20) Perylene-d12 (I)

23.484min (+0.273) 0.40ng/ul

response 1556

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.57
265.00	103.50	341.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:48:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

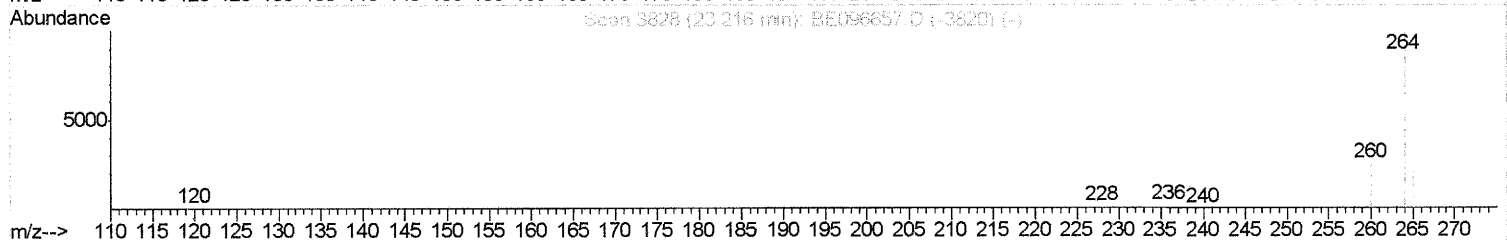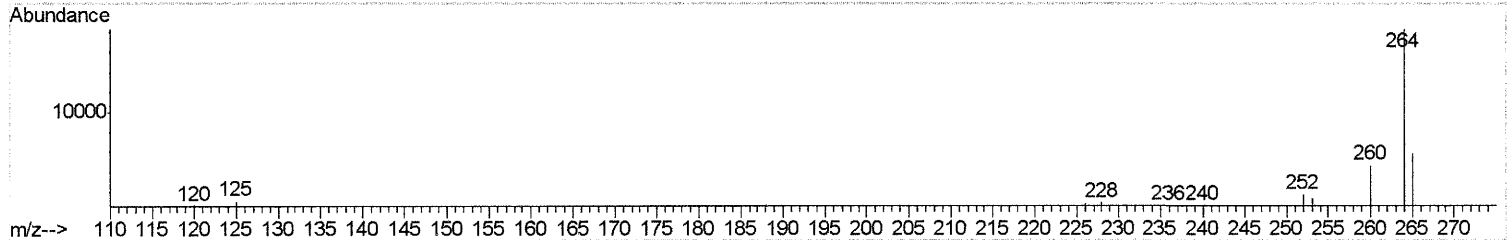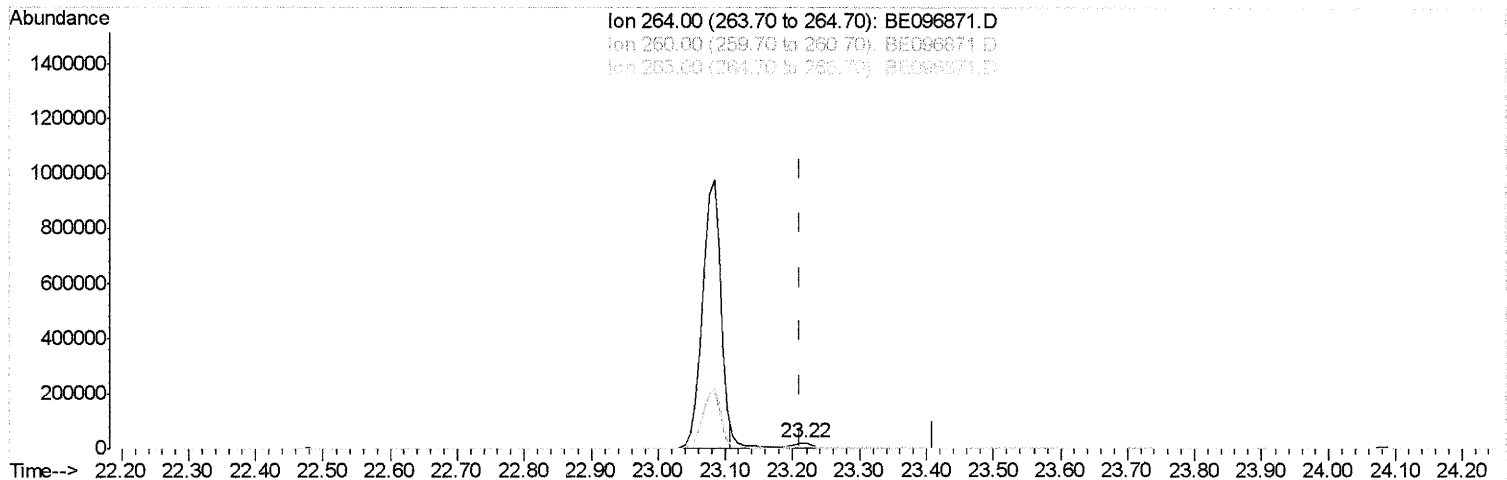

TIC: BE096871.D

(20) Perylene-d12 (I)

23.216min (+0.006) 0.40ng/ul m

response 27110

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.20
265.00	103.50	31.63#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

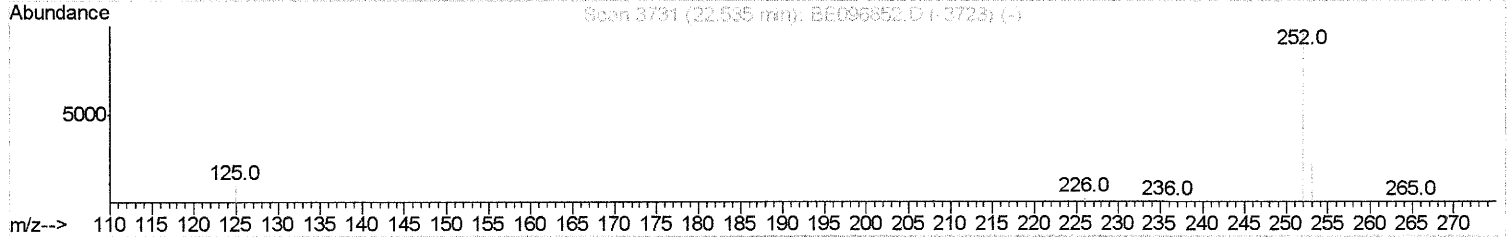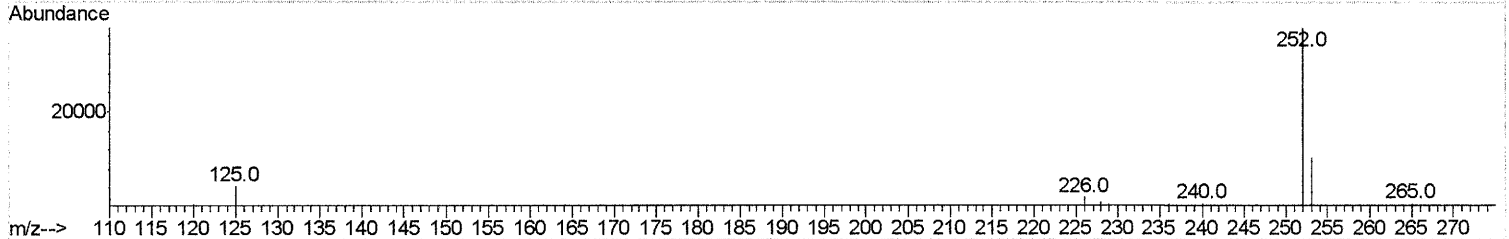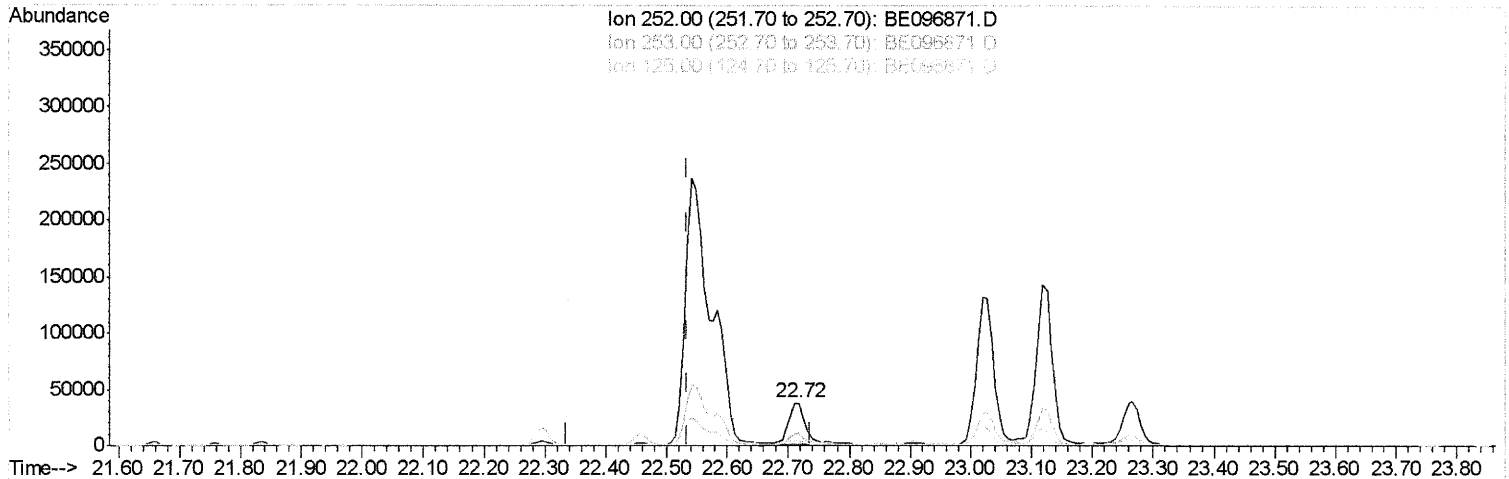

TIC: BE096871.D

(21) Benzo(b)fluoranthene

22.717min (+0.182) 0.89ng/ul

response 74757

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.39
125.00	17.50	11.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

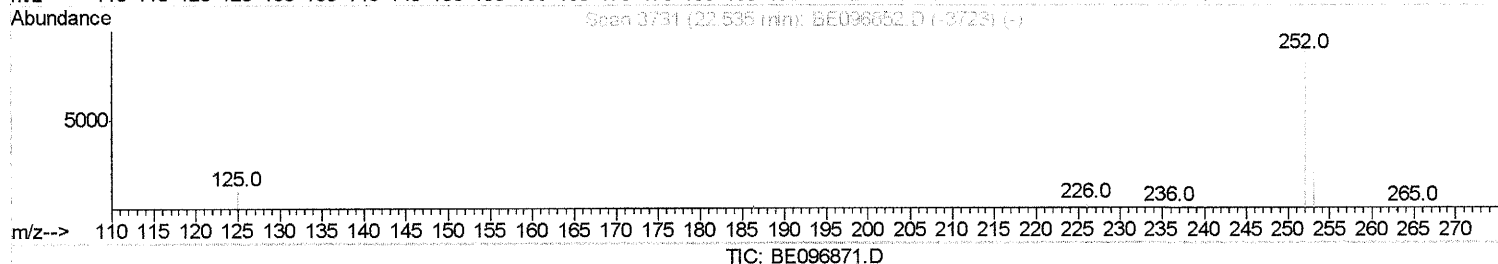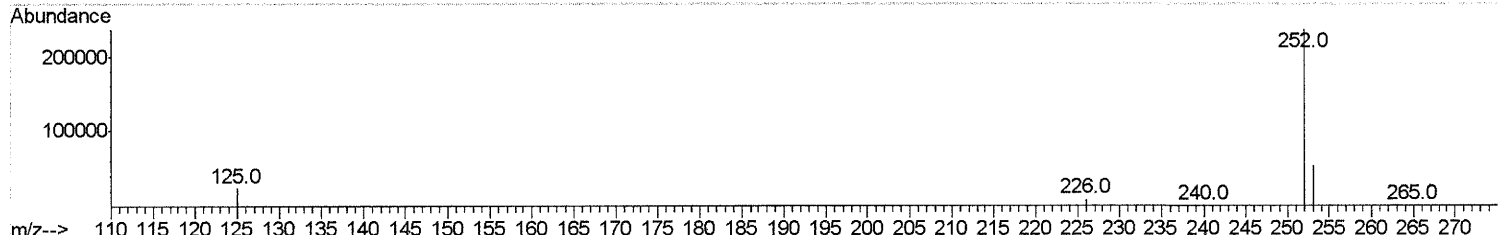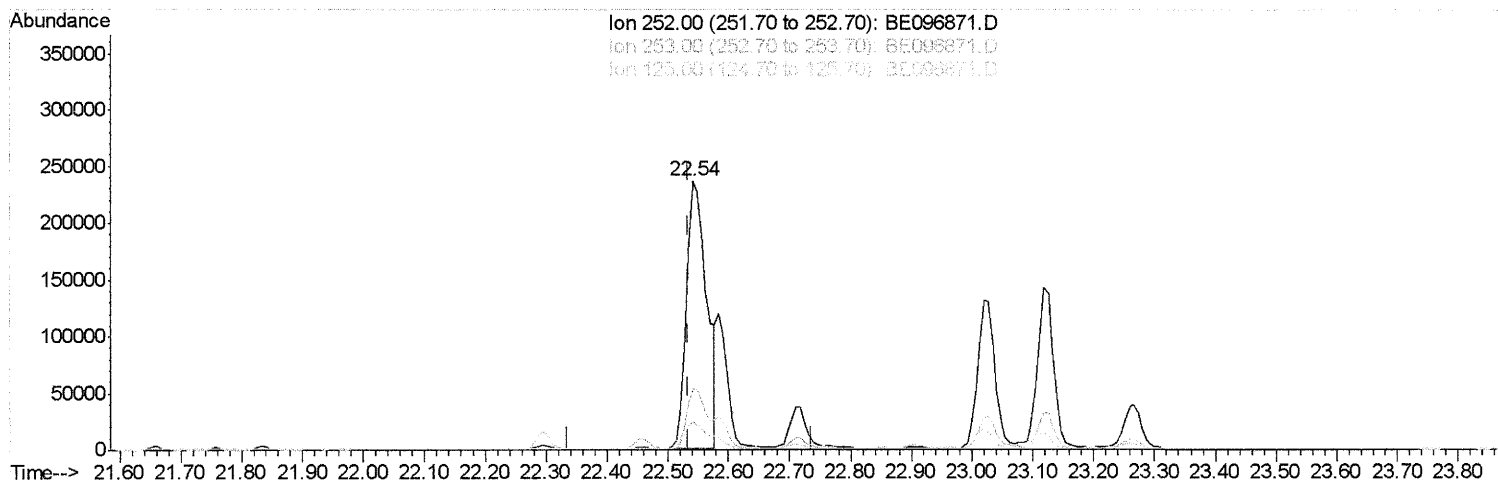

(21) Benzo(b)fluoranthene

22.541min (+0.006) 6.61ng/ul m

SJ 7/11/18

response 557250

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.84
125.00	17.50	10.29
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

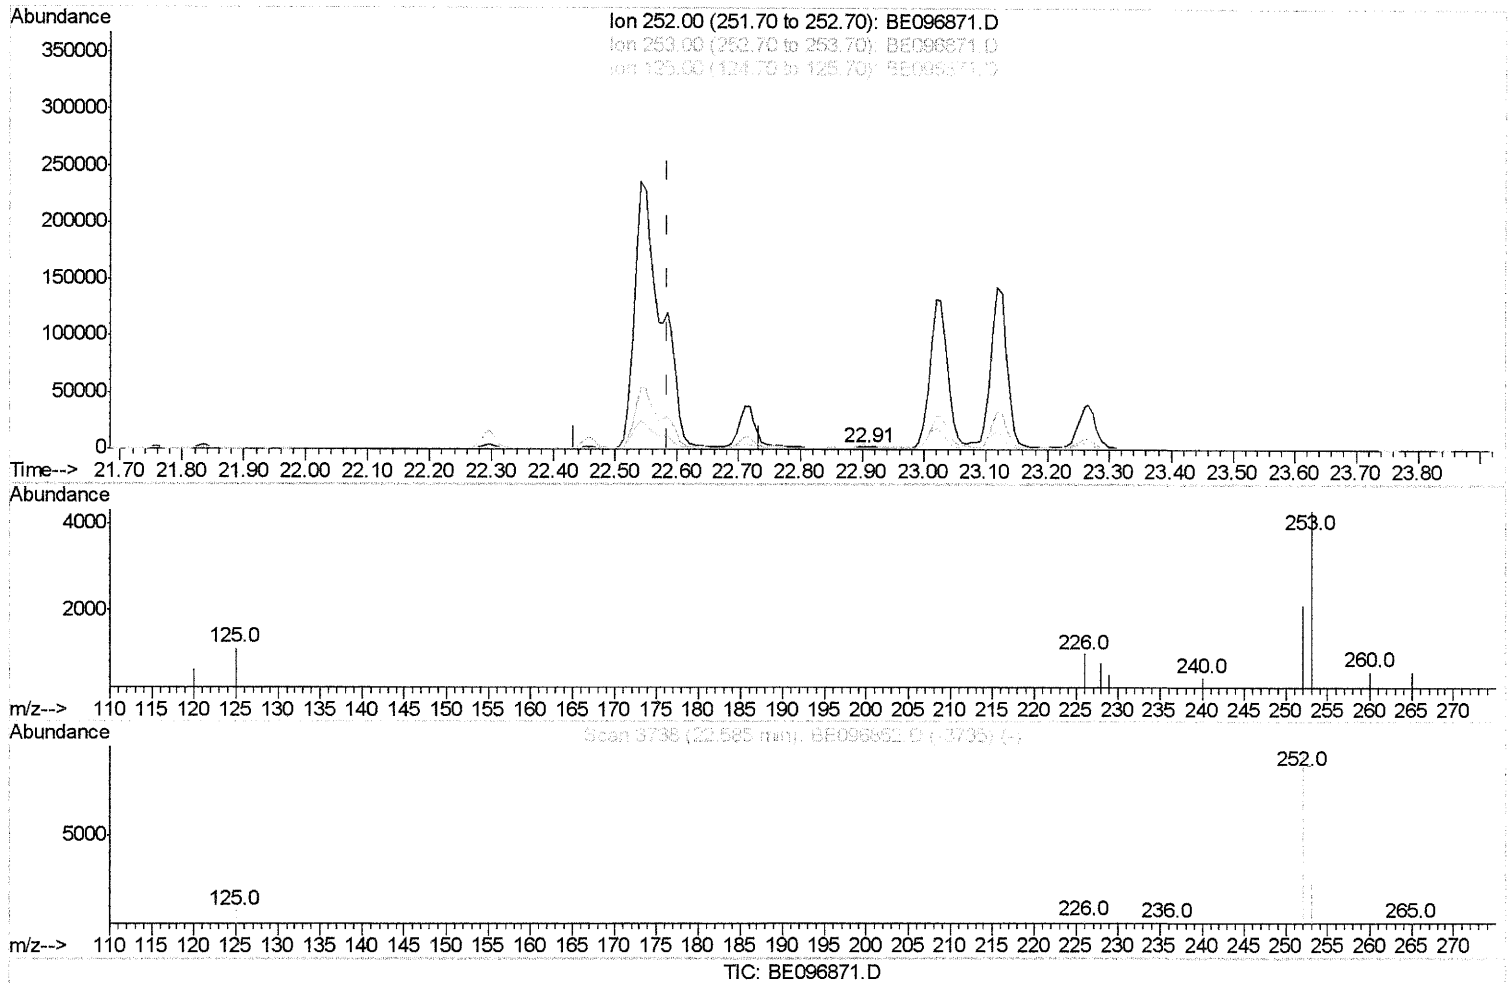

(22) Benzo(k)fluoranthene

22.907min (+0.322) 0.02ng/ul

response 2020

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	205.27#
125.00	17.10	52.11#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

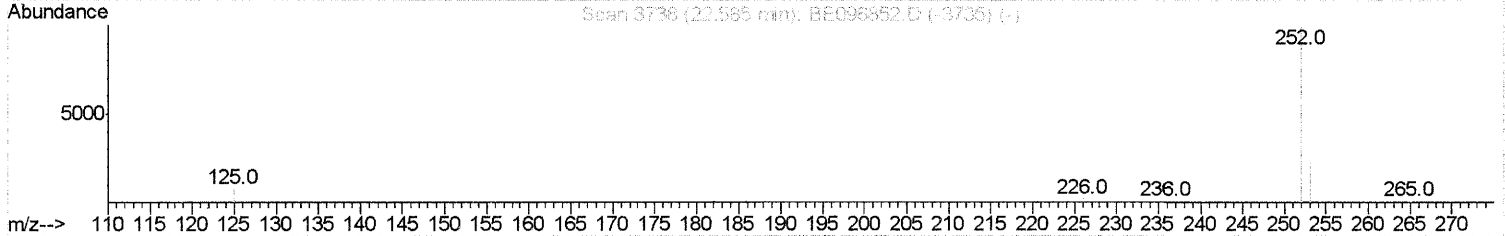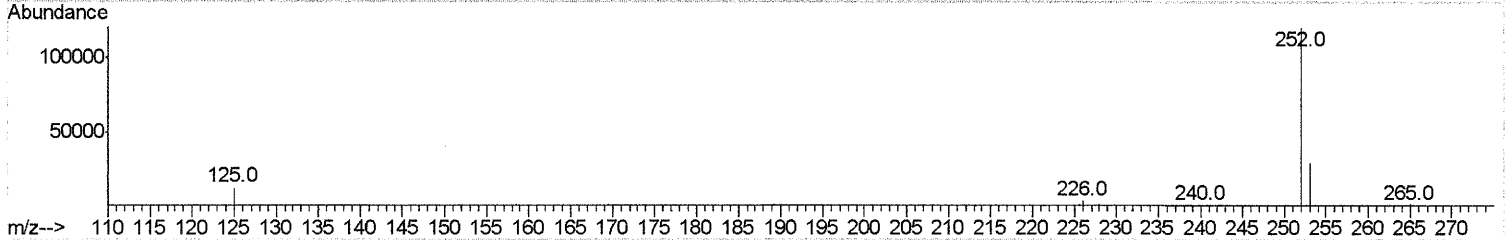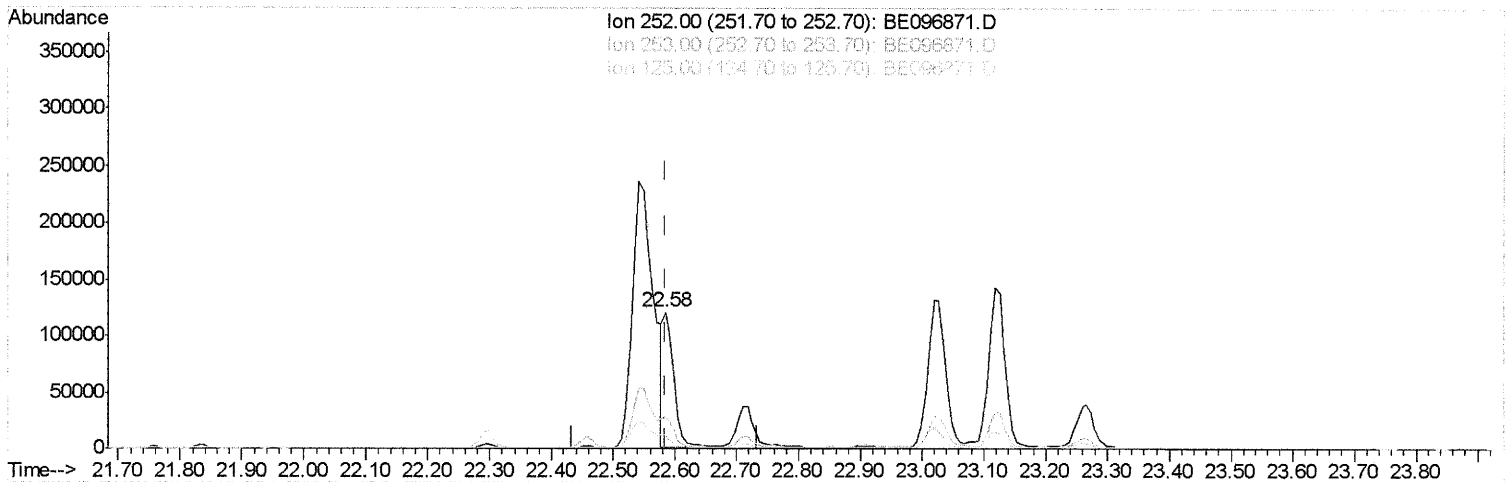

TIC: BE096871.D

(22) Benzo(k)fluoranthene

22.584min (-0.001) 1.51ng/ul m

response 139133

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.97#
125.00	17.10	9.89#
0.00	0.00	0.00

SJ 7/11/18

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

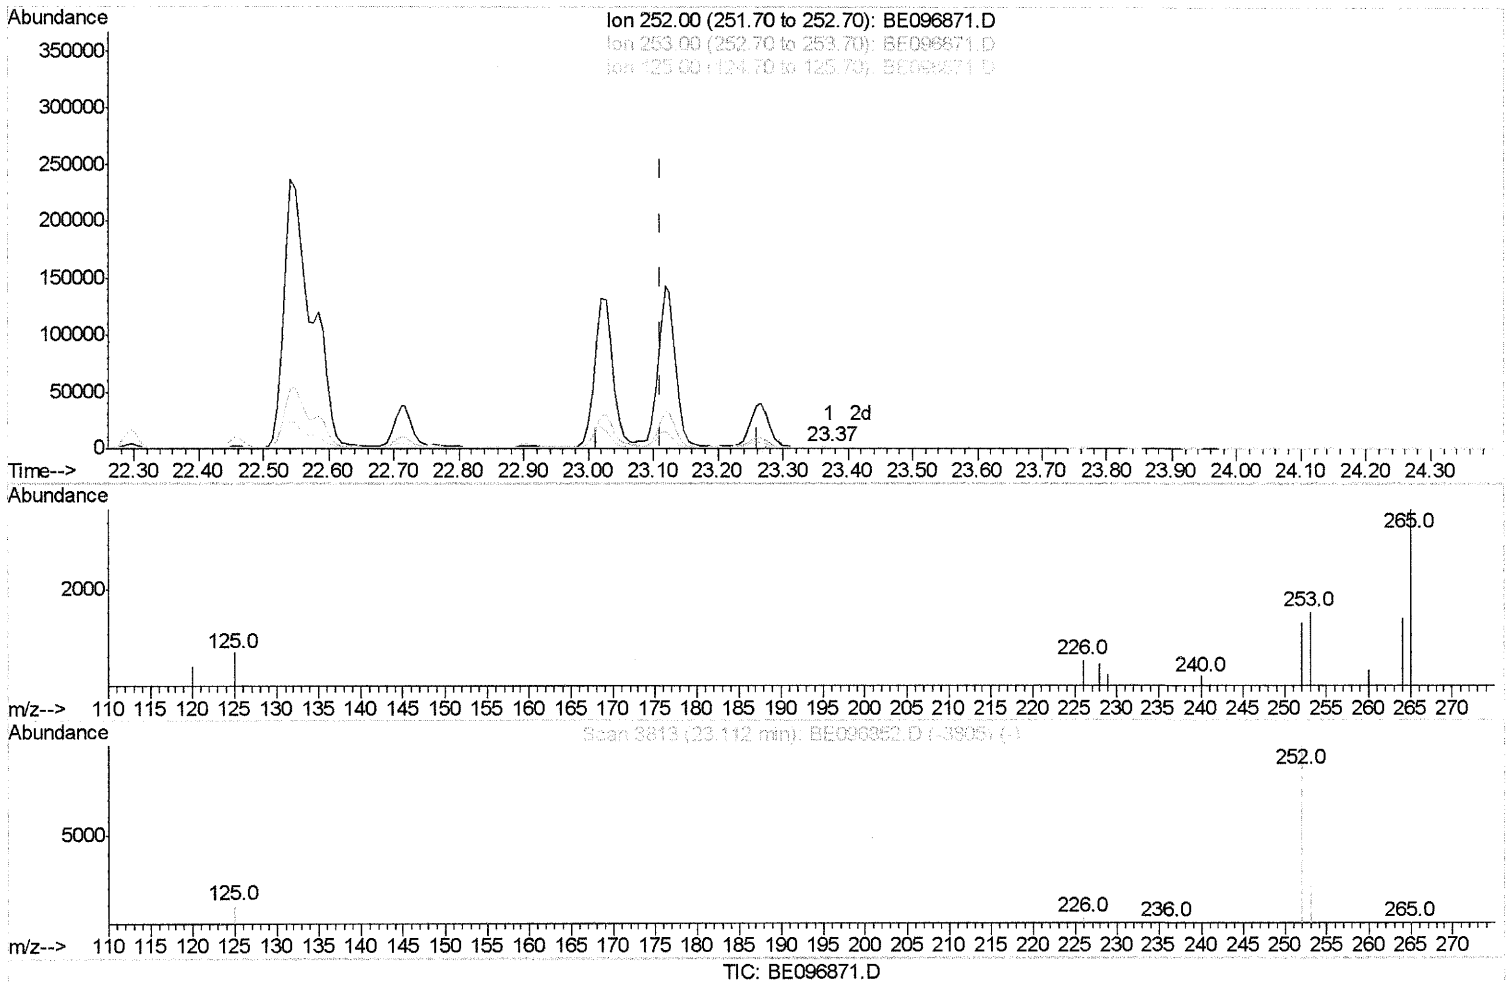

(23) Benzo(a)pyrene (C)
 23.371min (+0.259) 0.01ng/ul
 response 763

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	113.75#
125.00	22.60	62.61#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

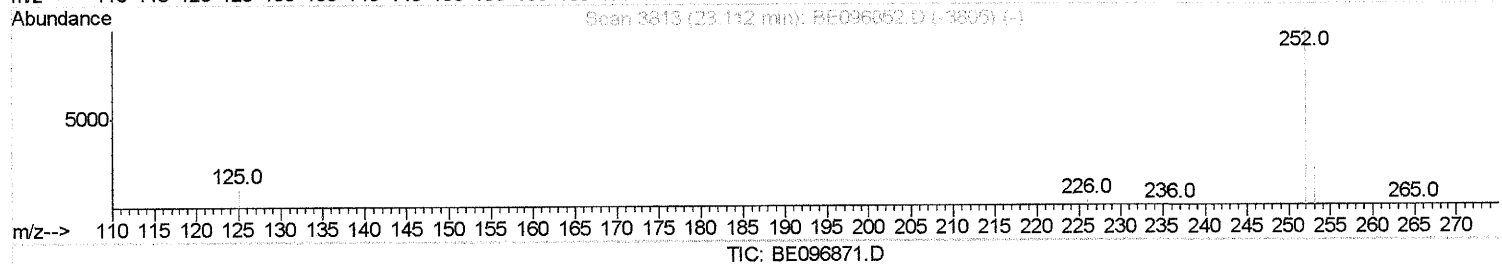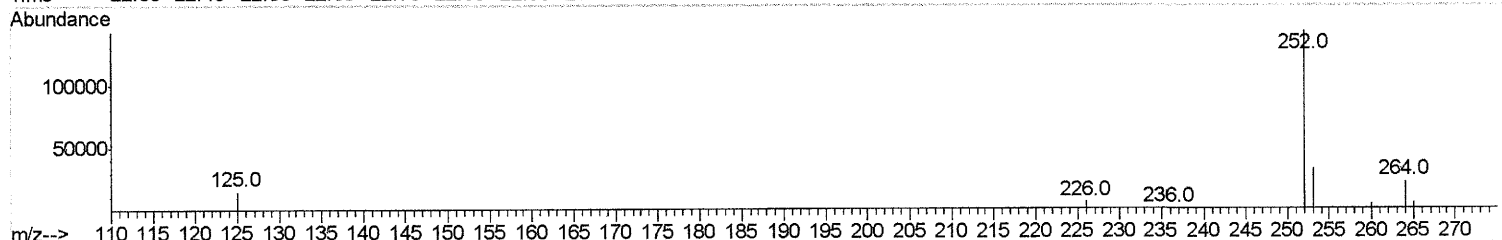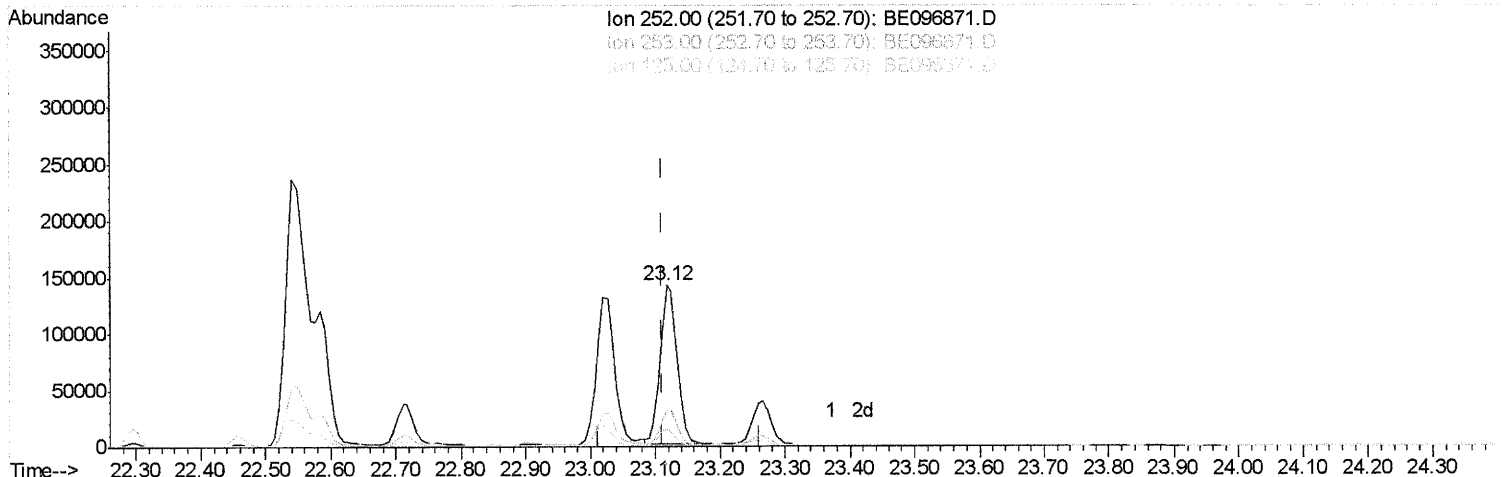

(23) Benzo(a)pyrene (C)

23.118min (+0.006) 3.54ng/ul m

response 252483

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.07#
125.00	22.60	10.92#
0.00	0.00	0.00

SJ 7/11/18

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

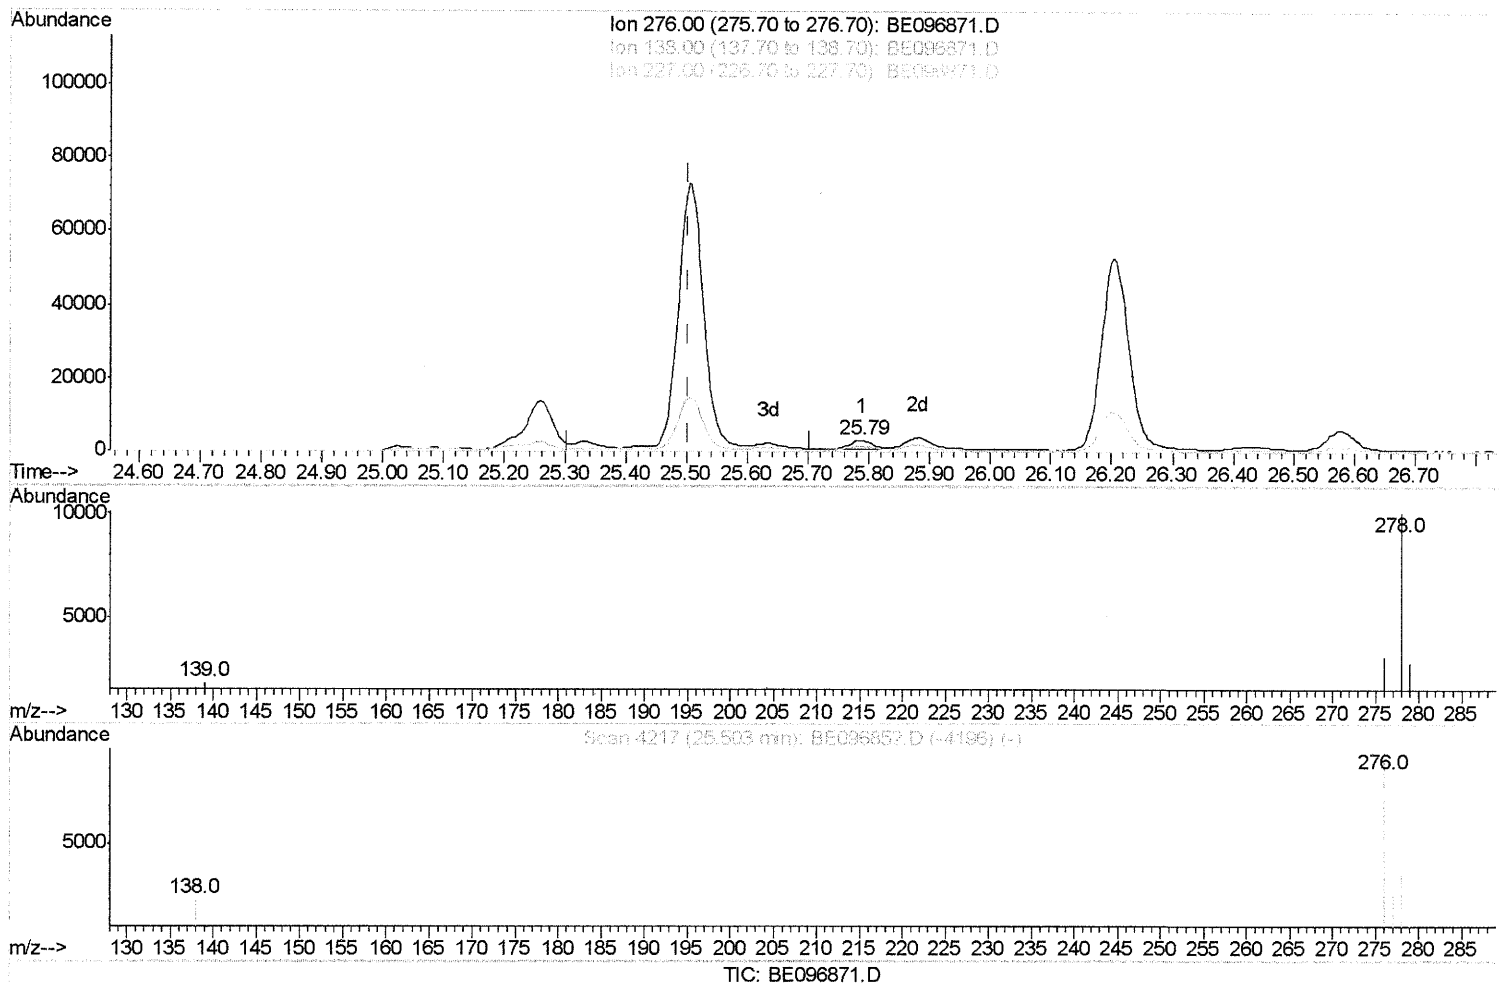

(24) Indeno(1,2,3-cd)pyrene

25.789min (+0.286) 0.09ng/ul

response 7024

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	50.88#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

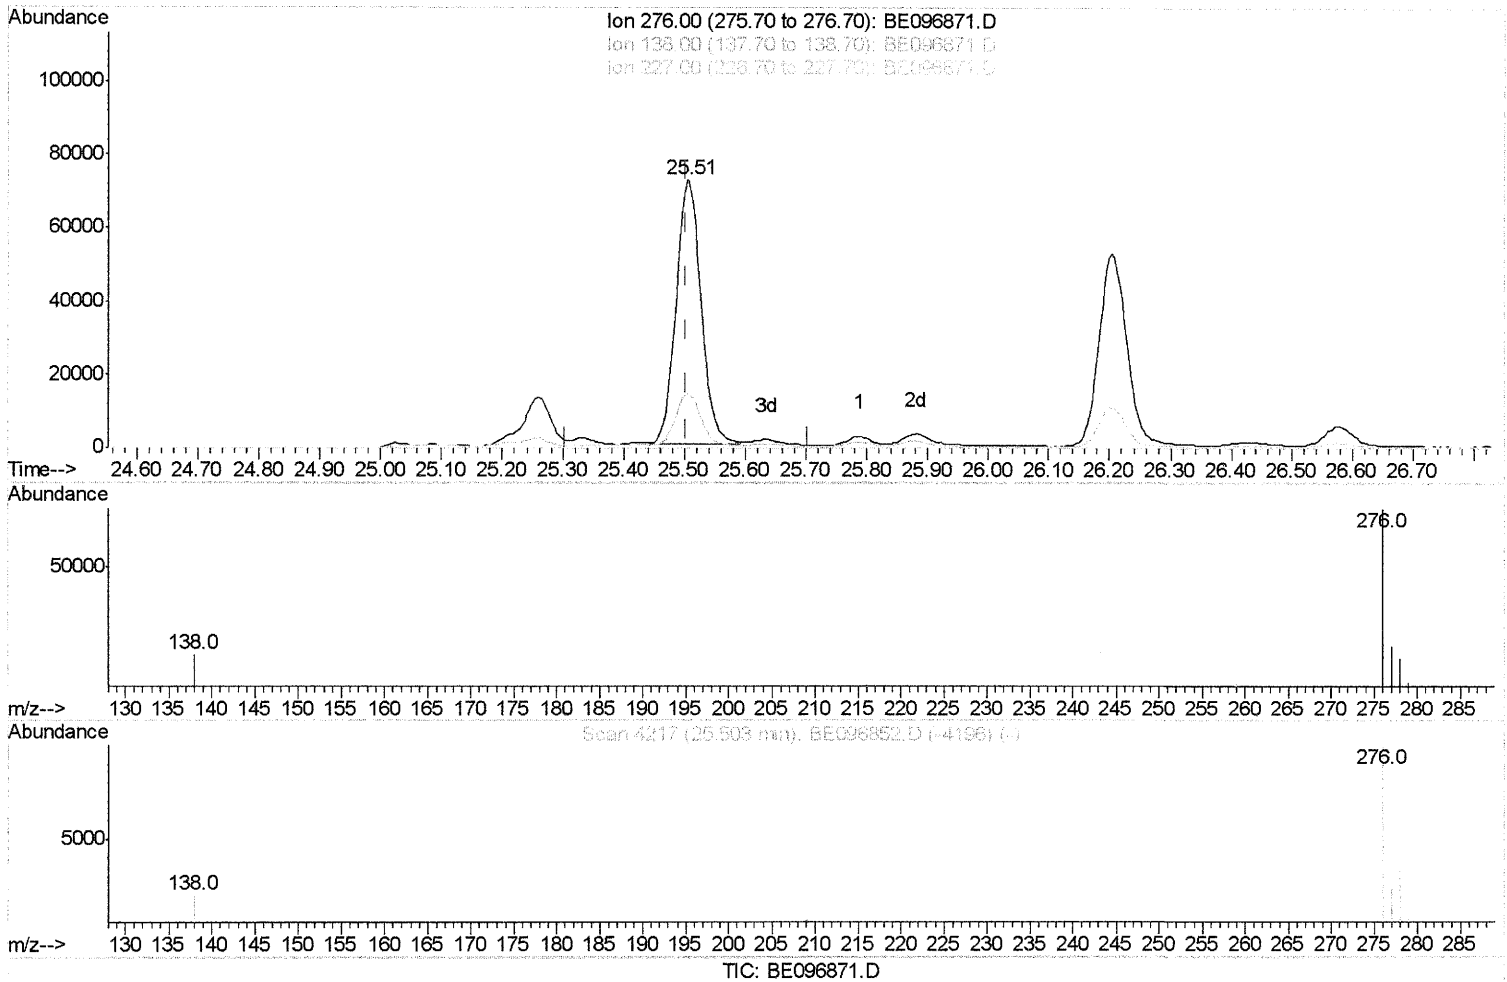

(24) Indeno(1,2,3-cd)pyrene

25.507min (+0.004) 2.78ng/ul m

response 206021

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	1.73#
227.00	10.00	0.00#
0.00	0.00	0.00

SJ 7/11/18

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

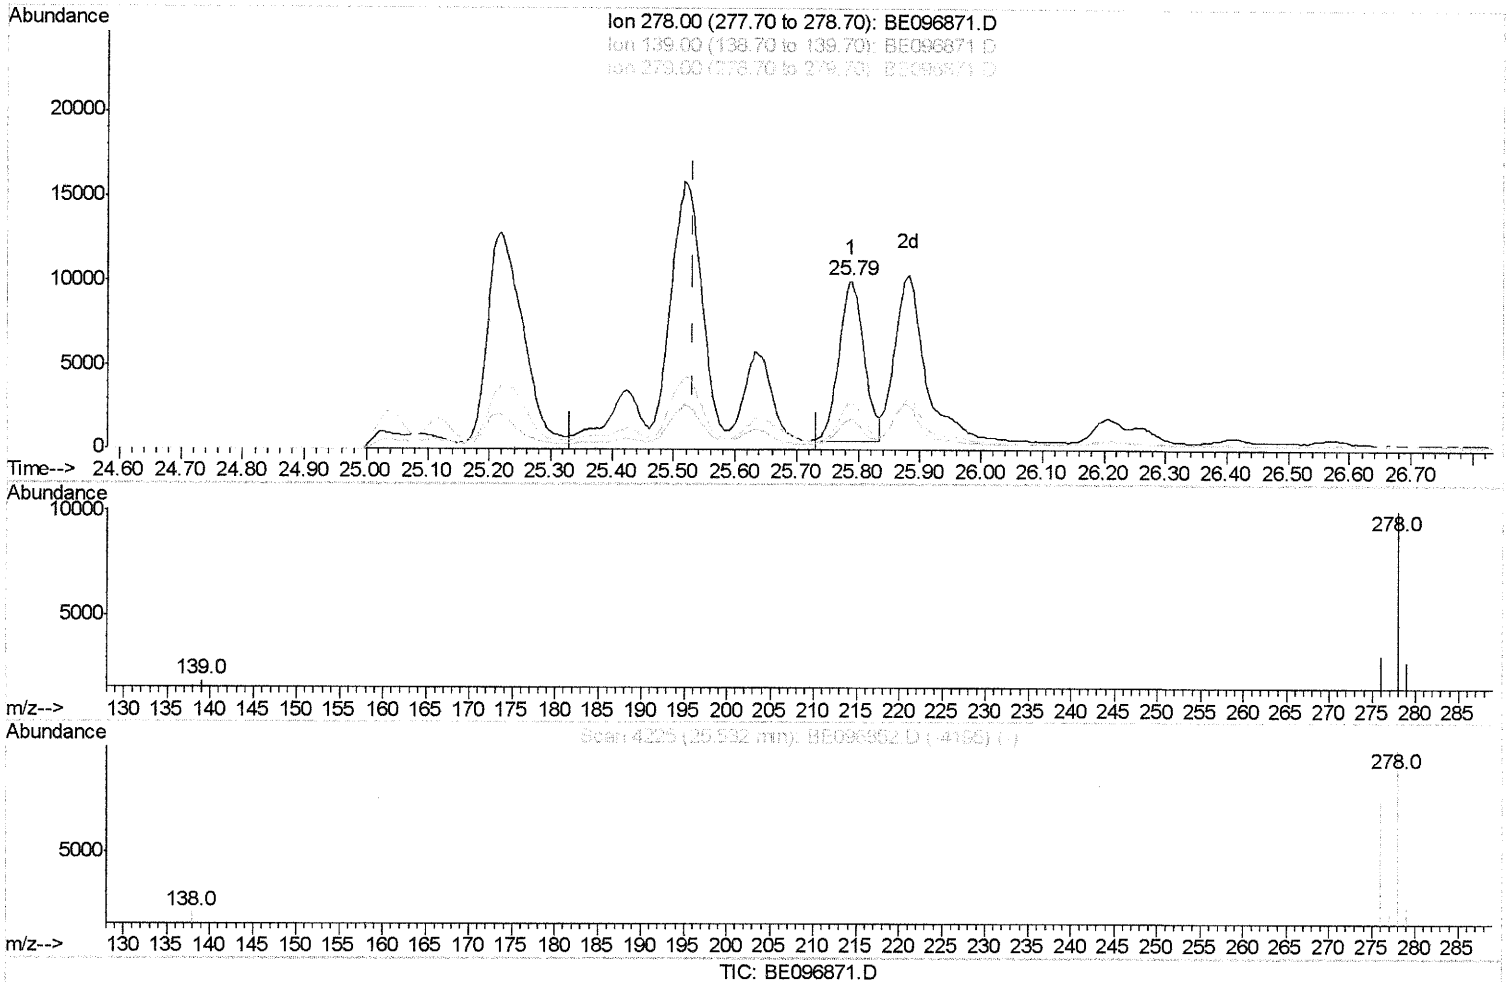

(25) Dibenzo(a,h)anthracene

25.789min (+0.257) 0.46ng/ul

response 27237

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	18.72
279.00	32.40	28.31
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

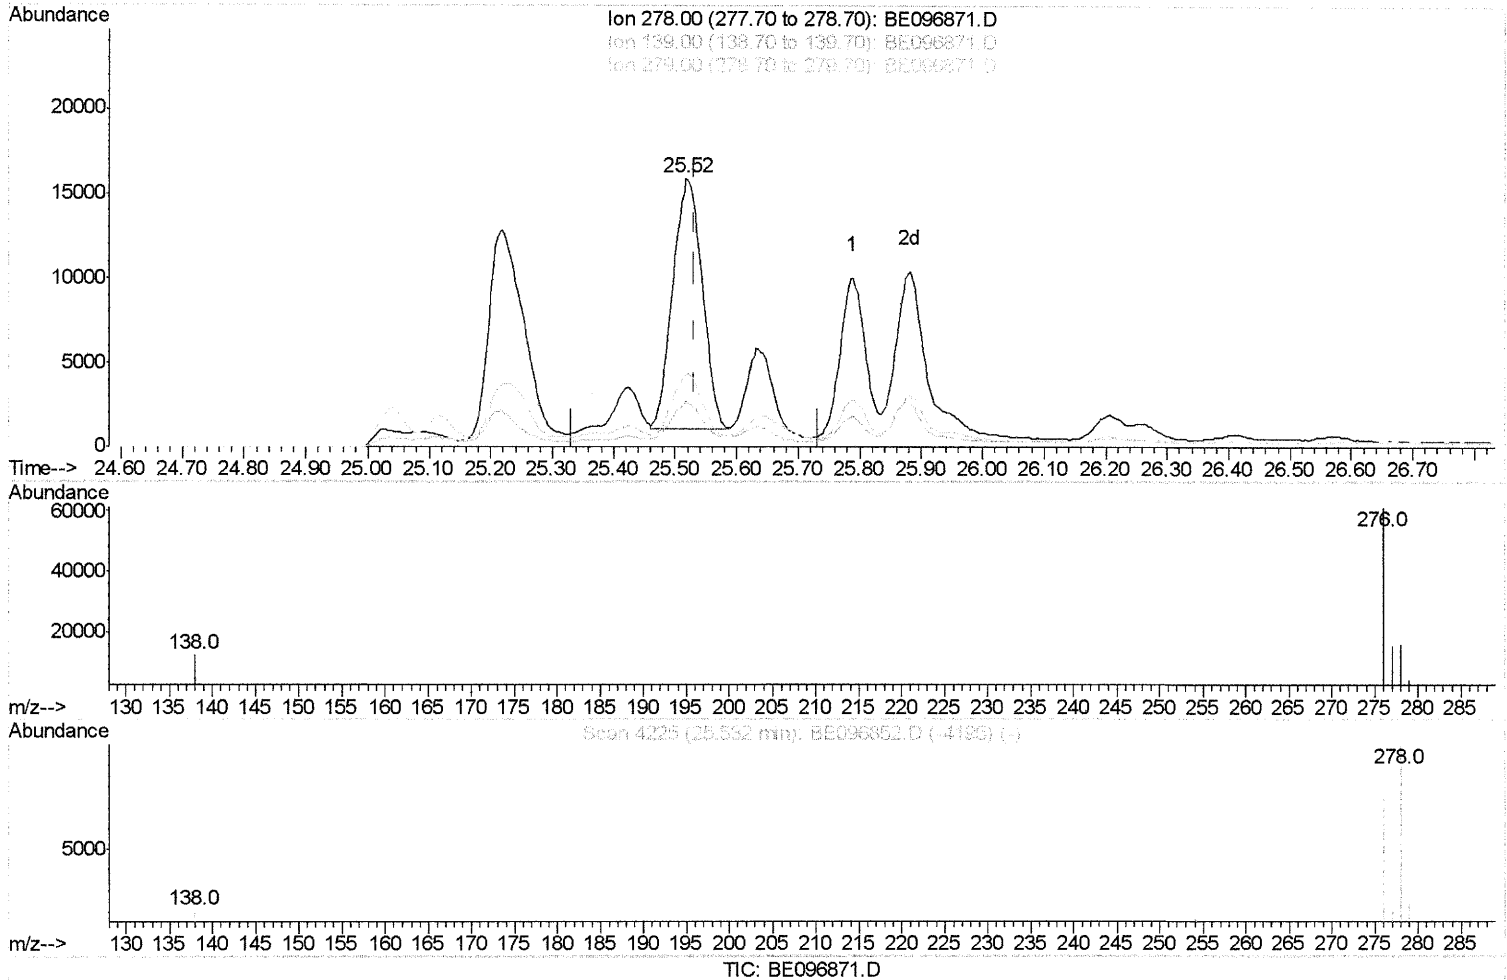

(25) Dibenzo(a,h)anthracene

25.518min (-0.014) 0.84ng/ul m

response 49355

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	17.06#
279.00	32.40	27.07
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

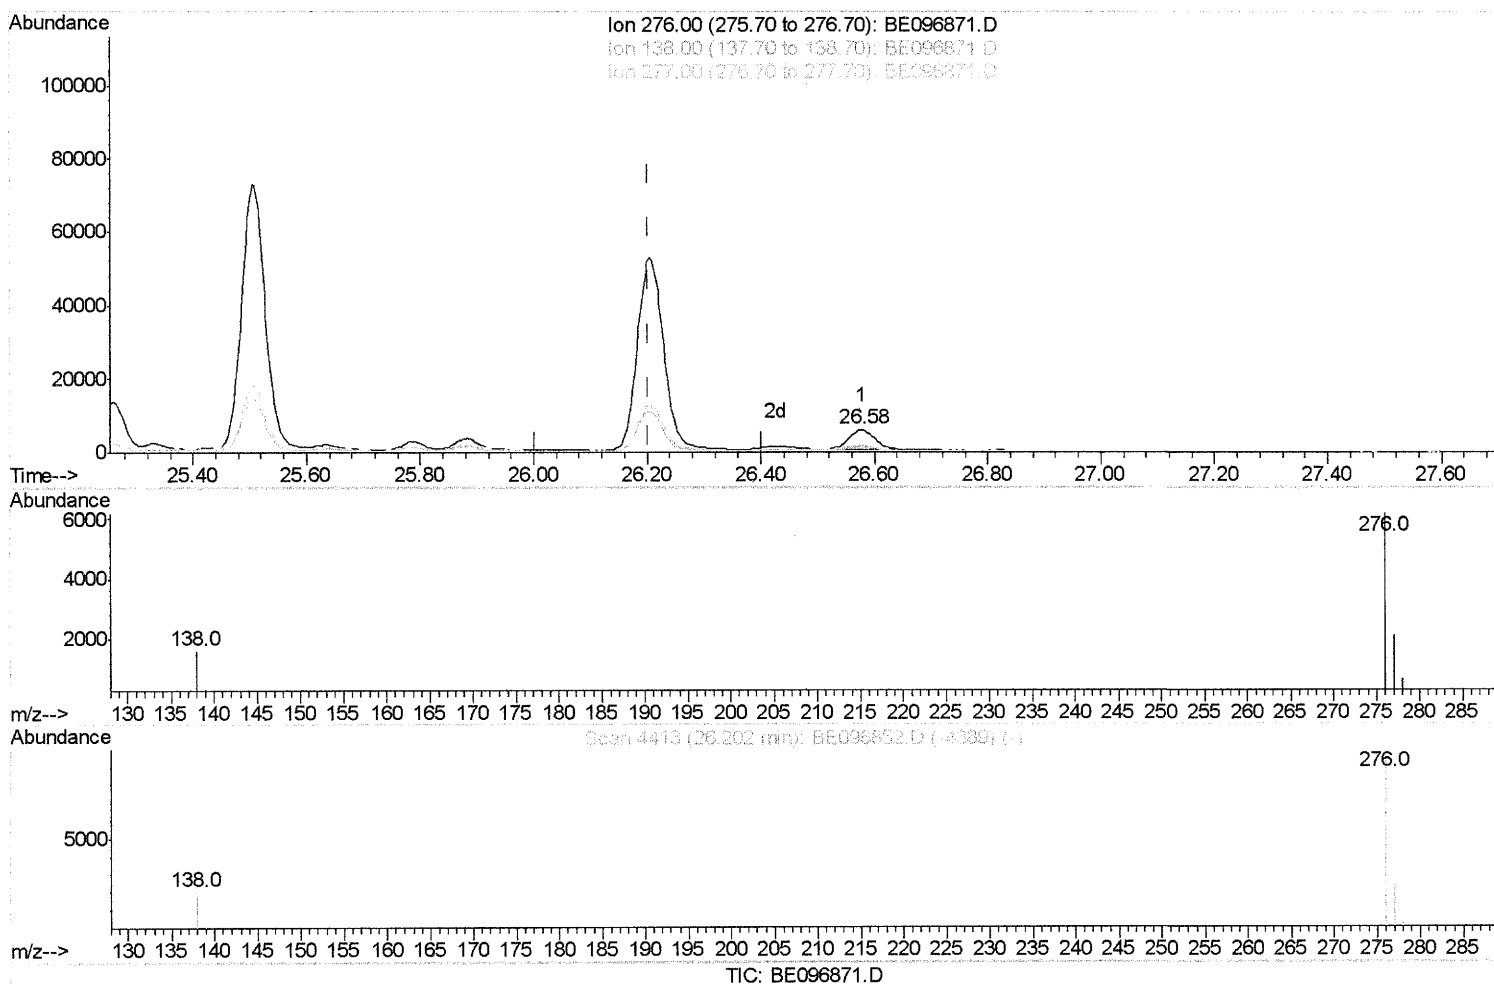

(26) Benzo(g,h,i)perylene

26.577min (+0.375) 0.26ng/ul

response 18810

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	26.48
277.00	25.60	34.06#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
 Data File : BE096871.D
 Acq On : 7 Jul 2018 2:11
 Operator : SJ/JU
 Sample : J3765-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1H08

Manual Integrations
 APPROVED

Sohil
 7/9/2018 4:14:16 PM

Quant Time: Jul 07 06:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 06 16:55:25 2018
 Response via : Initial Calibration

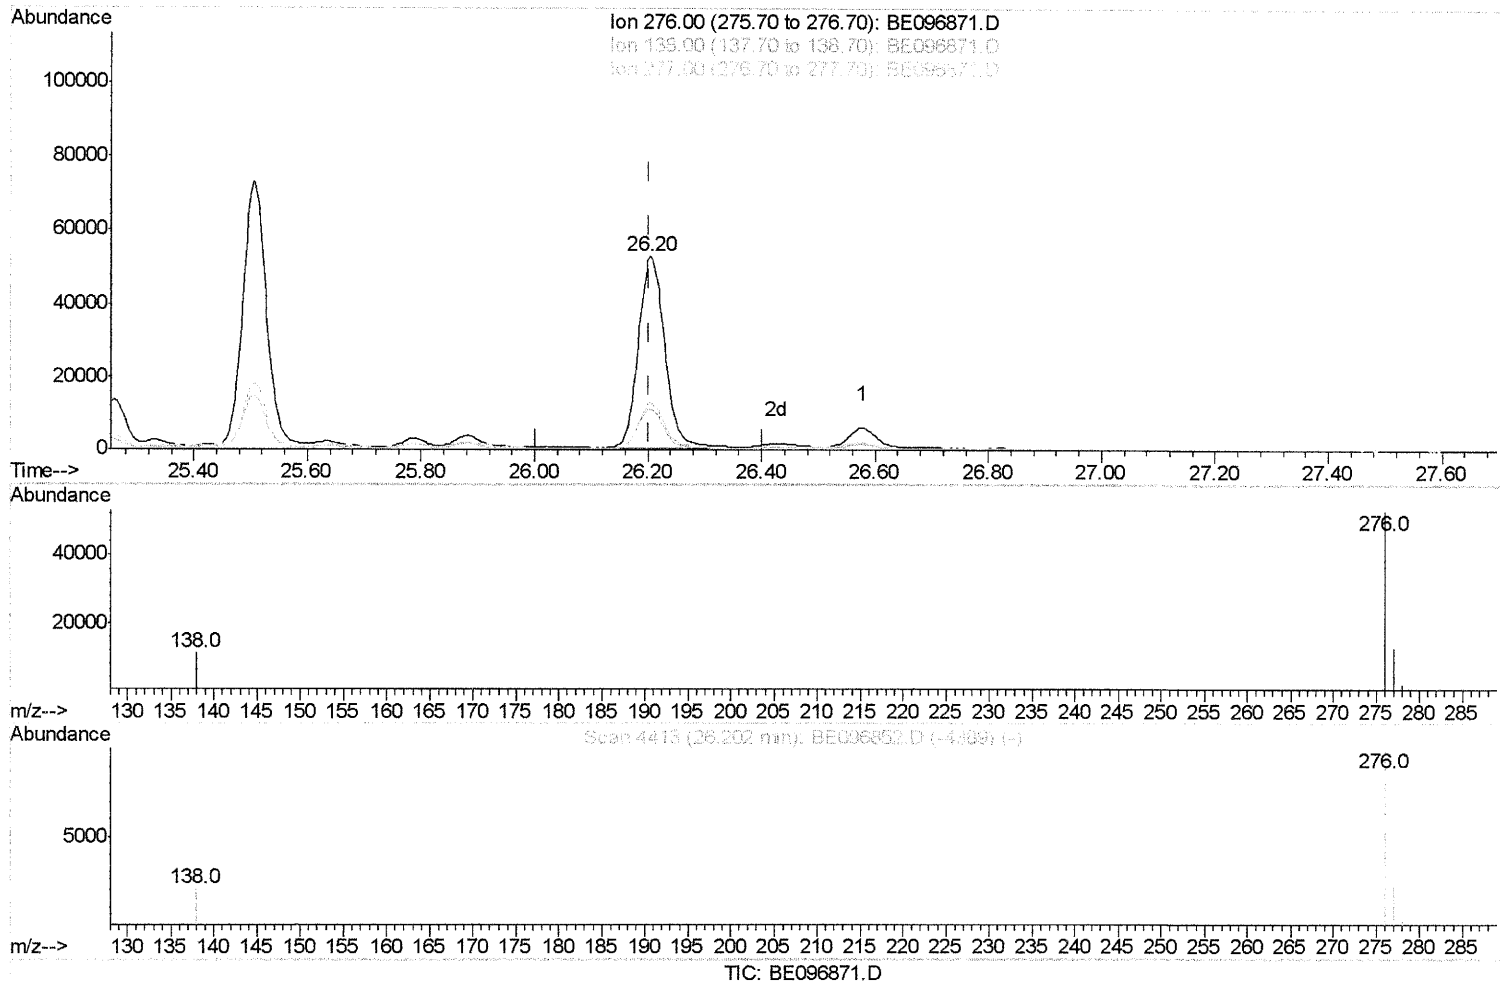

(26) Benzo(g,h,i)perylene

26.203min (+0.000) 2.35ng/ul m

SJ 7/11/18

response 168688

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	21.11#
277.00	25.60	24.24
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
Client Sampled :
F1H08

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070618\
Data File : BE096871.D
Acq On : 7 Jul 2018 2:11
Operator : SJ/JU
Sample : J3765-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
7/9/2018 4:14:16 PM

Quant Time: Jul 09 05:43:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE070618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 06 16:55:25 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	3436	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	18289	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	12291	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.78	188	28818m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	28348m	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	27110m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.74	152	8184	0.27	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	22063m	0.31	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.19	128	10246	0.232	ng/ul#	91
5) 2-Methylnaphthalene	11.81	142	5741	0.191	ng/ul	98
7) Acenaphthylene	13.74	152	21049	0.418	ng/ul	97
8) Acenaphthene	14.09	153	1650	0.040	ng/ul#	91
9) Fluorene	15.08	166	13123	0.306	ng/ul	90
12) Phenanthrene	16.82	178	60835m	0.819	ng/ul	
13) Anthracene	16.91	178	413925m	6.560	ng/ul	
15) Fluoranthene	18.85	202	209418m	2.646	ng/ul	
17) Pyrene	19.21	202	279410	3.003	ng/ul#	81
18) Benzo(a)anthracene	20.96	228	167292m	2.502	ng/ul	
19) Chrysene	21.02	228	251625	2.905	ng/ul	99
21) Benzo(b)fluoranthene	22.54	252	557250m	7.531	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	139133m	1.722	ng/ul	
23) Benzo(a)pyrene	23.12	252	252483m	4.034	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.51	276	206021m	3.171	ng/ul	
25) Dibenzo(a,h)anthracene	25.52	278	49355m	0.956	ng/ul	
26) Benzo(a,h,i)perylene	26.20	276	168688m	2.675	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed