
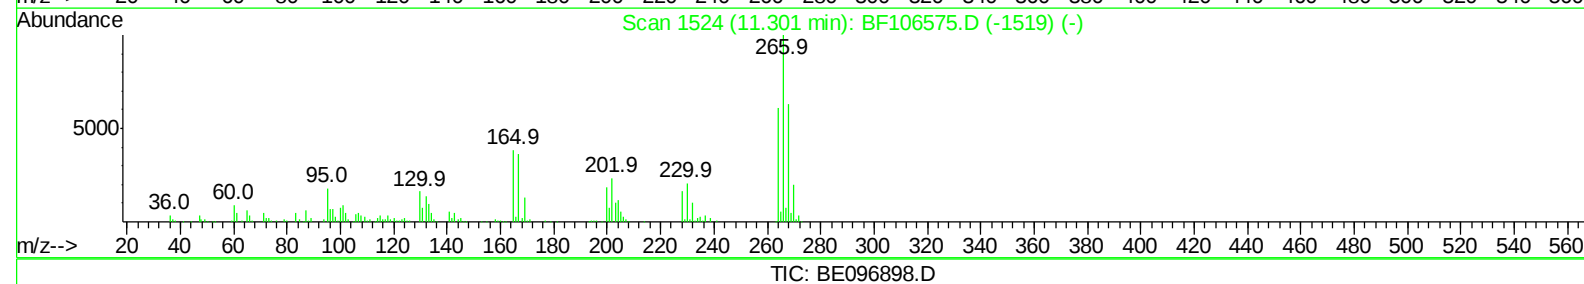
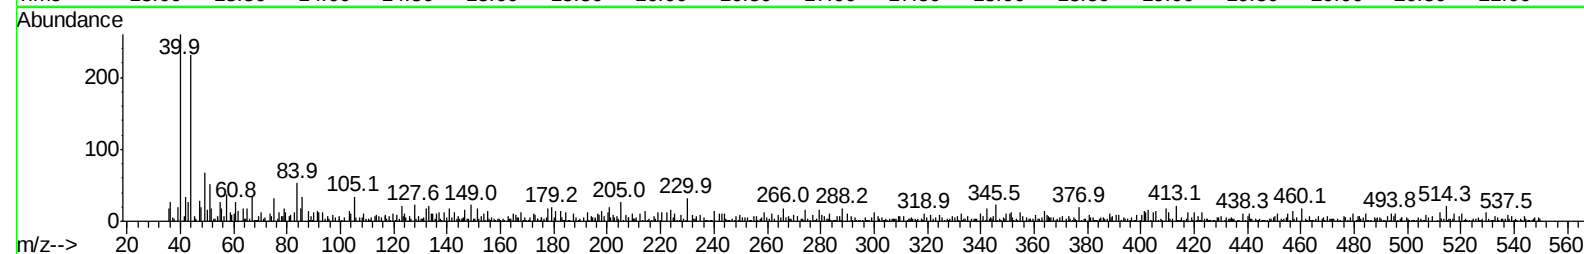


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071318\
Data File : BE096898.D
Acq On : 13 Jul 2018 9:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:17:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 13 11:54:53 2018
Response via : Initial Calibration

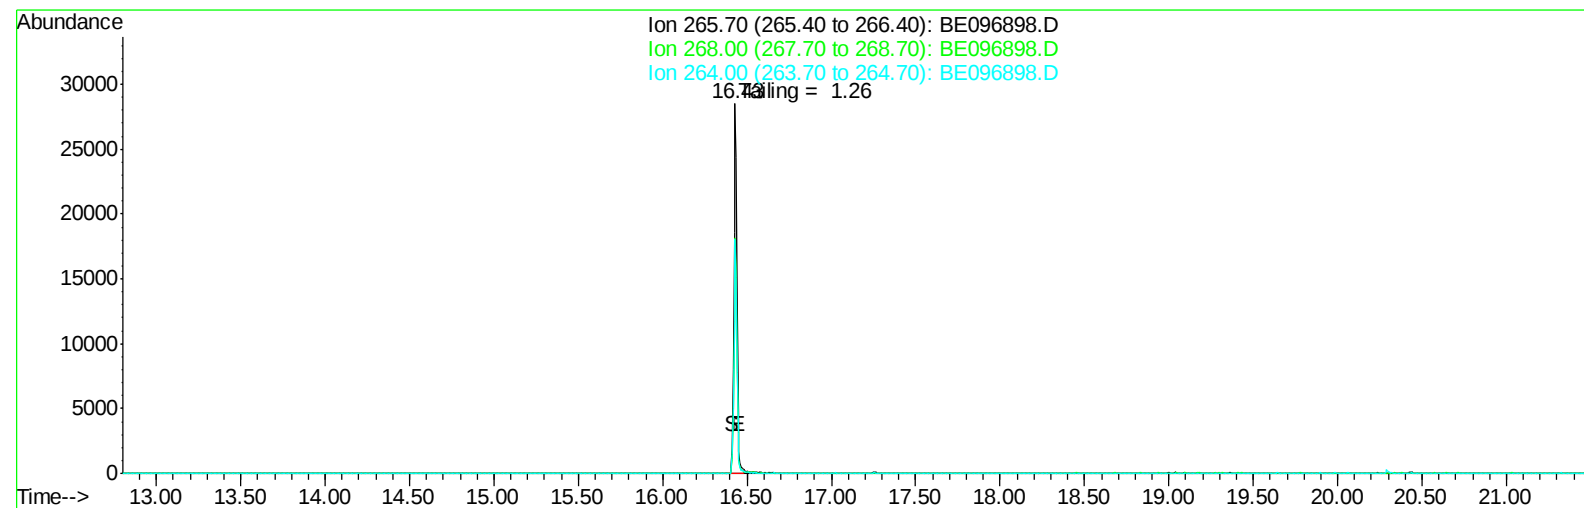

TIC: BE096898.D

(69) Pentachlorophenol (C)




11.330min (+0.035) 256.72ng

response 16

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.56
264.00	61.90	50.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071318\
 Data File : BE096898.D
 Acq On : 13 Jul 2018 9:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 01:17:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 13 11:54:53 2018
 Response via : Initial Calibration

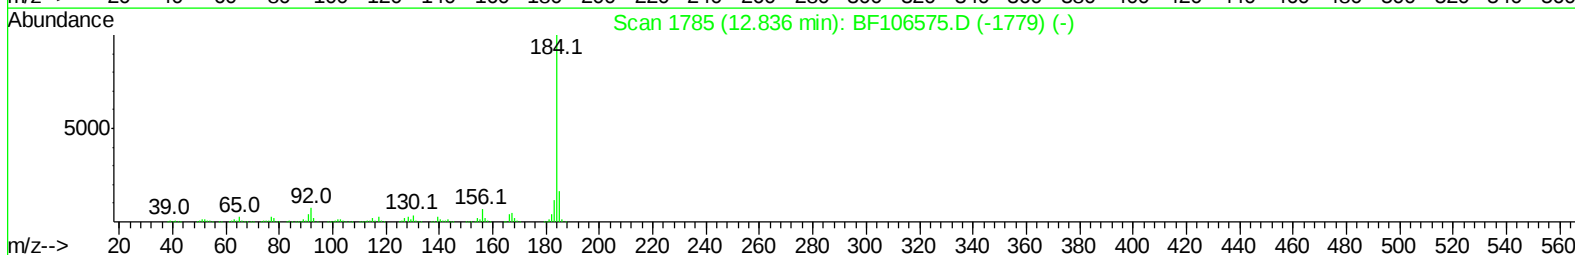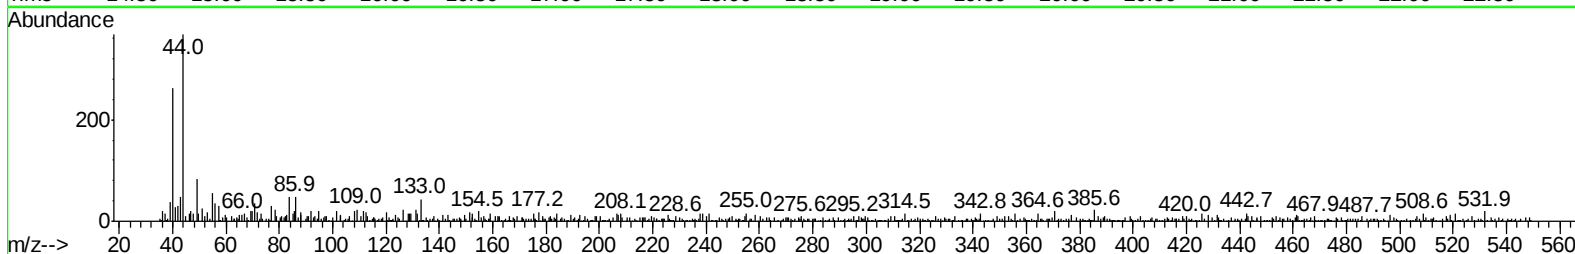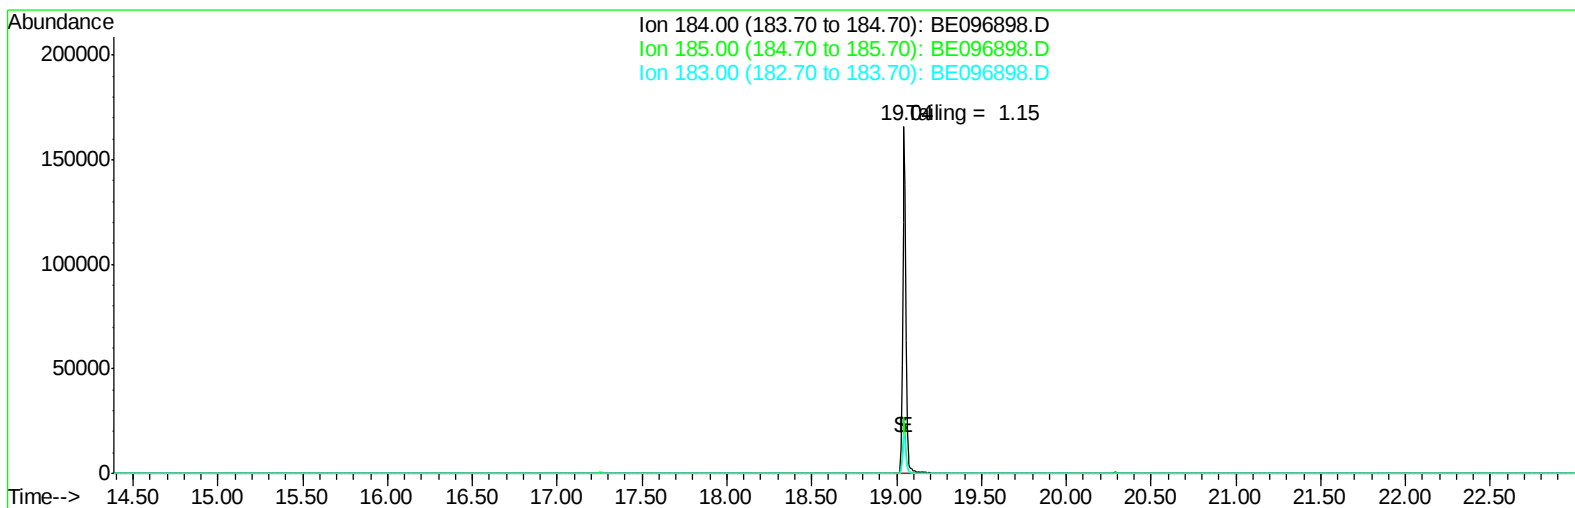

TIC: BE096898.D

(76) Benzidine

12.840min (+0.021) 21.95ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	26.67#
183.00	11.60	73.33#
0.00	0.00	0.00