

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071318\
 Data File : BE096931.D
 Acq On : 14 Jul 2018 8:46
 Operator : SJ/JU
 Sample : J3170-10DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 GW01-071118DL

Quant Time: Jul 16 00:37:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 13 17:02:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	2357	0.40	ng	0.01
7) Naphthalene-d8	10.14	136	12170	0.40	ng	0.00
13) Acenaphthene-d10	14.03	164	6627	0.40	ng	0.00
19) Phenanthrene-d10	16.78	188	16594	0.40	ng	0.01
27) Chrysene-d12	20.98	240	13674	0.40	ng	0.00
34) Perylene-d12	23.21	264	13922	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.05	112	248	0.05	ng	0.00
5) Phenol-d6	6.60	99	216	0.03	ng	0.01
8) Nitrobenzene-d5	8.53	82	784	0.11	ng	0.01
11) 2-Methylnaphthalene-d10	11.74	152	1578	0.09	ng	0.00
14) 2,4,6-Tribromophenol	15.53	330	146	0.23	ng	0.01
15) 2-Fluorobiphenyl	12.64	172	3082	0.13	ng	0.00
25) Fluoranthene-d10	18.82	212	13819	0.09	ng	0.00
29) Terphenyl-d14	19.43	244	3611	0.14	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.10	88	4733	1.340	ng	# 89
32) Bis(2-ethylhexyl)phthalate	20.93	149	1139	0.042	ng	# 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071318\
Data File : BE096931.D
Acq On : 14 Jul 2018 8:46
Operator : SJ/JU
Sample : J3170-10DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
GW01-071118DL

Quant Time: Jul 16 00:37:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 13 17:02:57 2018
Response via : Initial Calibration

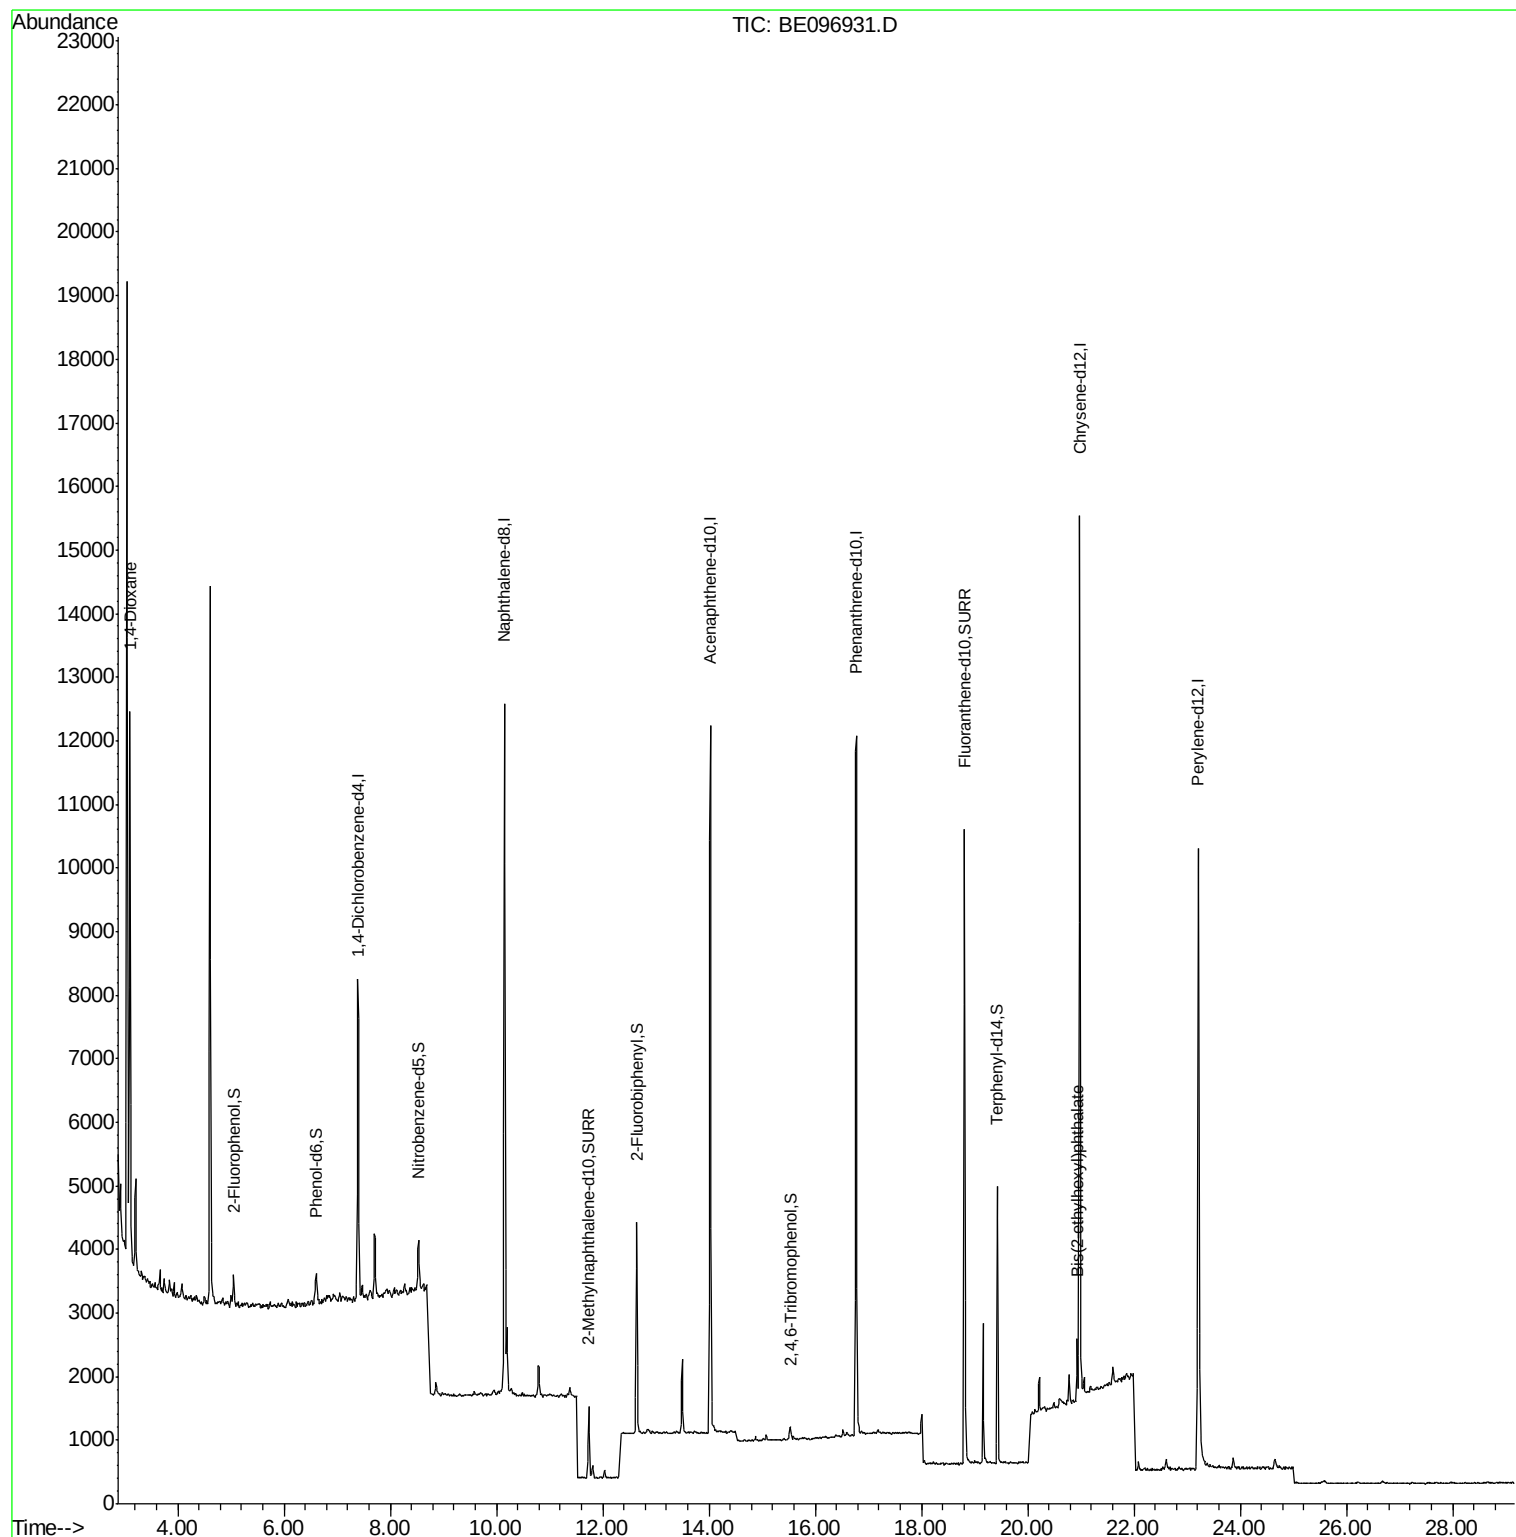



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.40 min Scan# 394

Delta R.T. 0.01 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL


Tot Ion:152 Resp: 2357

Ion Ratio Lower Upper

152 100

150 148.4 117.2 175.8




115 60.3 57.0 85.6

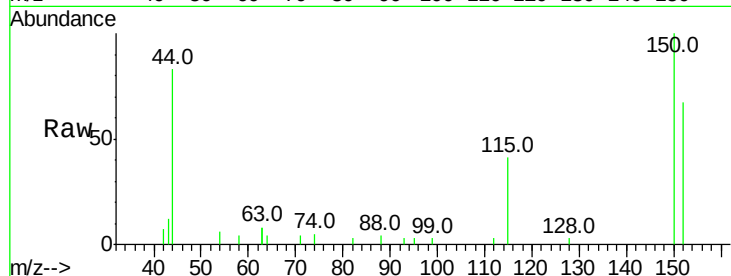

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

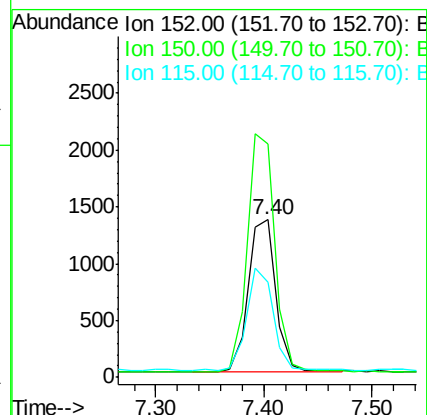

#2

1,4-Dioxane

Concen: 1.340 ng

RT: 3.10 min Scan# 20

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion: 88 Resp: 4733

Ion Ratio Lower Upper

88 100

58 82.7 63.2 94.8



43 37.0 41.2 61.8#




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

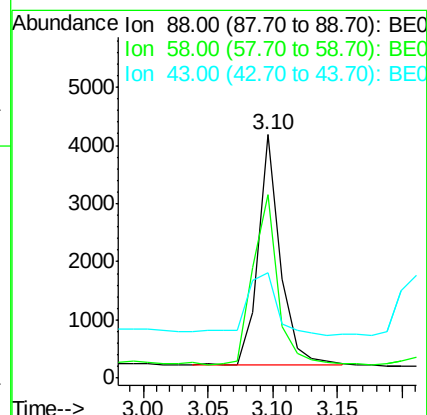

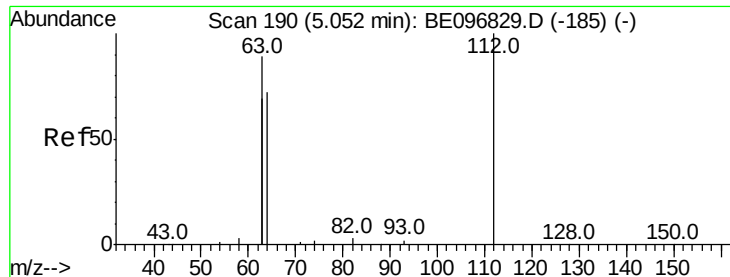

#4

2-Fluorophenol

Concen: 0.047 ng

RT: 5.05 min Scan# 190

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL


Tot Ion: 112 Resp: 248

Ion Ratio Lower Upper

112 100

64 71.0 60.1 90.1




63 152.0 116.8 175.2

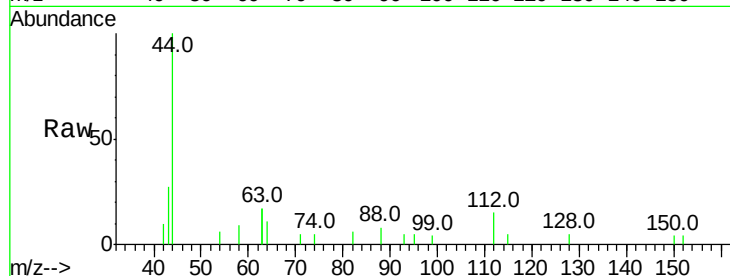

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

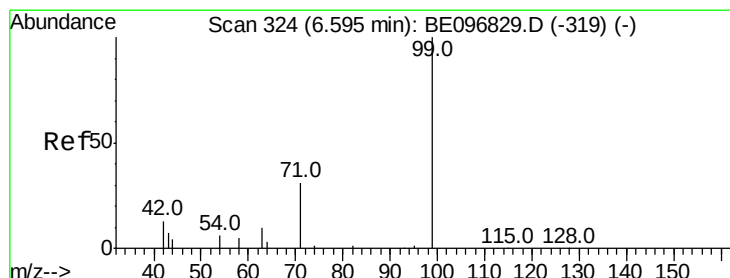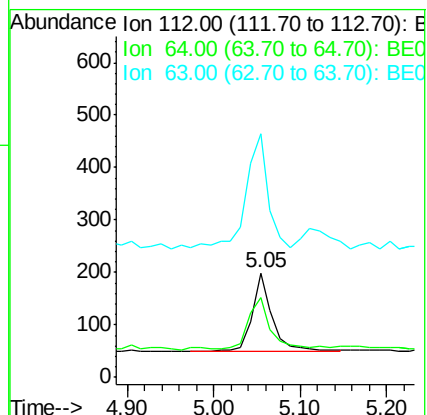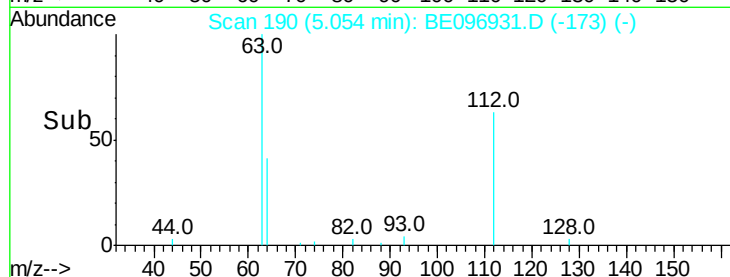

#5

Phenol-d6

Concen: 0.027 ng

RT: 6.60 min Scan# 324

Delta R.T. 0.01 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion: 99 Resp: 216

Ion Ratio Lower Upper

99 100

42 30.1 20.2 30.2



71 48.6 28.4 42.6#

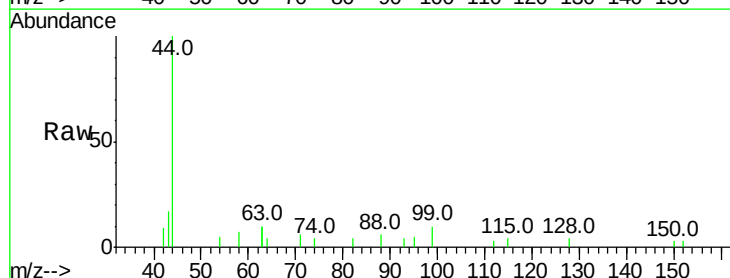


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

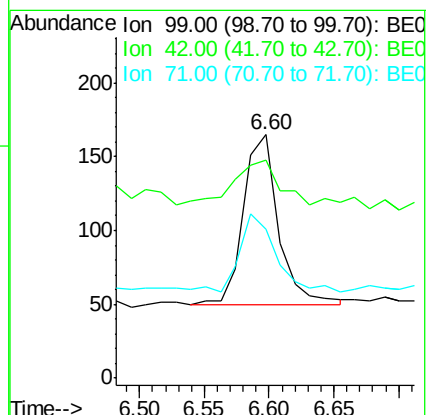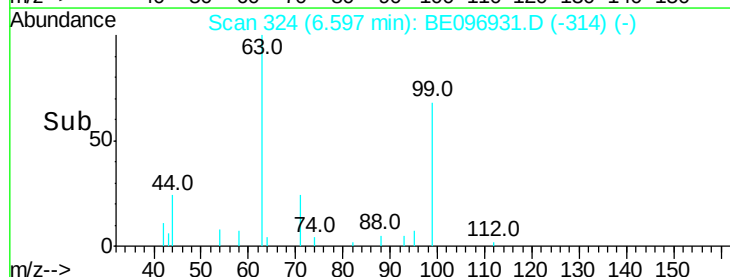

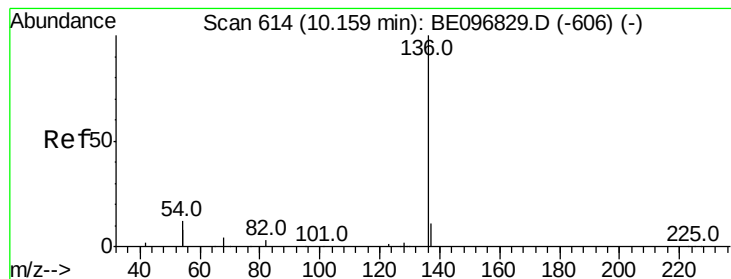

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.14 min Scan# 613

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL

Tot Ion:136 Resp: 12170





Ion Ratio Lower Upper

136 100

137 11.4 9.5 14.3

54 50.2 29.1 43.7#

68 9.3 6.2 9.2#

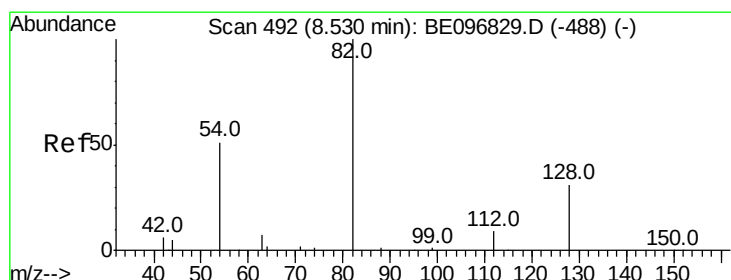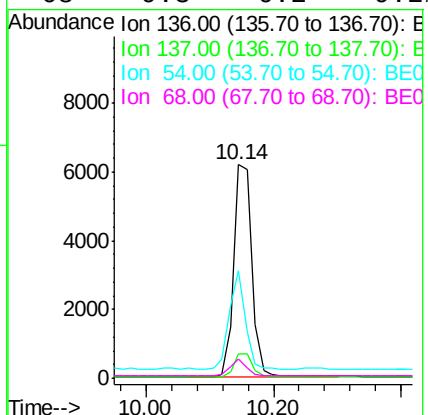

#8

Nitrobenzene-d5

Concen: 0.106 ng

RT: 8.53 min Scan# 492

Delta R.T. 0.01 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46




Tgt Ion: 82 Resp: 784


Ion Ratio Lower Upper

82 100

128 41.4 24.0 36.0#

54 56.5 40.0 60.0

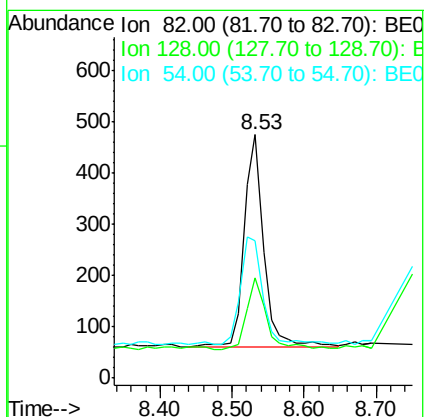

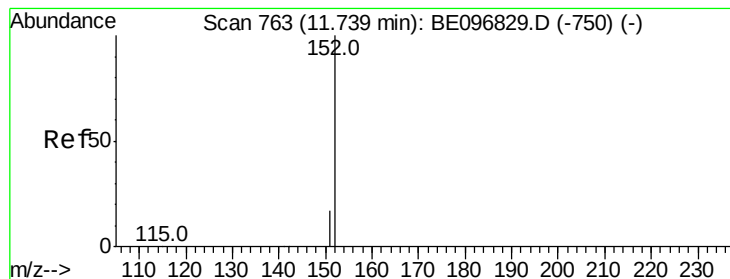

#11

2-Methylnaphthalene-d10

Concen: 0.090 ng

RT: 11.74 min Scan# 762

Delta R.T. 0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :


GW01-071118DL

Tot Ion:152 Resp: 1578

Ion Ratio Lower Upper




152 100

151 19.7 15.4 23.0

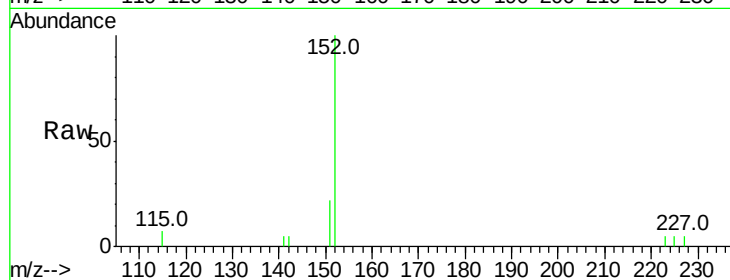

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

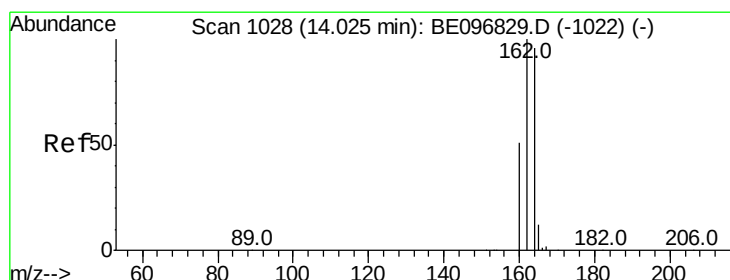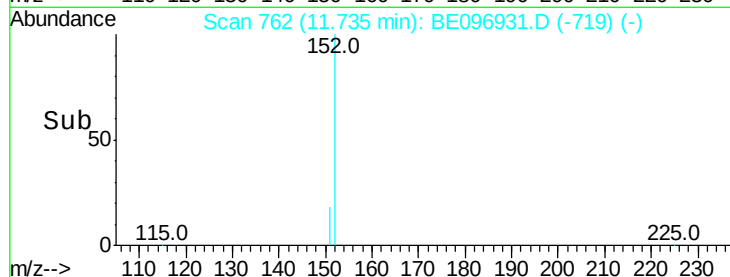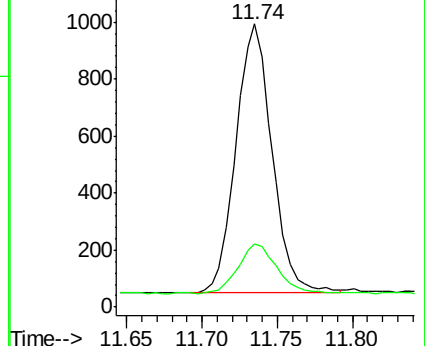

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.03 min Scan# 1028

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion:164 Resp: 6627

Ion Ratio Lower Upper

164 100

162 102.3 83.1 124.7



160 51.3 37.1 55.7

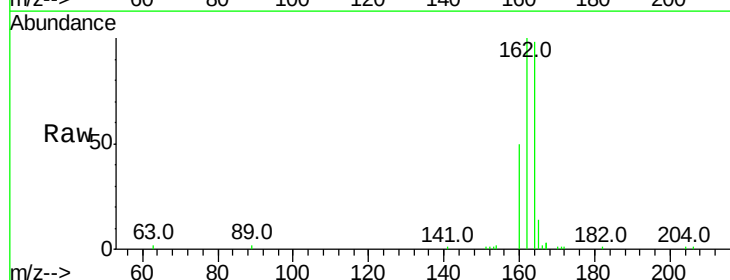


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

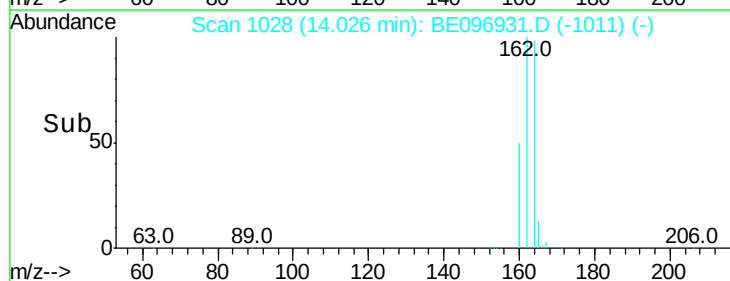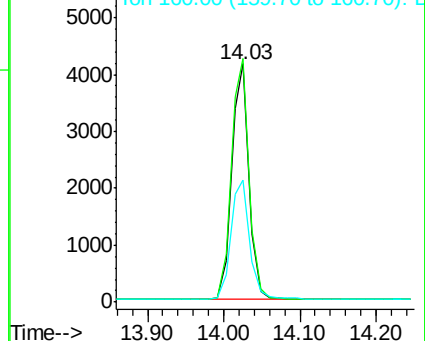



#14

2,4,6-Tribromophenol

Concen: 0.228 ng

RT: 15.53 min Scan# 1154

Delta R.T. 0.01 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL


Tot Ion:330 Resp: 146

Ion Ratio Lower Upper




330 100

332 94.5 152.7 229.1#

141 43.2 33.7 50.5

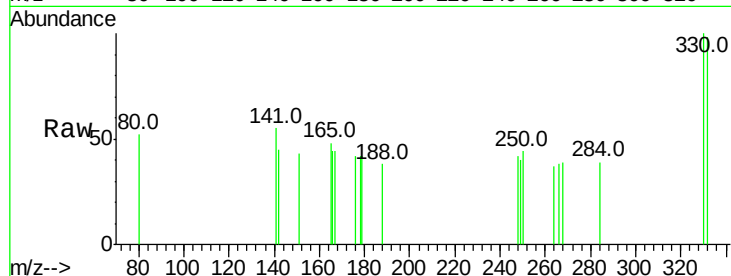

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

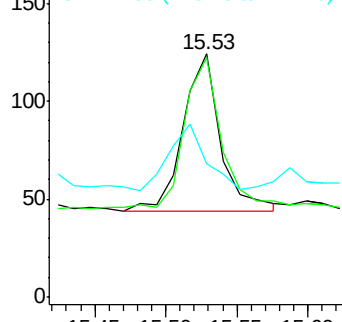

#15

2-Fluorobiphenyl

Concen: 0.127 ng

RT: 12.64 min Scan# 908

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion:172 Resp: 3082

Ion Ratio Lower Upper



172 100


171 34.6 29.9 44.9

170 24.3 21.8 32.8



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

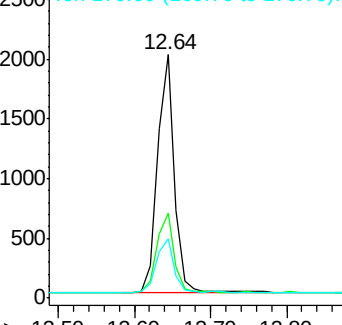

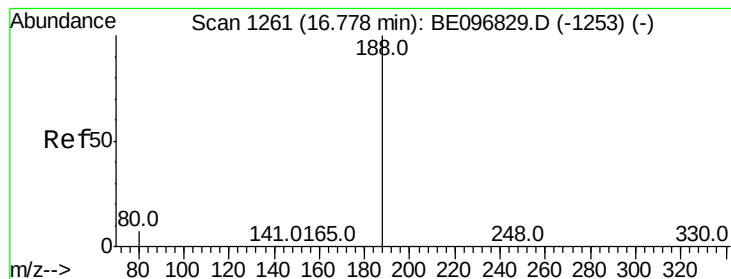

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.78 min Scan# 1261

Delta R.T. 0.01 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL


Tot Ion:188 Resp: 16594

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 7.5 3.6 5.4#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

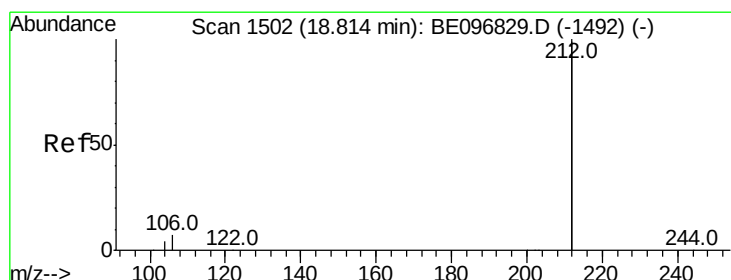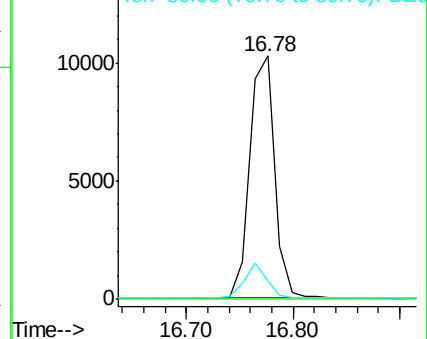

#25

Fluoranthene-d10

Concen: 0.095 ng

RT: 18.82 min Scan# 1503

Delta R.T. 0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion:212 Resp: 13819

Ion Ratio Lower Upper

212 100

106 3.5 2.8 4.2



104 2.0 1.6 2.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

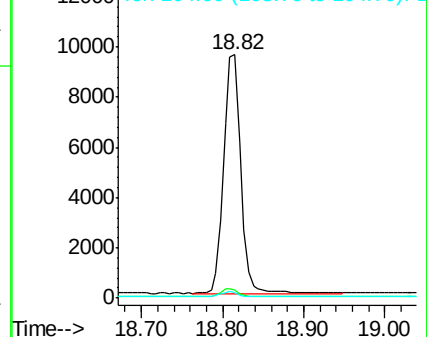



#27

Chrysene-d12

Concen: 0.400 ng

RT: 20.98 min Scan# 1787

Delta R.T. 0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleID :

GW01-071118DL


Tot Ion:240 Resp: 13674

Ion Ratio Lower Upper

240 100

120 6.7 5.5 8.3




236 27.4 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

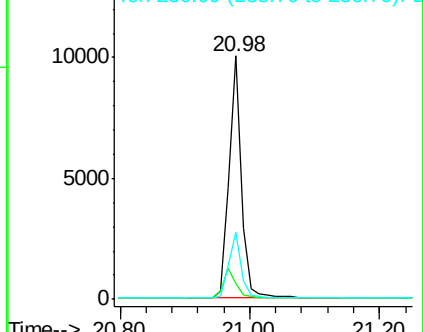

#29

Terphenyl-d14

Concen: 0.137 ng

RT: 19.43 min Scan# 1610

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion:244 Resp: 3611

Ion Ratio Lower Upper

244 100

212 37.6 25.4 38.0



122 13.8 8.1 12.1#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

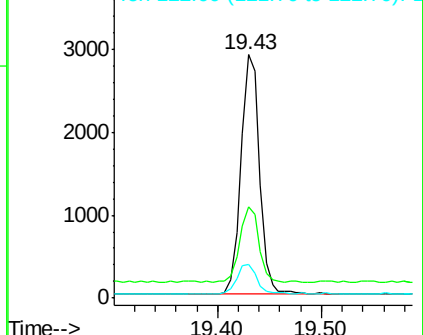



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.042 ng

RT: 20.93 min Scan# 1783

Delta R.T. 0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46

Instrument :

BNA_E

ClientSampleId :

GW01-071118DL


Tot Ion:149 Resp: 1139

Ion Ratio Lower Upper

149 100

167 6.8 5.4 8.0




279 1.1 0.7 1.1#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

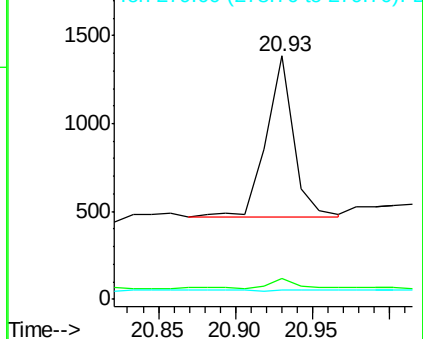

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.21 min Scan# 2205

Delta R.T. -0.00 min

Lab File: BE096931.D

Acq: 14 Jul 2018 8:46


Tgt Ion:264 Resp: 13922

Ion Ratio Lower Upper

264 100

260 26.0 20.5 30.7

265 24.2 22.8 34.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

