


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071318\
 Data File : BE096898.D
 Acq On : 13 Jul 2018 9:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 13 17:02:57 2018

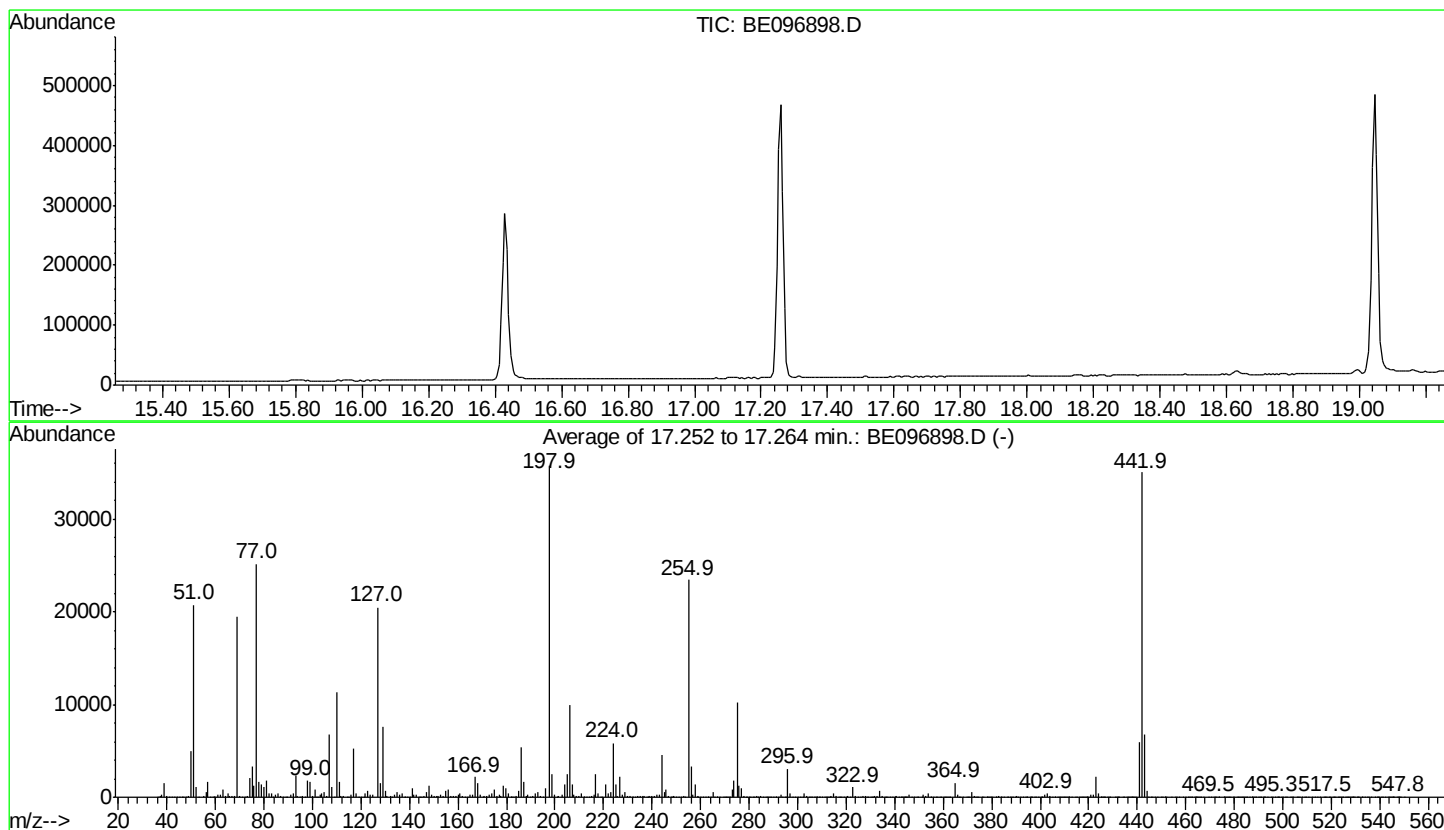

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.0	20747	PASS
68	69	0.00	2	0.5	105	PASS
69	198	0.00	100	54.5	19510	PASS
70	69	0.00	2	0.7	140	PASS
127	198	10	80	57.3	20487	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35776	PASS
199	198	5	9	7.0	2504	PASS
275	198	10	60	28.8	10291	PASS
365	198	1	100	4.4	1580	PASS
441	443	0.01	100	88.1	5968	PASS
442	198	50	100	98.2	35123	PASS
443	442	15	24	19.3	6771	PASS