


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071318\
Data File : BE096917.D
Acq On : 14 Jul 2018 00:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 13 17:02:57 2018

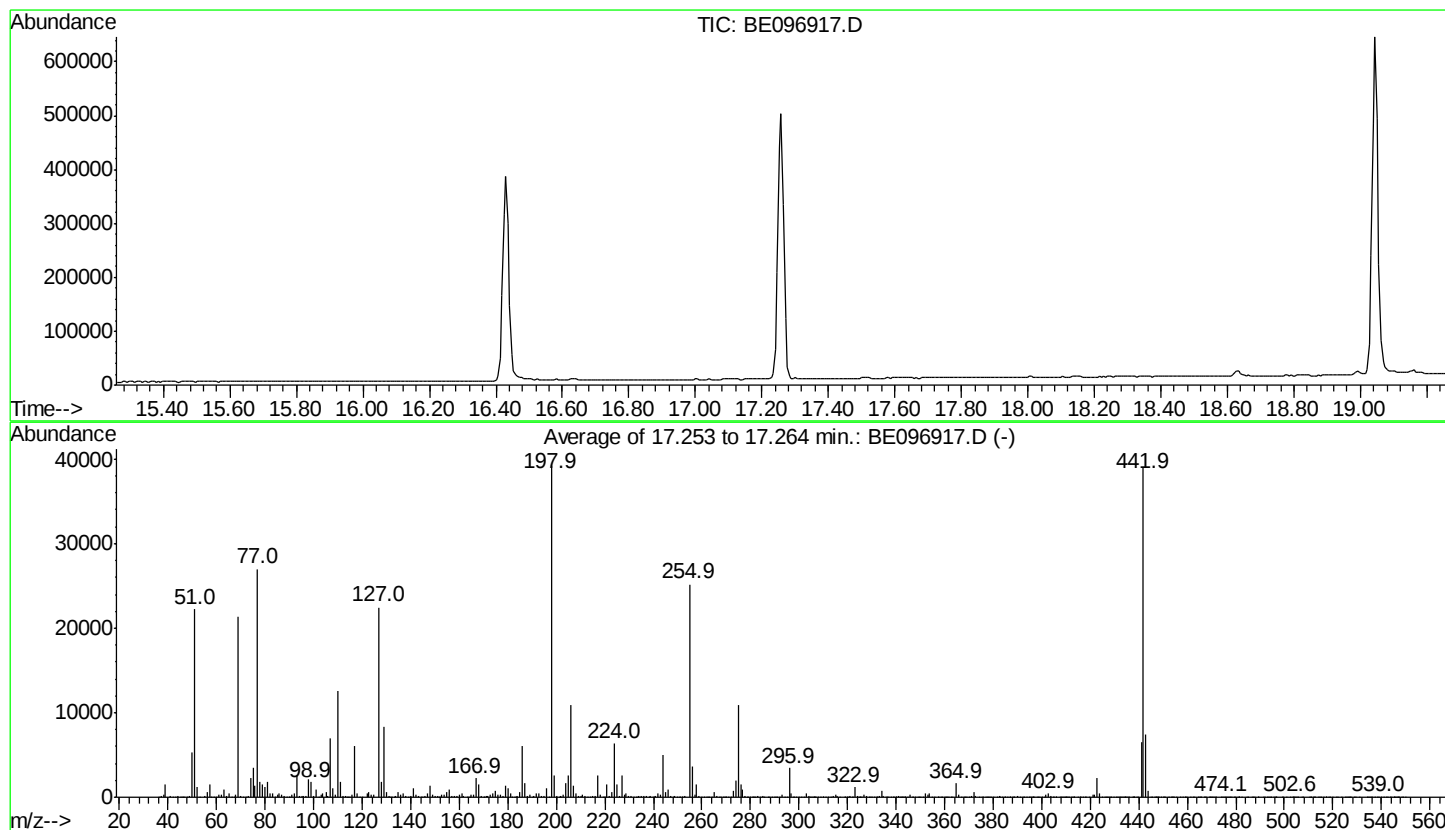

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	22253	PASS
68	69	0.00	2	1.7	365	PASS
69	198	0.00	100	54.3	21281	PASS
70	69	0.00	2	0.5	102	PASS
127	198	10	80	57.2	22446	PASS
197	198	0.00	2	0.2	64	PASS
198	198	100	100	100.0	39219	PASS
199	198	5	9	6.8	2651	PASS
275	198	10	60	27.8	10885	PASS
365	198	1	100	4.2	1633	PASS
441	443	0.01	100	88.7	6581	PASS
442	198	50	100	99.5	39042	PASS
443	442	15	24	19.0	7423	PASS