


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071618\
Data File : BE096933.D
Acq On : 16 Jul 2018 9:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 17 15:02:56 2018

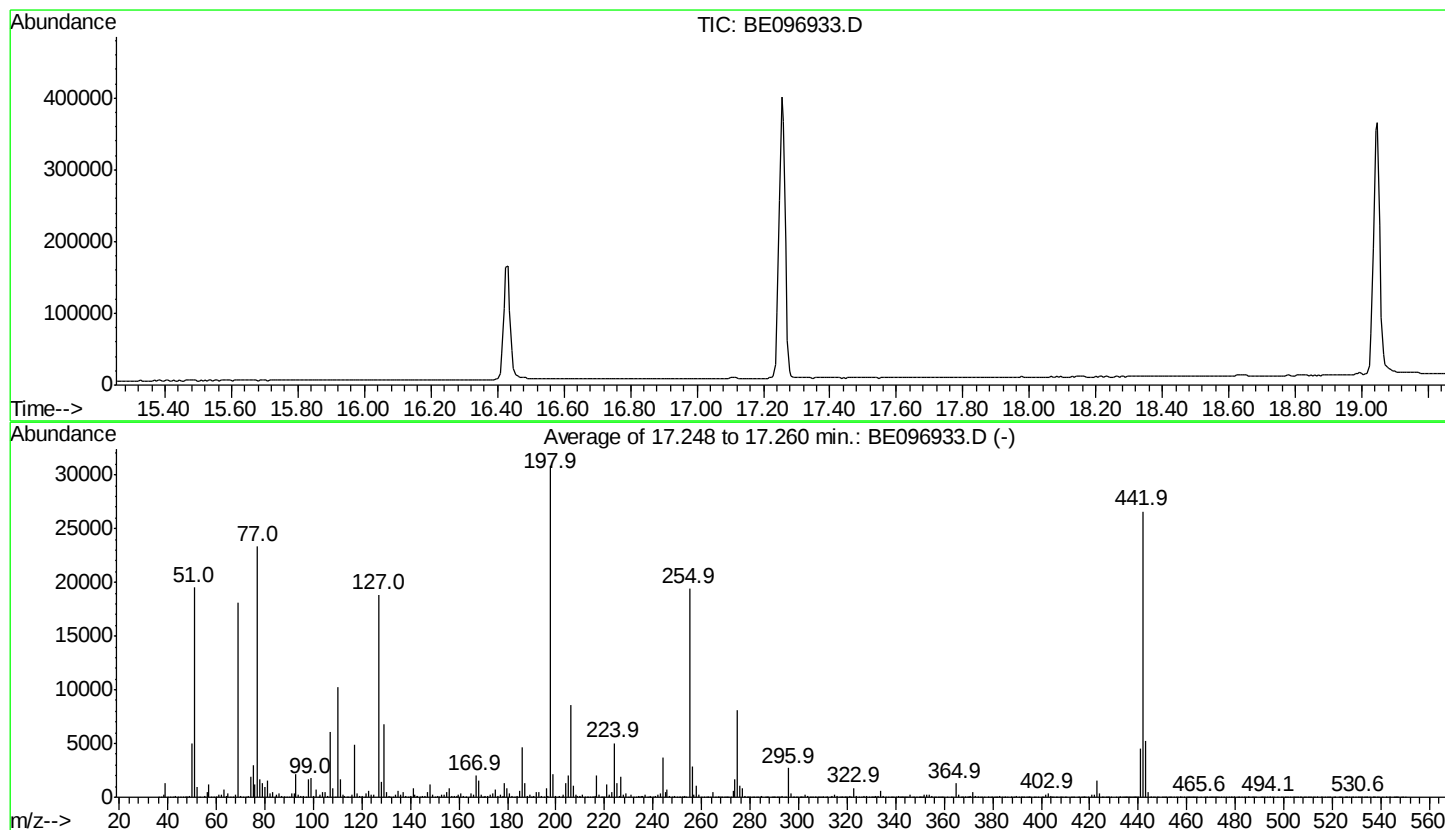

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.2	19492	PASS
68	69	0.00	2	1.2	225	PASS
69	198	0.00	100	58.6	18076	PASS
70	69	0.00	2	0.7	127	PASS
127	198	10	80	61.1	18853	PASS
197	198	0.00	2	0.3	79	PASS
198	198	100	100	100.0	30860	PASS
199	198	5	9	6.8	2090	PASS
275	198	10	60	26.4	8152	PASS
365	198	1	100	4.2	1297	PASS
441	443	0.01	100	86.8	4580	PASS
442	198	50	100	86.2	26615	PASS
443	442	15	24	19.8	5274	PASS