


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071619\
 Data File : BE100435.D
 Acq On : 16 Jul 2019 6:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 16 14:03:26 2019

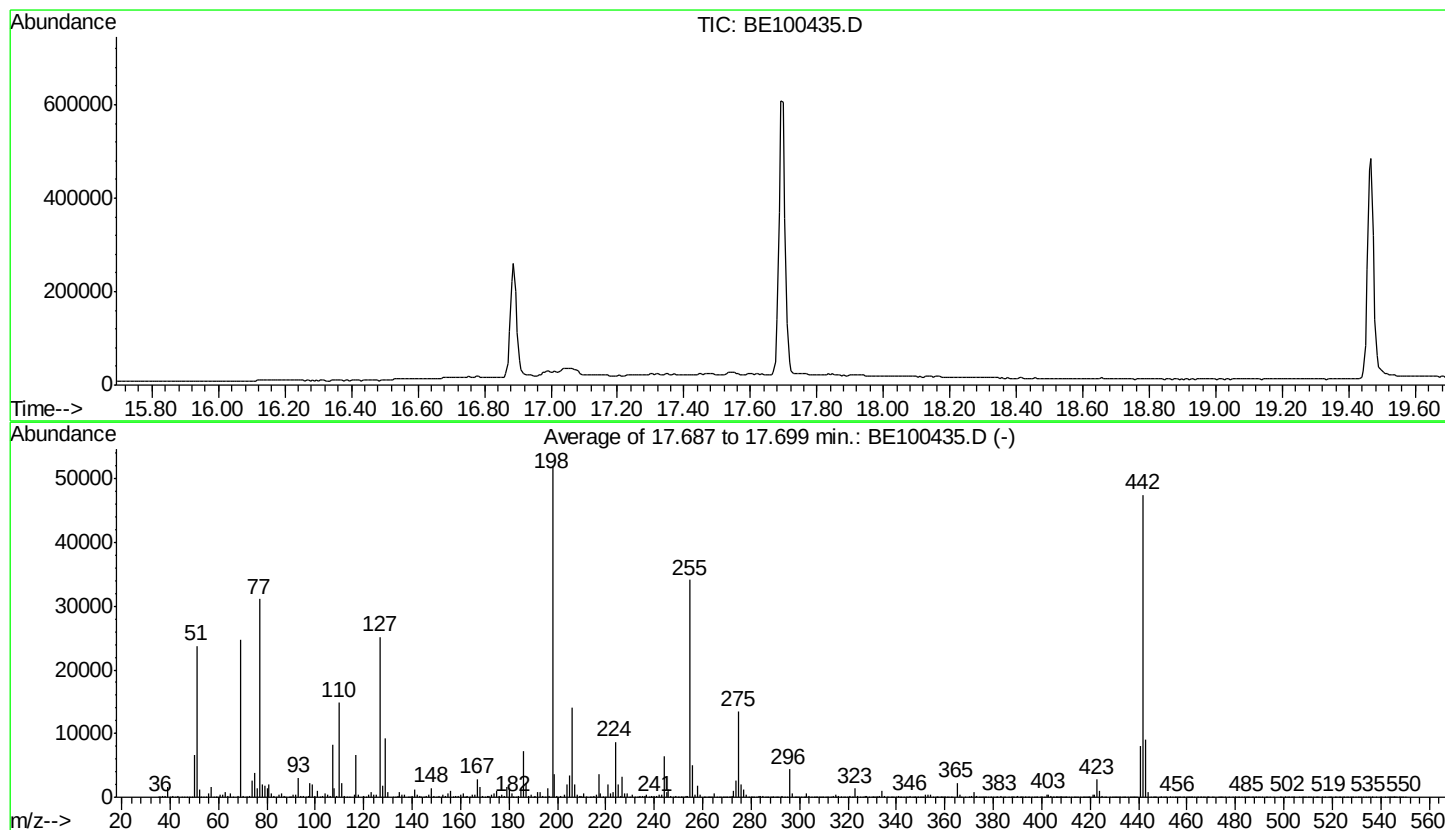

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	23811	PASS
68	69	0.00	2	0.6	139	PASS
69	198	0.00	100	47.4	24707	PASS
70	69	0.00	2	0.4	109	PASS
127	198	10	80	48.4	25222	PASS
197	198	0.00	2	0.4	210	PASS
198	198	100	100	100.0	52074	PASS
199	198	5	9	6.8	3555	PASS
275	198	10	60	25.9	13463	PASS
365	198	1	100	4.3	2262	PASS
441	198	0.01	100	15.4	8005	PASS
442	198	50	100	91.1	47452	PASS
443	442	15	24	19.0	9002	PASS