

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096970.D
 Acq On : 17 Jul 2018 22:58
 Operator : SJ/JU
 Sample : PB111127BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jul 18 03:42:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1818	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	9552	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	6093	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	1373566	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	23735	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.74	152	6242	0.41	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
9) Fluorene	15.03	166	1999	0.091	ng/ul#	19
23) Benzo(a)pyrene	23.08	252	5506	0.093	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096970.D
Acq On : 17 Jul 2018 22:58
Operator : SJ/JU
Sample : PB111127BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jul 18 03:42:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

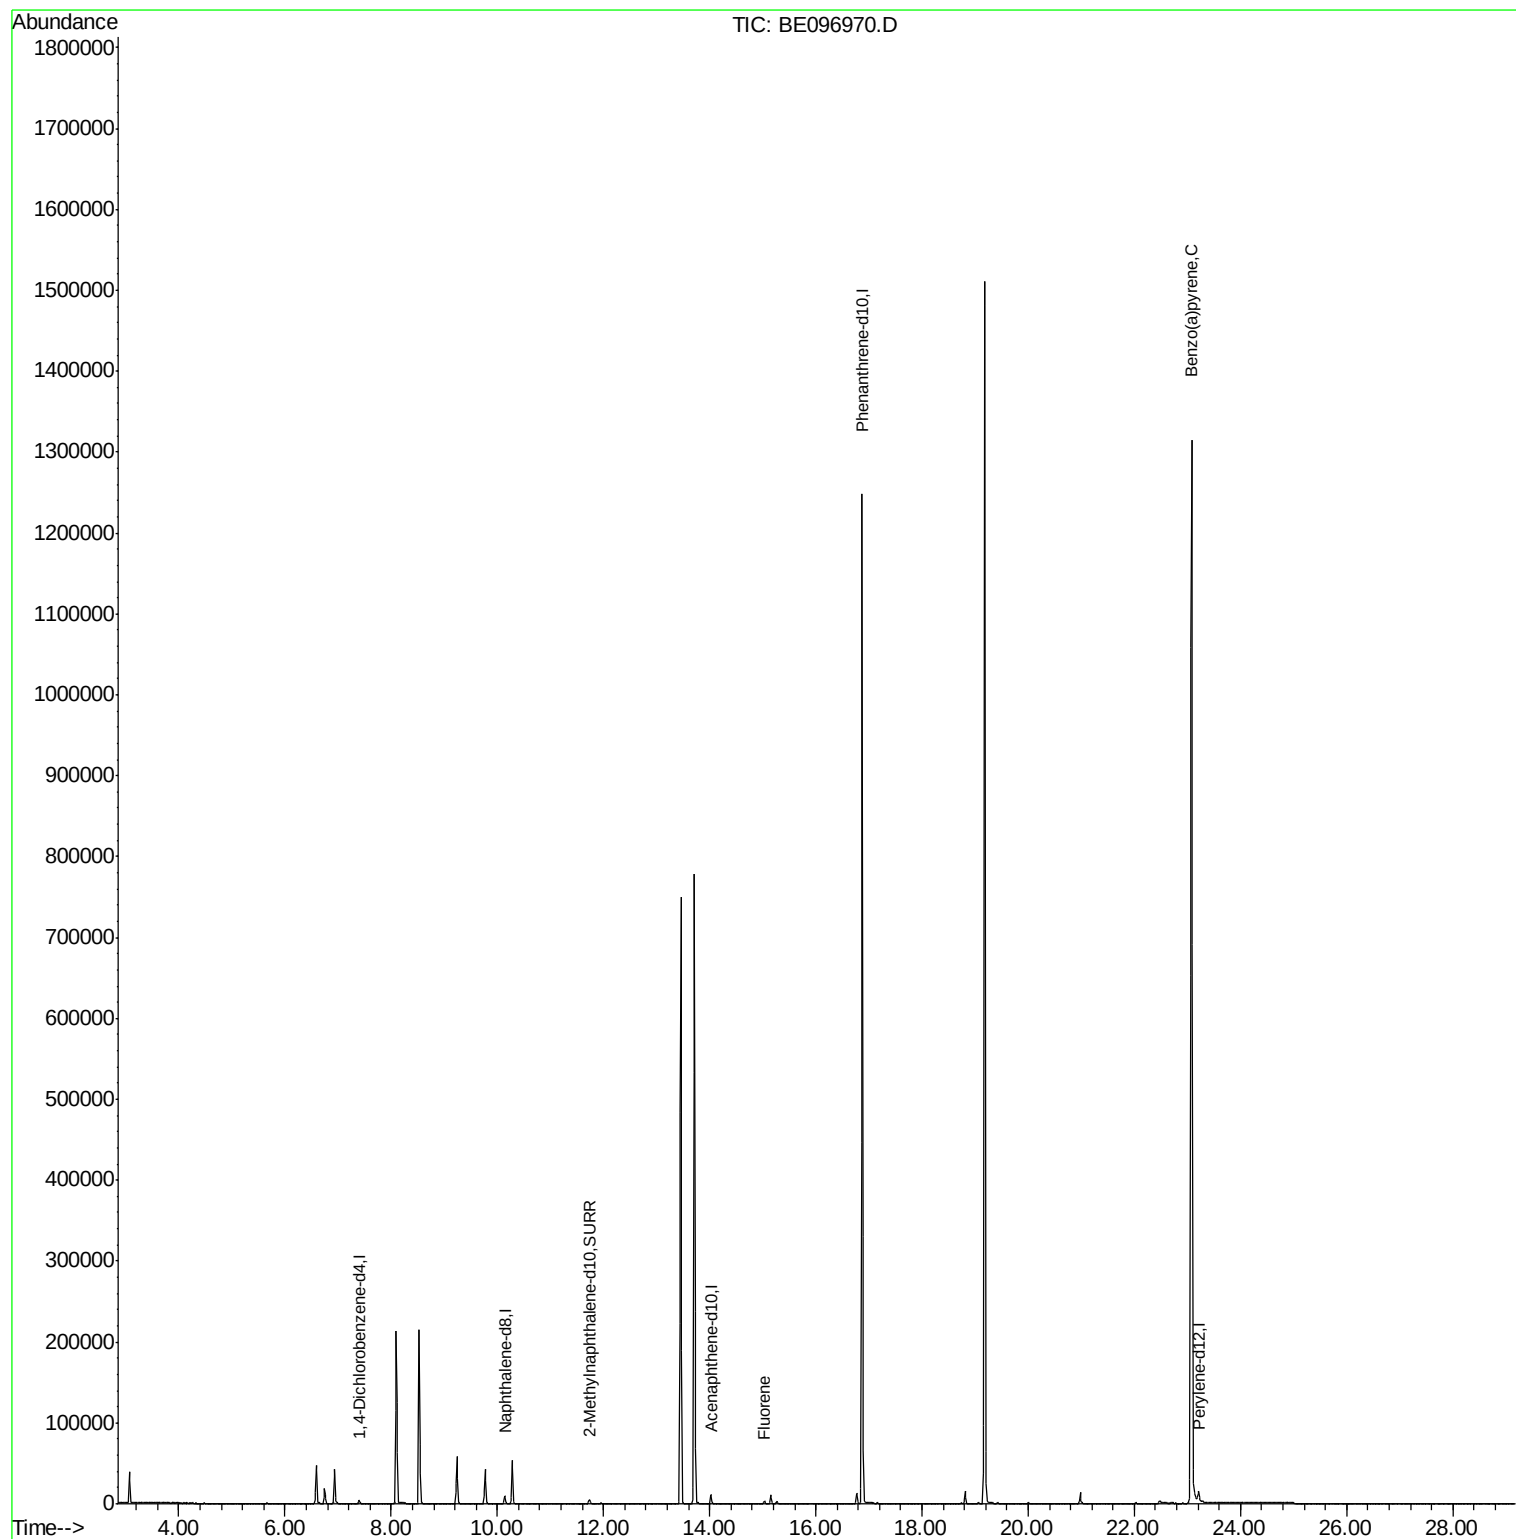

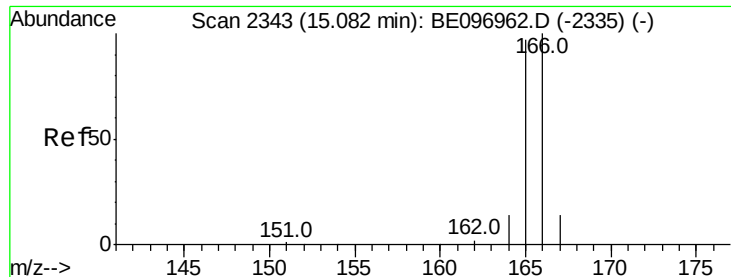

#9

Fluorene

Concen: 0.091 ng/ul

RT: 15.03 min Scan# 2334

Delta R.T. -0.05 min

Lab File: BE096970.D

Acq: 17 Jul 2018 22:58

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 1999

Ion Ratio Lower Upper

166 100

165 7.5 73.4 110.2#




167 38.2 14.6 22.0#

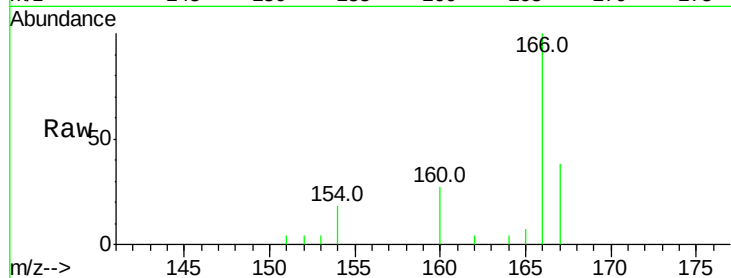

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

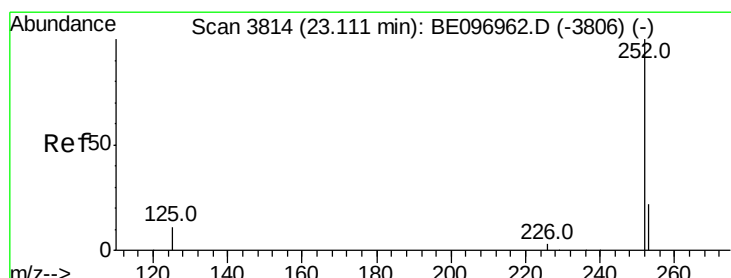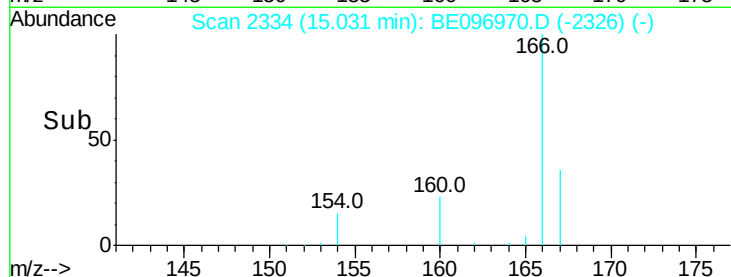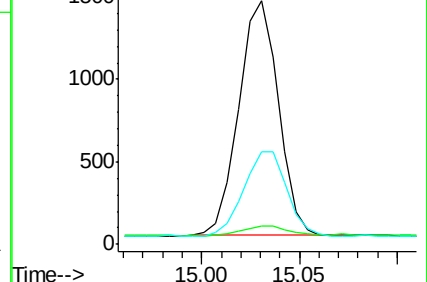

#23

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 23.08 min Scan# 3809

Delta R.T. -0.03 min

Lab File: BE096970.D

Acq: 17 Jul 2018 22:58


Tgt Ion:252 Resp: 5506

Ion Ratio Lower Upper

252 100

253 28.0 28.5 42.7#

125 17.8 18.1 27.1#

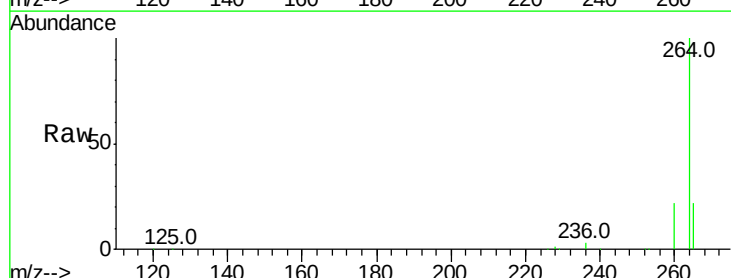

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

