

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
 Data File : BE096971.D
 Acq On : 17 Jul 2018 23:34
 Operator : SJ/JU
 Sample : J3967-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jul 18 03:42:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 03:40:41 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	1969	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	9990	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.03	164	6108	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	1262367	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	26151	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	5605	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.08	252	5289	0.081	ng/ul	Ovalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071718\
Data File : BE096971.D
Acq On : 17 Jul 2018 23:34
Operator : SJ/JU
Sample : J3967-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jul 18 03:42:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE071718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 03:40:41 2018
Response via : Initial Calibration

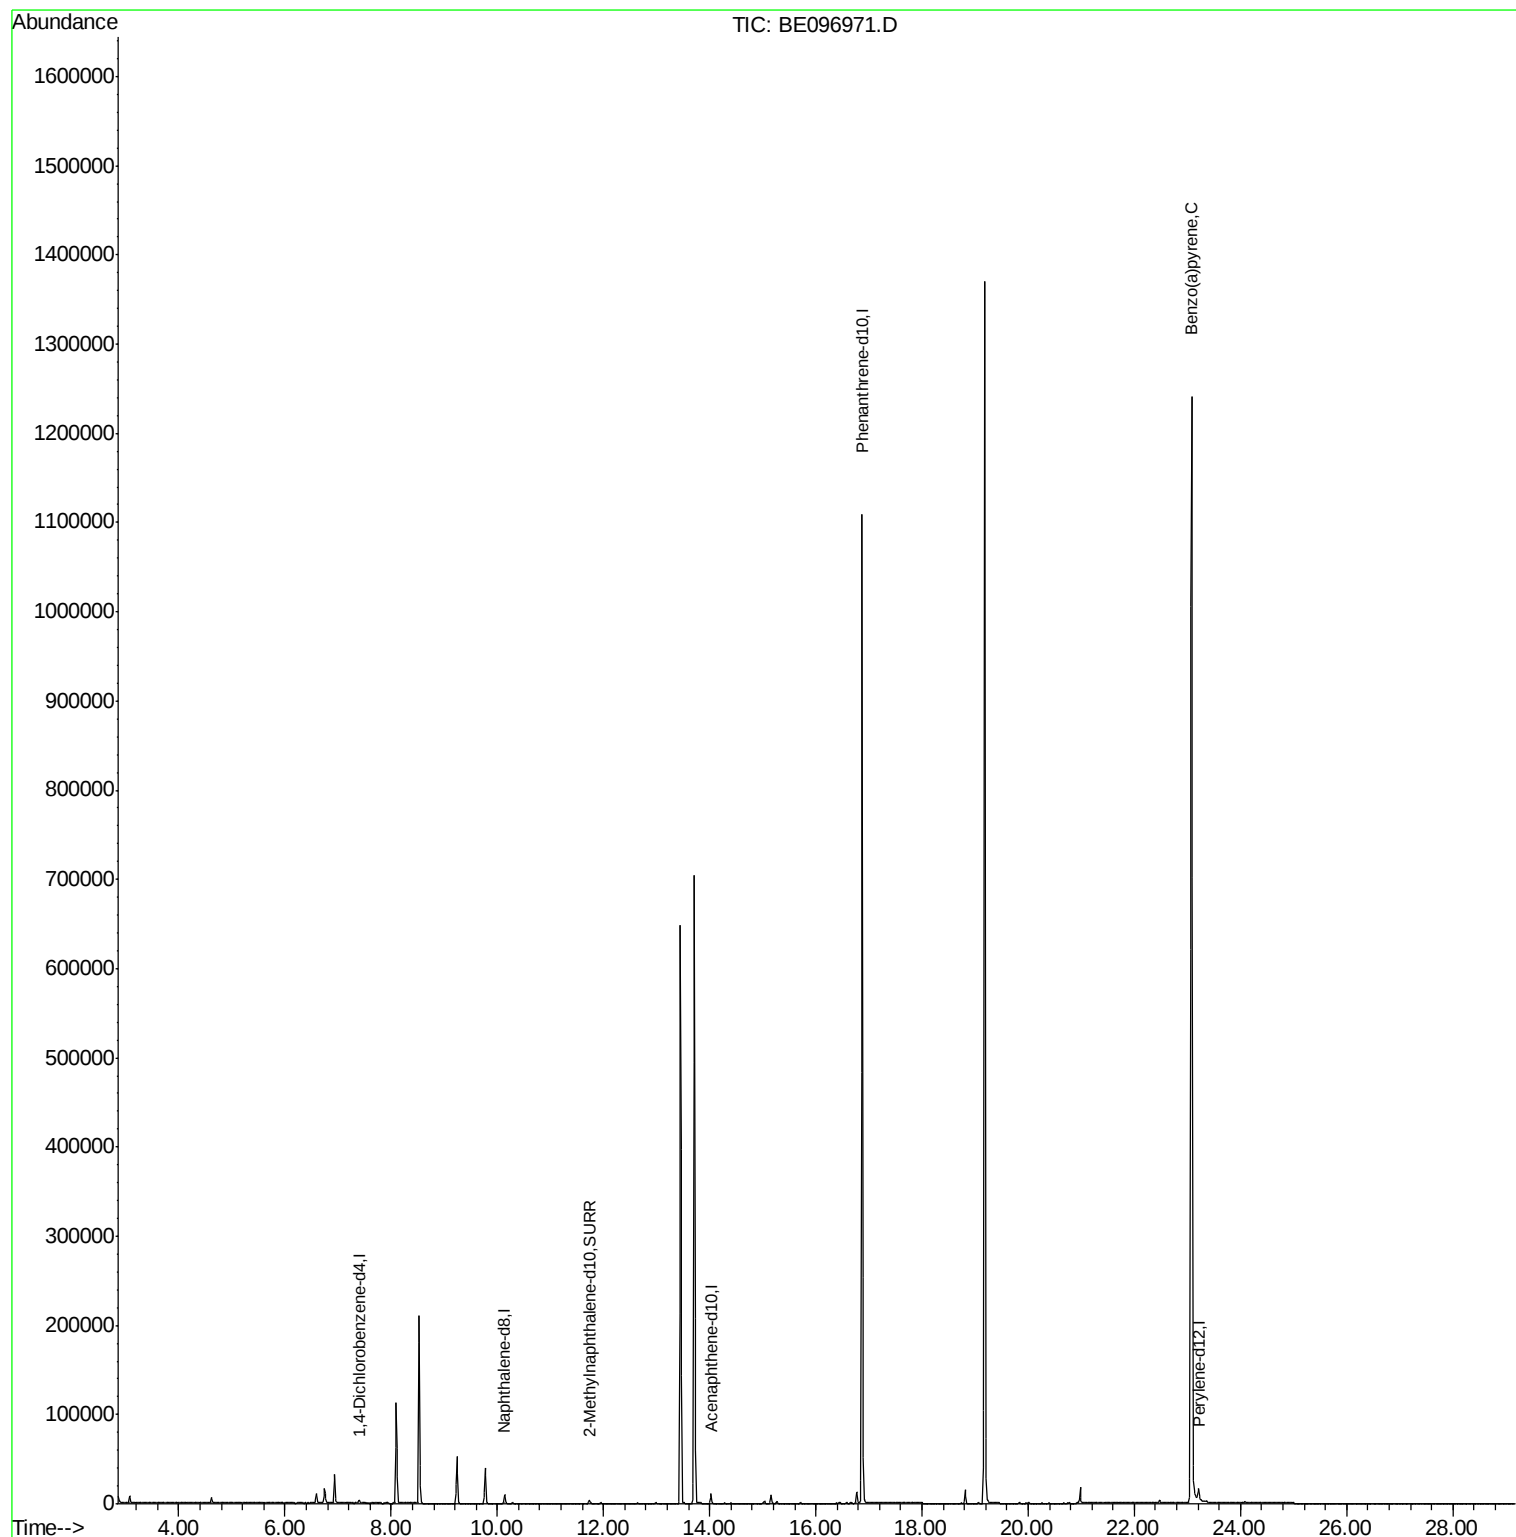

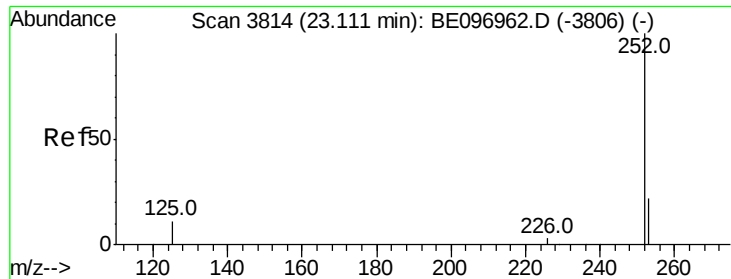

#23

Benzo(a)pyrene

Concen: 0.081 ng/ul

RT: 23.08 min Scan# 3809

Delta R.T. -0.03 min


Lab File: BE096971.D

Acq: 17 Jul 2018 23:34

Instrument :

BNA_E

ClientSampleId :

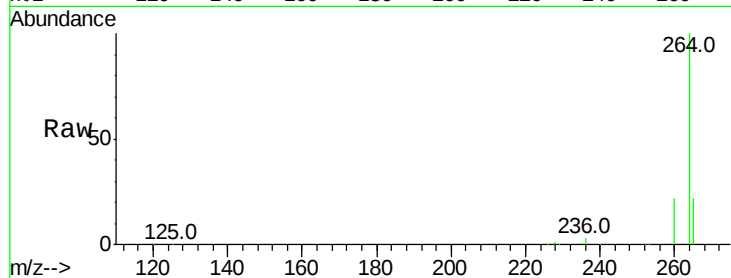

Tot Ion: 252 Resp: 5289

Ion Ratio Lower Upper

252 100

253 30.3 28.5 42.7

125 18.9 18.1 27.1

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

